

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021320\
 Data File : BG044432.D
 Acq On : 14 Feb 2020 00:33
 Operator : CG/JU
 Sample : L1511-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 LAYDOWN-SOFT-AREA

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.010	321	327	334	rBV2	19603	32591	1.83%	0.213%
2	5.486	401	408	420	rBV	642194	1069906	60.19%	6.996%
3	7.079	671	679	698	rBV	665303	1201781	67.61%	7.858%
4	7.907	812	820	828	rBV	317290	554070	31.17%	3.623%
5	8.230	867	875	883	rBV	548145	949223	53.40%	6.207%
6	9.059	1008	1016	1032	rBV	394637	763239	42.94%	4.991%
7	10.704	1286	1296	1315	rBV	449725	828012	46.58%	5.414%
8	13.166	1707	1715	1726	rBV	1071402	1654104	93.05%	10.816%
9	14.000	1851	1857	1866	rVB	31101	54082	3.04%	0.354%
10	14.546	1943	1950	1958	rBV	683712	1111173	62.51%	7.266%
11	16.033	2196	2203	2219	rBV	745414	1187716	66.82%	7.766%
12	17.290	2410	2417	2422	rBV	789630	1221023	68.69%	7.984%
13	17.325	2422	2423	2429	rVB	54831	63268	3.56%	0.414%
14	18.360	2594	2599	2602	rBV3	20394	34673	1.95%	0.227%
15	19.341	2762	2766	2773	rBV	95359	133789	7.53%	0.875%
16	19.699	2824	2827	2833	rVB	85703	120160	6.76%	0.786%
17	19.905	2856	2862	2868	rBV	1340738	1777612	100.00%	11.623%
18	21.532	3133	3139	3145	rBV2	755750	1253299	70.50%	8.195%
19	24.623	3658	3665	3682	rVB2	418504	1283976	72.23%	8.395%


Sum of corrected areas: 15293697

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021320\
Data File : BG044432.D
Acq On : 14 Feb 2020 00:33
Operator : CG/JU
Sample : L1511-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
LAYDOWN-SOFT-AREA

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

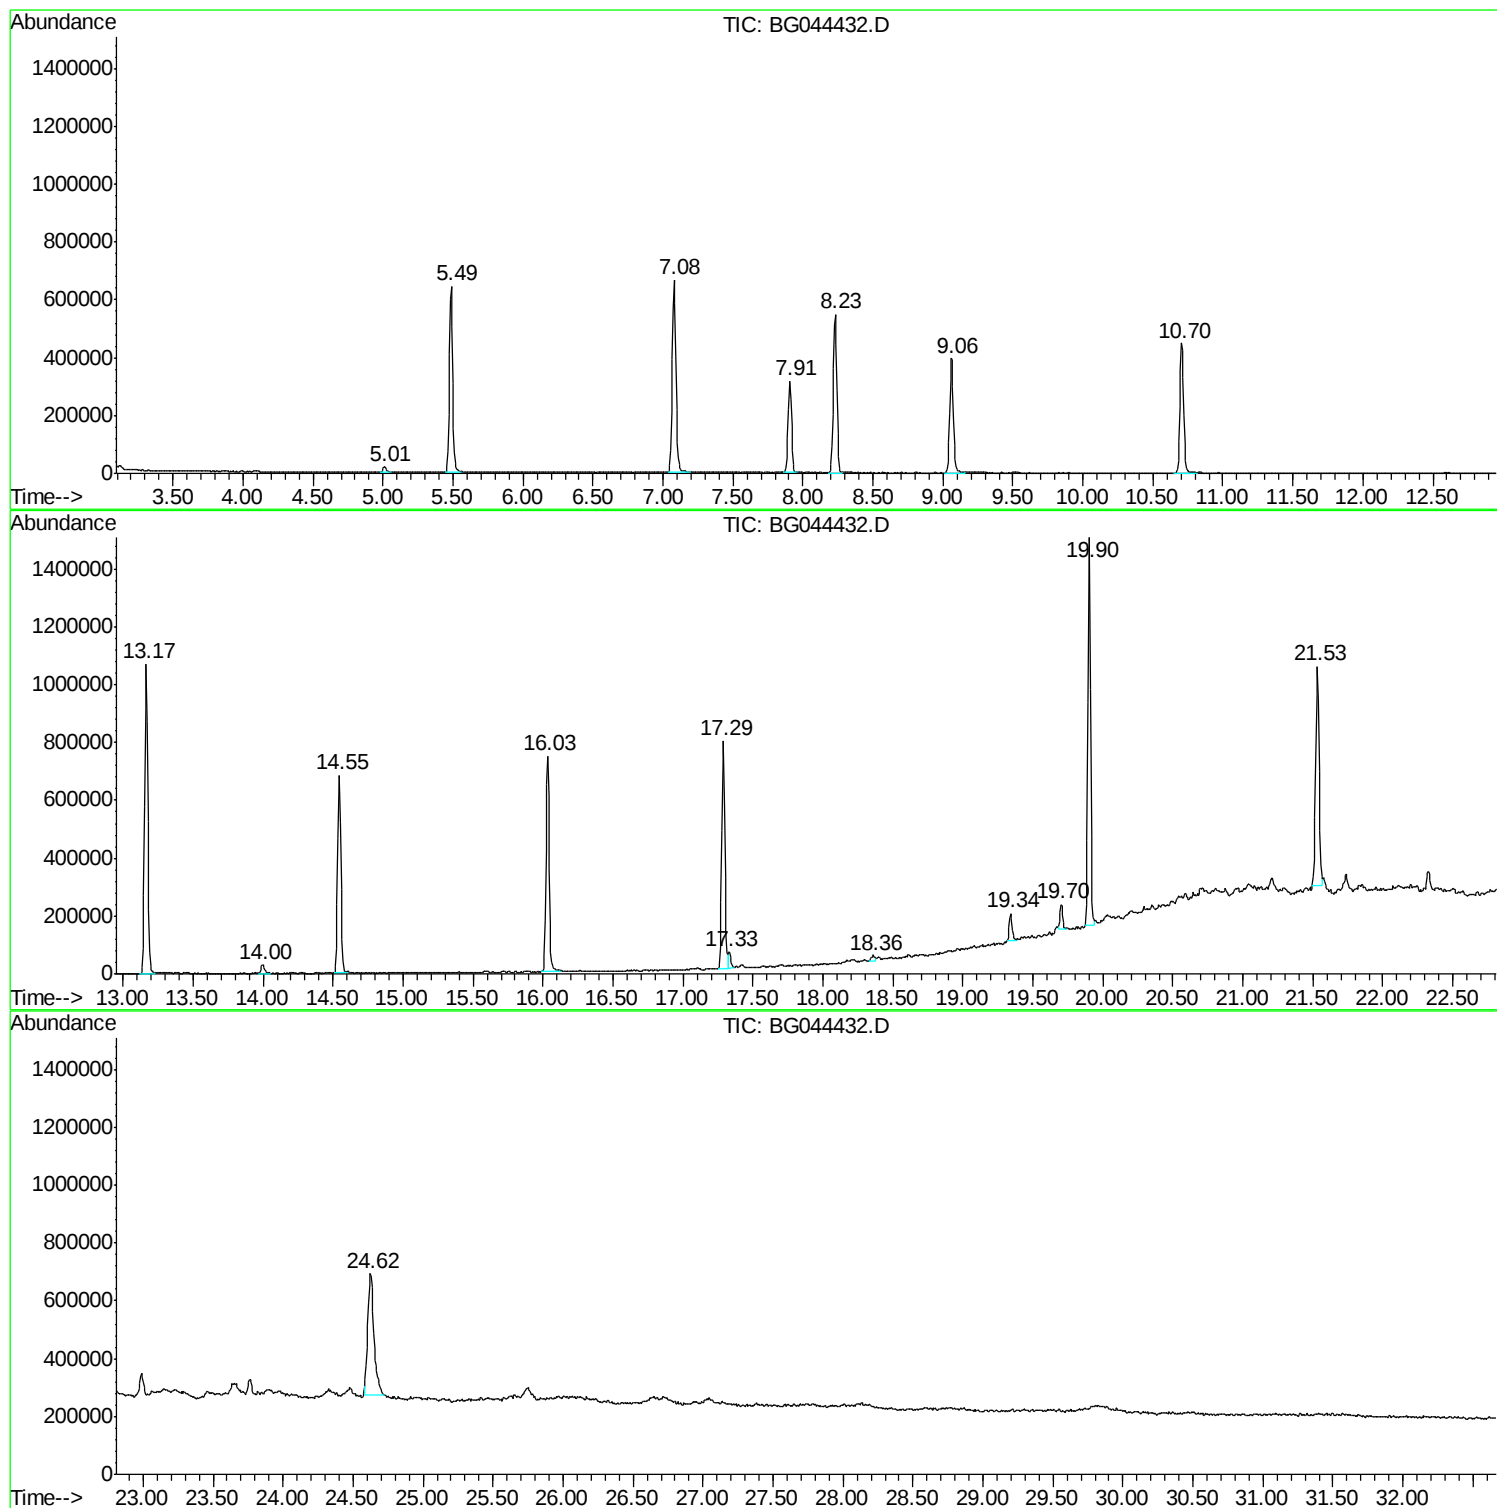

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021320\
Data_File : BG044432.D
Acq_On : 14 Feb 2020 00:333
Operator : CG/JUU
Sample : L1511-011
Misc :
ALS_Vial : 14 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
LAYDOWN-SOFT-AREA

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
