


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021320\
 Data File : BG044419.D
 Acq On : 13 Feb 2020 15:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 10 16:11:50 2020

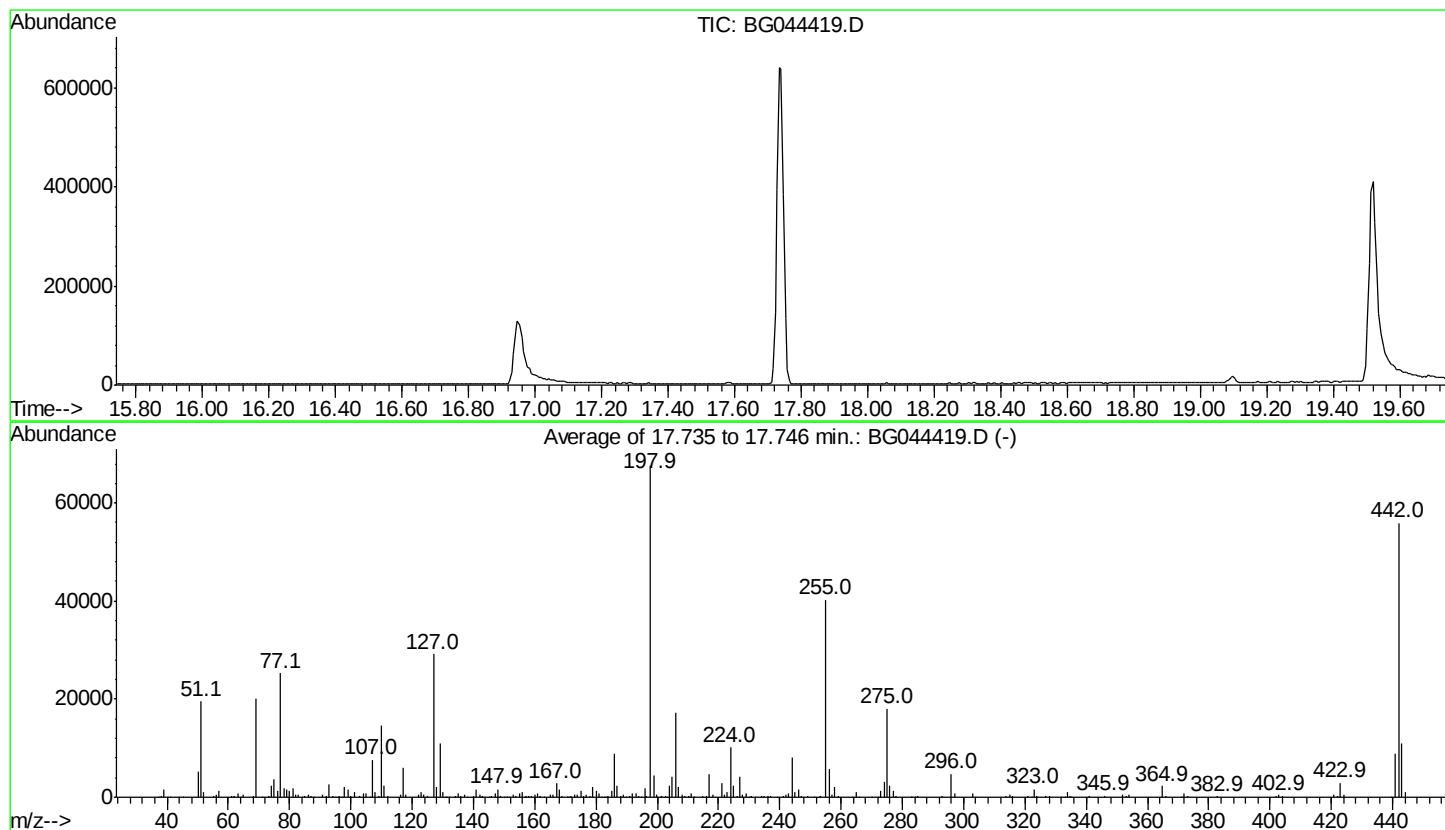

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	19578	PASS
68	69	0.00	2	1.6	326	PASS
69	198	0.00	100	29.8	20160	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.1	29128	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67616	PASS
199	198	5	9	6.7	4507	PASS
275	198	10	60	26.7	18035	PASS
365	198	1	100	3.4	2329	PASS
441	198	0.01	100	13.2	8914	PASS
442	198	50	100	82.8	55981	PASS
443	442	15	24	19.5	10916	PASS