
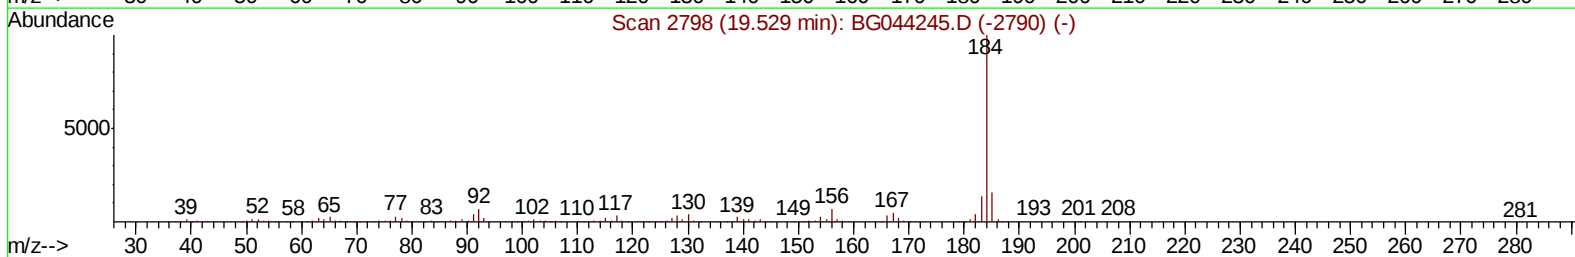
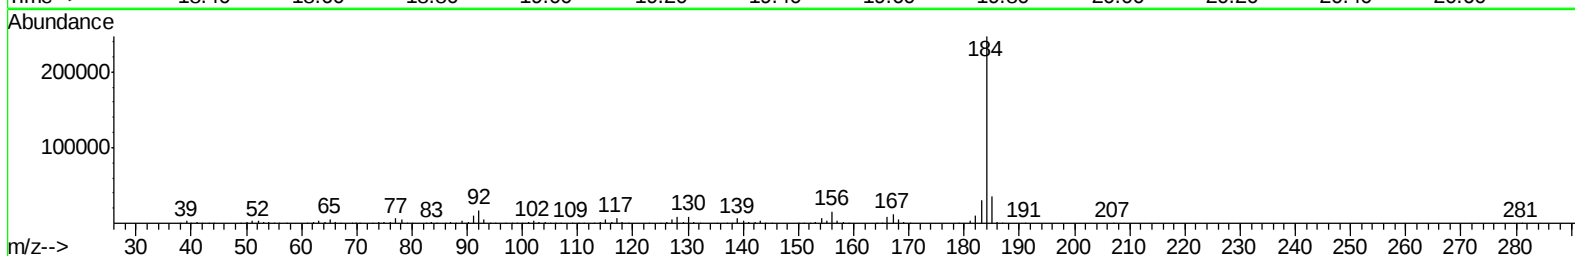


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021420\
 Data File : BG044436.D
 Acq On : 14 Feb 2020 13:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 17 00:38:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 10 16:11:50 2020
 Response via : Initial Calibration

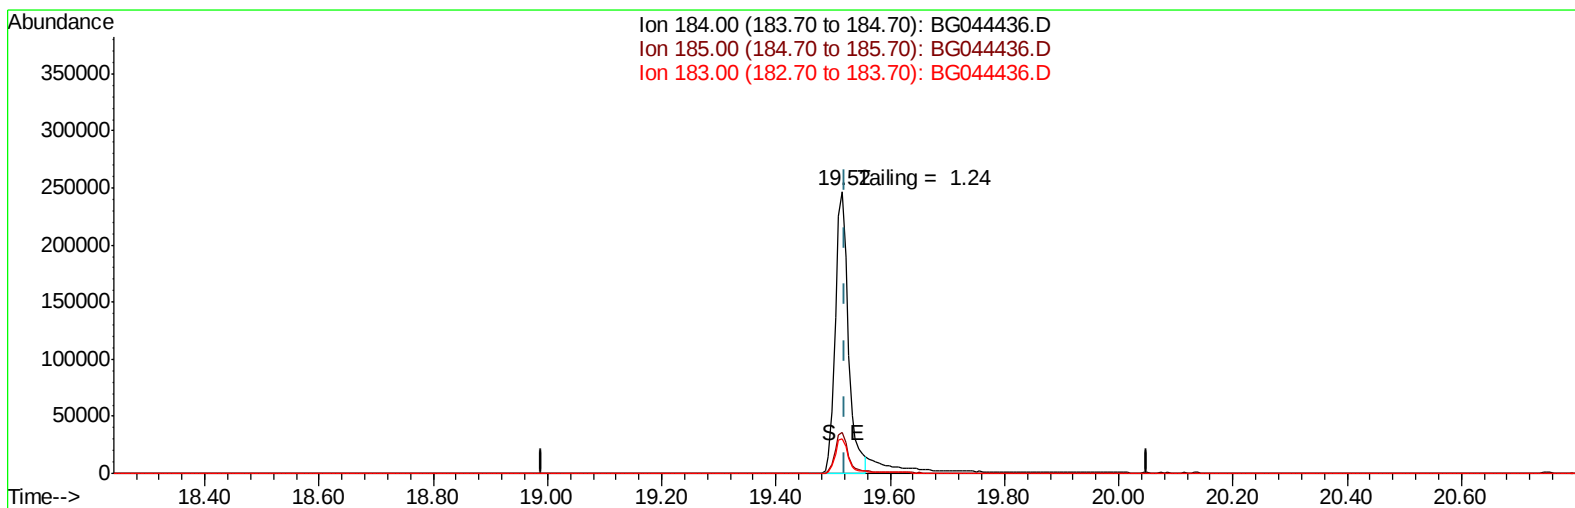

TIC: BG044436.D

(77) Benzidine




19.516min (-0.006) 0.00ng

response 439364

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	14.47
183.00	13.50	12.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021420\
 Data File : BG044436.D
 Acq On : 14 Feb 2020 13:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 17 00:38:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 10 16:11:50 2020
 Response via : Initial Calibration

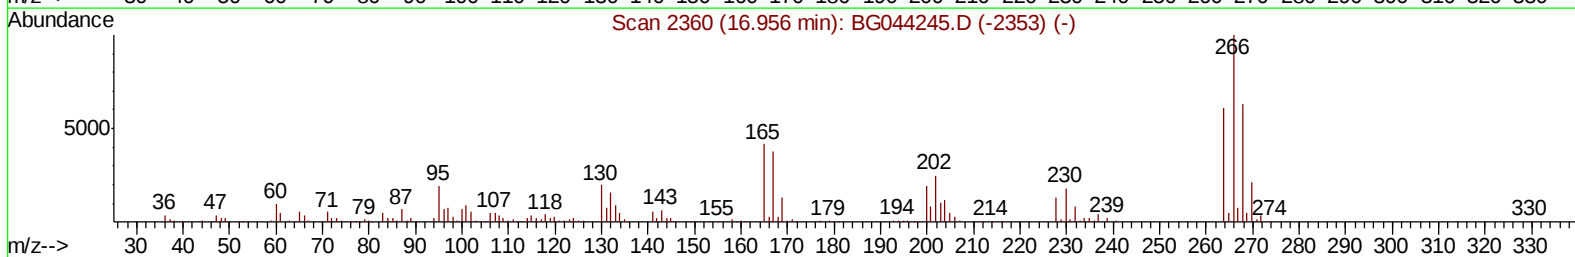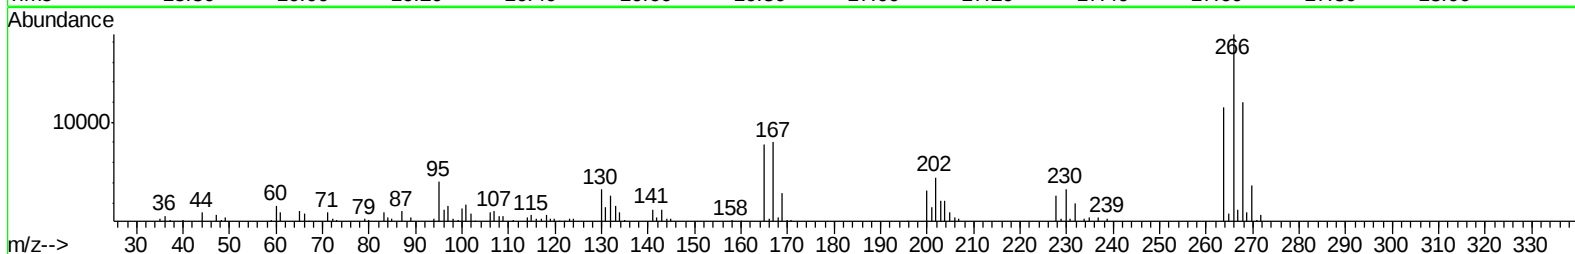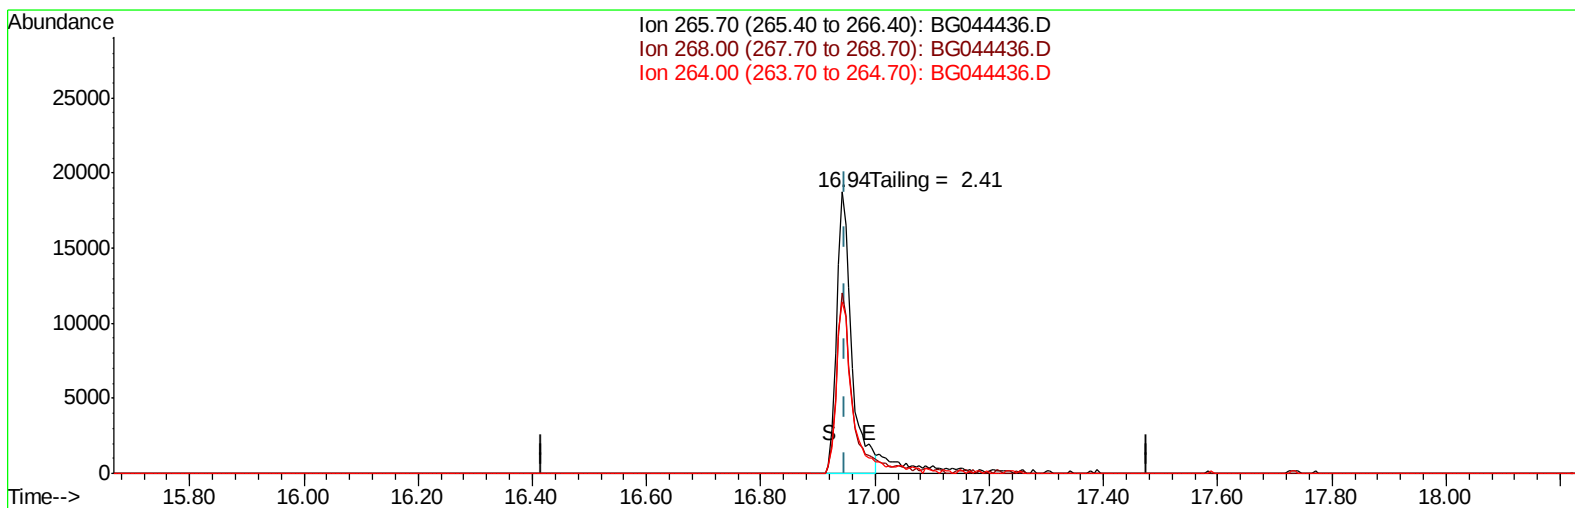

TIC: BG044436.D

(70) Pentachlorophenol (C)

16.942min (-0.006) 13808.75ng

response 37430

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	64.12
264.00	60.90	60.99
0.00	0.00	0.00