


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021420\
 Data File : BG044436.D
 Acq On : 14 Feb 2020 13:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 10 16:11:50 2020

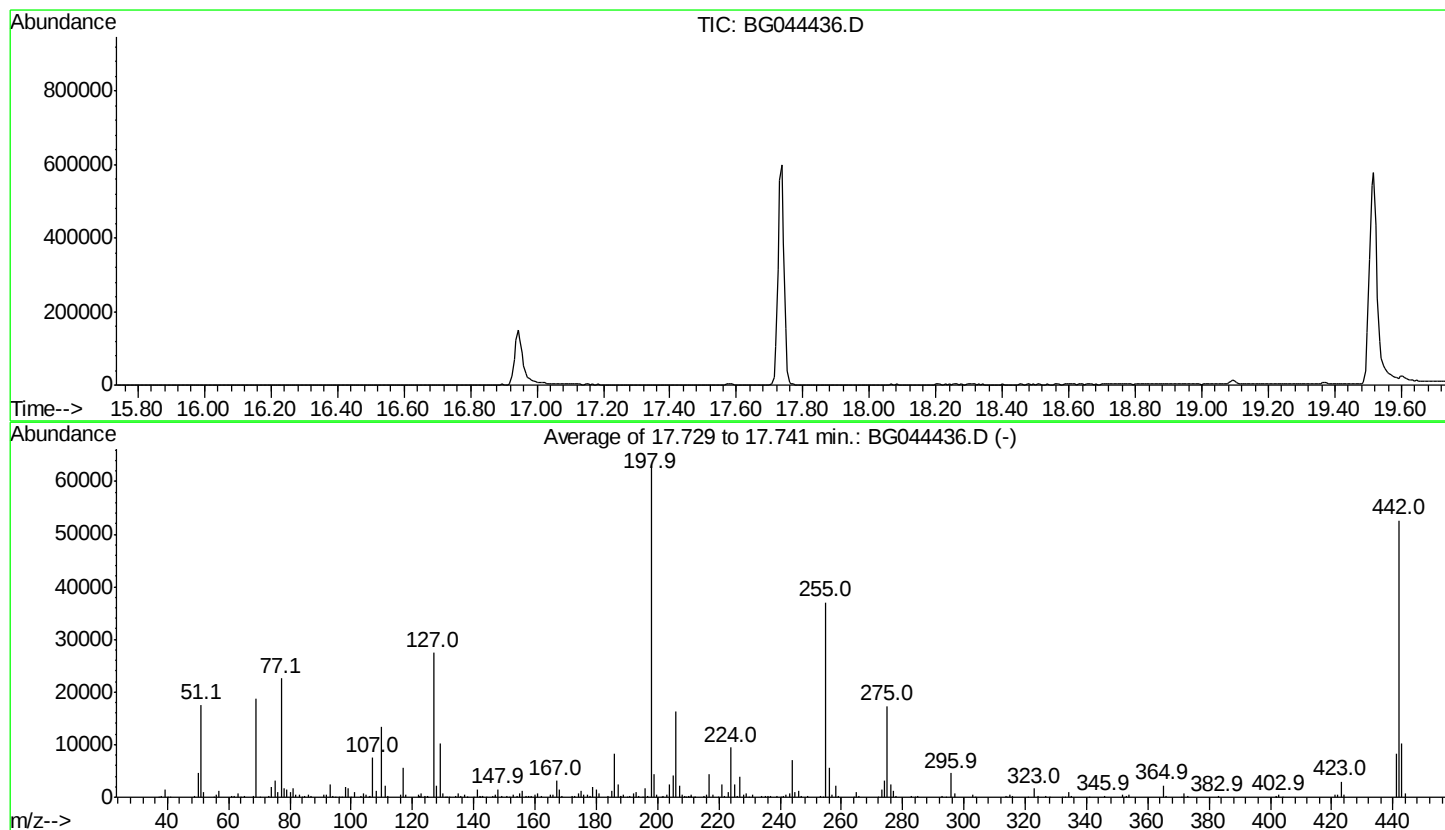

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	17582	PASS
68	69	0.00	2	1.2	227	PASS
69	198	0.00	100	29.6	18681	PASS
70	69	0.00	2	0.3	57	PASS
127	198	10	80	43.6	27480	PASS
197	198	0.00	2	0.4	242	PASS
198	198	100	100	100.0	63024	PASS
199	198	5	9	7.0	4416	PASS
275	198	10	60	27.5	17346	PASS
365	198	1	100	3.6	2259	PASS
441	198	0.01	100	13.3	8389	PASS
442	198	50	100	83.5	52594	PASS
443	442	15	24	19.5	10271	PASS