
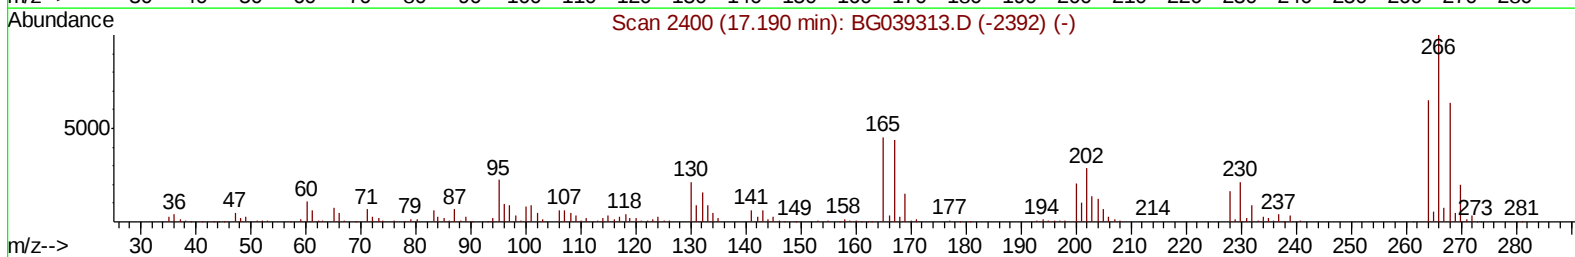
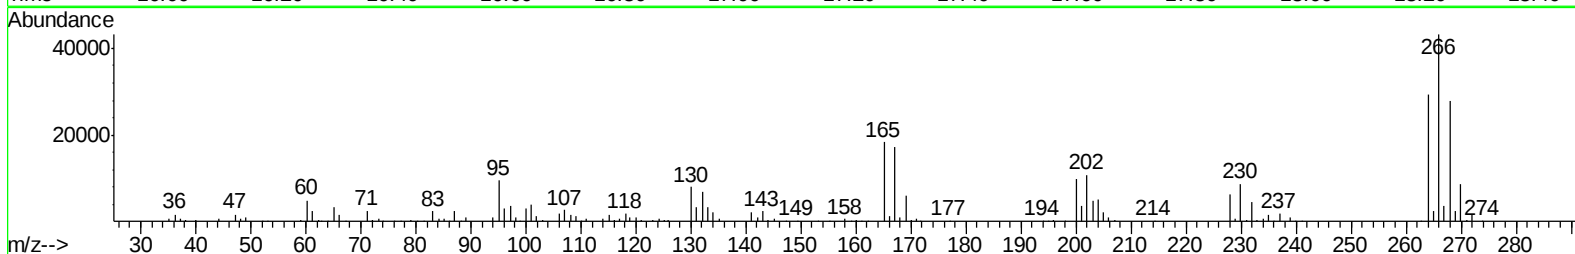


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021519\
Data File : BG039523.D
Acq On : 15 Feb 2019 14:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 03:31:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

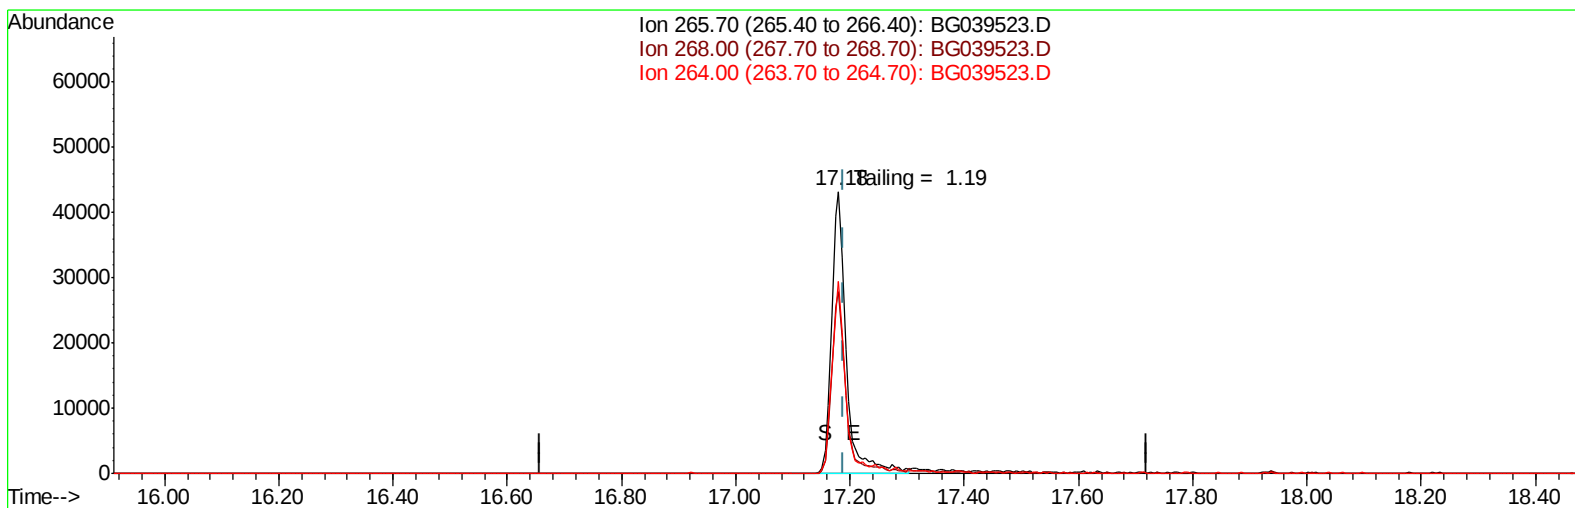

TIC: BG039523.D

(70) Pentachlorophenol (C)




17.180min (-0.010) 47541.64ng

response 74291

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.64
264.00	65.10	68.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021519\
Data File : BG039523.D
Acq On : 15 Feb 2019 14:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 03:31:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

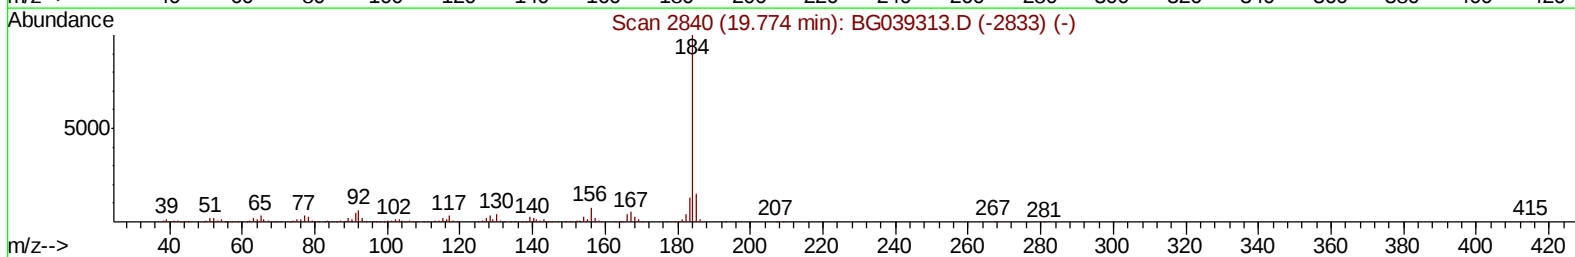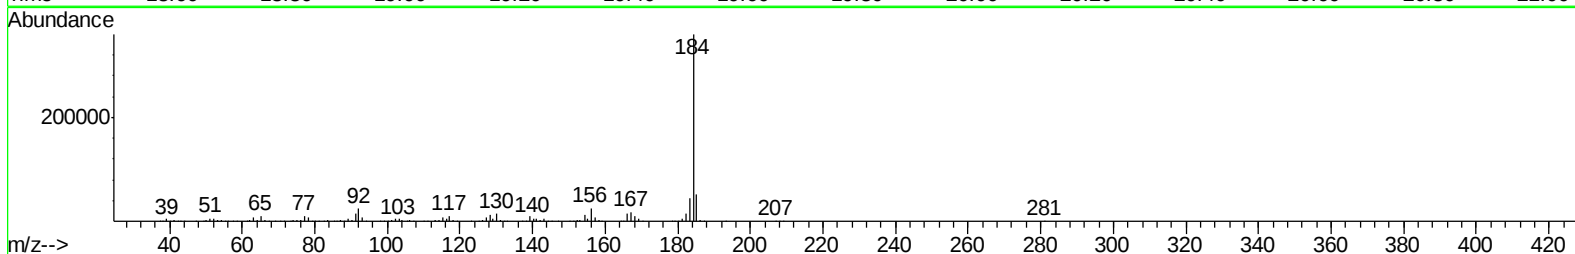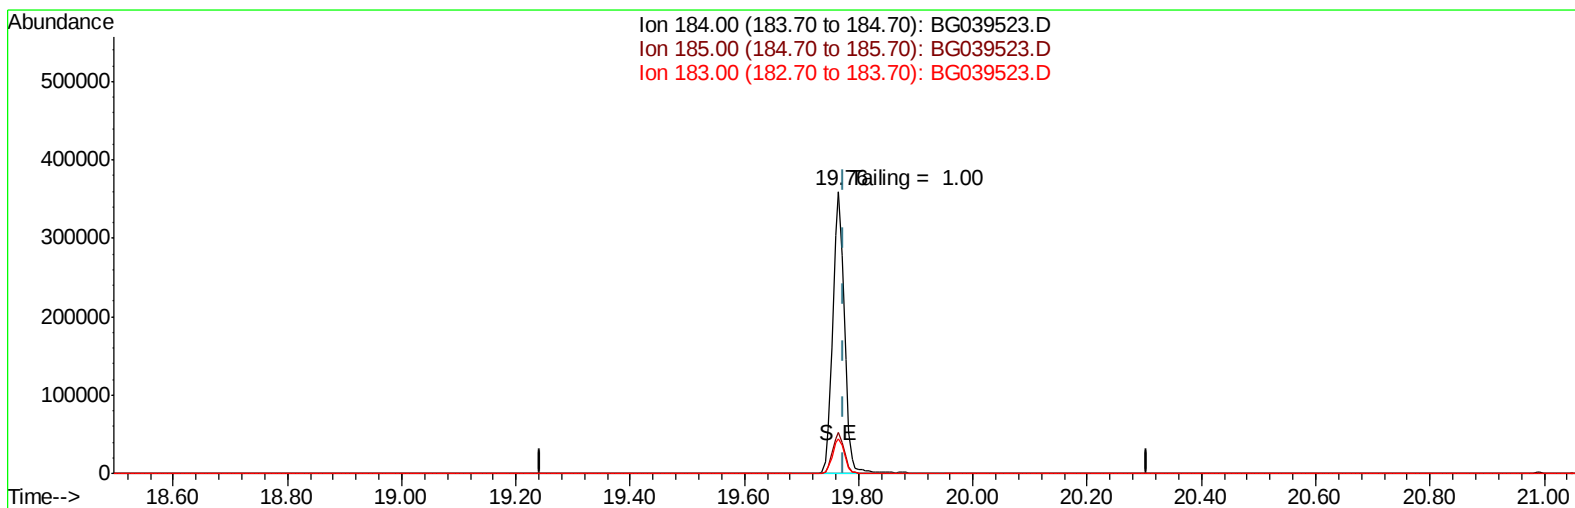

TIC: BG039523.D

(77) Benzidine

19.765min (-0.010) 52541.77ng

response 503003

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.34
183.00	13.20	12.45
0.00	0.00	0.00