

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021519\
 Data File : BG039530.D
 Acq On : 15 Feb 2019 20:44
 Operator : JU/SJ
 Sample : K1358-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TR-04-021419

Quant Time: Feb 16 03:31:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	48549	20.00	ng	0.00
21) Naphthalene-d8	10.99	136	215160	20.00	ng	-0.02
39) Acenaphthene-d10	14.79	164	154743	20.00	ng	-0.02
64) Phenanthrene-d10	17.54	188	379739	20.00	ng	-0.02
76) Chrysene-d12	21.83	240	402352	20.00	ng	-0.02
87) Perylene-d12	25.22	264	400098	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	416277	146.75	ng	0.00
7) Phenol-d6	7.32	99	569480	136.39	ng	0.00
23) Nitrobenzene-d5	9.35	82	393822	114.35	ng	-0.01
42) 2,4,6-Tribromophenol	16.28	330	215479	129.31	ng	0.00
45) 2-Fluorobiphenyl	13.42	172	958309	88.84	ng	-0.02
79) Terphenyl-d14	20.13	244	1620080	85.23	ng	-0.02


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021519\
Data File : BG039530.D
Acq On : 15 Feb 2019 20:44
Operator : JU/SJ
Sample : K1358-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TR-04-021419

Quant Time: Feb 16 03:31:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

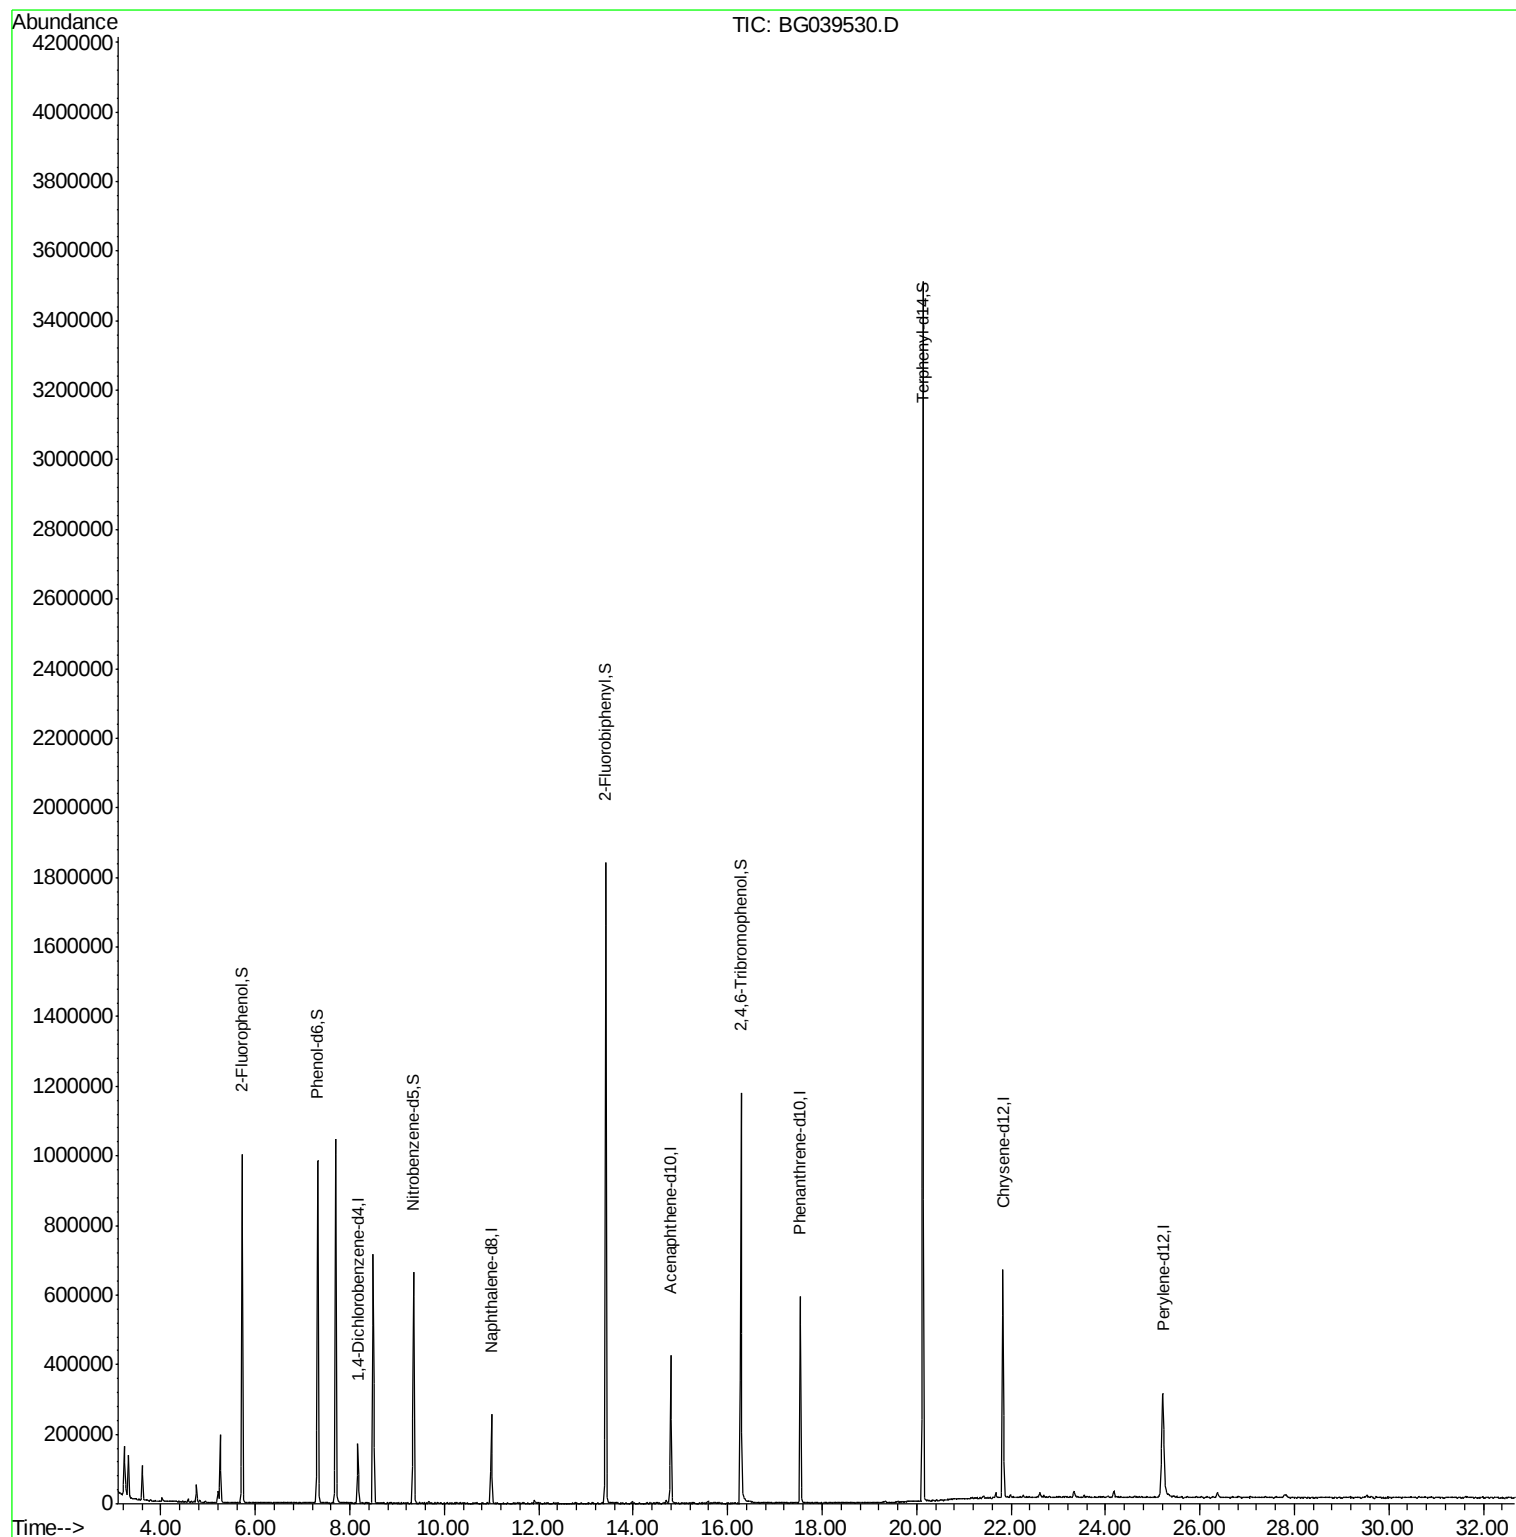




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.17 min Scan# 866
Delta R.T. -0.01 min
Lab File: BG039530.D
Acq: 15 Feb 2019 20:44

Instrument :
BNA_G
ClientSampleId :
TR-04-021419

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.4	123.7	185.5
115	61.2	45.9	68.9



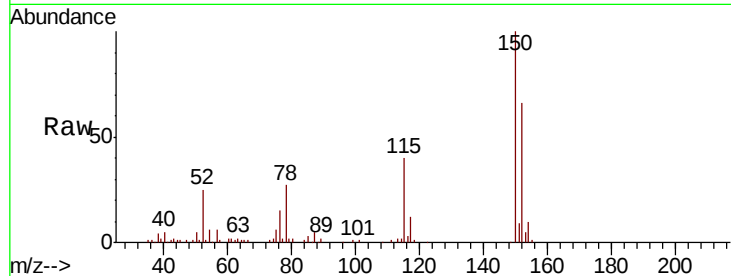


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

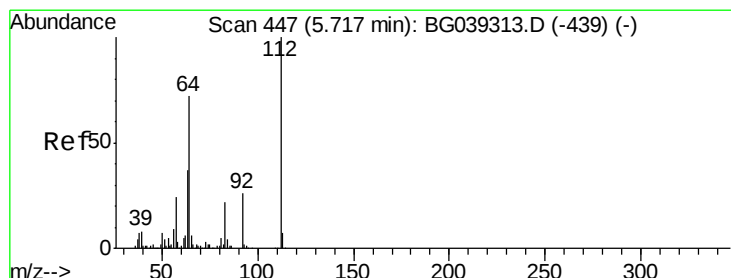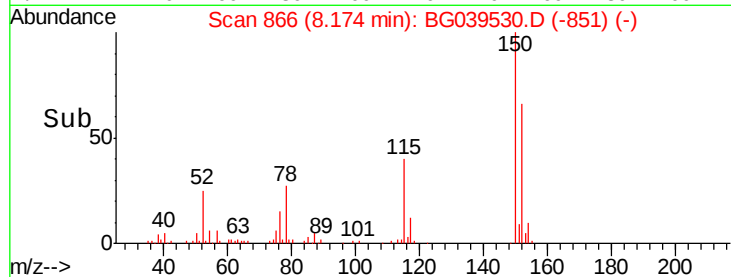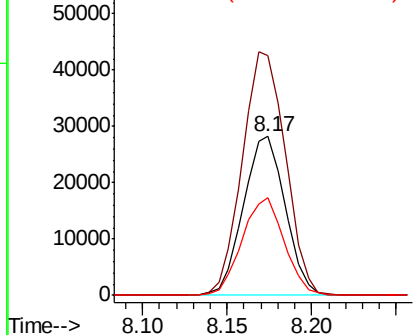

#5

2-Fluorophenol
Concen: 146.751 ng
RT: 5.72 min Scan# 448
Delta R.T. 0.00 min
Lab File: BG039530.D
Acq: 15 Feb 2019 20:44

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.6	57.8	86.8
63	36.9	29.8	44.6


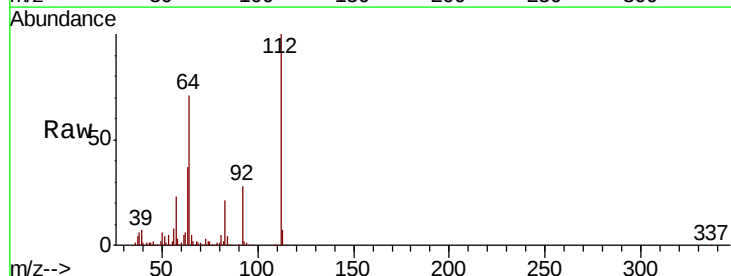


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG0

Ion 63.00 (62.70 to 63.70): BG0

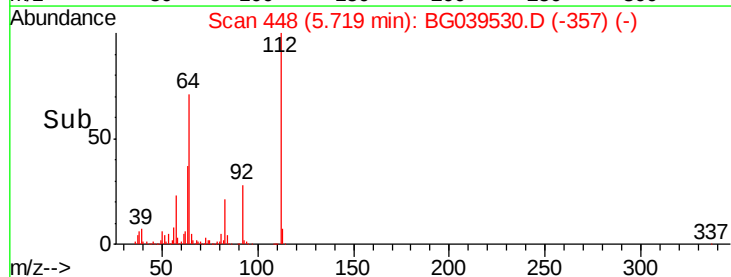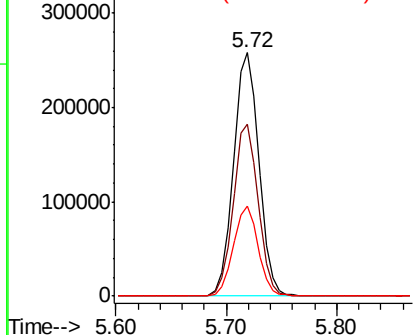



#7

Phenol-d6

Concen: 136.388 ng

RT: 7.32 min Scan# 720

Delta R.T. -0.00 min

Lab File: BG039530.D

Acq: 15 Feb 2019 20:44

Instrument :

BNA_G

ClientSampleId :

TR-04-021419


Tot Ion: 99 Resp: 569480

Ion Ratio Lower Upper




99 100

42 19.8 18.2 27.2

71 36.0 28.0 42.0

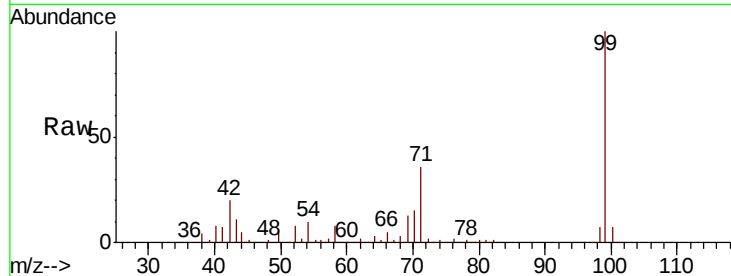

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

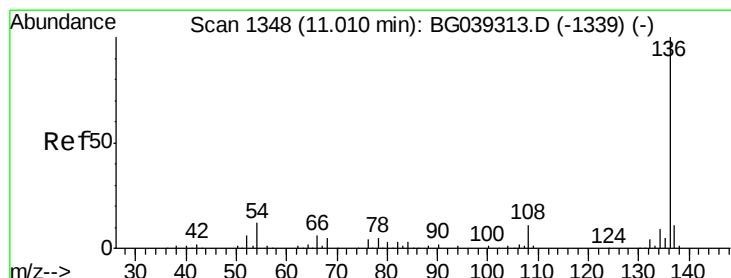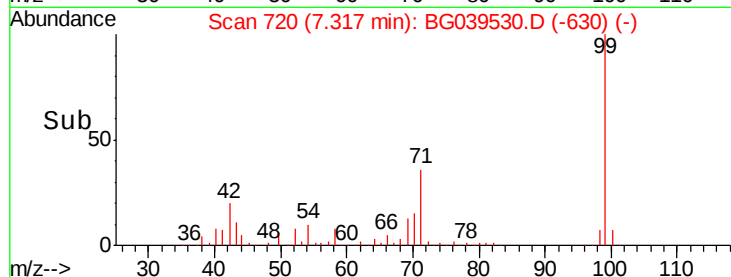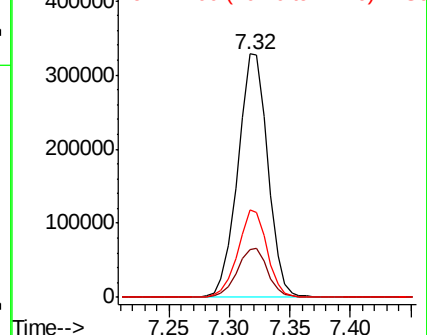

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.99 min Scan# 1346

Delta R.T. -0.02 min

Lab File: BG039530.D

Acq: 15 Feb 2019 20:44

Tgt Ion: 136 Resp: 215160


Ion Ratio Lower Upper

136 100



137 11.1 9.1 13.7

54 10.7 9.4 14.2

68 5.8 4.2 6.4

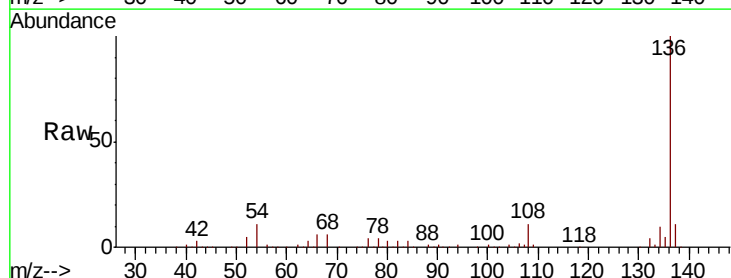

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



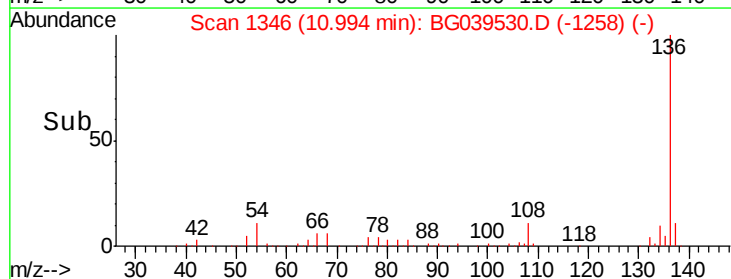
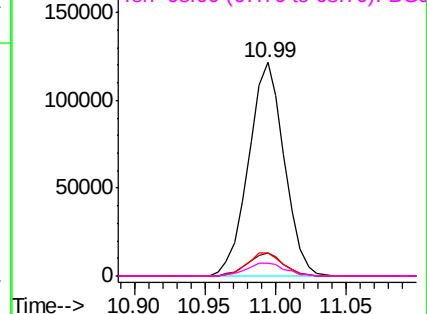




#23
Nitrobenzene-d5
Concen: 114.346 ng
RT: 9.35 min Scan# 1066
Delta R.T. -0.01 min
Lab File: BG039530.D
Acq: 15 Feb 2019 20:44




Instrument :
BNA_G
ClientSampleId :
TR-04-021419

Tot Ion	Ratio	Lower	Upper
82	100		
128	44.3	31.3	46.9
54	59.8	50.9	76.3

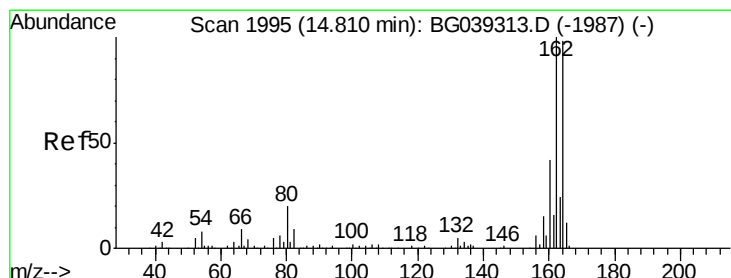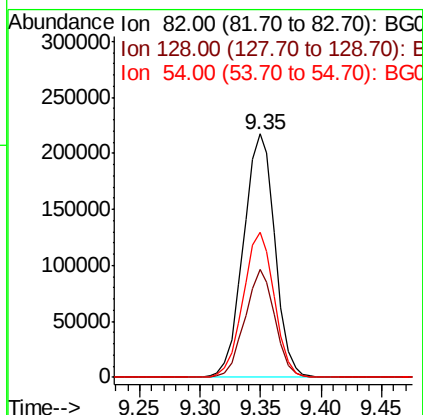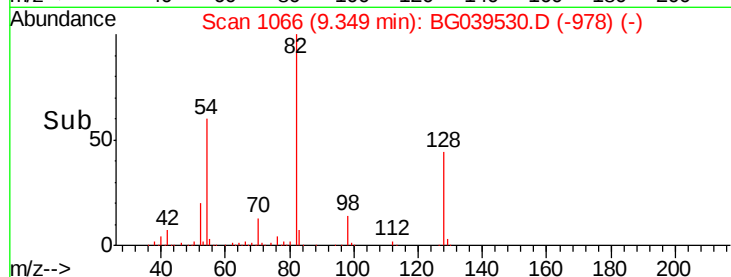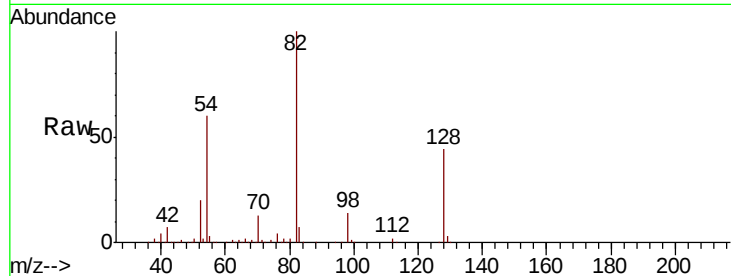

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.79 min Scan# 1993
Delta R.T. -0.02 min
Lab File: BG039530.D
Acq: 15 Feb 2019 20:44

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.1	81.6	122.4
160	44.7	34.2	51.2

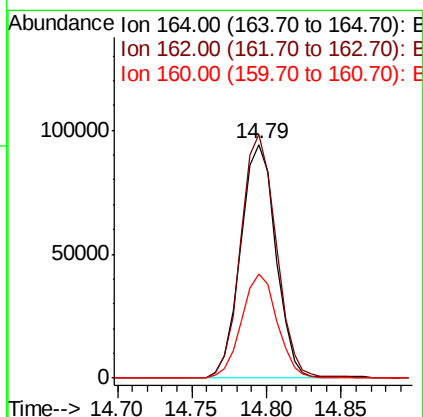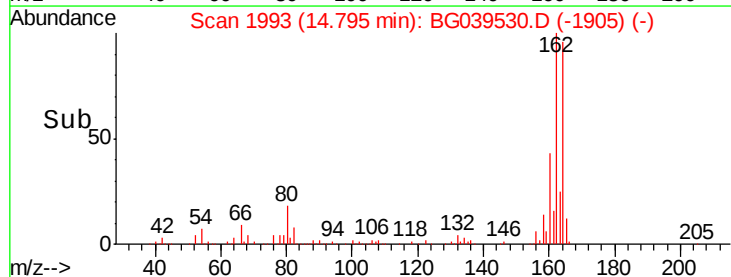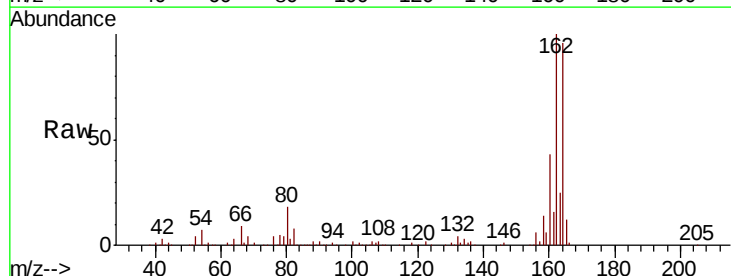






#42
 2,4,6-Tribromophenol
 Concen: 129.315 ng
 RT: 16.28 min Scan# 2246
 Delta R.T. -0.01 min
 Lab File: BG039530.D
 Acq: 15 Feb 2019 20:44

Instrument :
 BNA_G
 ClientSampleId :
 TR-04-021419

Tot Ion:330 Resp: 215479
 Ion Ratio Lower Upper
 330 100
 332 96.3 75.7 113.5
 141 41.4 35.6 53.4

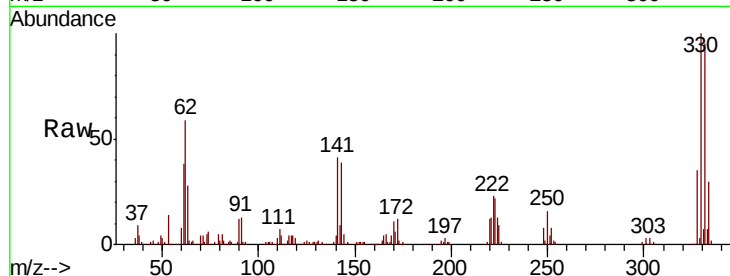


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

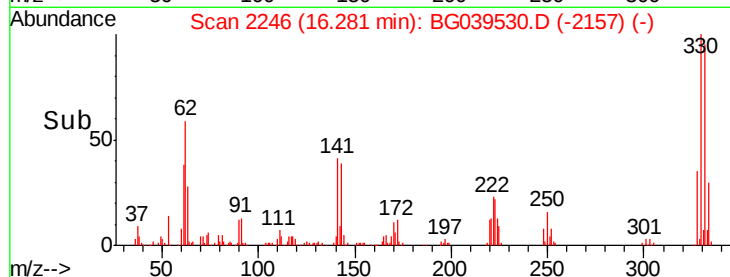
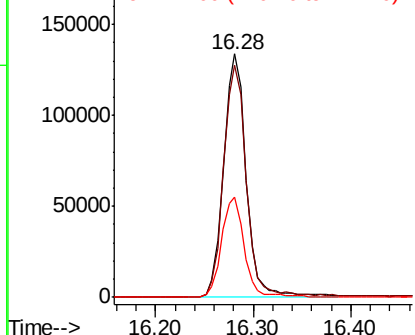



#45
 2-Fluorobiphenyl
 Concen: 88.840 ng
 RT: 13.42 min Scan# 1759
 Delta R.T. -0.02 min
 Lab File: BG039530.D
 Acq: 15 Feb 2019 20:44

Tgt Ion:172 Resp: 958309
 Ion Ratio Lower Upper
 172 100
 171 37.1 30.8 46.2
 170 25.4 20.2 30.4

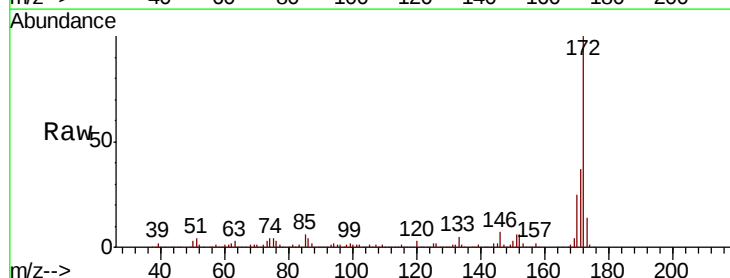

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

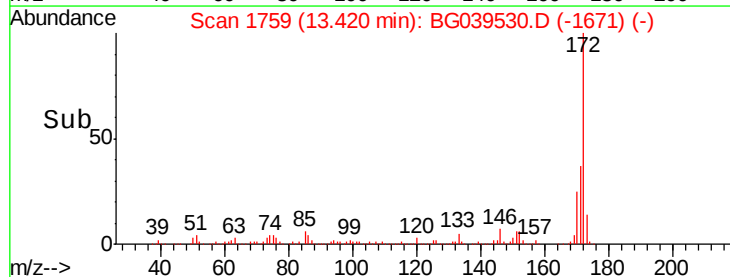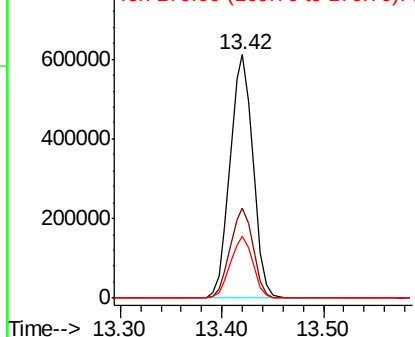

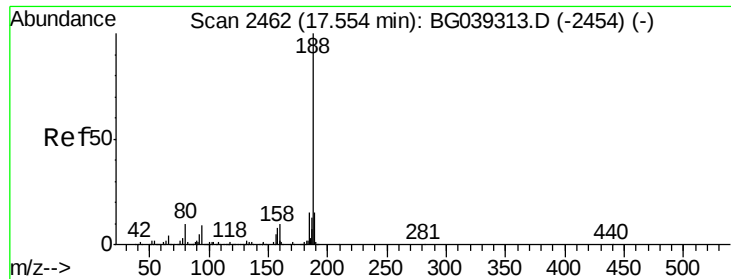

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.54 min Scan# 2460

Delta R.T. -0.02 min

Lab File: BG039530.D

Acq: 15 Feb 2019 20:44

Instrument :

BNA_G

ClientSampleId :

TR-04-021419


Tot Ion:188 Resp: 379739

Ion Ratio Lower Upper

188 100

94 8.1 6.9 10.3




80 8.9 8.1 12.1

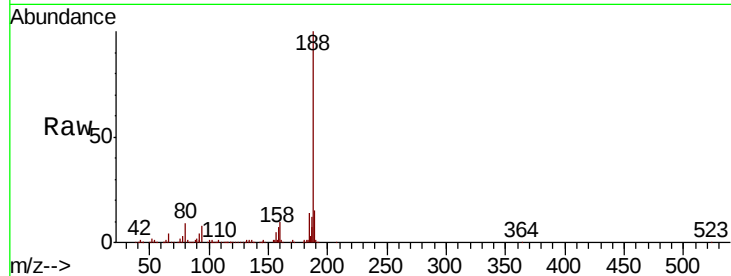

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG0

Ion 80.00 (79.70 to 80.70): BG0

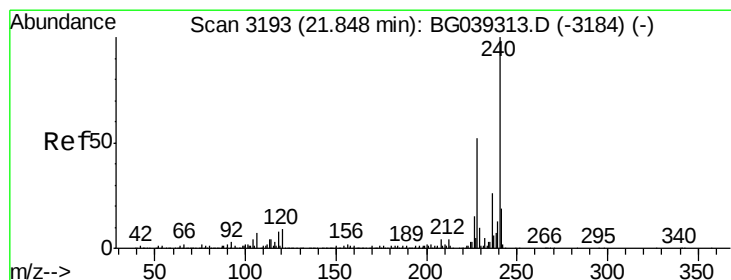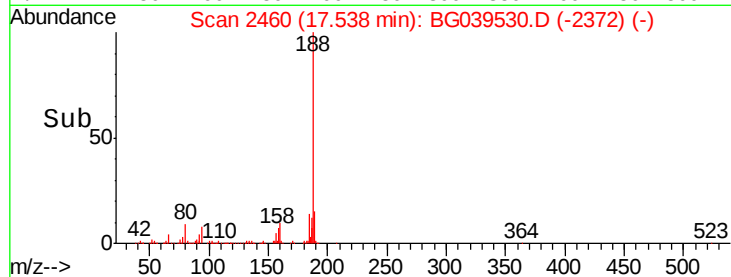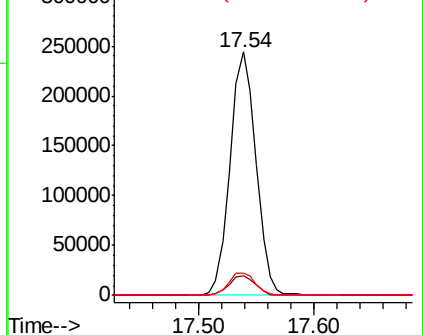

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.83 min Scan# 3190

Delta R.T. -0.02 min

Lab File: BG039530.D

Acq: 15 Feb 2019 20:44


Tgt Ion:240 Resp: 402352

Ion Ratio Lower Upper

240 100

120 8.9 7.0 10.6



236 26.3 21.0 31.4

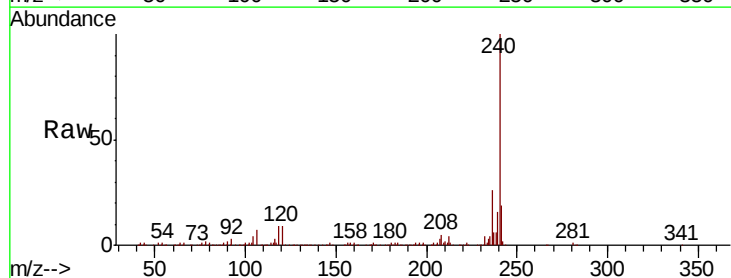

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

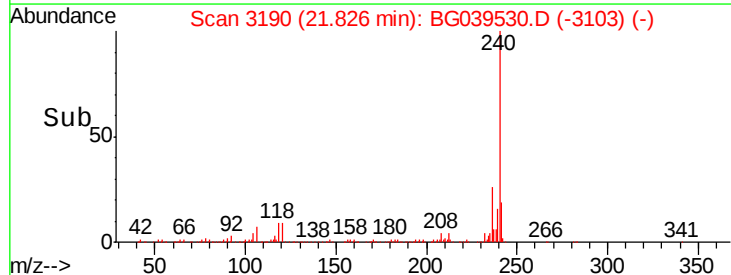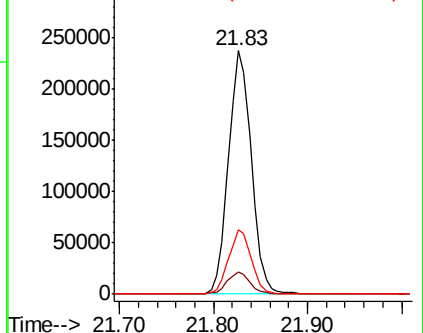



#79

Terphenyl-d14

Concen: 85.229 ng

RT: 20.13 min Scan# 2902

Delta R.T. -0.02 min

Lab File: BG039530.D

Acq: 15 Feb 2019 20:44

Instrument :


BNA_G

ClientSampleId :

TR-04-021419

Tot Ion:244 Resp: 1620080

Ion	Ratio	Lower	Upper
244	100		
212	9.9	7.3	10.9
122	10.1	8.4	12.6



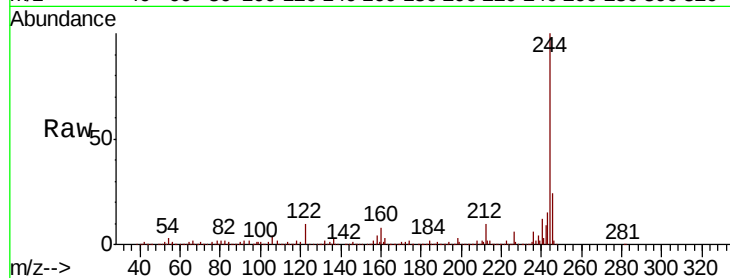


Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

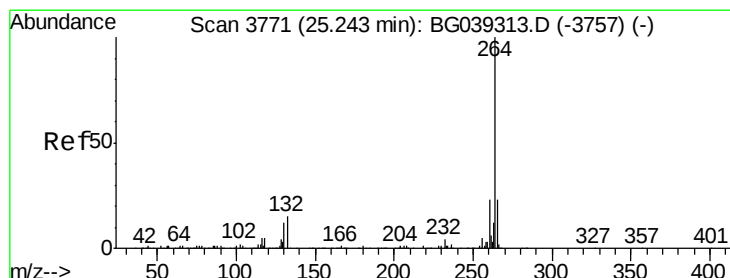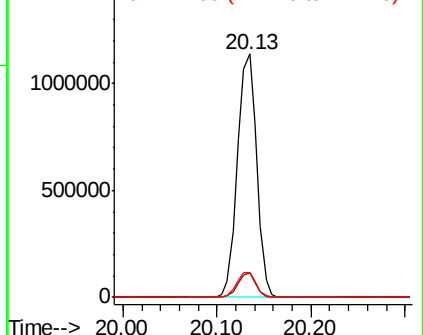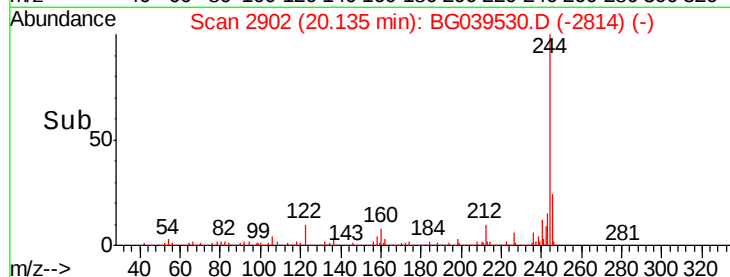

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.22 min Scan# 3767


Delta R.T. -0.03 min

Lab File: BG039530.D

Acq: 15 Feb 2019 20:44

Tgt Ion:264 Resp: 400098

Ion	Ratio	Lower	Upper
264	100		
260	23.5	18.2	27.4
265	21.0	18.5	27.7

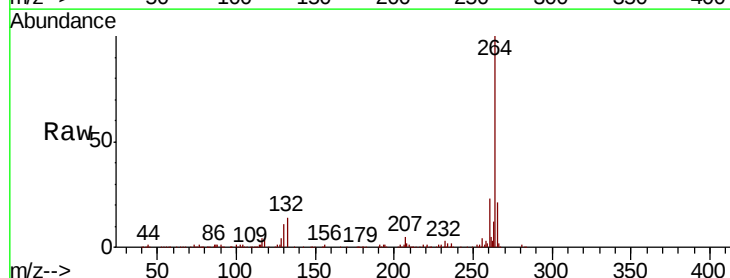

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

