


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021519\
 Data File : BG039523.D
 Acq On : 15 Feb 2019 14:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 29 15:41:51 2019

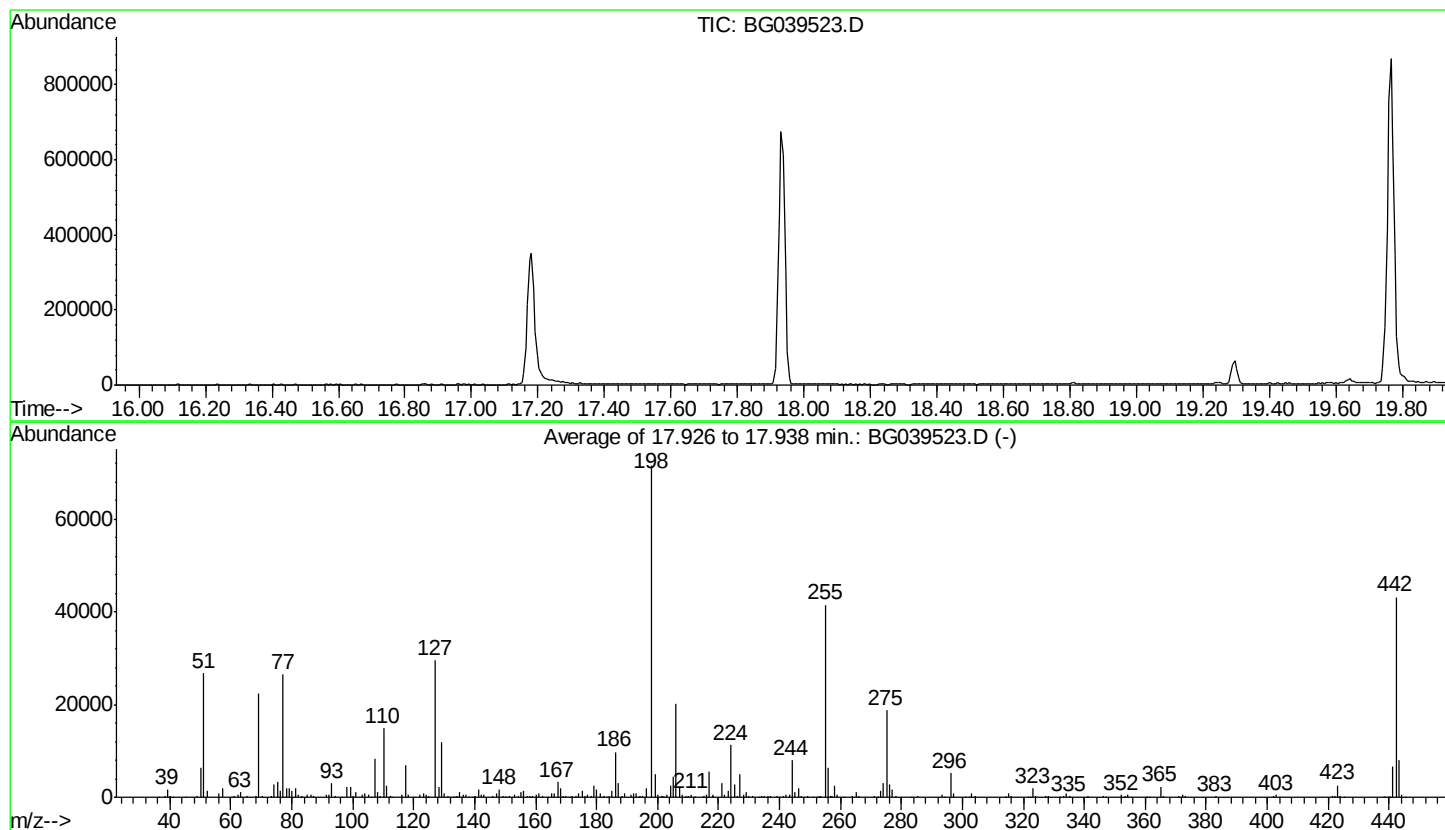

AutoFind: Scans 2526, 2527, 2528; Background Corrected with Scan 2520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	26698	PASS
68	69	0.00	2	1.6	356	PASS
69	198	0.00	100	31.2	22352	PASS
70	69	0.00	2	1.0	226	PASS
127	198	10	80	41.3	29514	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71549	PASS
199	198	5	9	7.1	5050	PASS
275	198	10	60	26.1	18708	PASS
365	198	1	100	3.2	2280	PASS
441	198	0.01	100	9.3	6673	PASS
442	198	50	100	60.3	43173	PASS
443	442	15	24	18.3	7884	PASS