
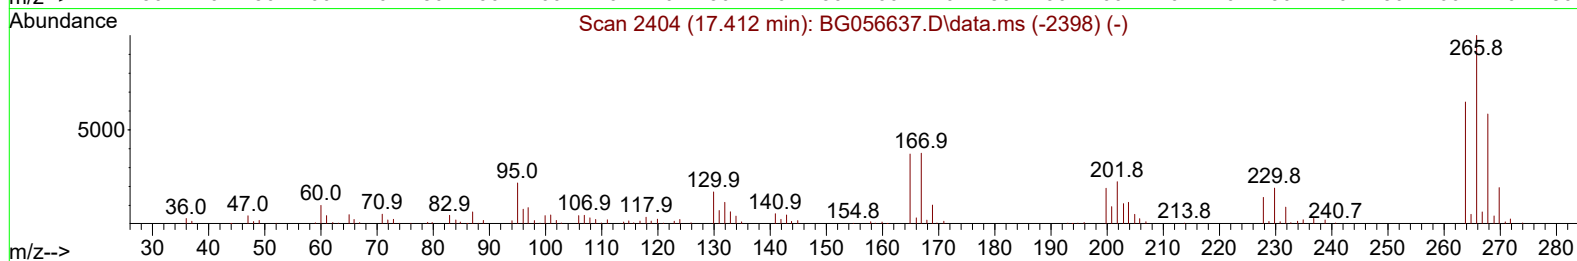
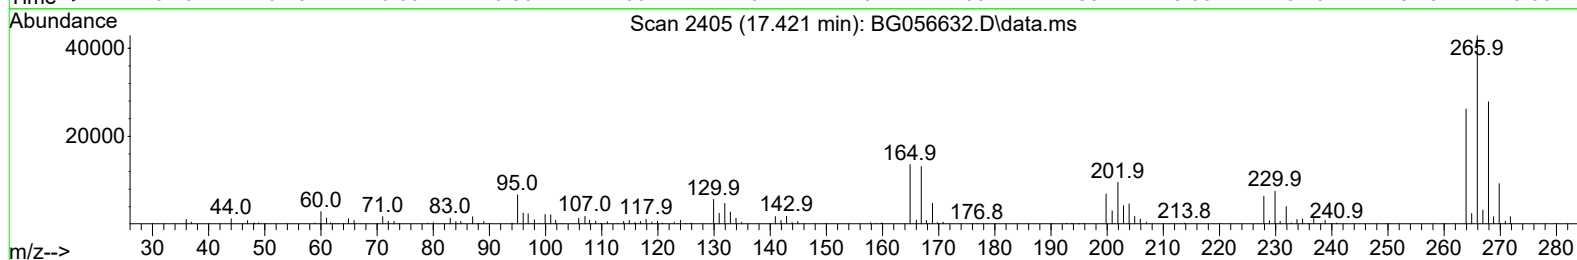


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021523\
Data File : BG056632.D
Acq On : 15 Feb 2023 13:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 04:22:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 16 01:33:33 2023
Response via : Initial Calibration

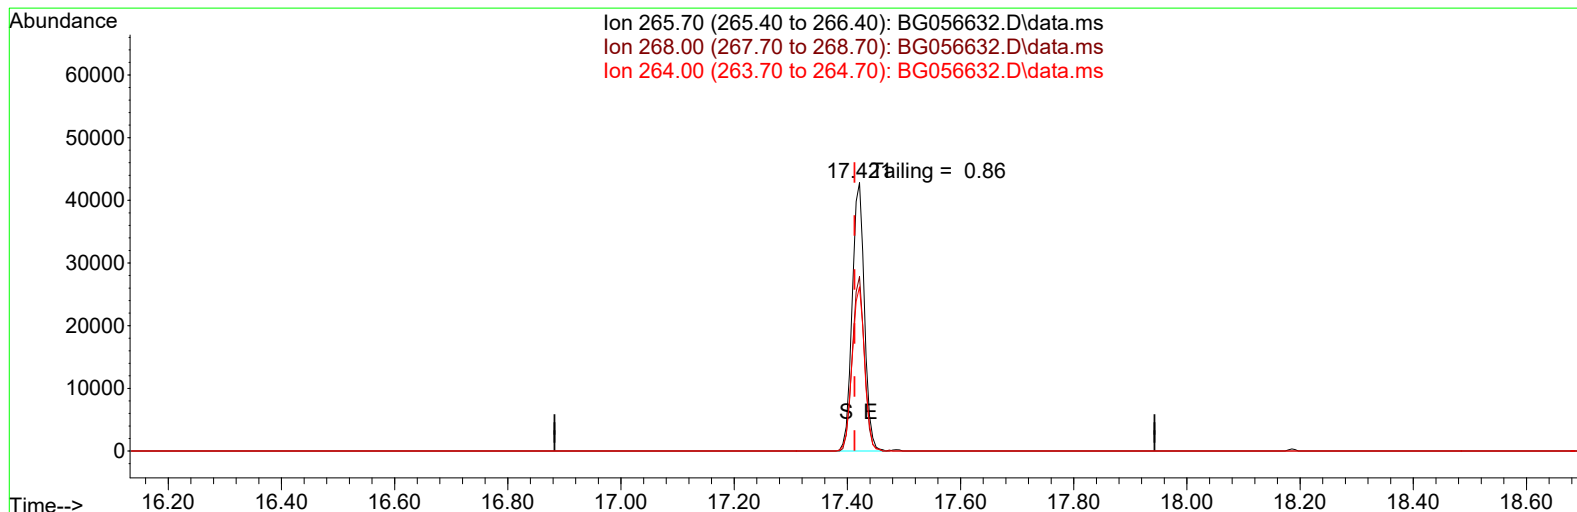

TIC: BG056632.D\data.ms

(70) Pentachlorophenol (C)




17.421min (+ 0.009) 18142.14 ng

response 64278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	58.40	64.99
264.00	64.70	61.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021523\
Data File : BG056632.D
Acq On : 15 Feb 2023 13:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 04:22:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 16 01:33:33 2023
Response via : Initial Calibration

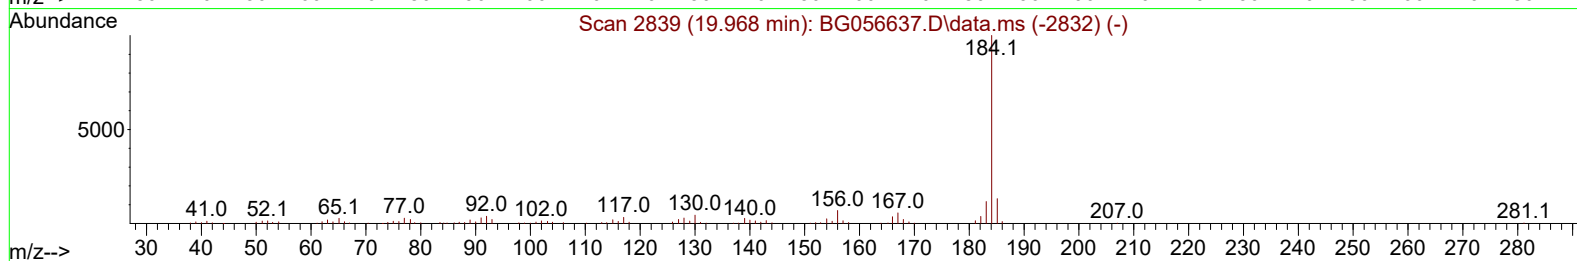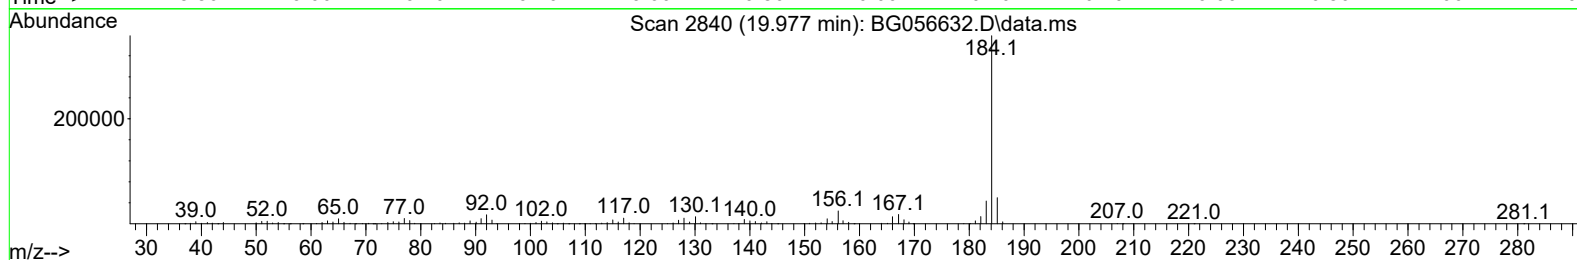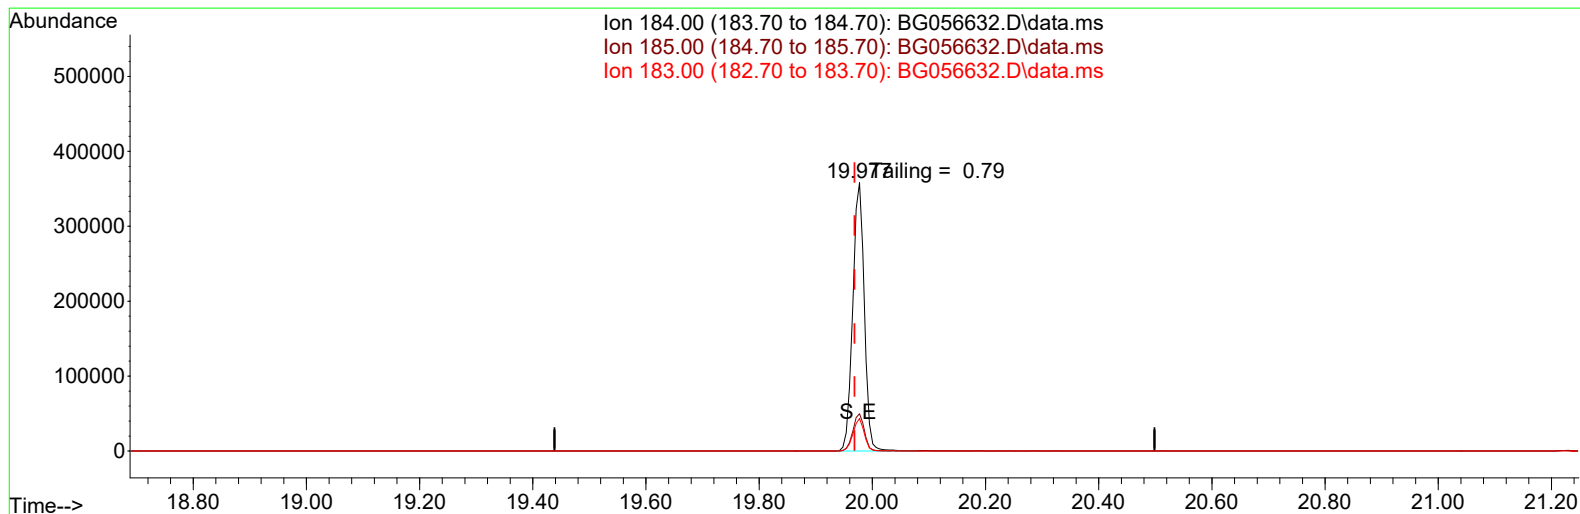

TIC: BG056632.D\data.ms

(77) Benzidine

19.977min (+ 0.009) 0.00 ng

response 509056

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.20	13.88
183.00	11.70	12.14
0.00	0.00	0.00