
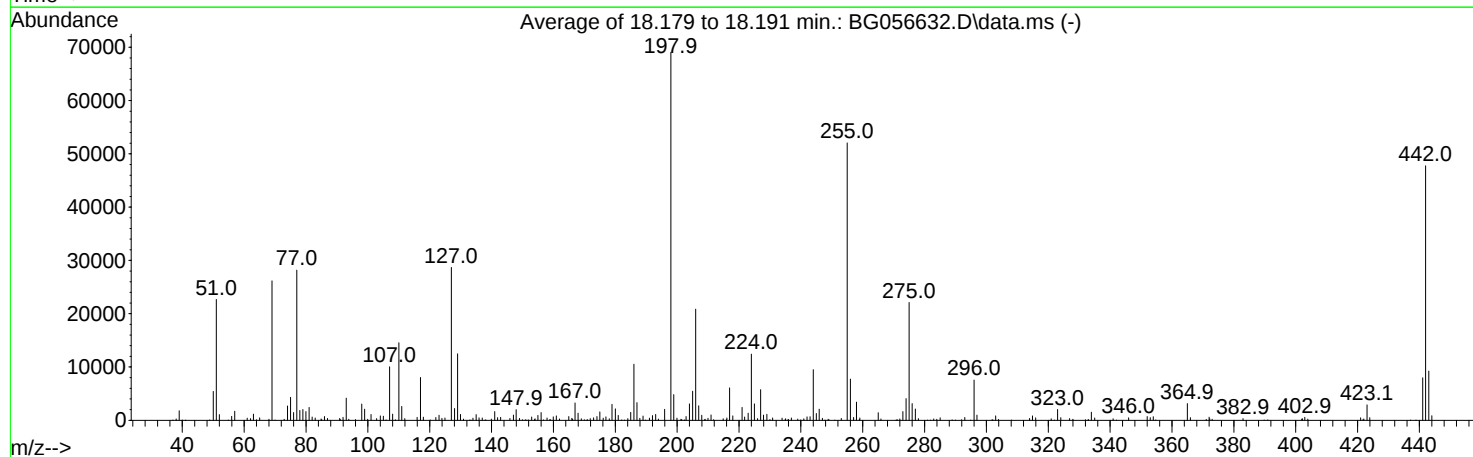


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021523\
Data File : BG056632.D
Acq On : 15 Feb 2023 13:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 16 01:33:33 2023

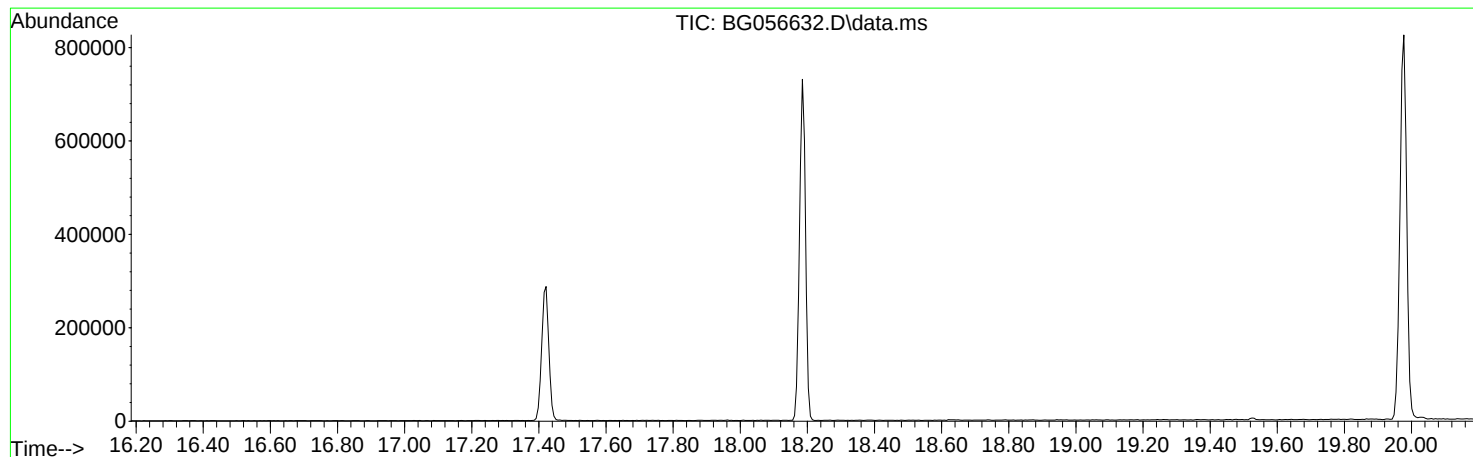




AutoFind: Scans 2534, 2535, 2536; Background Corrected with Scan 2527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	22696	PASS
68	69	0.00	2	0.8	210	PASS
69	198	0.00	100	37.9	26187	PASS
70	69	0.00	2	0.2	59	PASS
127	198	10	80	41.5	28680	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69032	PASS
199	198	5	9	7.0	4820	PASS
275	198	10	60	32.0	22117	PASS
365	198	1	100	4.5	3126	PASS
441	198	0.01	100	11.6	7978	PASS
442	442	50	100	100.0	47752	PASS
443	442	15	24	19.3	9236	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021523\
Data File : BG056632.D
Acq On : 15 Feb 2023 13:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 16 04:22:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 16 01:33:33 2023
Response via : Initial Calibration

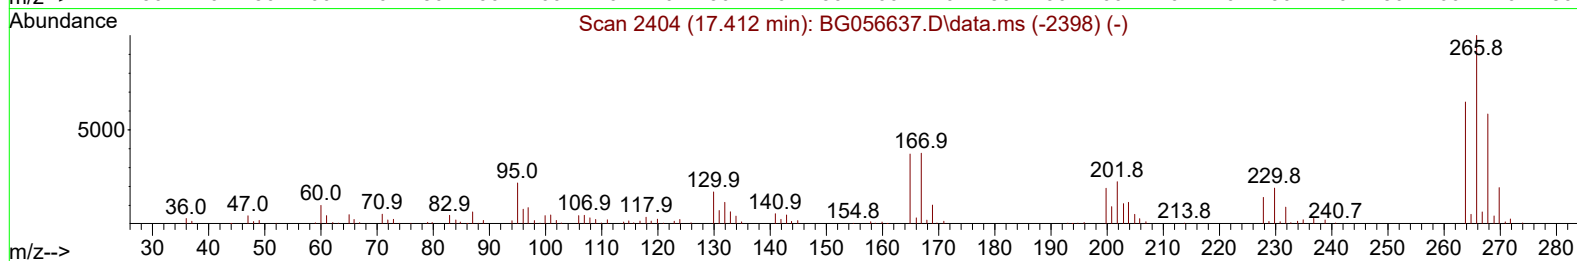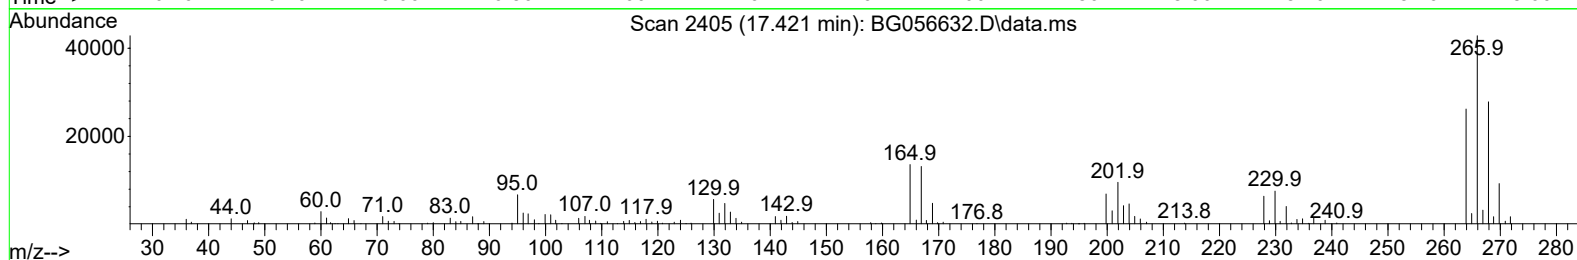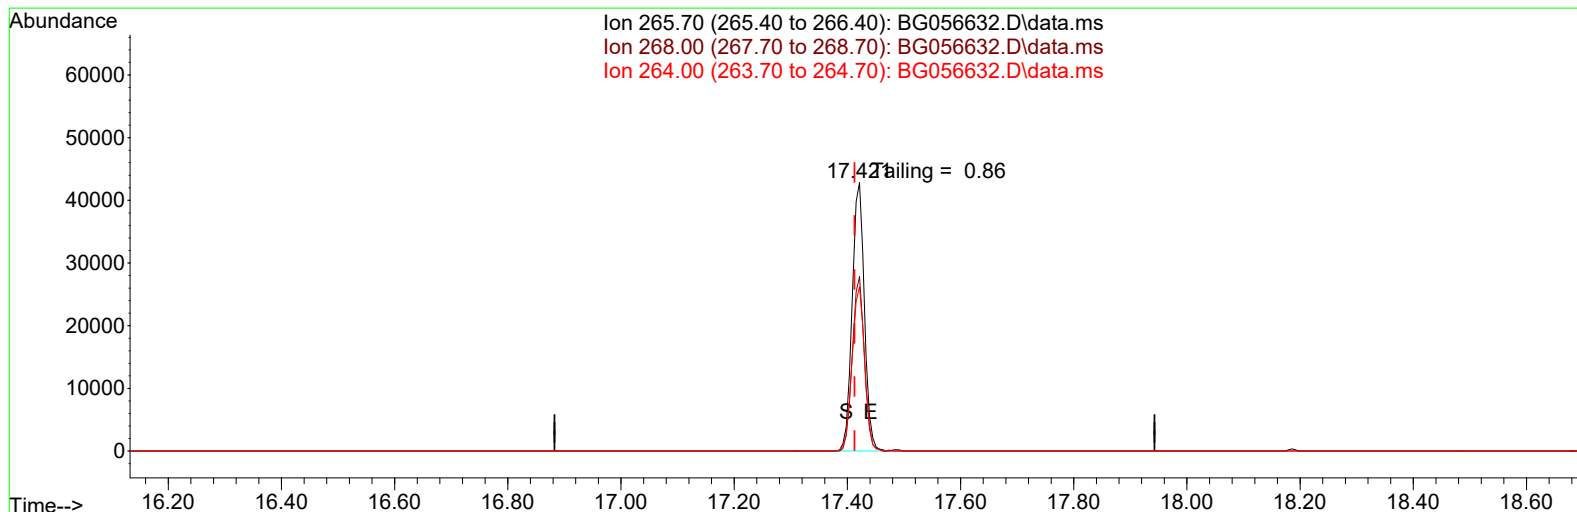

TIC: BG056632.D\data.ms

(70) Pentachlorophenol (C)

17.421min (+ 0.009) 18142.14 ng




response 64278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	58.40	64.99
264.00	64.70	61.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021523\
Data File : BG056632.D
Acq On : 15 Feb 2023 13:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 16 04:22:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 16 01:33:33 2023
Response via : Initial Calibration

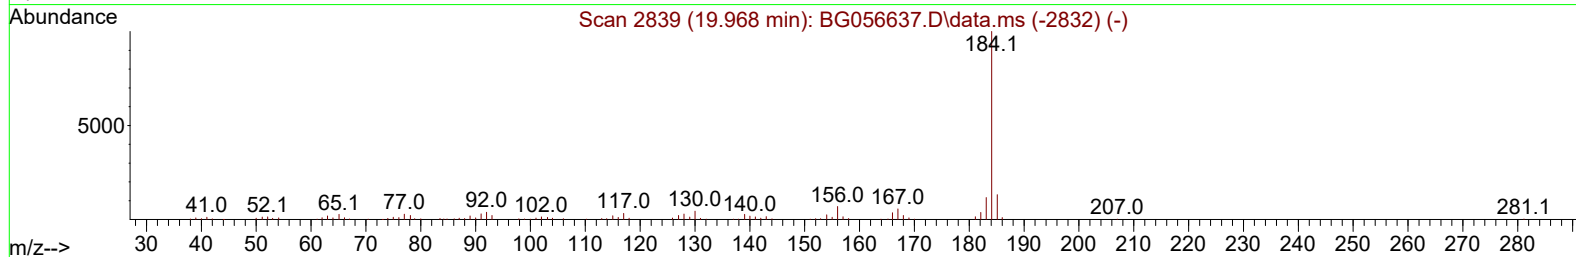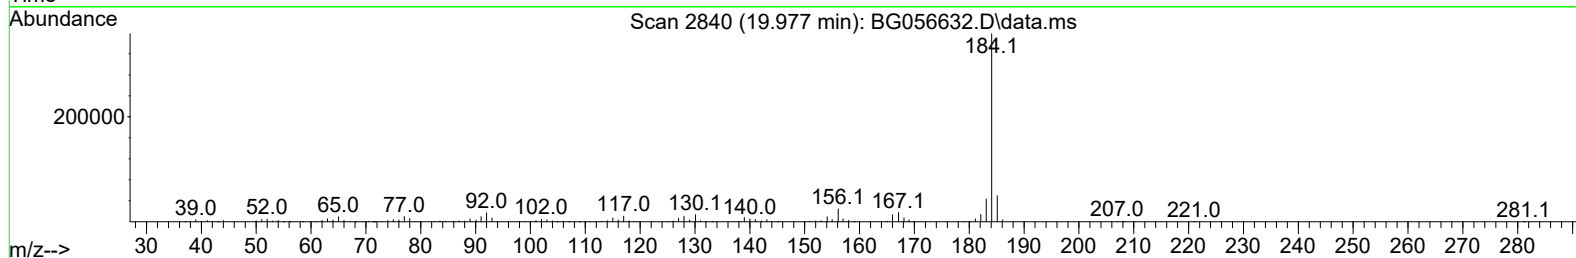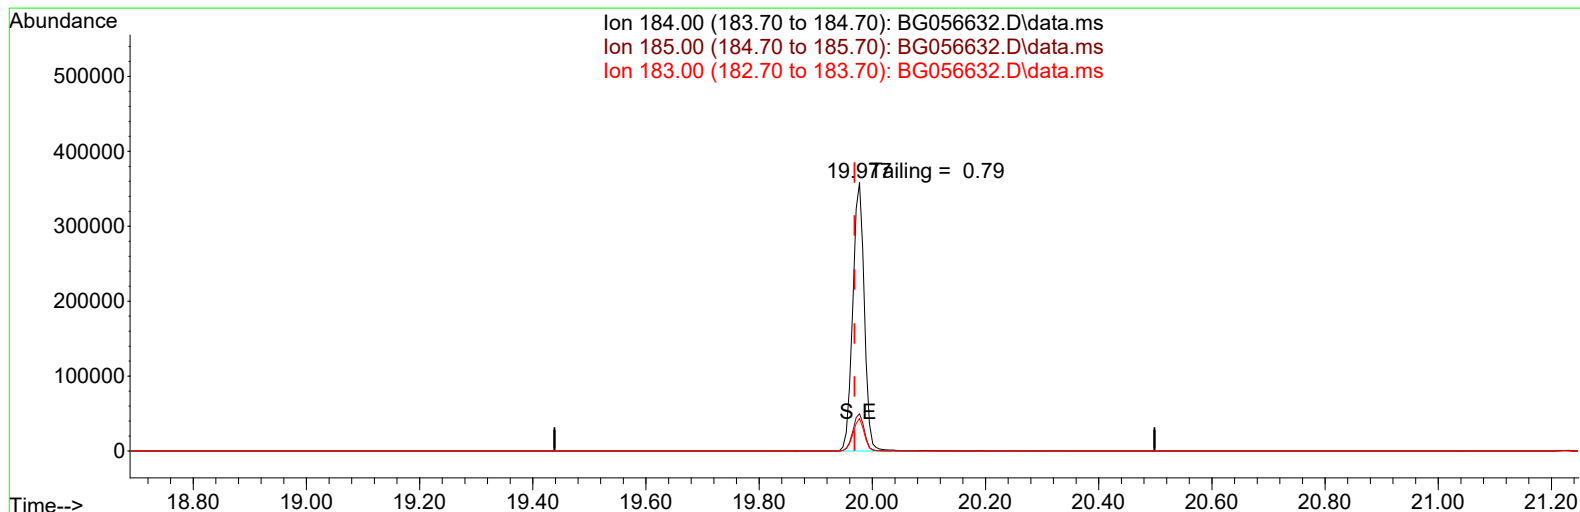

TIC: BG056632.D\data.ms

(77) Benzidine

19.977min (+ 0.009) 0.00 ng

response 509056

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.20	13.88
183.00	11.70	12.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/15/2023	BNA_G	<u>BG056632.D</u>
Compound Name	Response	Retention Time
DDT	167933	21.229
DDD	1715	20.812
DDE	0	20.47
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1715	169648	1.01

Instrument :
BNA_G
ClientSampleId :
DFTPP