
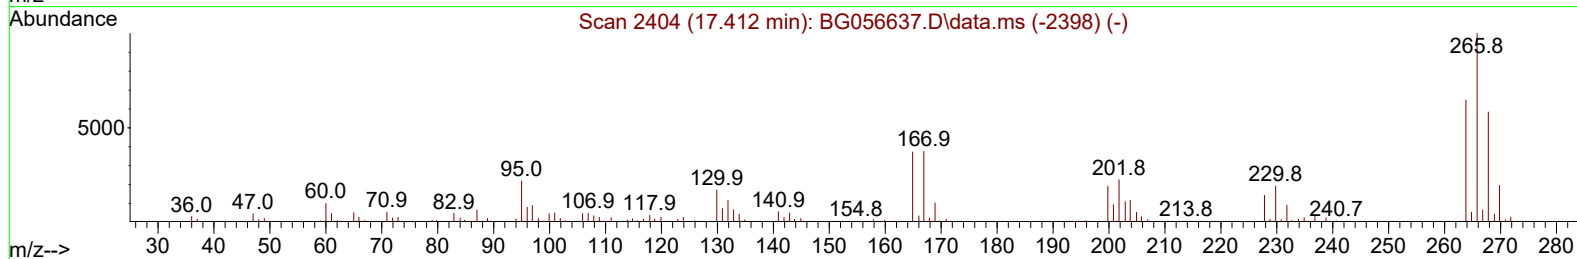
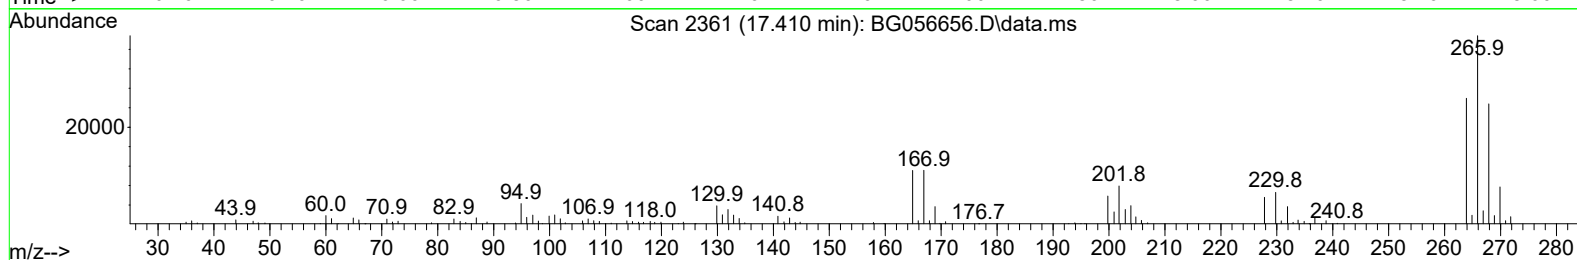


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021723\
Data File : BG056656.D
Acq On : 17 Feb 2023 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 04:03:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 16 01:33:33 2023
Response via : Initial Calibration

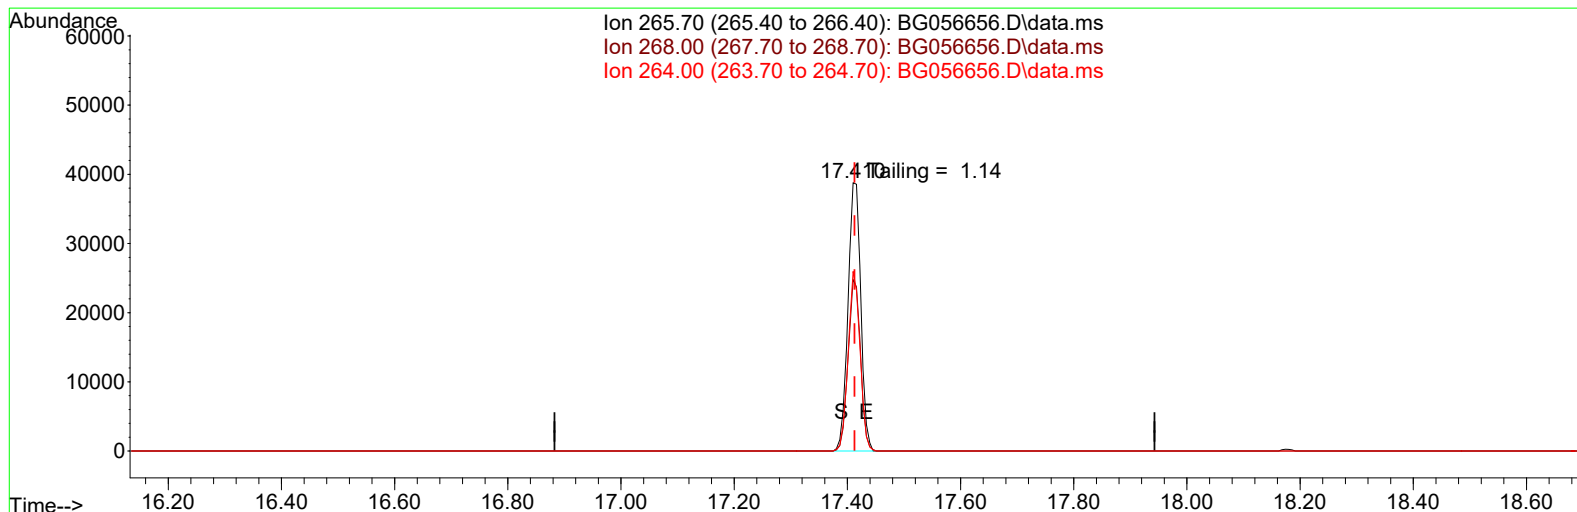

TIC: BG056656.D\data.ms

(70) Pentachlorophenol (C)




17.410min (-0.002) 18135.13 ng

response 60797

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	58.40	63.88
264.00	64.70	66.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021723\
Data File : BG056656.D
Acq On : 17 Feb 2023 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 04:03:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 16 01:33:33 2023
Response via : Initial Calibration

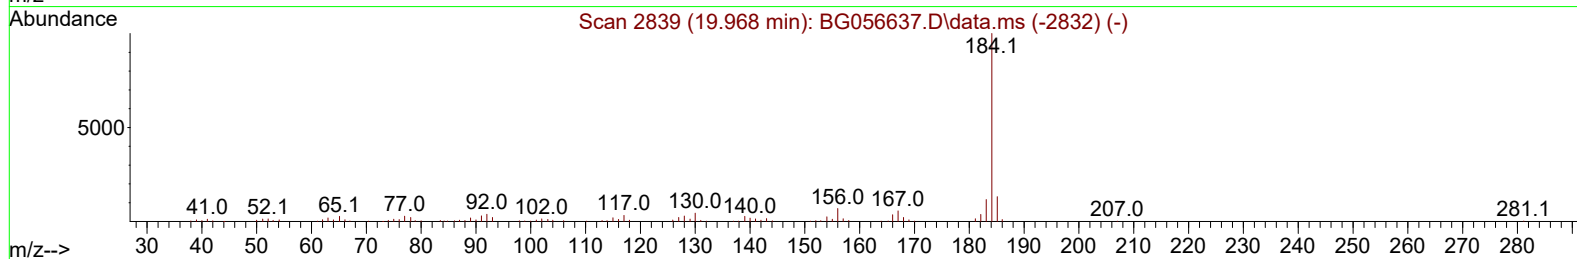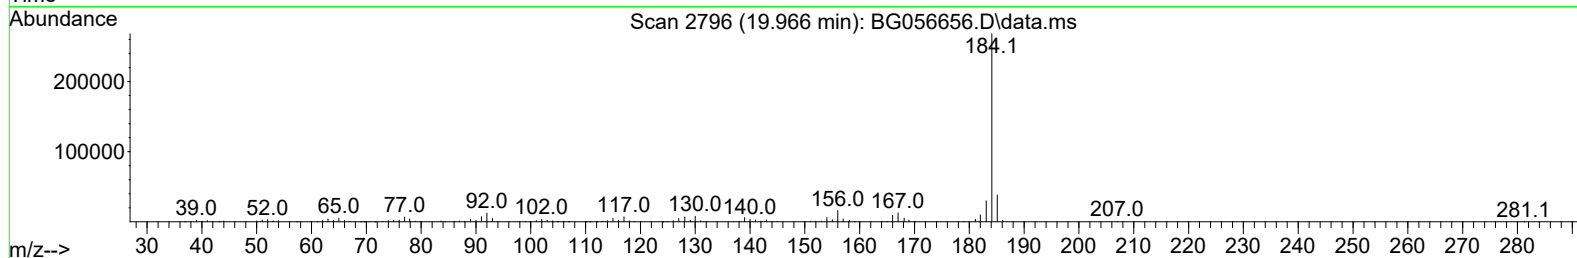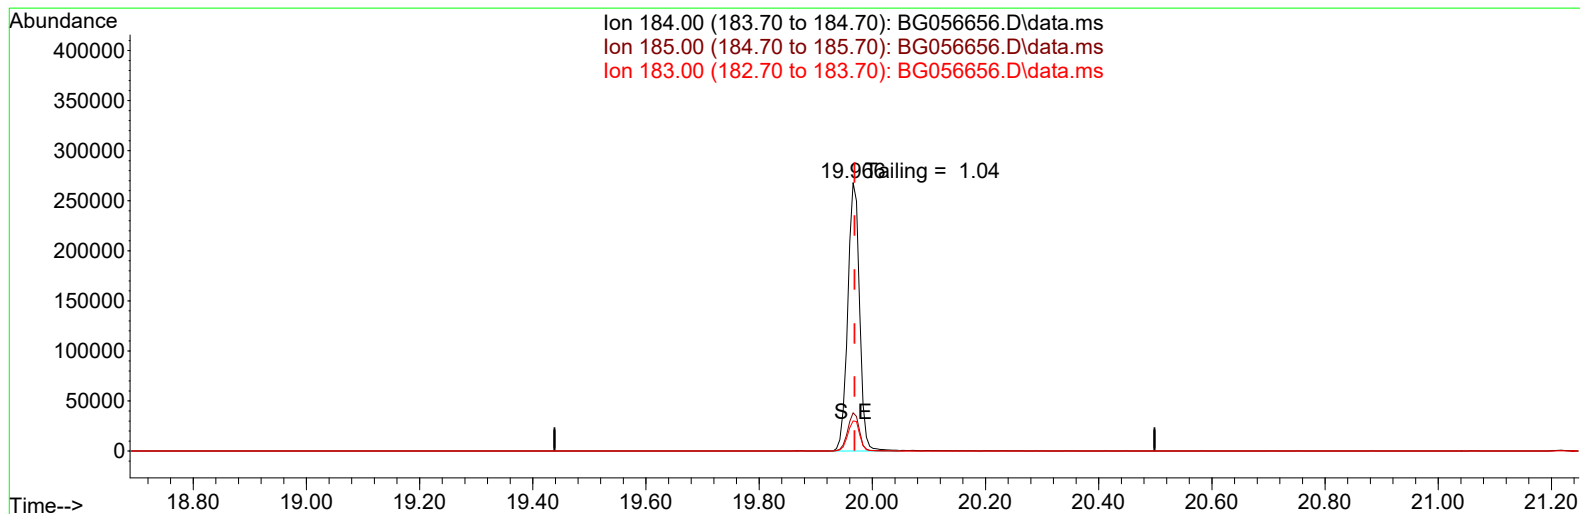

TIC: BG056656.D\data.ms

(77) Benzidine

19.966min (-0.002) 0.00 ng

response 389541

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.20	14.25
183.00	11.70	11.20
0.00	0.00	0.00