

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021723\
 Data File : BG056658.D
 Acq On : 17 Feb 2023 16:13
 Operator : CG/JU
 Sample : PB150923BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB150923BL

Quant Time: Feb 18 00:04:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 16 01:33:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.427	152	14398	20.000	ng	-0.01
21) Naphthalene-d8	11.271	136	59496	20.000	ng	0.00
39) Acenaphthene-d10	15.037	164	47591	20.000	ng	0.00
64) Phenanthrene-d10	17.775	188	129203	20.000	ng	0.00
76) Chrysene-d12	22.088	240	130731	20.000	ng	-0.01
86) Perylene-d12	25.631	264	139415	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.936	112	127943	144.584	ng	0.00
7) Phenol-d6	7.552	99	183551	140.422	ng	0.00
23) Nitrobenzene-d5	9.608	82	87204	75.046	ng	0.00
42) 2,4,6-Tribromophenol	16.512	330	68194	104.660	ng	0.00
45) 2-Fluorobiphenyl	13.668	172	310836	87.459	ng	0.00
79) Terphenyl-d14	20.343	244	738472	92.421	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021723\
Data File : BG056658.D
Acq On : 17 Feb 2023 16:13
Operator : CG/JU
Sample : PB150923BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150923BL


Quant Time: Feb 18 00:04:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 16 01:33:33 2023
Response via : Initial Calibration

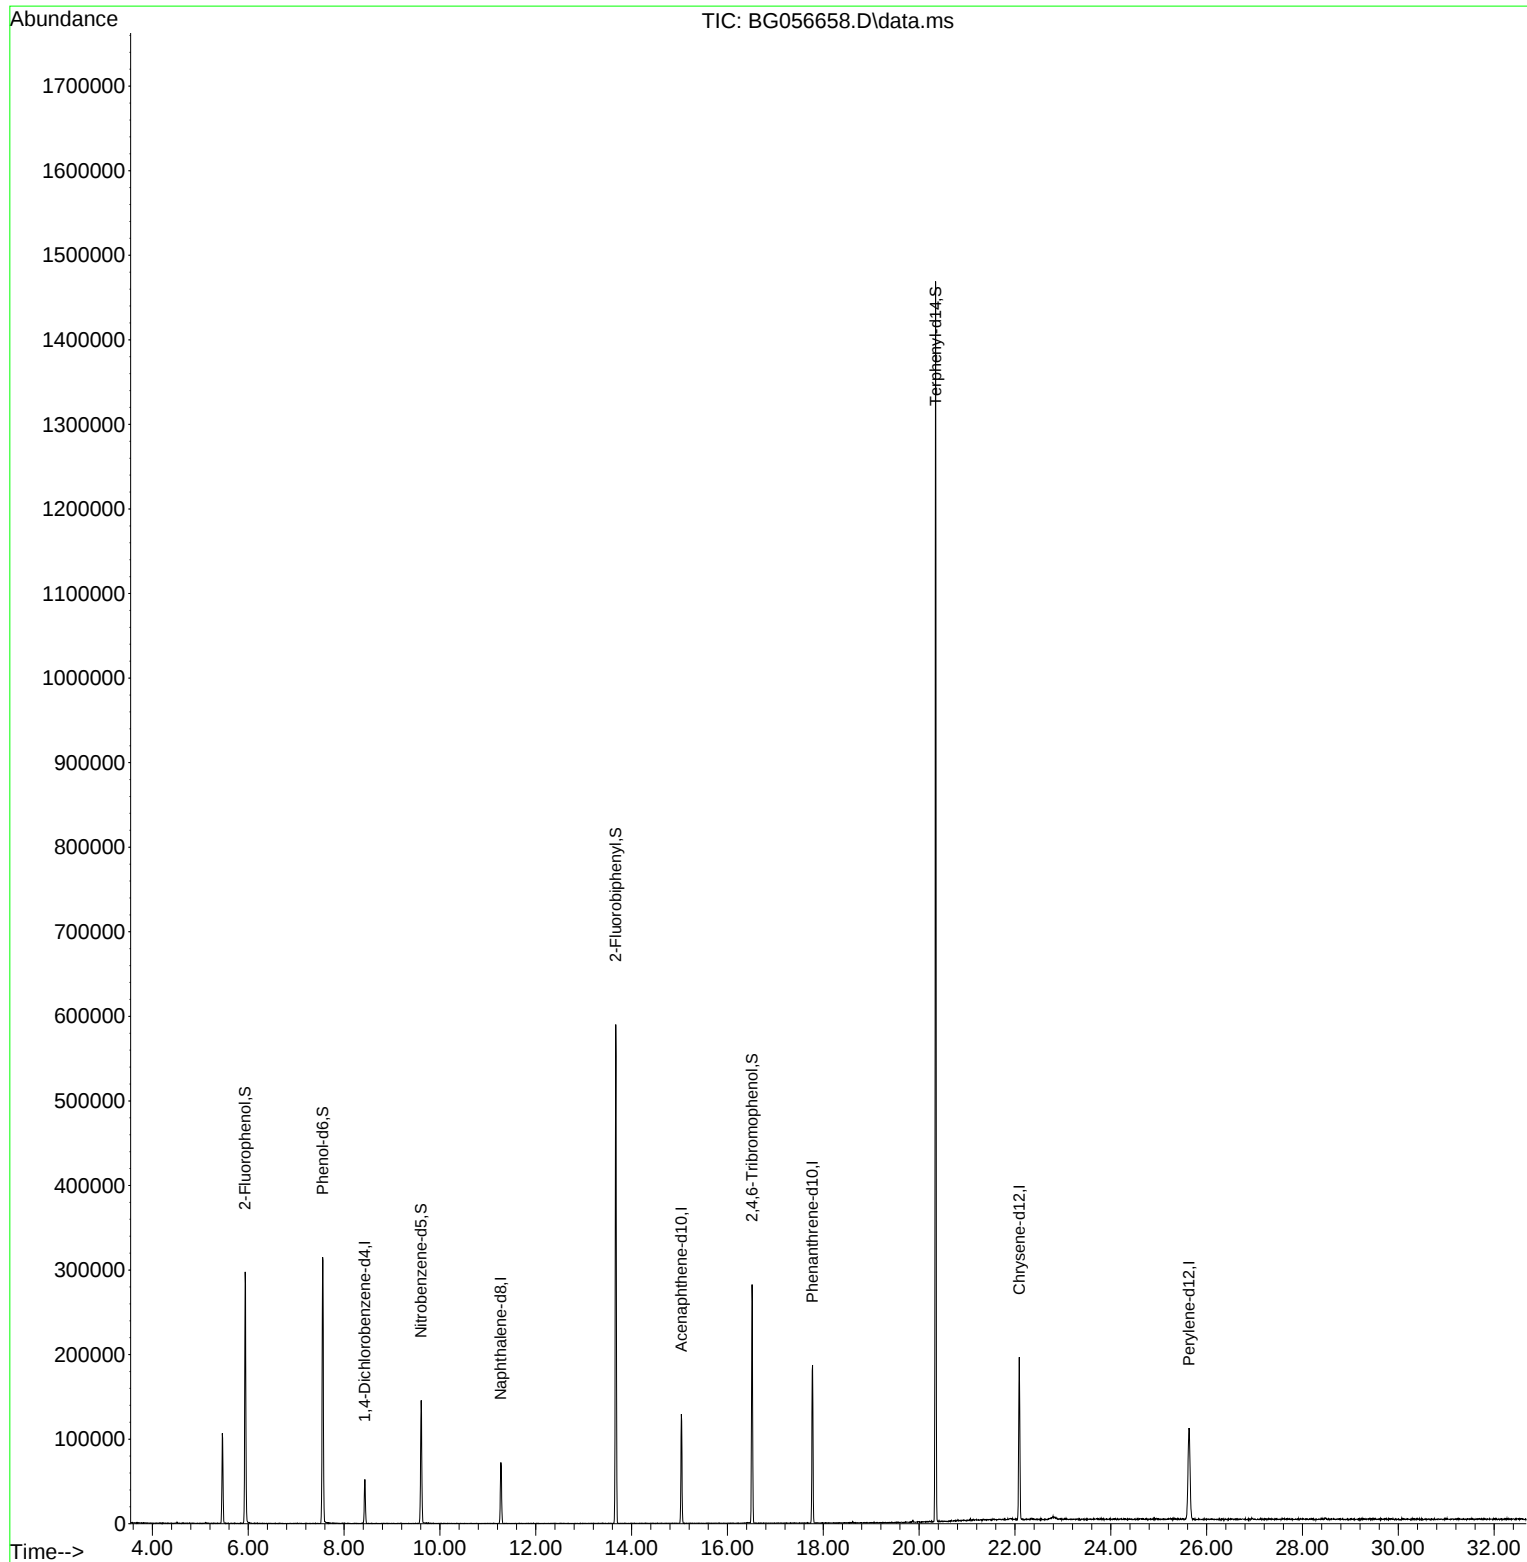



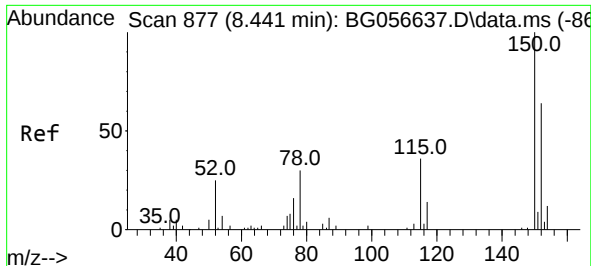


#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.427 min Scan# 81
Delta R.T. -0.014 min
Lab File: BG056658.D
Acq: 17 Feb 2023 16:13


Instrument :
BNA_G
ClientSampleId :
PB150923BL





Tgt Ion:152 Resp: 14398
Ion Ratio Lower Upper
152 100
150 137.6 124.8 187.2
115 53.5 44.7 67.1

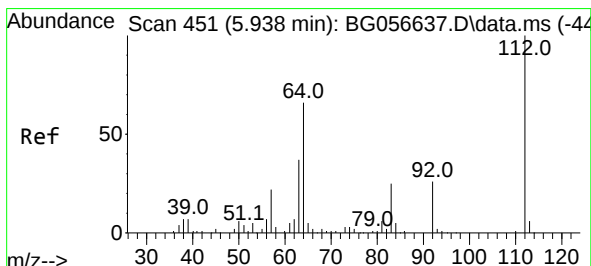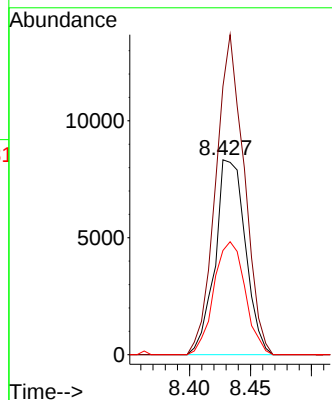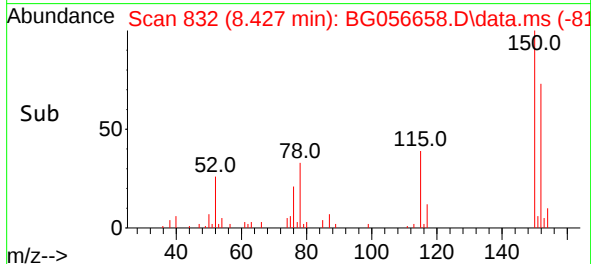


#5
2-Fluorophenol
Concen: 144.584 ng
RT: 5.936 min Scan# 408
Delta R.T. -0.002 min
Lab File: BG056658.D
Acq: 17 Feb 2023 16:13

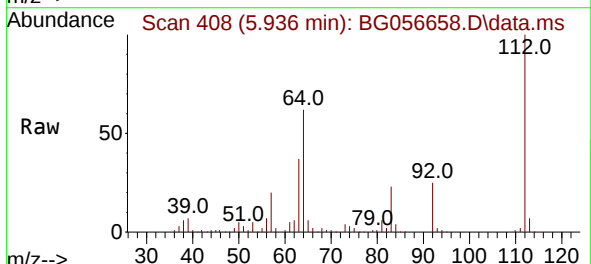

Tgt Ion:112 Resp: 127943
Ion Ratio Lower Upper
112 100
64 61.6 52.6 78.8
63 36.9 29.8 44.6



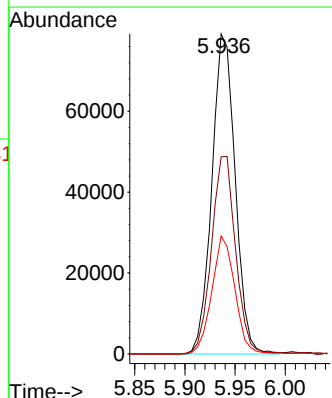



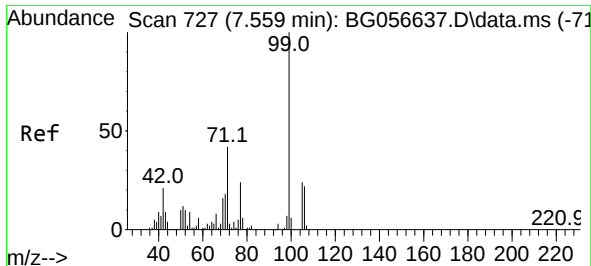

#7
Phenol-d6
Concen: 140.422 ng
RT: 7.552 min Scan# 61
Delta R.T. -0.007 min
Lab File: BG056658.D
Acq: 17 Feb 2023 16:13




Instrument :
BNA_G
ClientSampleId :
PB150923BL


Tgt Ion: 99 Resp: 183551
Ion Ratio Lower Upper
99 100
42 19.2 16.8 25.2
71 41.9 33.9 50.9

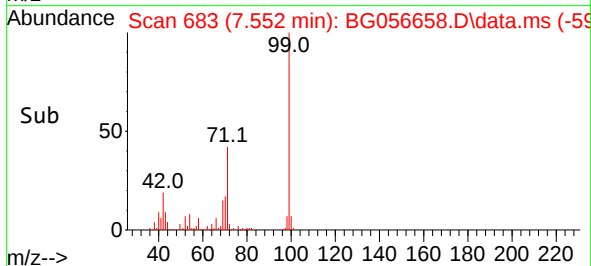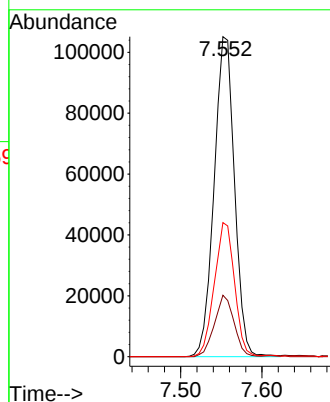

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.271 min Scan# 1316
Delta R.T. -0.007 min
Lab File: BG056658.D
Acq: 17 Feb 2023 16:13

Tgt Ion:136 Resp: 59496
Ion Ratio Lower Upper
136 100
137 11.5 9.7 14.5
54 8.9 7.7 11.5
68 5.5 4.8 7.2


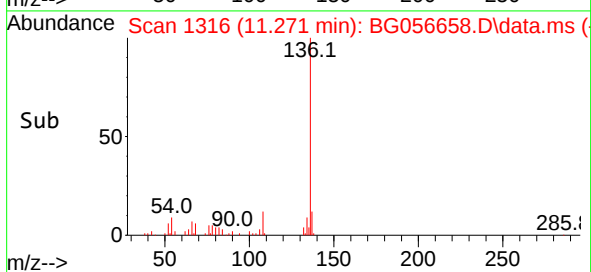
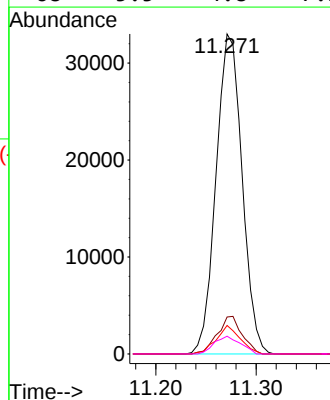
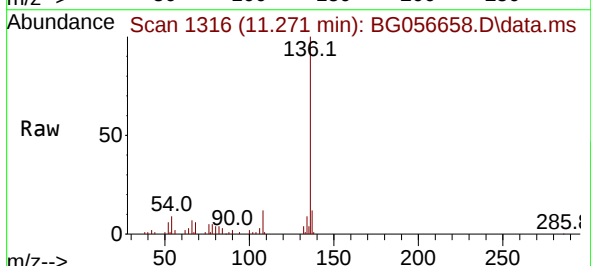




#23
Nitrobenzene-d5
Concen: 75.046 ng
RT: 9.608 min Scan# 1077
Delta R.T. -0.008 min
Lab File: BG056658.D
Acq: 17 Feb 2023 16:13




Instrument :
BNA_G
ClientSampleId :
PB150923BL


Tgt Ion: 82 Resp: 87204
Ion Ratio Lower Upper
82 100
128 39.1 29.4 44.2
54 46.0 37.8 56.6

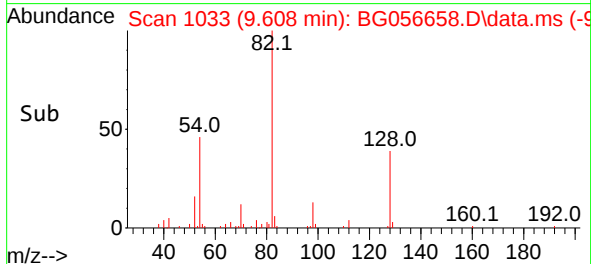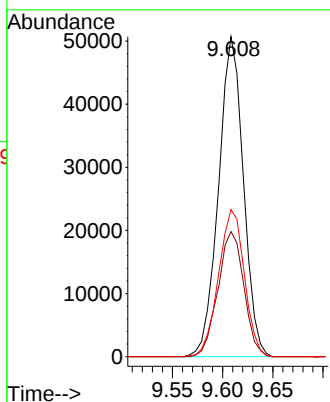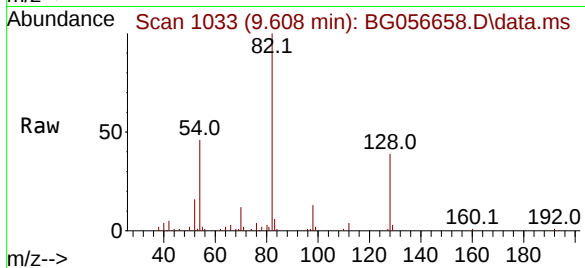

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 15.037 min Scan# 1957
Delta R.T. -0.007 min
Lab File: BG056658.D
Acq: 17 Feb 2023 16:13

Tgt Ion: 164 Resp: 47591
Ion Ratio Lower Upper
164 100
162 104.9 81.3 121.9
160 43.8 35.2 52.8


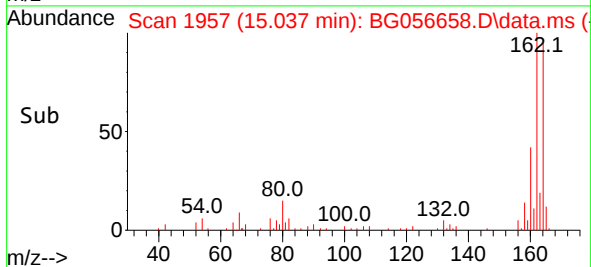
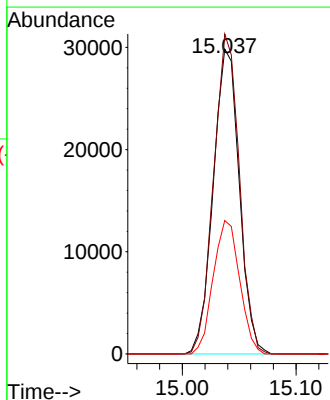
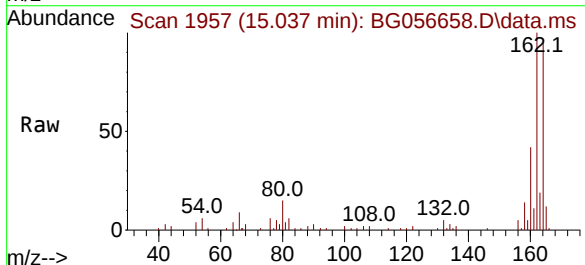


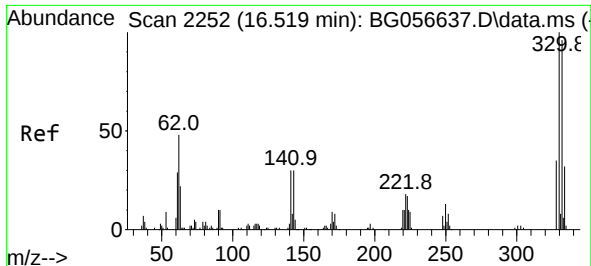

#42
2,4,6-Tribromophenol
Concen: 104.660 ng
RT: 16.512 min Scan# 21
Delta R.T. -0.007 min
Lab File: BG056658.D
Acq: 17 Feb 2023 16:13




Instrument :
BNA_G
ClientSampleId :
PB150923BL


Tgt Ion:330 Resp: 68194
Ion Ratio Lower Upper
330 100
332 96.0 75.7 113.5
141 22.5 24.6 37.0#

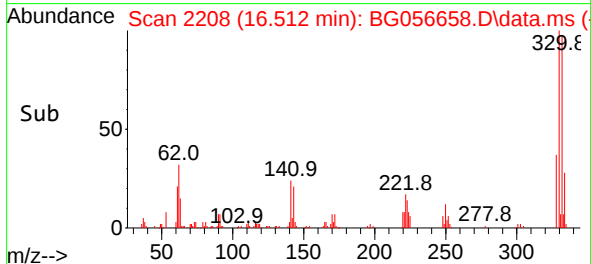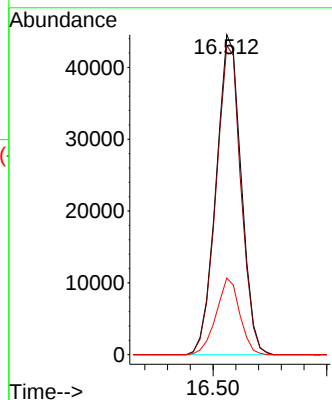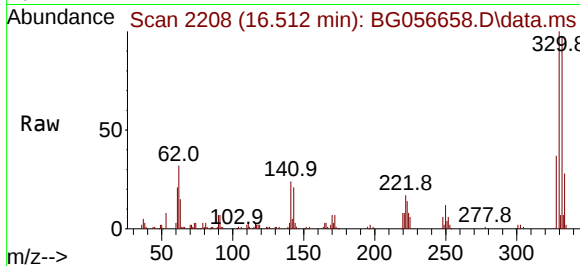

#45
2-Fluorobiphenyl
Concen: 87.459 ng
RT: 13.668 min Scan# 1724
Delta R.T. -0.007 min
Lab File: BG056658.D
Acq: 17 Feb 2023 16:13

Tgt Ion:172 Resp: 310836
Ion Ratio Lower Upper
172 100
171 36.1 28.6 43.0
170 23.7 19.4 29.0


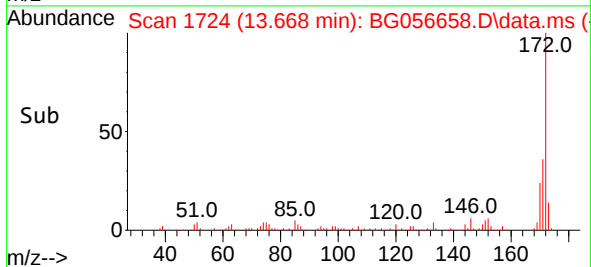
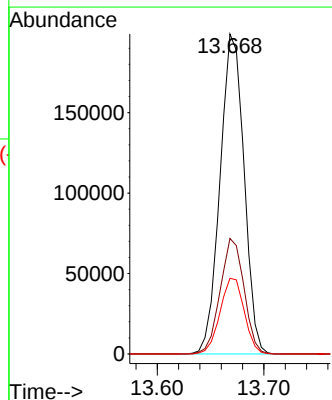
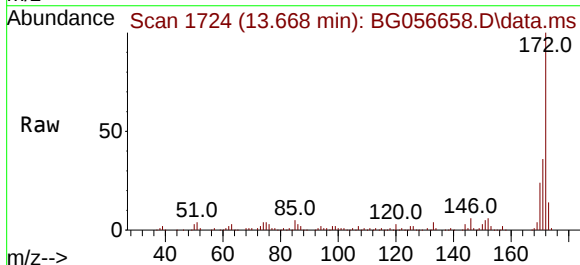


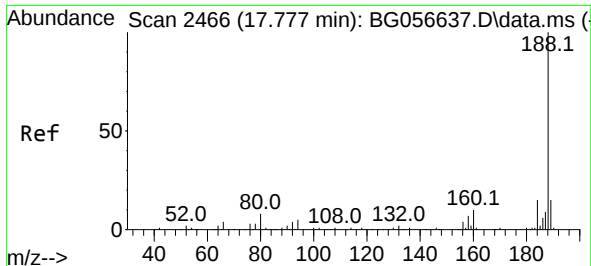

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.775 min Scan# 24
Delta R.T. -0.002 min
Lab File: BG056658.D
Acq: 17 Feb 2023 16:13




Instrument :
BNA_G
ClientSampleId :
PB150923BL


Tgt Ion:188 Resp: 129203
Ion Ratio Lower Upper
188 100
94 5.3 4.0 6.0
80 6.9 6.3 9.5

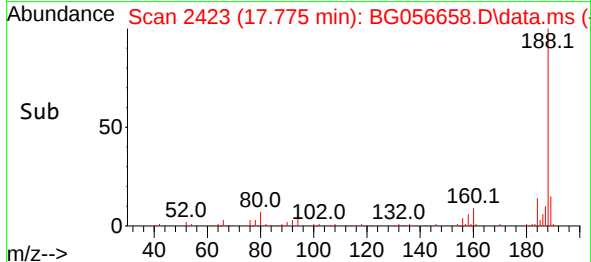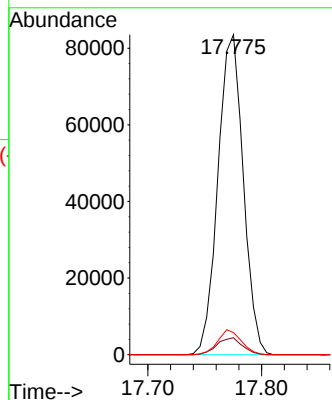

#76
Chrysene-d12
Concen: 20.000 ng
RT: 22.088 min Scan# 3157
Delta R.T. -0.013 min
Lab File: BG056658.D
Acq: 17 Feb 2023 16:13

Tgt Ion:240 Resp: 130731
Ion Ratio Lower Upper
240 100
120 4.5 3.5 5.3
236 25.7 21.5 32.3


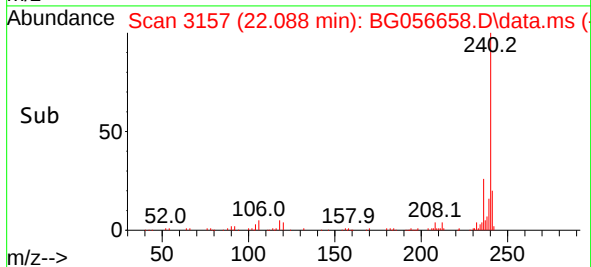
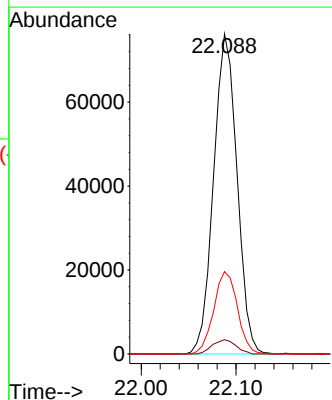
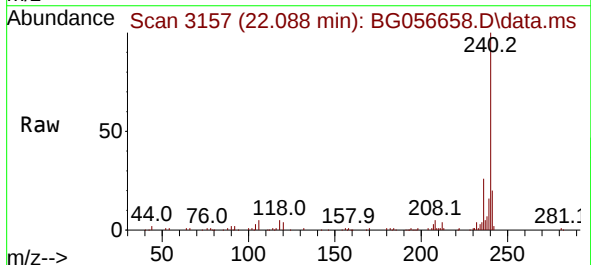


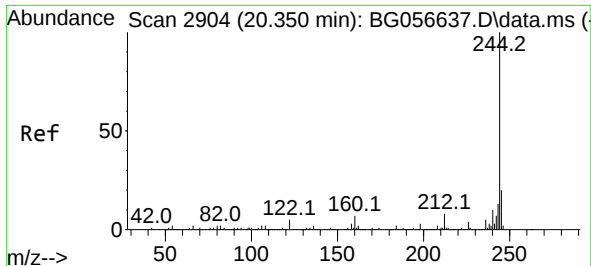

#79
 Terphenyl-d14
 Concen: 92.421 ng
 RT: 20.343 min Scan# 21
 Delta R.T. -0.007 min
 Lab File: BG056658.D
 Acq: 17 Feb 2023 16:13

Instrument :
 BNA_G
 ClientSampleId :
 PB150923BL

Tgt Ion:244 Resp: 738472
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.0 9.0
 122 5.4 3.8 5.8

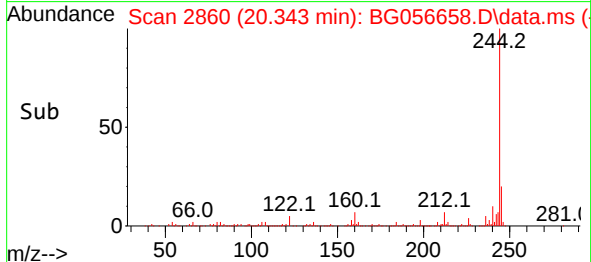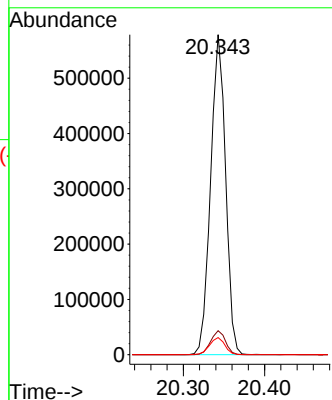

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.631 min Scan# 3760
 Delta R.T. -0.007 min
 Lab File: BG056658.D
 Acq: 17 Feb 2023 16:13

Tgt Ion:264 Resp: 139415
 Ion Ratio Lower Upper
 264 100
 260 23.4 18.6 27.8
 265 20.5 17.0 25.4

