


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021723\
Data File : BG056656.D
Acq On : 17 Feb 2023 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 16 01:33:33 2023

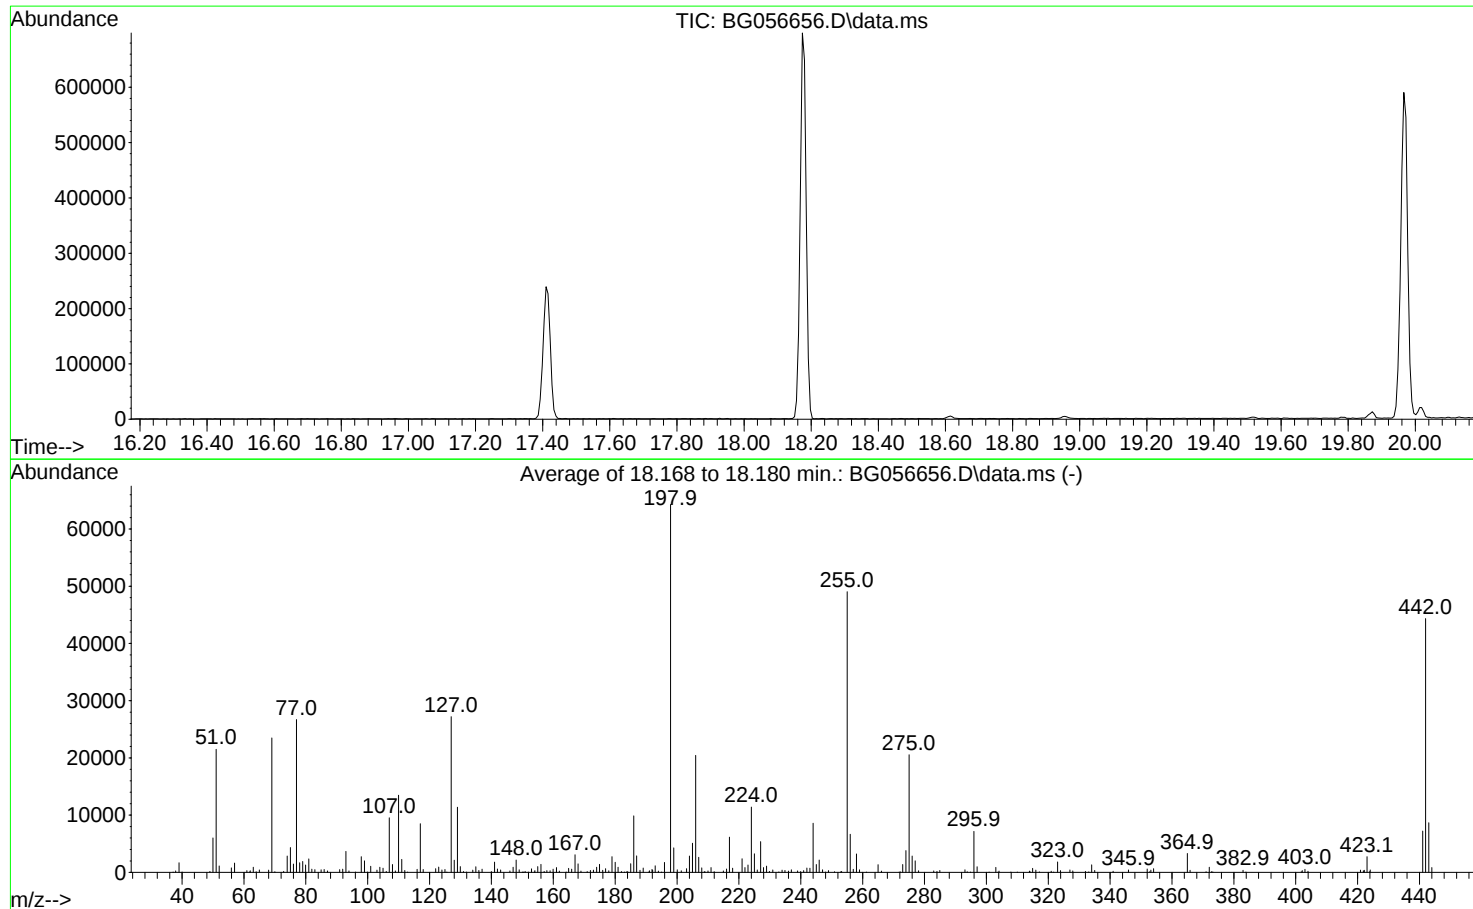




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	21507	PASS
68	69	0.00	2	1.7	398	PASS
69	198	0.00	100	36.5	23488	PASS
70	69	0.00	2	0.5	124	PASS
127	198	10	80	42.3	27200	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64283	PASS
199	198	5	9	6.7	4285	PASS
275	198	10	60	32.0	20565	PASS
365	198	1	100	5.1	3308	PASS
441	198	0.01	100	11.2	7219	PASS
442	442	50	100	100.0	44344	PASS
443	442	15	24	19.6	8671	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021723\
Data File : BG056656.D
Acq On : 17 Feb 2023 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 18 04:03:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 16 01:33:33 2023
Response via : Initial Calibration

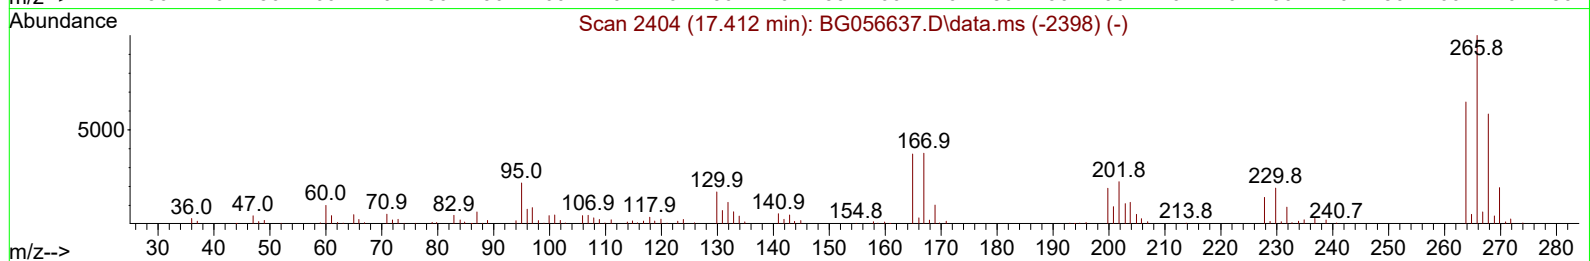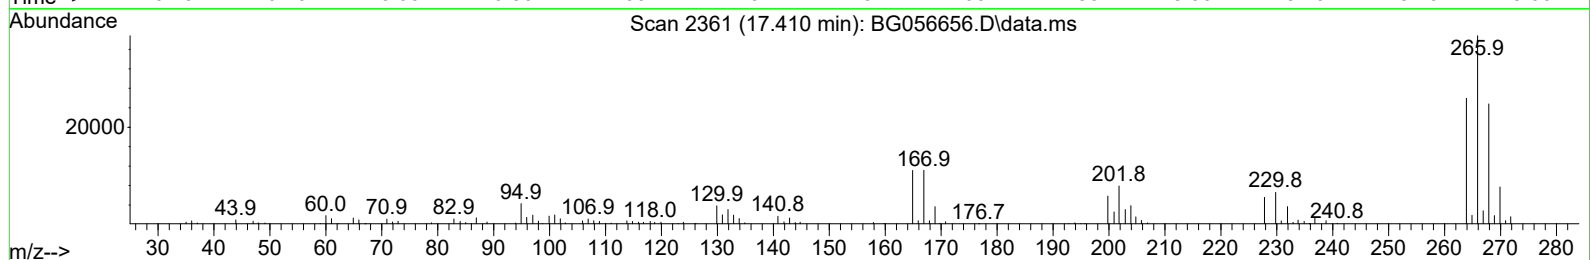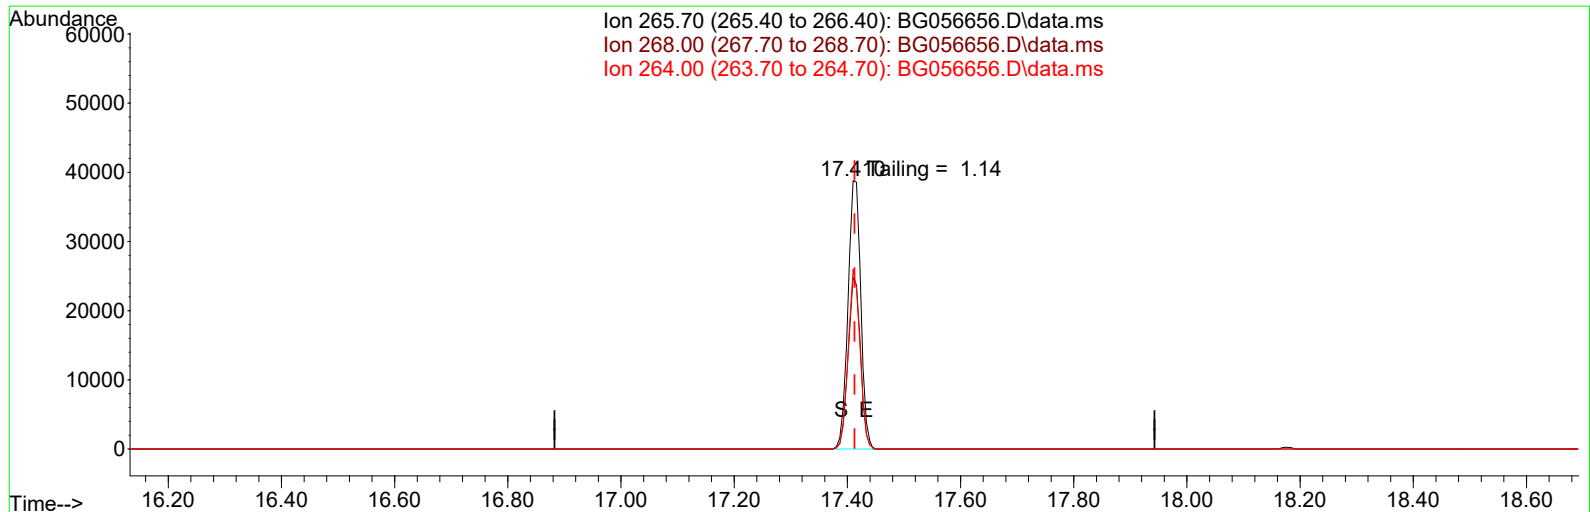

TIC: BG056656.D\data.ms

(70) Pentachlorophenol (C)

17.410min (-0.002) 18135.13 ng




response 60797

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	58.40	63.88
264.00	64.70	66.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021723\
Data File : BG056656.D
Acq On : 17 Feb 2023 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 18 04:03:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 16 01:33:33 2023
Response via : Initial Calibration

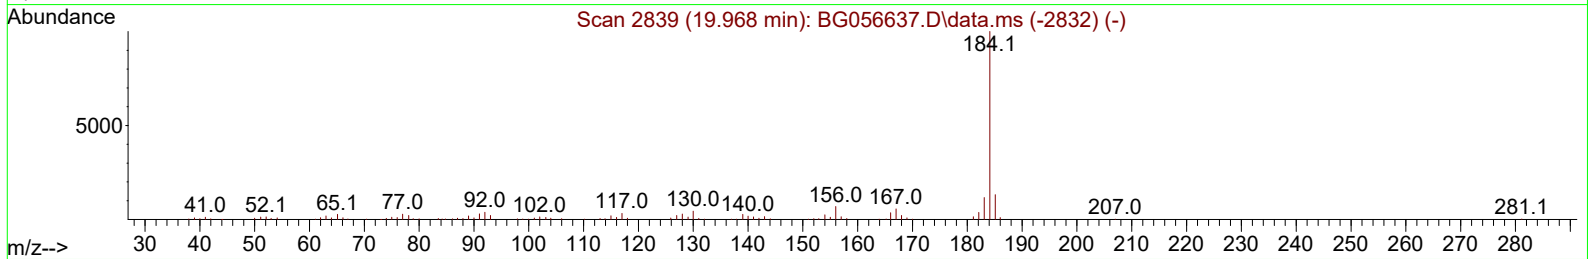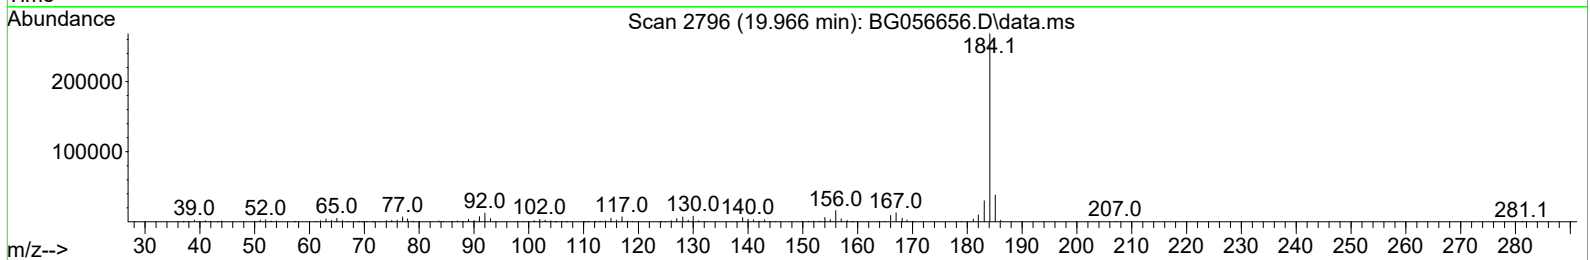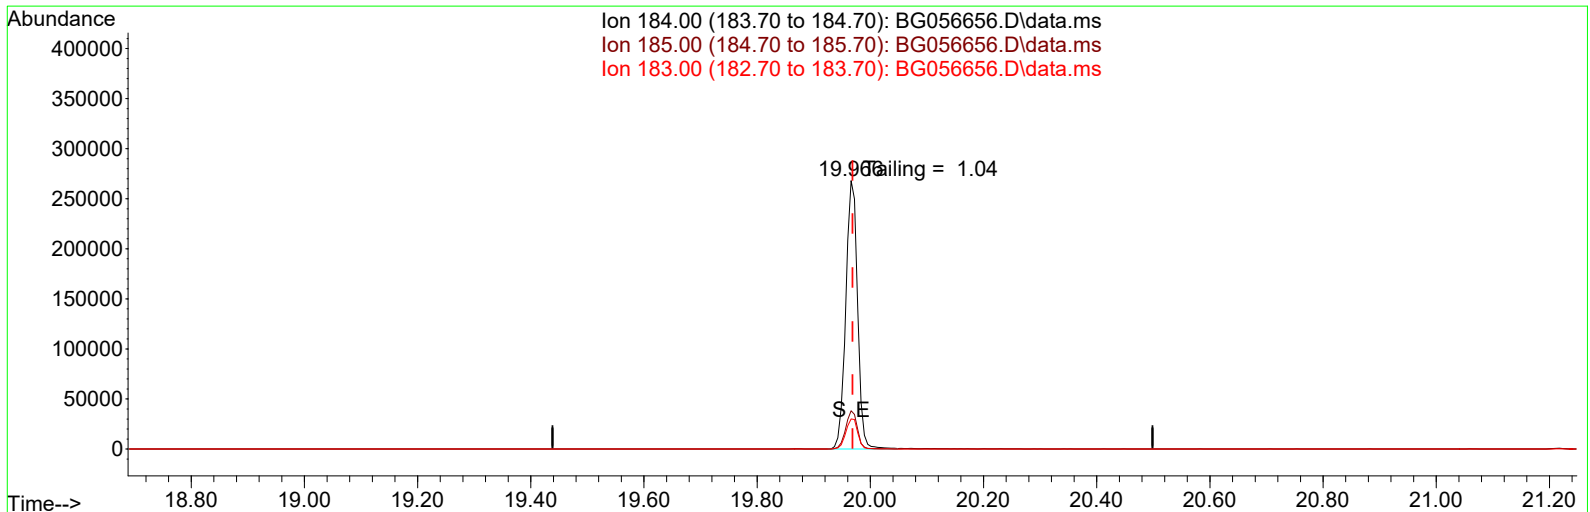

TIC: BG056656.D\data.ms

(77) Benzidine

19.966min (-0.002) 0.00 ng

response 389541

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.20	14.25
183.00	11.70	11.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/17/2023	BNA_G	BG056656.D
Compound Name	Response	Retention Time
DDT	136809	21.212
DDD	3964	20.747
DDE	0	20.47
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3964	140773	2.82

Instrument :
BNA_G
ClientSampleId :
DFTPP