
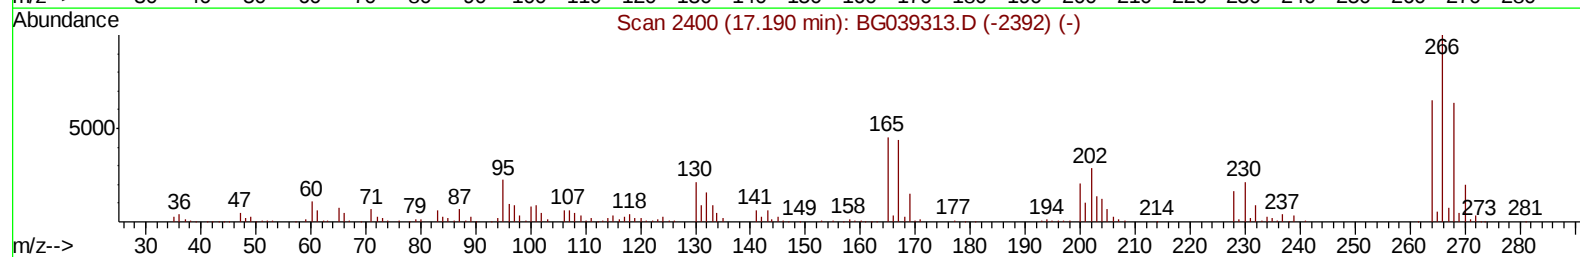
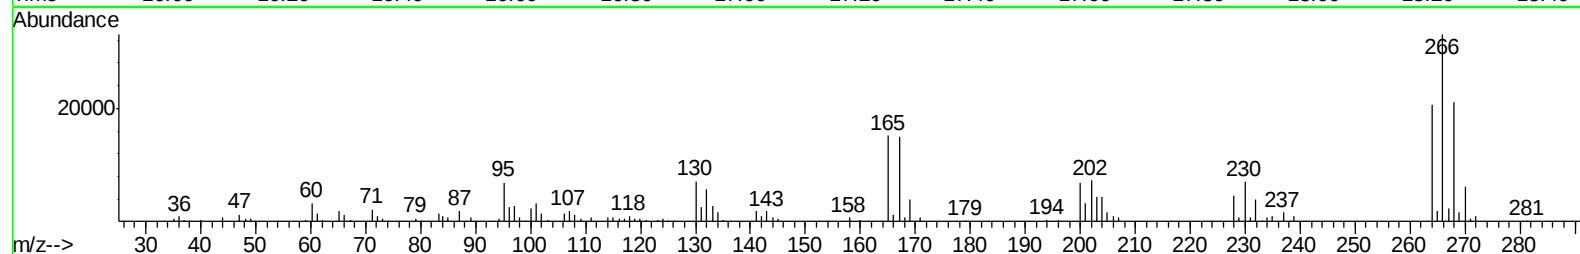


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021919\
Data File : BG039555.D
Acq On : 19 Feb 2019 14:18
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 02:03:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

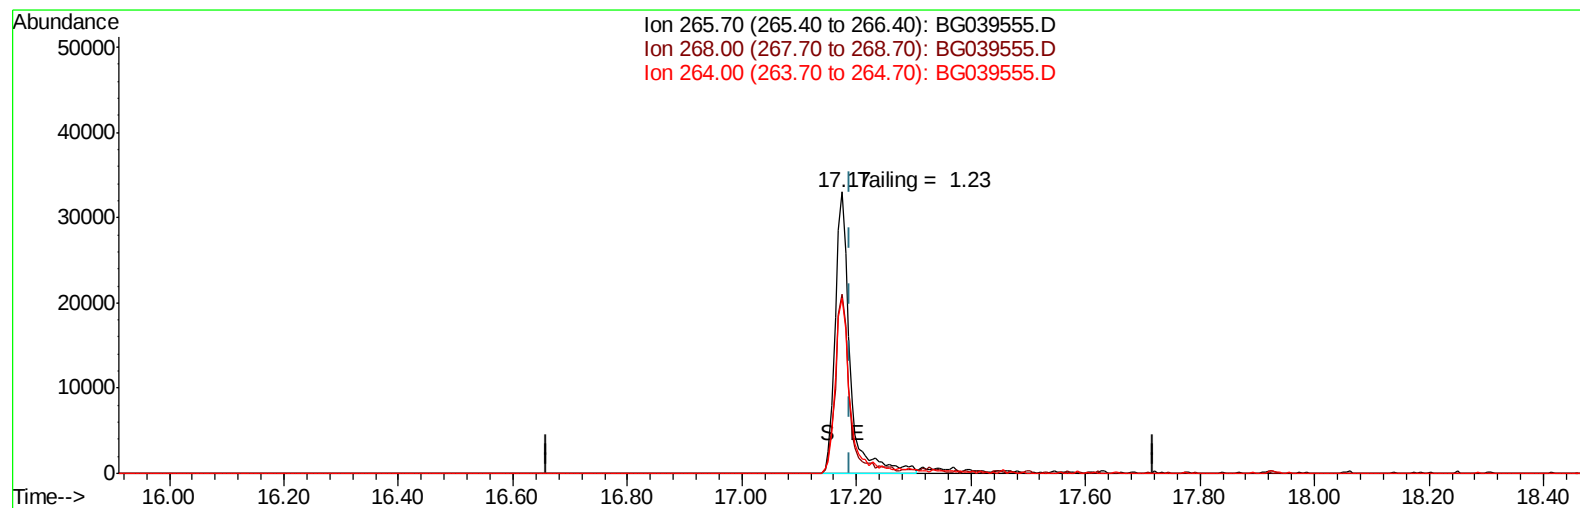

TIC: BG039555.D

(70) Pentachlorophenol (C)




17.175min (-0.015) 115766.01ng

response 58211

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.73
264.00	65.10	62.20
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021919\
Data File : BG039555.D
Acq On : 19 Feb 2019 14:18
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 02:03:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

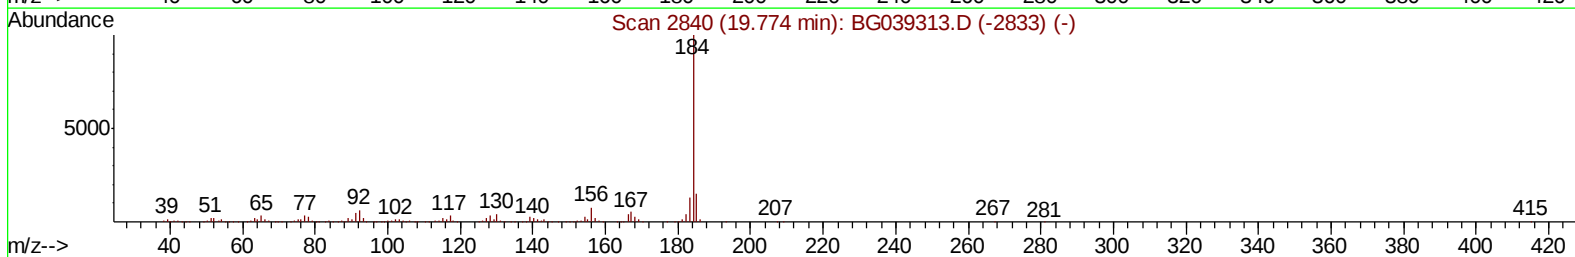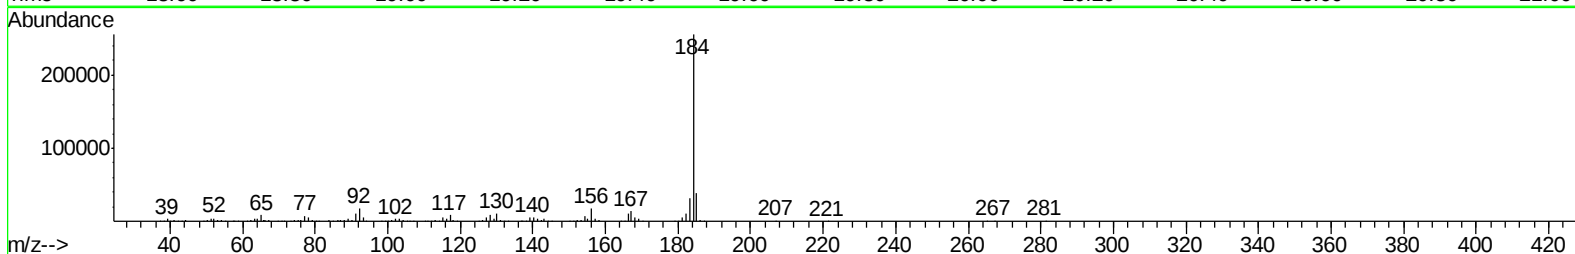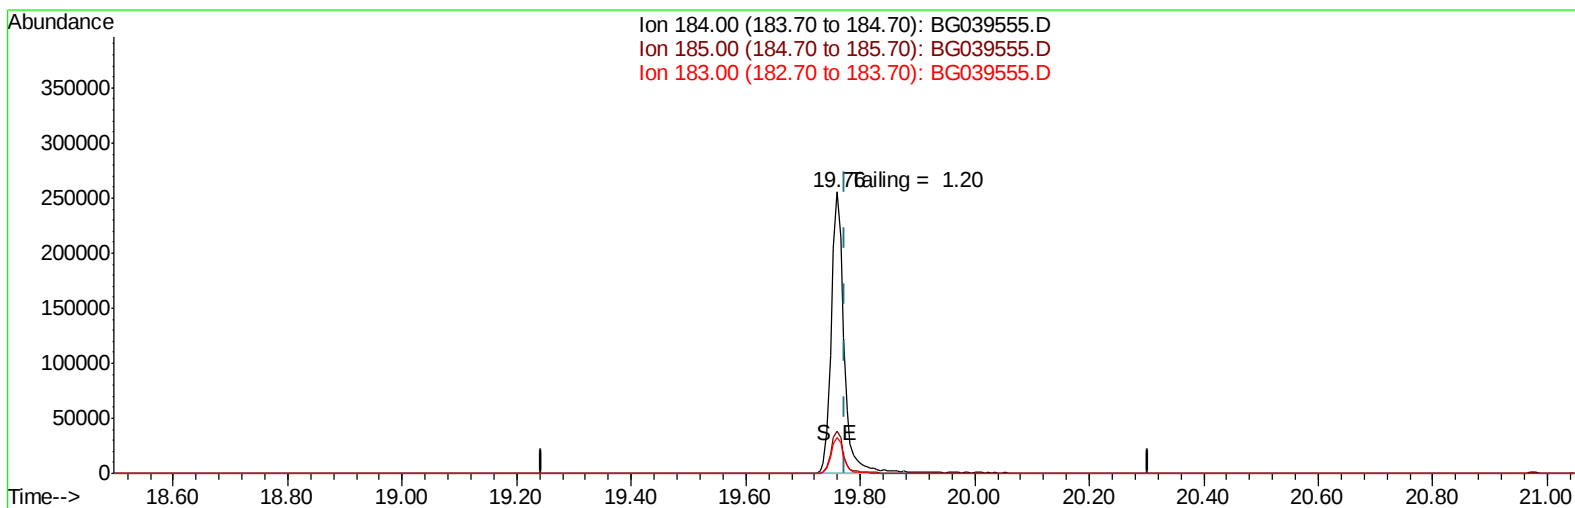

TIC: BG039555.D

(77) Benzidine

19.759min (-0.015) 64087.71ng

response 397118

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.94
183.00	13.20	12.52
0.00	0.00	0.00