
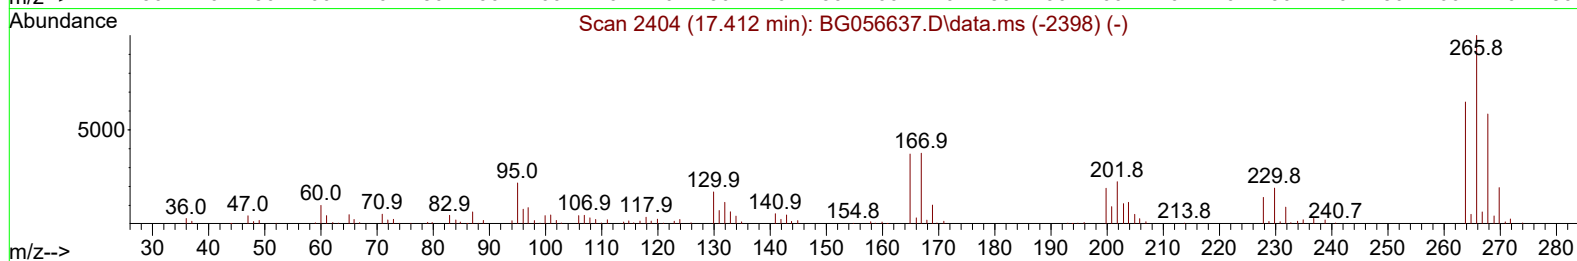
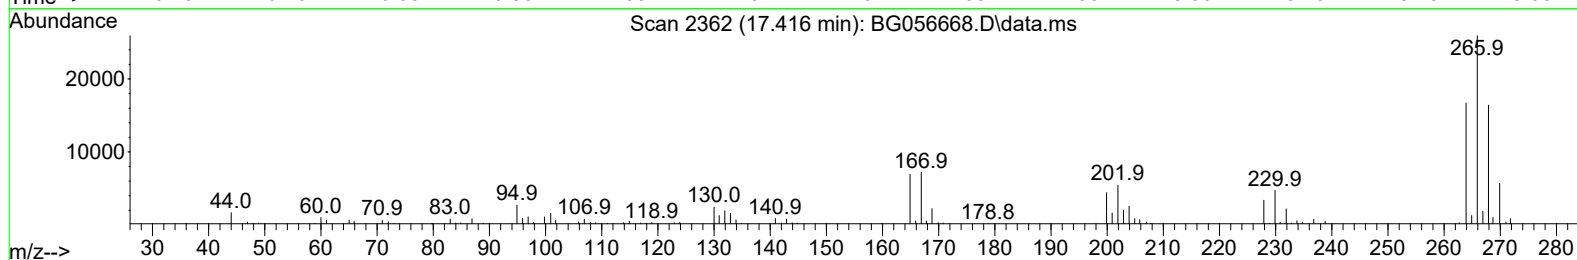


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022023\
 Data File : BG056668.D
 Acq On : 20 Feb 2023 11:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 04:33:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 16 01:33:33 2023
 Response via : Initial Calibration

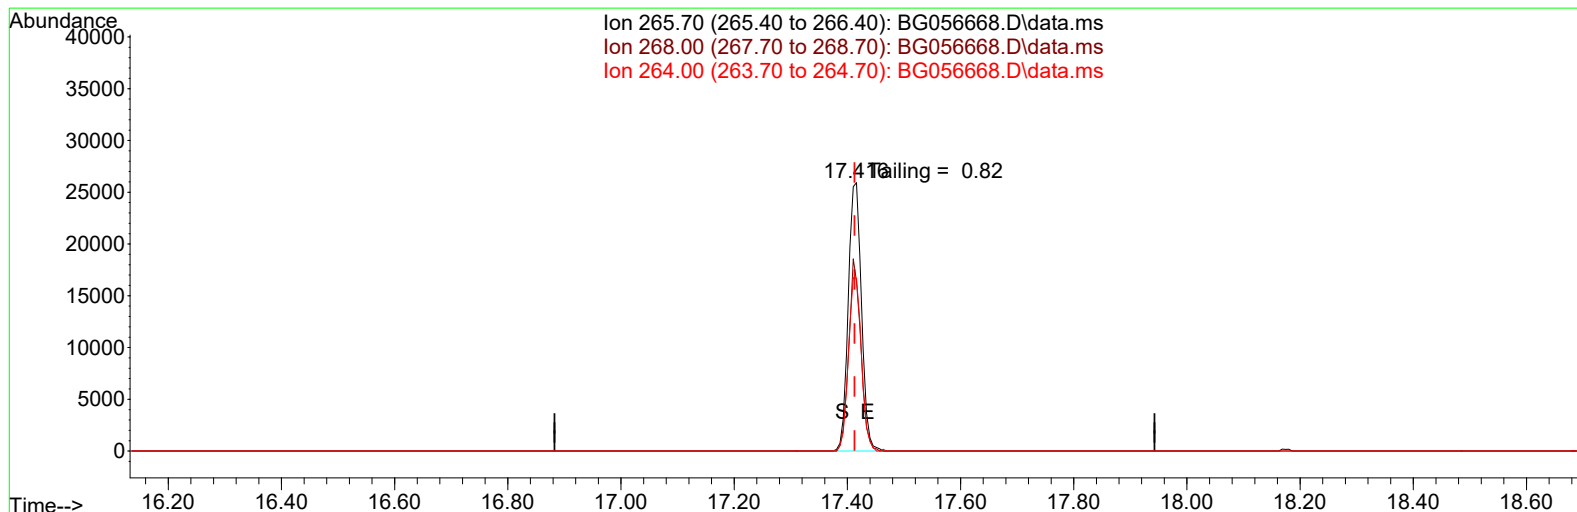

TIC: BG056668.D\data.ms

(70) Pentachlorophenol (C)




17.416min (+ 0.004) 25237.08 ng

response 41975

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	58.40	67.14
264.00	64.70	64.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022023\
 Data File : BG056668.D
 Acq On : 20 Feb 2023 11:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 04:33:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 16 01:33:33 2023
 Response via : Initial Calibration

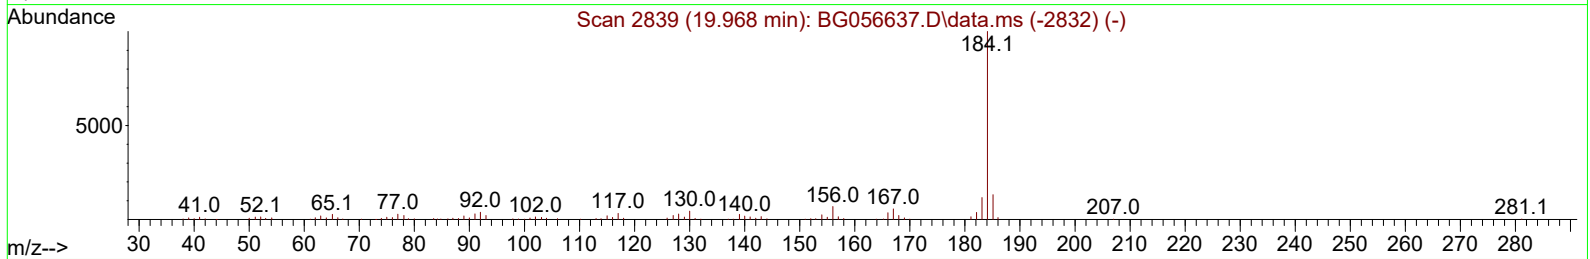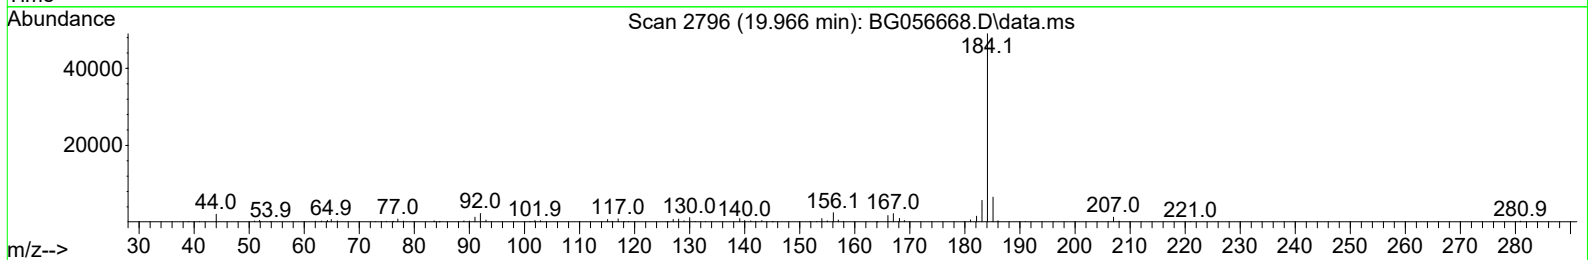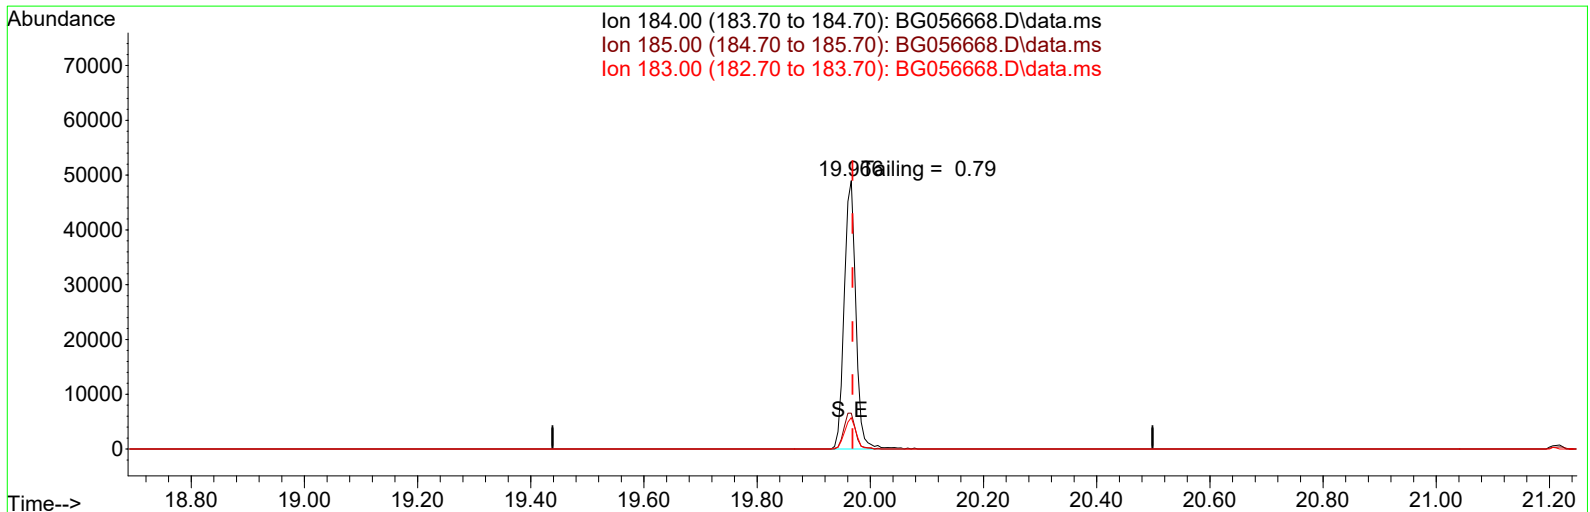

TIC: BG056668.D\data.ms

(77) Benzidine

19.966min (-0.002) 0.00 ng

response 69438

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.20	13.39
183.00	11.70	11.71
0.00	0.00	0.00