


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022023\
Data File : BG056668.D
Acq On : 20 Feb 2023 11:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 16 01:33:33 2023

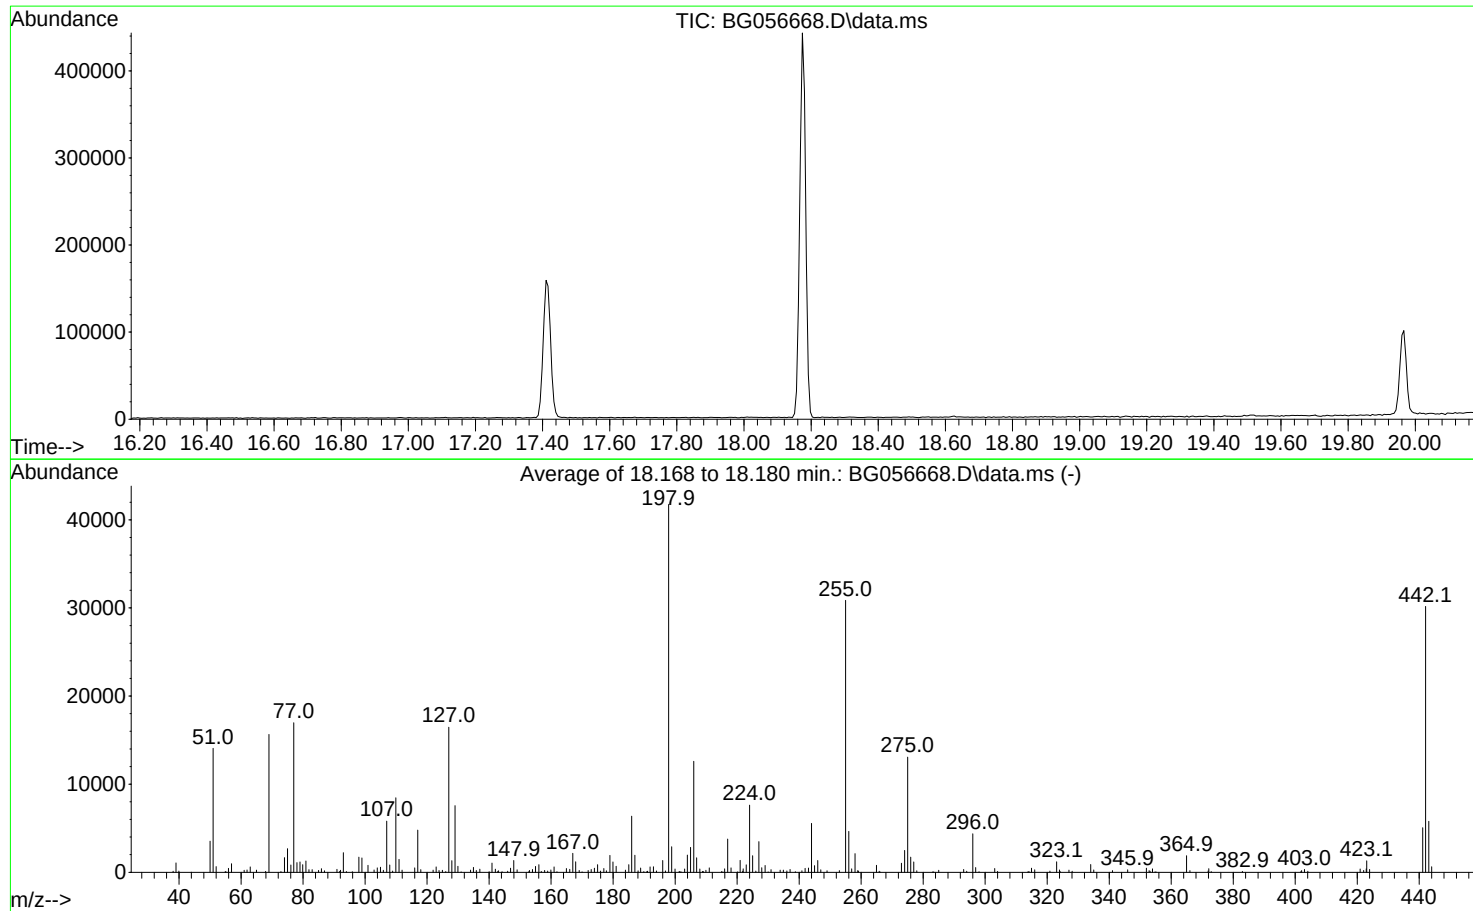




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	14066	PASS
68	69	0.00	2	0.6	96	PASS
69	198	0.00	100	37.5	15648	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.4	16466	PASS
197	198	0.00	2	0.3	146	PASS
198	198	100	100	100.0	41749	PASS
199	198	5	9	6.9	2897	PASS
275	198	10	60	31.3	13061	PASS
365	198	1	100	4.5	1875	PASS
441	198	0.01	100	12.1	5051	PASS
442	442	50	100	100.0	30171	PASS
443	442	15	24	19.2	5783	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022023\
Data File : BG056668.D
Acq On : 20 Feb 2023 11:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 21 04:33:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 16 01:33:33 2023
Response via : Initial Calibration

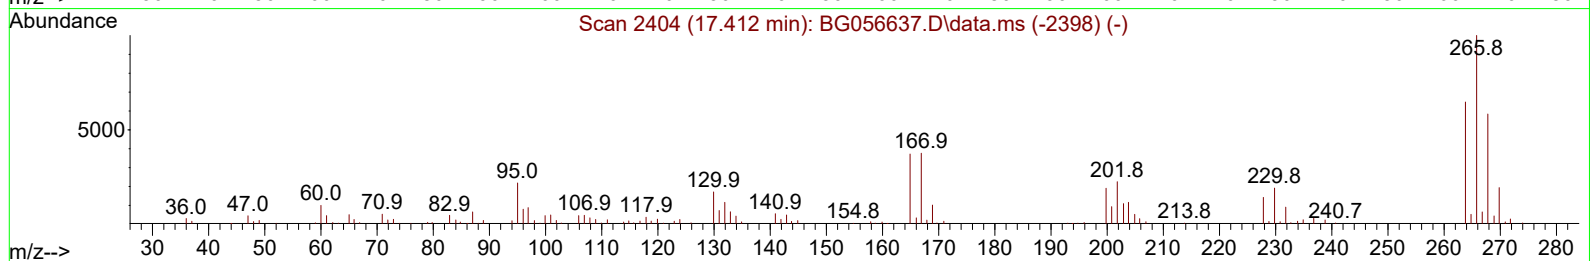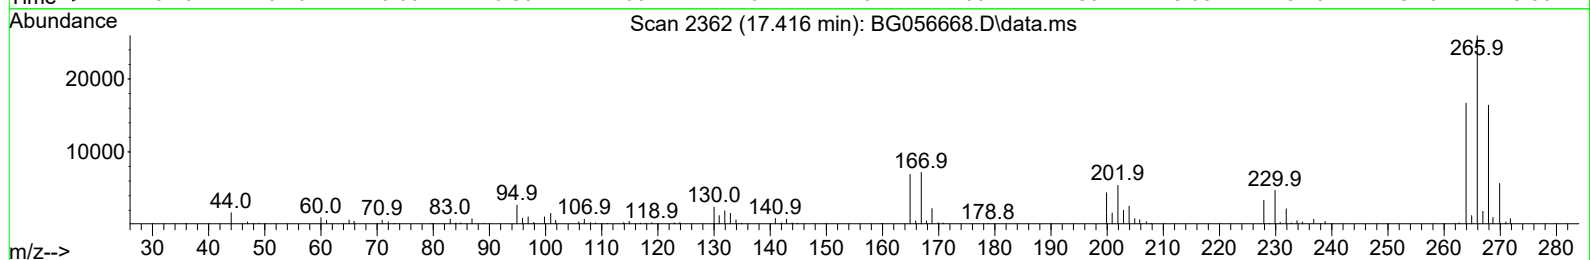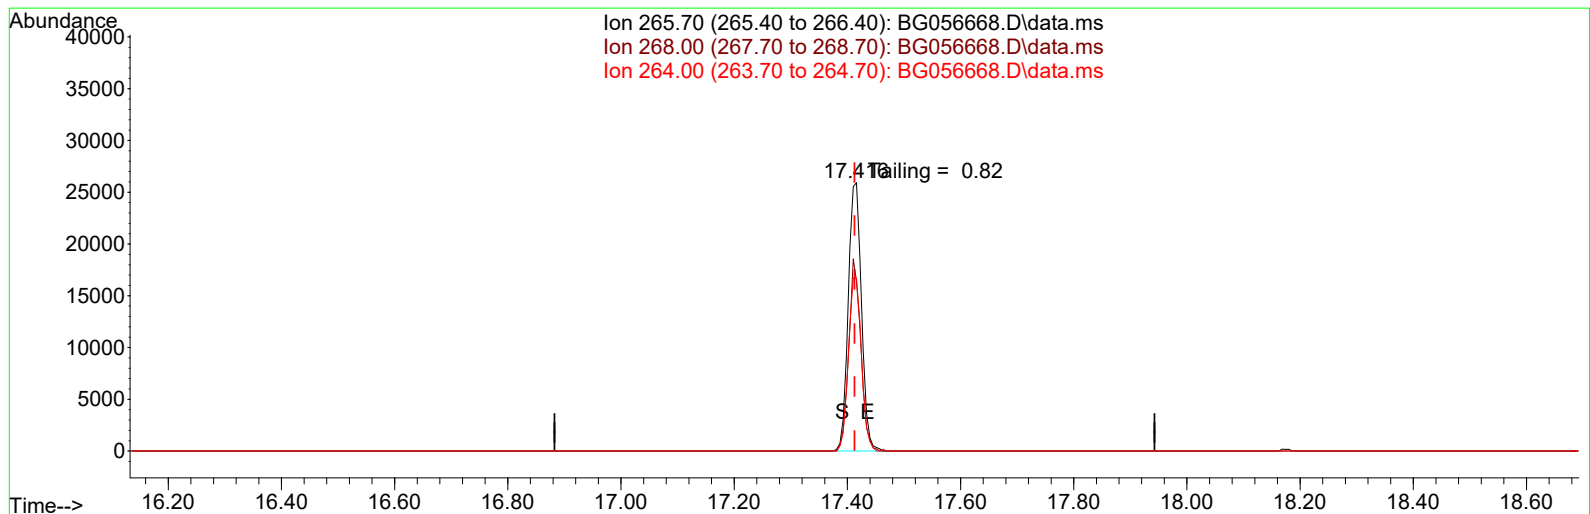

TIC: BG056668.D\data.ms

(70) Pentachlorophenol (C)

17.416min (+ 0.004) 25237.08 ng




response 41975

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	58.40	67.14
264.00	64.70	64.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022023\
 Data File : BG056668.D
 Acq On : 20 Feb 2023 11:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Feb 21 04:33:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 16 01:33:33 2023
 Response via : Initial Calibration

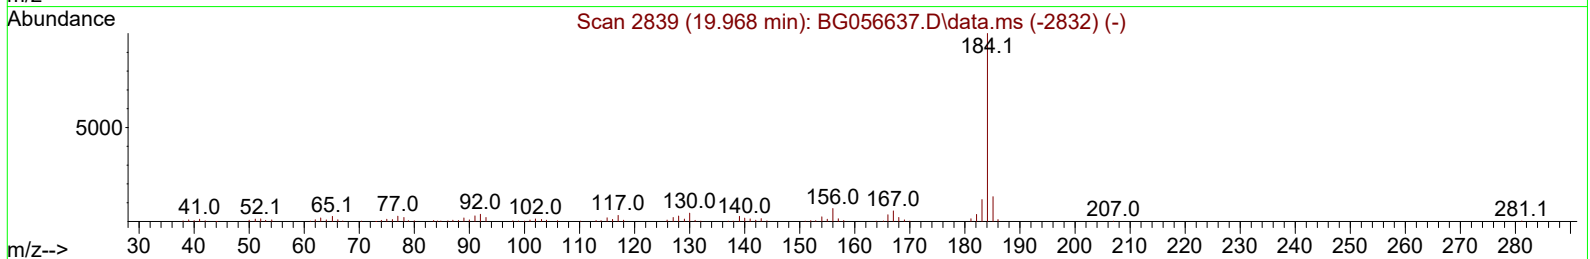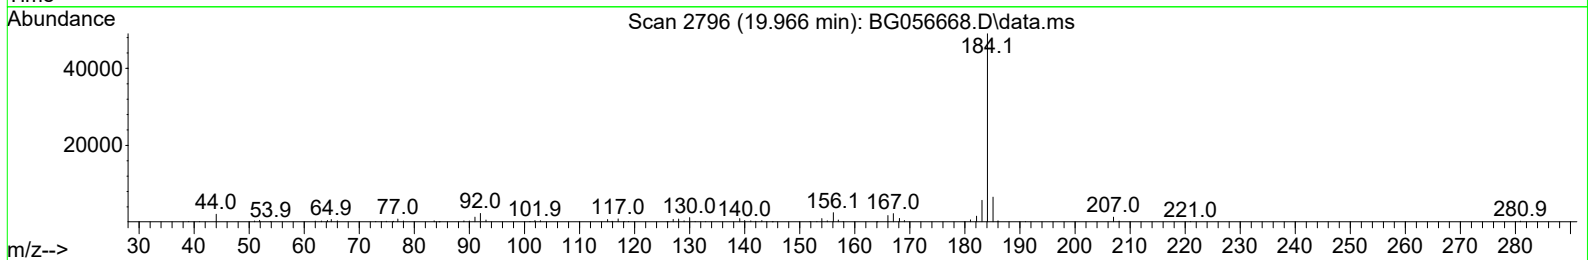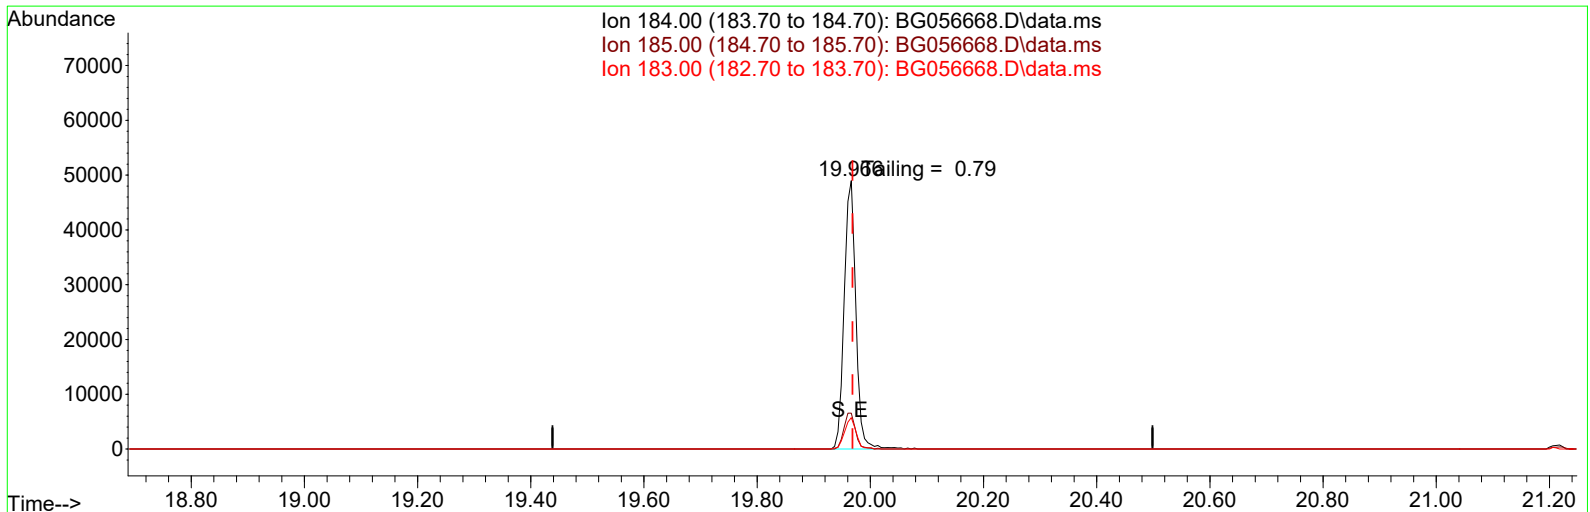

TIC: BG056668.D\data.ms

(77) Benzidine

19.966min (-0.002) 0.00 ng

response 69438

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.20	13.39
183.00	11.70	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/20/2023	BNA_G	<u>BG056668.D</u>
Compound Name	Response	Retention Time
DDT	97214	21.212
DDD	3606	20.748
DDE	68	20.254
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3674	100888	3.64

Instrument :
BNA_G
ClientSampleId :
DFTPP