
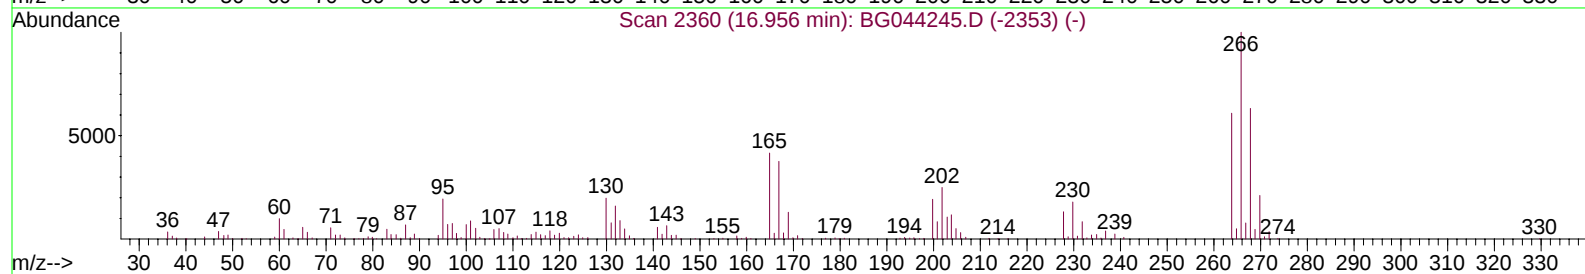
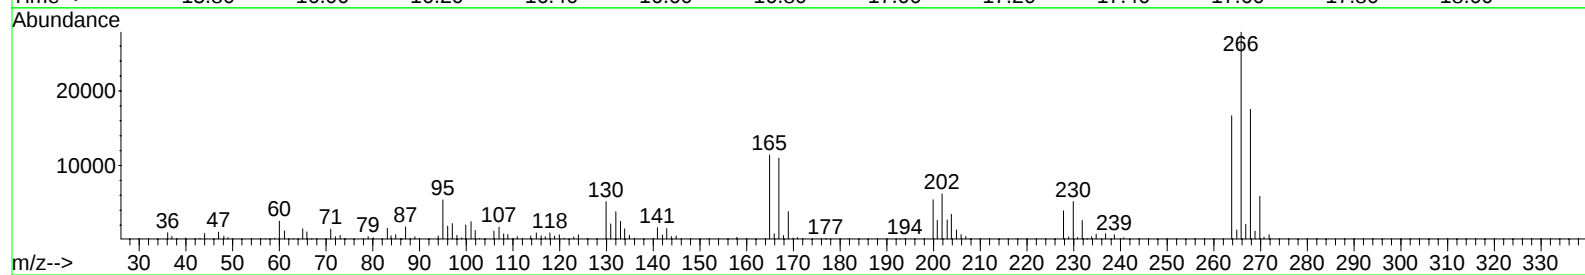


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG022120\
Data File : BG044541.D
Acq On : 21 Feb 2020 9:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 17:45:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 21 16:02:12 2020
Response via : Initial Calibration

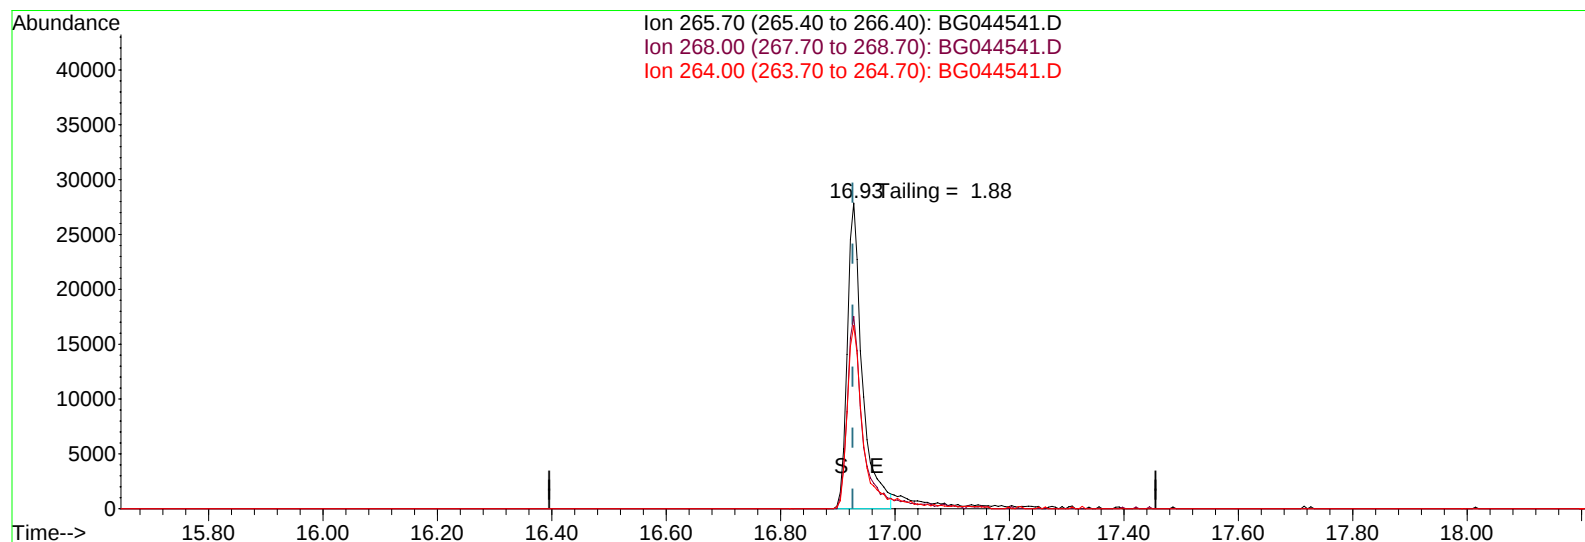

TIC: BG044541.D

(70) Pentachlorophenol (C)




16.928min (+0.002) 34732.70ng

response 54666

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	62.89
264.00	62.30	59.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG022120\
 Data File : BG044541.D
 Acq On : 21 Feb 2020 9:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 17:45:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 21 16:02:12 2020
 Response via : Initial Calibration

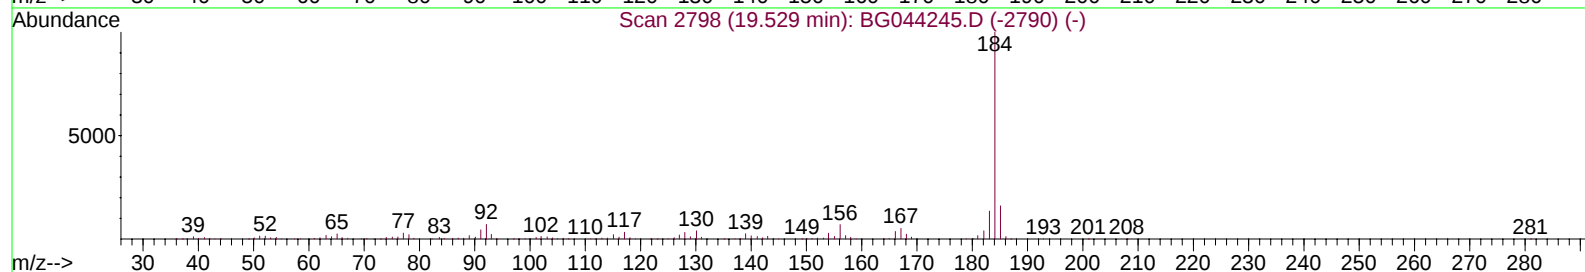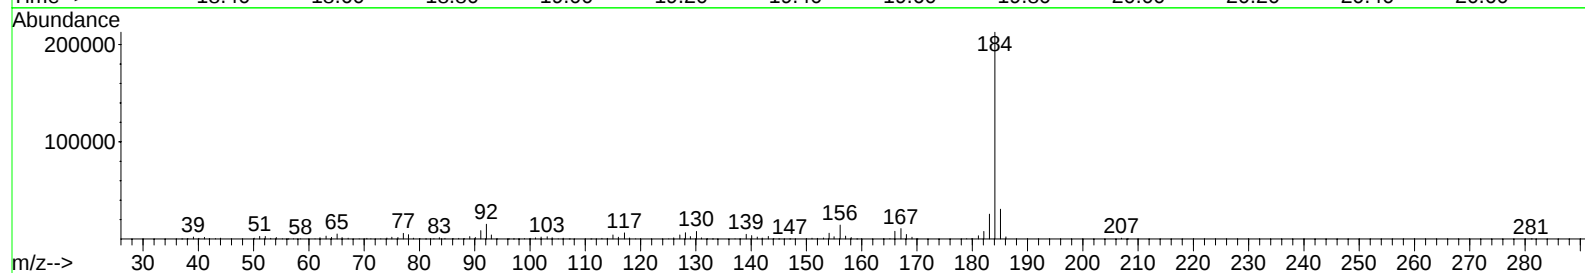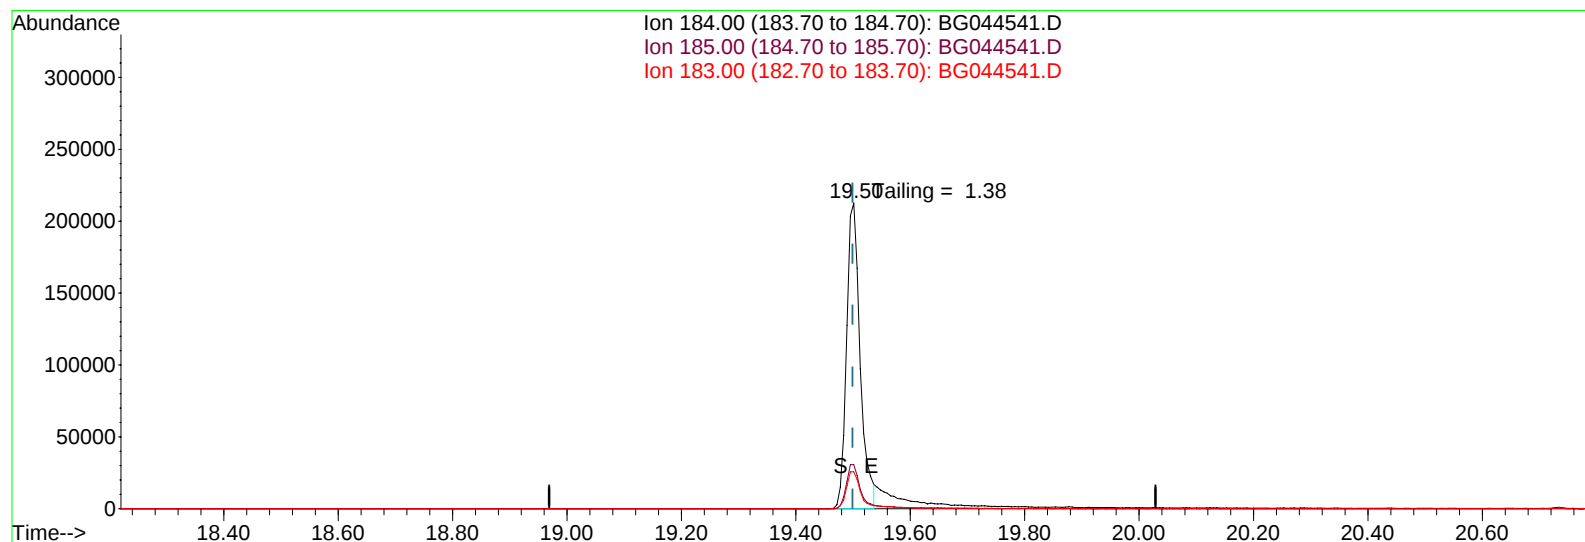

TIC: BG044541.D

(77) Benzidine

19.501min (+0.002) 0.00ng

response 406170

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	14.44
183.00	13.70	12.09
0.00	0.00	0.00