

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022120\
 Data File : BG044546.D
 Acq On : 21 Feb 2020 12:58
 Operator : CG/JU
 Sample : PB126914BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB126914BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	396	403	418	rBV	804183	1327897	26.85%	7.083%
2	7.055	667	675	695	rBV	790249	1405424	28.41%	7.496%
3	7.878	808	815	825	rBV	158757	274615	5.55%	1.465%
4	8.201	863	870	884	rBV	661675	1139454	23.04%	6.078%
5	9.036	1004	1012	1028	rBV	474046	887462	17.94%	4.733%
6	10.681	1284	1292	1311	rBV	196018	394327	7.97%	2.103%
7	13.142	1704	1711	1735	rBV	1421071	2327254	47.05%	12.413%
8	14.523	1939	1946	1958	rBV	376436	625434	12.64%	3.336%
9	16.010	2192	2199	2221	rBV	1239351	2012285	40.68%	10.733%
10	17.267	2406	2413	2427	rBV	550046	881931	17.83%	4.704%
11	19.882	2852	2858	2874	rBV	3698926	4946320	100.00%	26.382%
12	21.509	3128	3135	3148	rBV	637737	1064520	21.52%	5.678%
13	21.709	3164	3169	3175	rBV	39290	59689	1.21%	0.318%
14	22.296	3263	3269	3276	rBV	48812	79885	1.62%	0.426%
15	22.954	3375	3381	3390	rVB2	51903	90224	1.82%	0.481%
16	23.724	3505	3512	3519	rBV2	36684	79456	1.61%	0.424%
17	24.576	3647	3657	3674	rBV2	389385	1152437	23.30%	6.147%


Sum of corrected areas: 18748614

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022120\
Data File : BG044546.D
Acq On : 21 Feb 2020 12:58
Operator : CG/JU
Sample : PB126914BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB126914BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

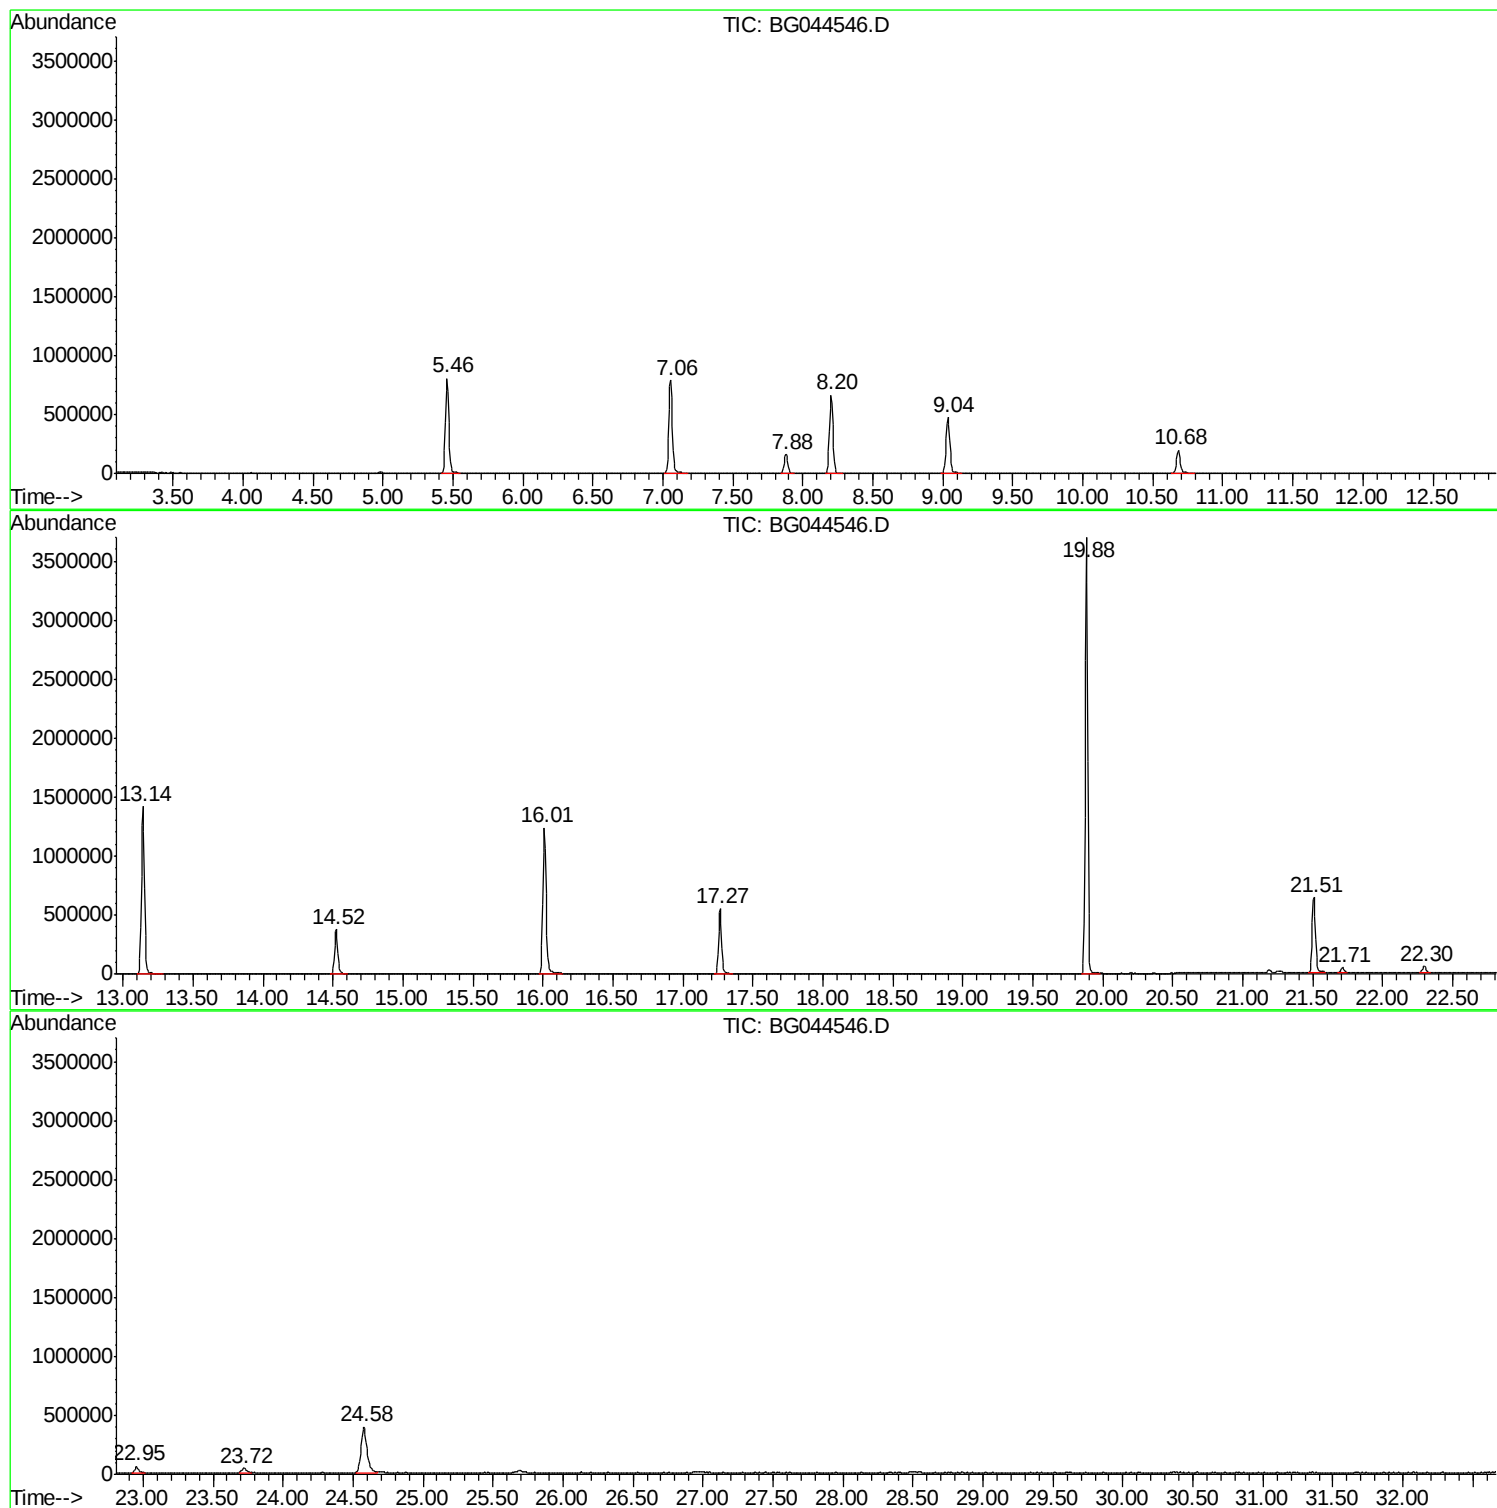

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG022120\
Data_File : BG044546.D
Acq_On : 21_Feb_2020 12:588
Operator : CG/JUU
Sample : PB126914BLL
Misc :
ALS_Vial : 6 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
PB126914BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
