


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022120\
 Data File : BG044541.D
 Acq On : 21 Feb 2020 9:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 21 16:02:12 2020

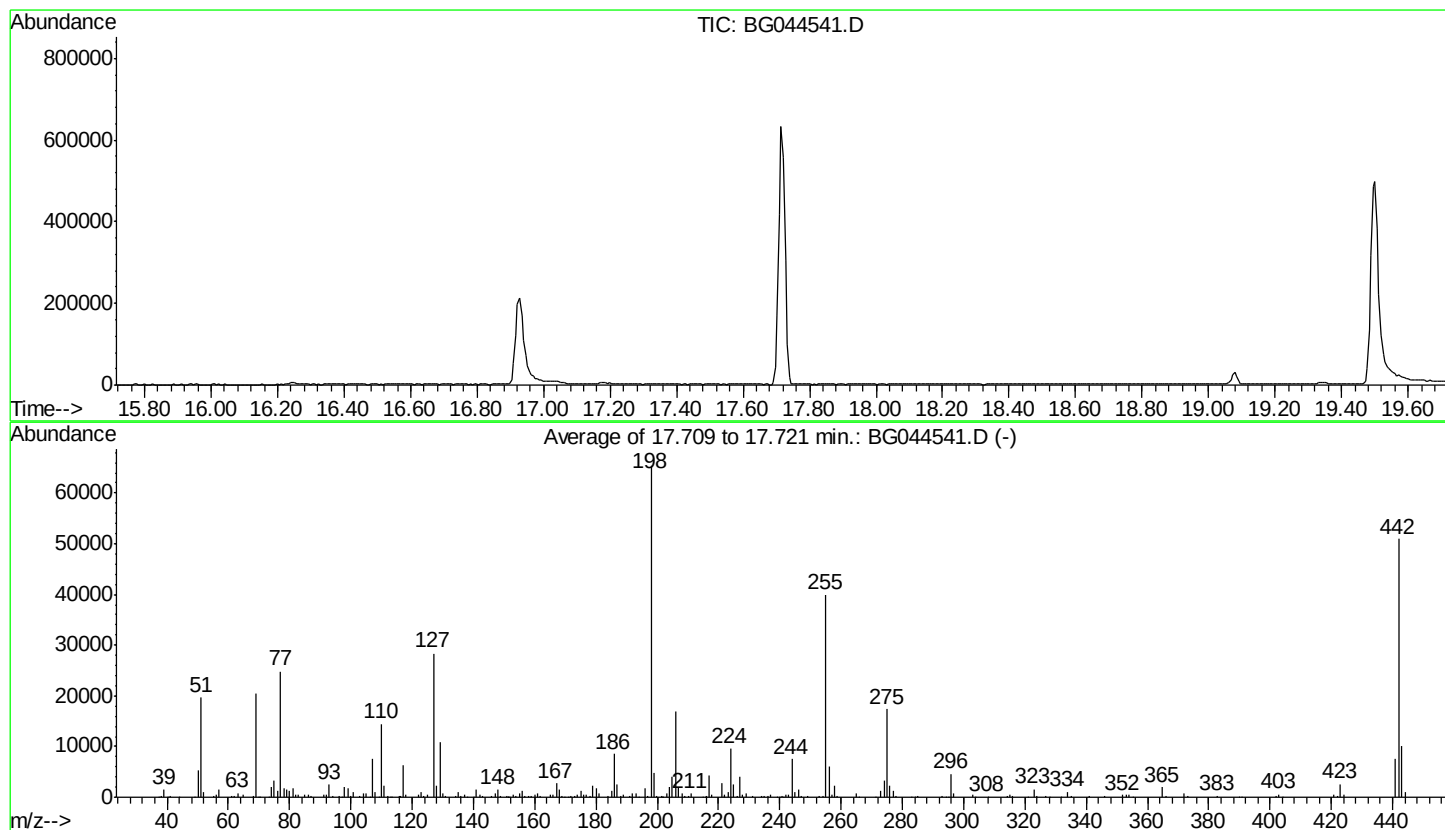

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	19610	PASS
68	69	0.00	2	0.8	163	PASS
69	198	0.00	100	31.4	20520	PASS
70	69	0.00	2	0.6	113	PASS
127	198	10	80	43.3	28322	PASS
197	198	0.00	2	0.3	203	PASS
198	198	100	100	100.0	65408	PASS
199	198	5	9	7.2	4734	PASS
275	198	10	60	26.6	17391	PASS
365	198	1	100	3.1	2016	PASS
441	198	0.01	100	11.7	7669	PASS
442	198	50	100	77.8	50888	PASS
443	442	15	24	19.7	10013	PASS