
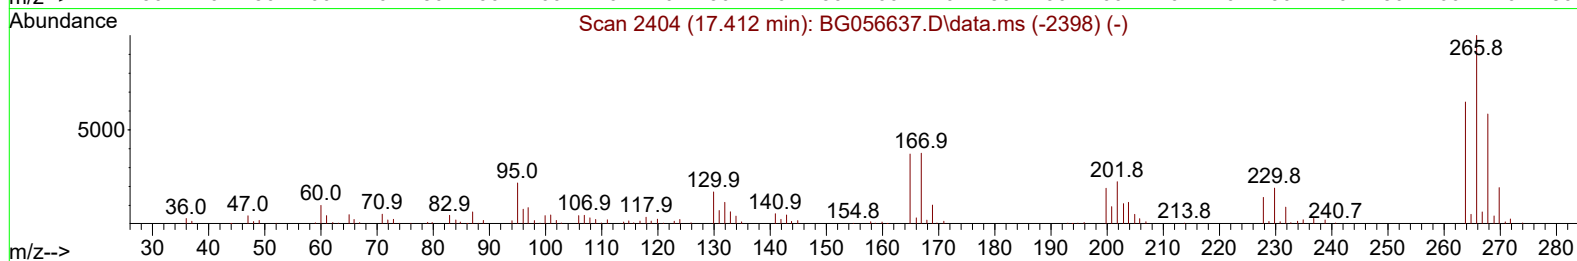
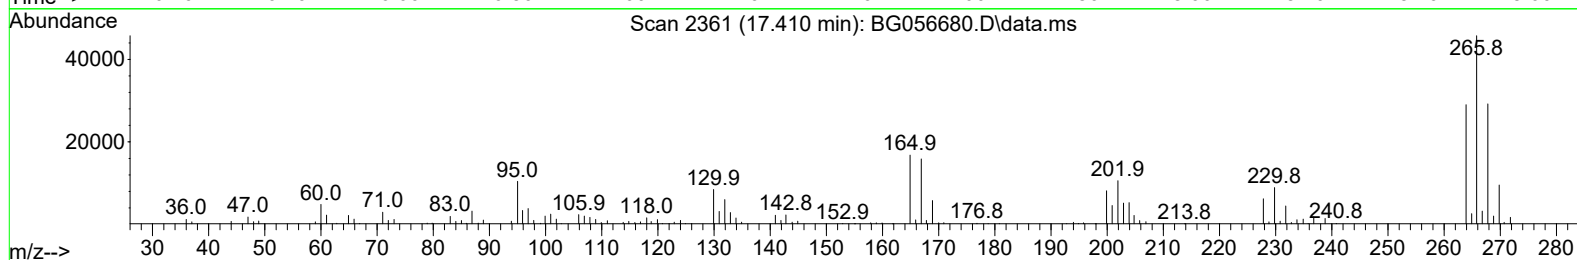


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022123\
Data File : BG056680.D
Acq On : 21 Feb 2023 10:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 03:19:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 21 18:07:35 2023
Response via : Initial Calibration

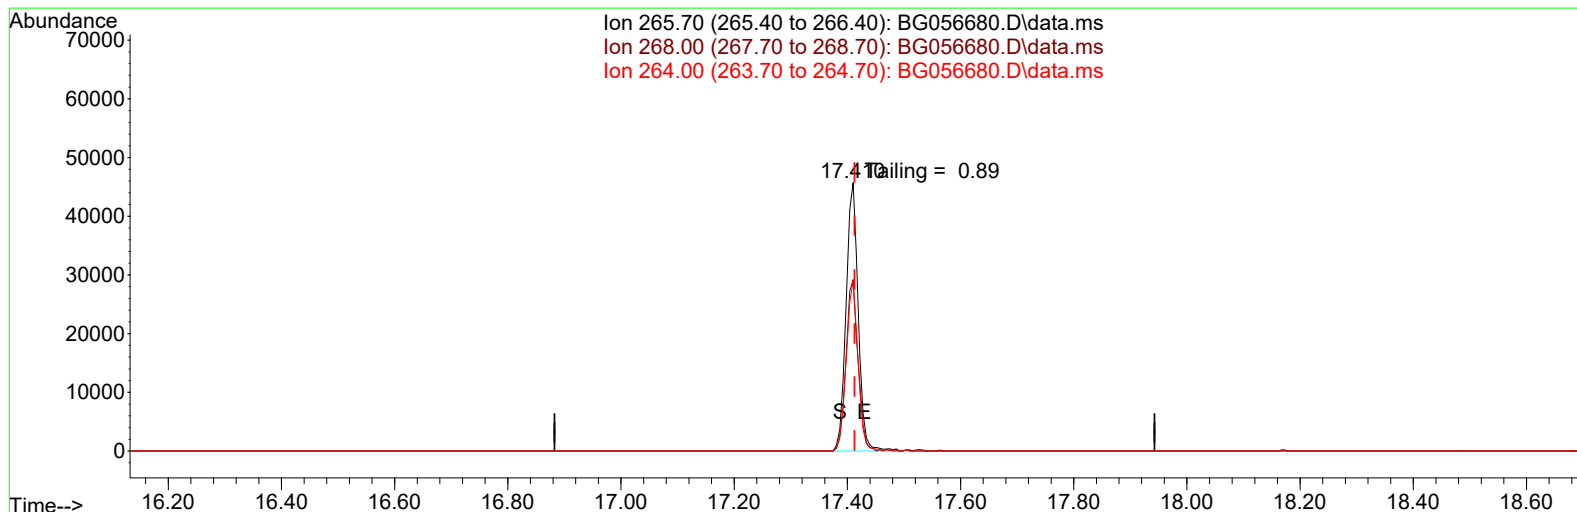

TIC: BG056680.D\data.ms

(70) Pentachlorophenol (C)




17.410min (-0.002) 25113.73 ng

response 67876

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	58.40	63.84
264.00	64.70	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022123\
 Data File : BG056680.D
 Acq On : 21 Feb 2023 10:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 03:19:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 21 18:07:35 2023
 Response via : Initial Calibration

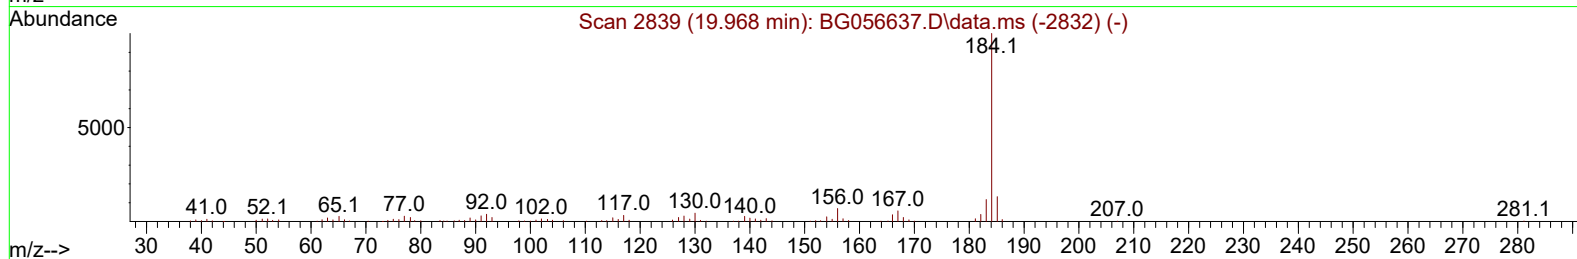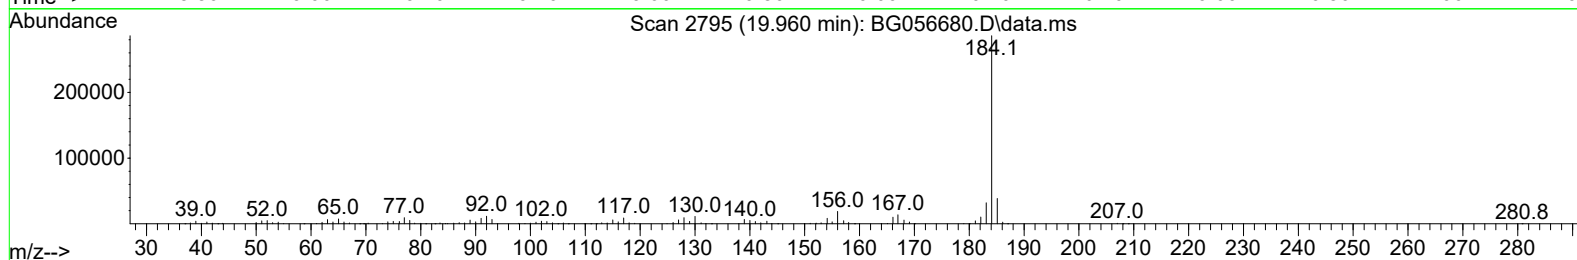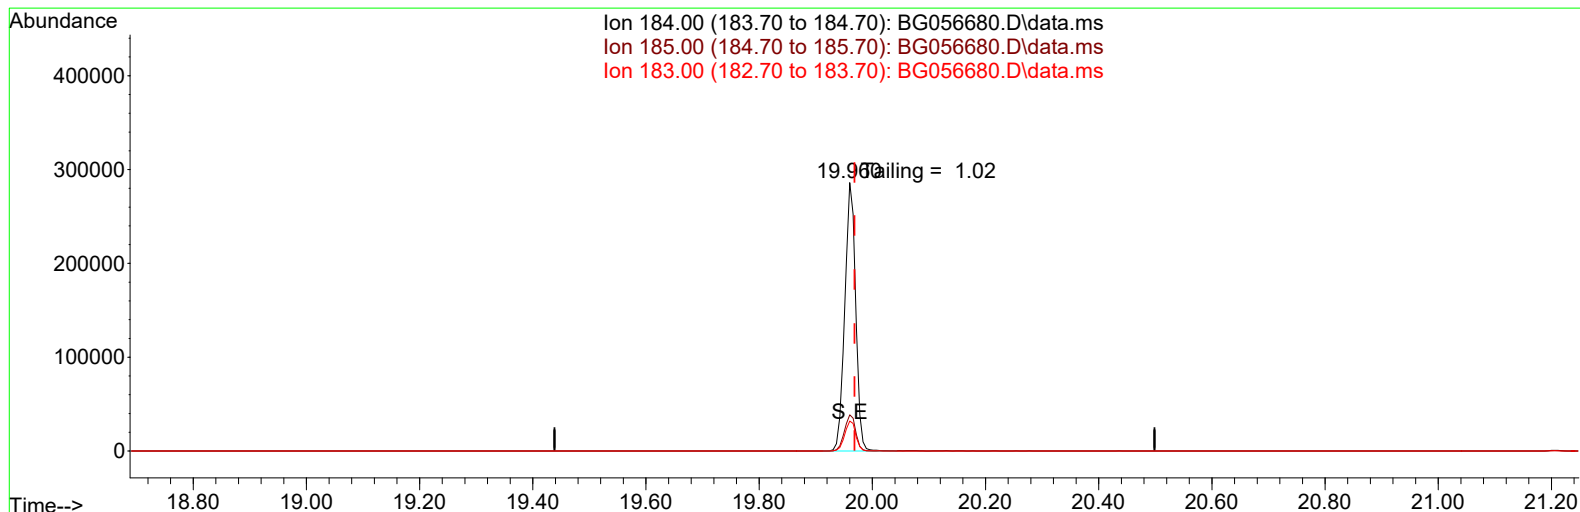

TIC: BG056680.D\data.ms

(77) Benzidine**19.960min (-0.008) 37701.86 ng****response 379633**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.20	13.48
183.00	11.70	11.16
0.00	0.00	0.00