
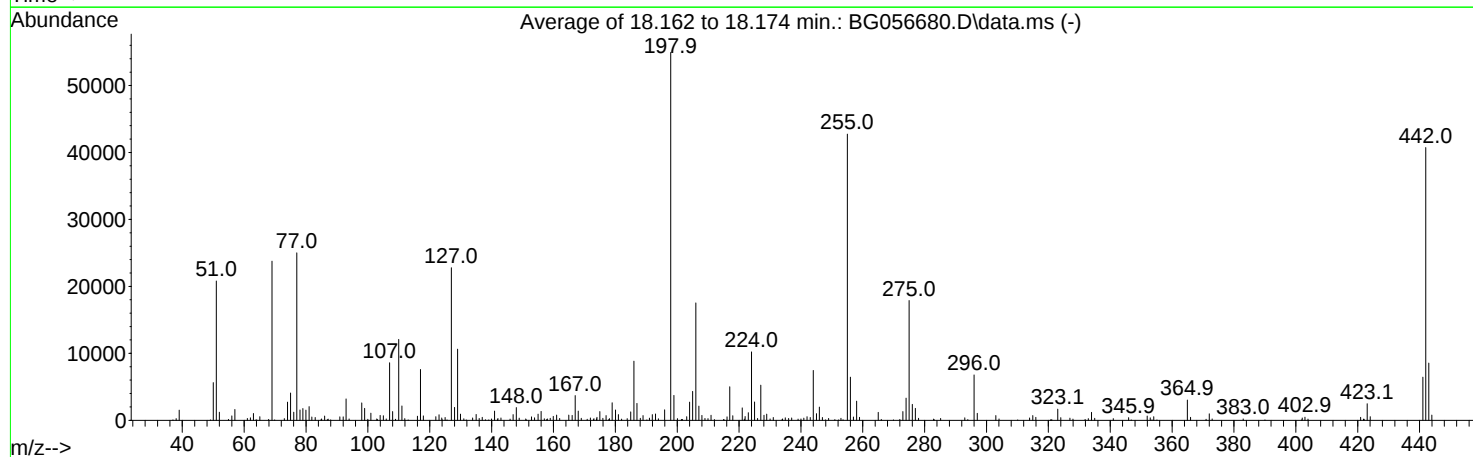


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022123\
 Data File : BG056680.D
 Acq On : 21 Feb 2023 10:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 21 18:07:35 2023

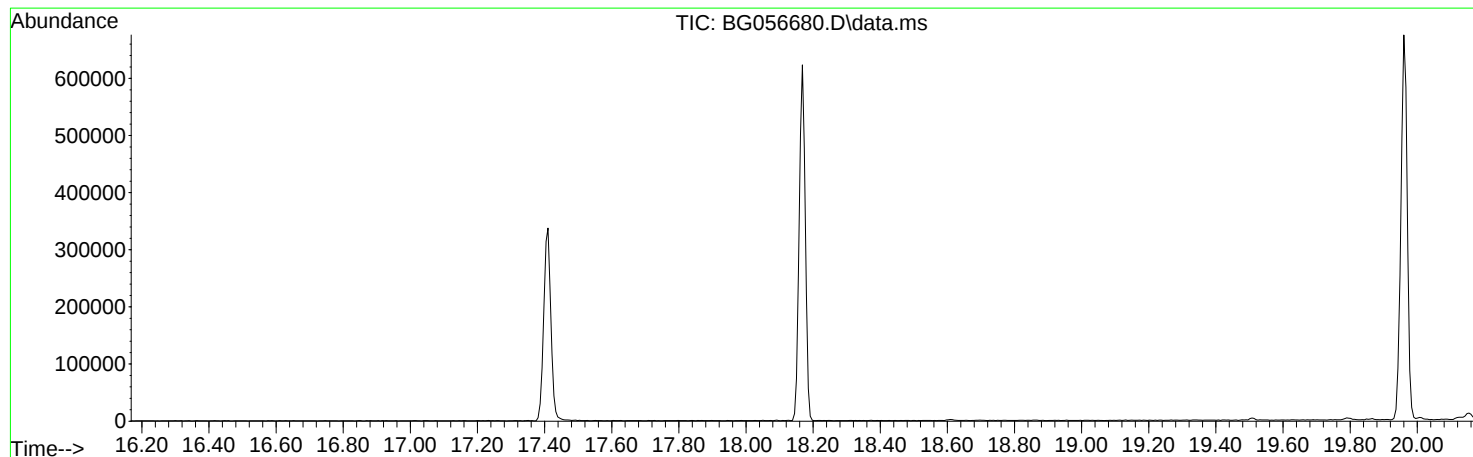




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	20811	PASS
68	69	0.00	2	0.5	129	PASS
69	198	0.00	100	43.3	23768	PASS
70	69	0.00	2	0.2	52	PASS
127	198	10	80	41.5	22781	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54941	PASS
199	198	5	9	6.8	3726	PASS
275	198	10	60	32.6	17894	PASS
365	198	1	100	5.5	3031	PASS
441	198	0.01	100	11.7	6431	PASS
442	442	50	100	100.0	40736	PASS
443	442	15	24	21.0	8548	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022123\
Data File : BG056680.D
Acq On : 21 Feb 2023 10:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 22 03:19:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 21 18:07:35 2023
Response via : Initial Calibration

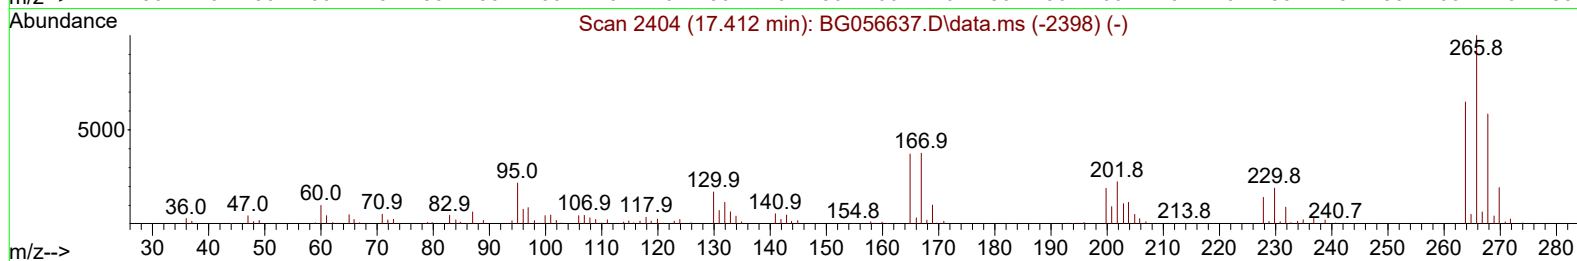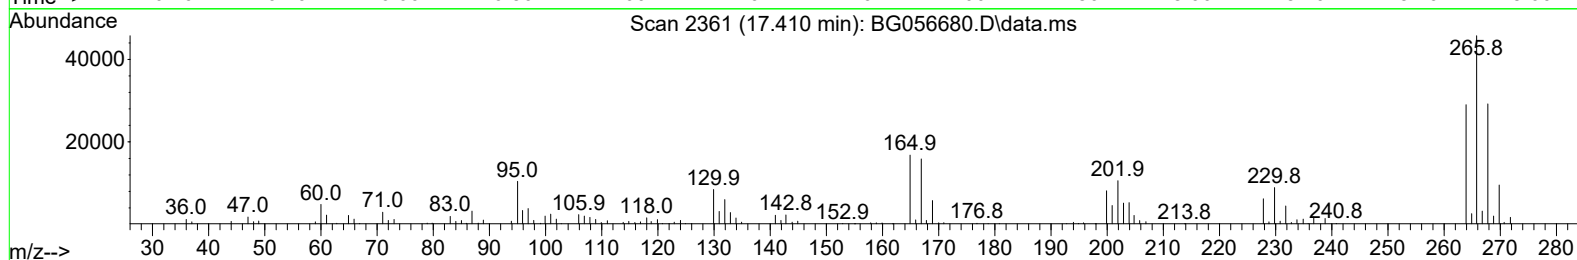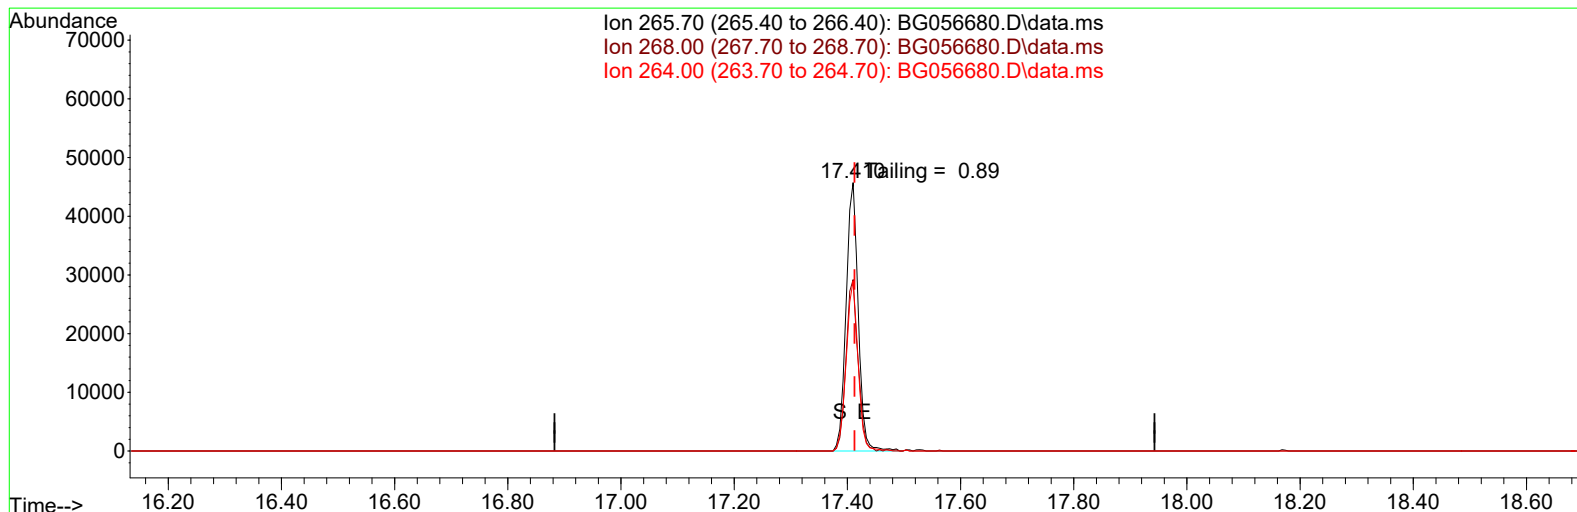

TIC: BG056680.D\data.ms

(70) Pentachlorophenol (C)

17.410min (-0.002) 25113.73 ng




response 67876

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	58.40	63.84
264.00	64.70	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022123\
 Data File : BG056680.D
 Acq On : 21 Feb 2023 10:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Feb 22 03:19:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 21 18:07:35 2023
 Response via : Initial Calibration

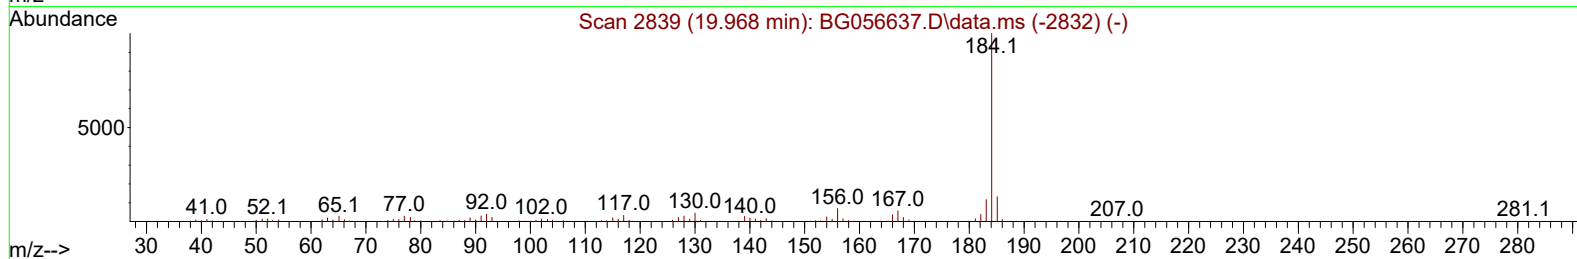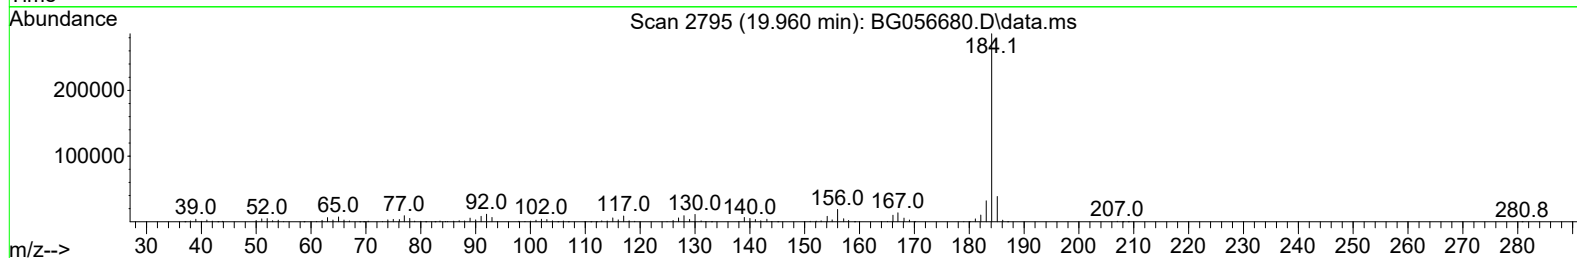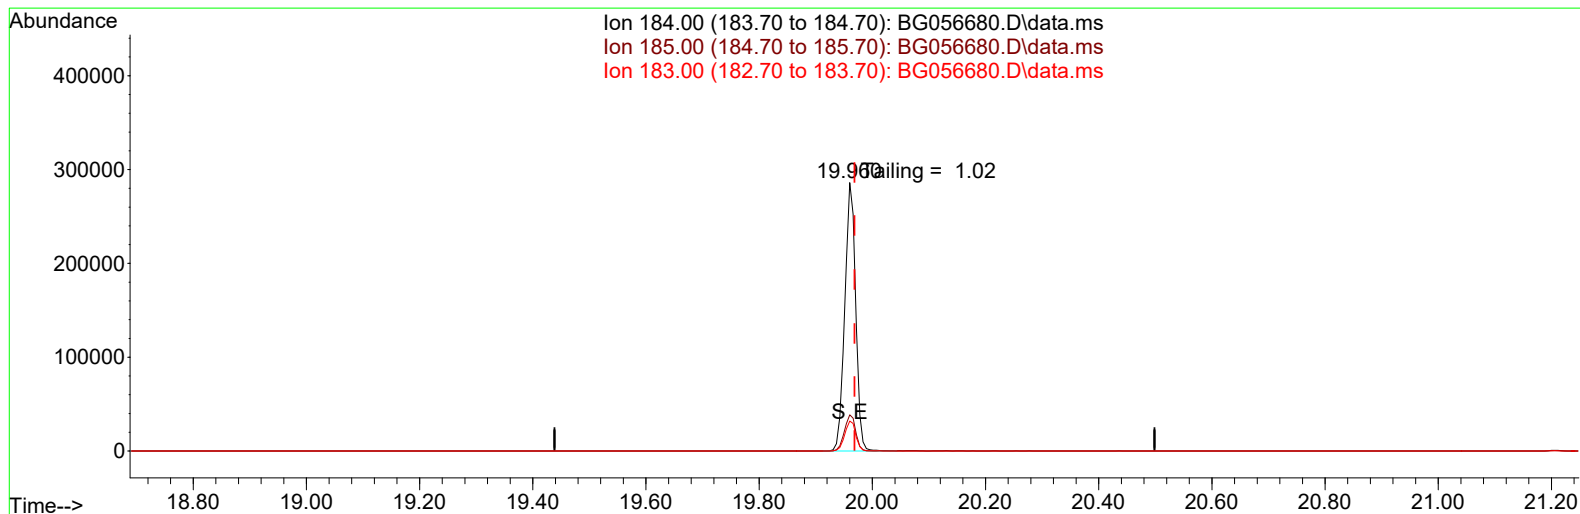

TIC: BG056680.D\data.ms

(77) Benzidine**19.960min (-0.008) 37701.86 ng****response 379633**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.20	13.48
183.00	11.70	11.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/21/2023	BNA_G	<u>BG056680.D</u>
Compound Name	Response	Retention Time
DDT	155467	21.206
DDD	4902	20.741
DDE	0	20.254
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4902	160369	3.06

Instrument :
BNA_G
ClientSampleId :
DFTPP