
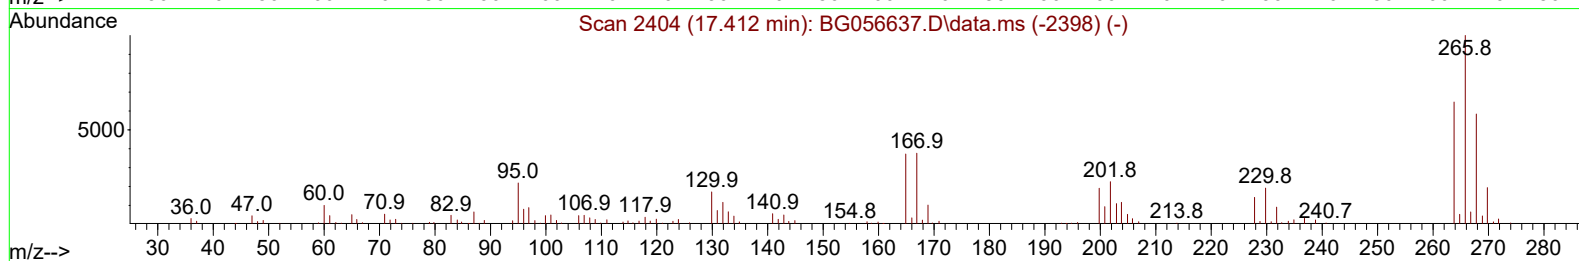
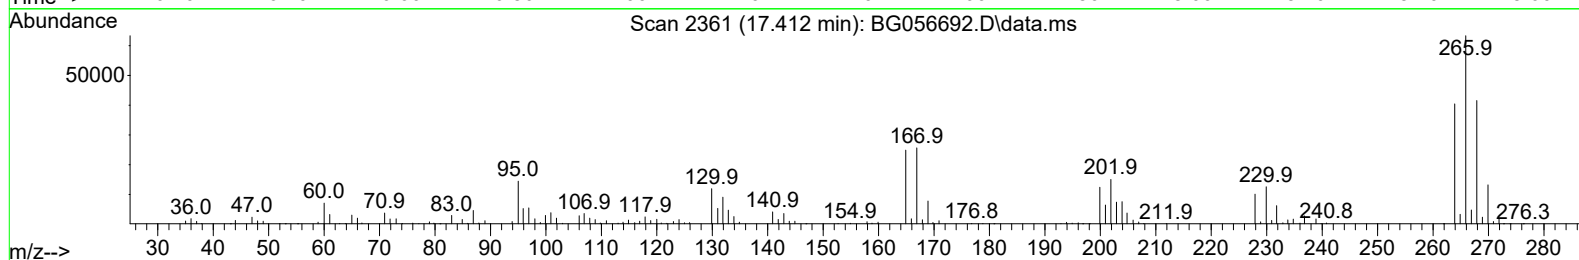


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022223\
Data File : BG056692.D
Acq On : 22 Feb 2023 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 04:22:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 23 01:45:41 2023
Response via : Initial Calibration

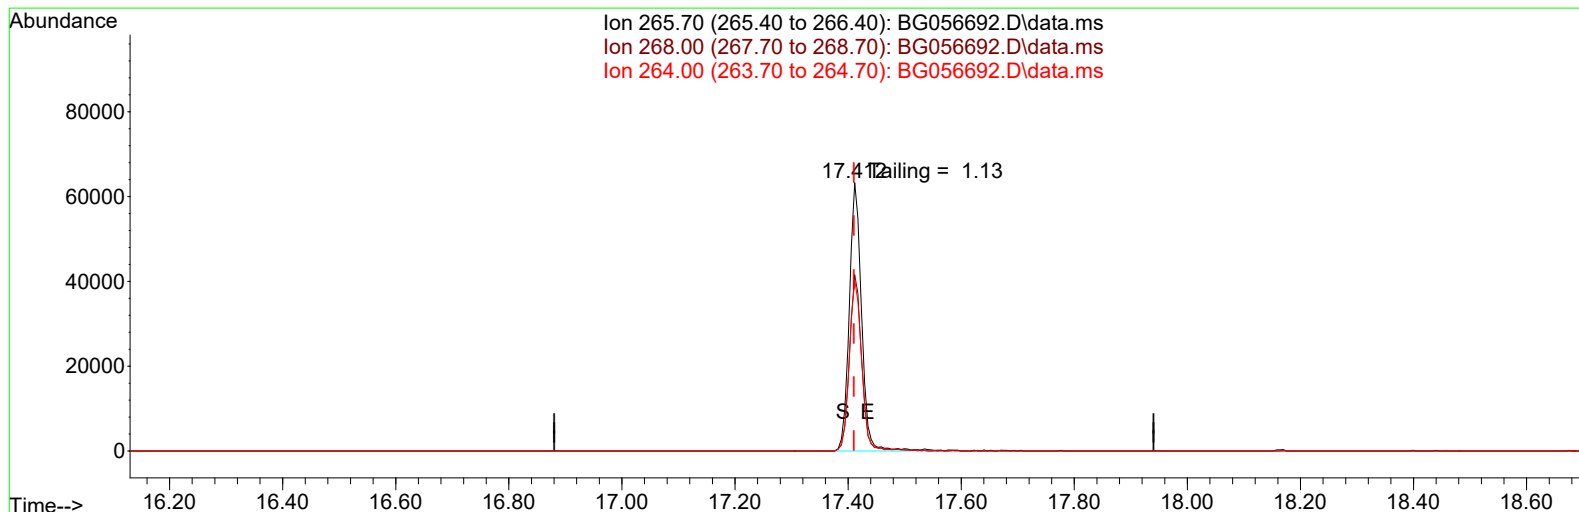

TIC: BG056692.D\data.ms

(70) Pentachlorophenol (C)




17.412min (+ 0.002) 18200.95 ng

response 94601

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	58.40	65.64
264.00	64.70	63.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022223\
 Data File : BG056692.D
 Acq On : 22 Feb 2023 10:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 04:22:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 23 01:45:41 2023
 Response via : Initial Calibration

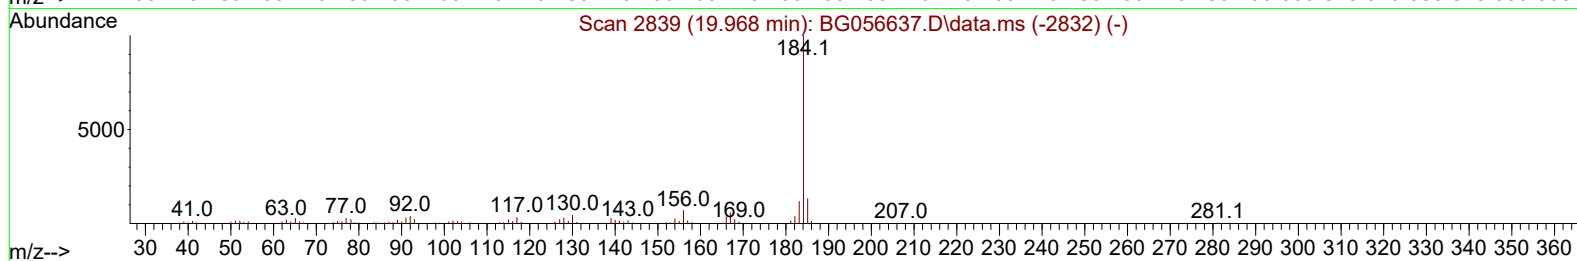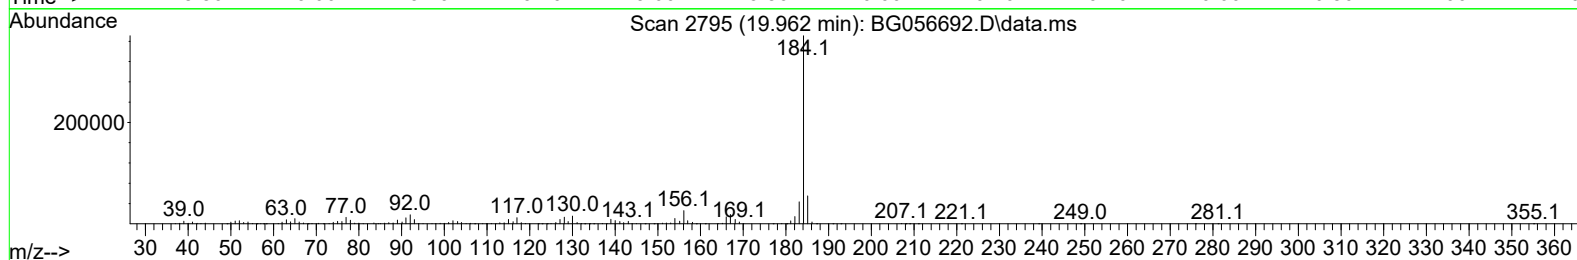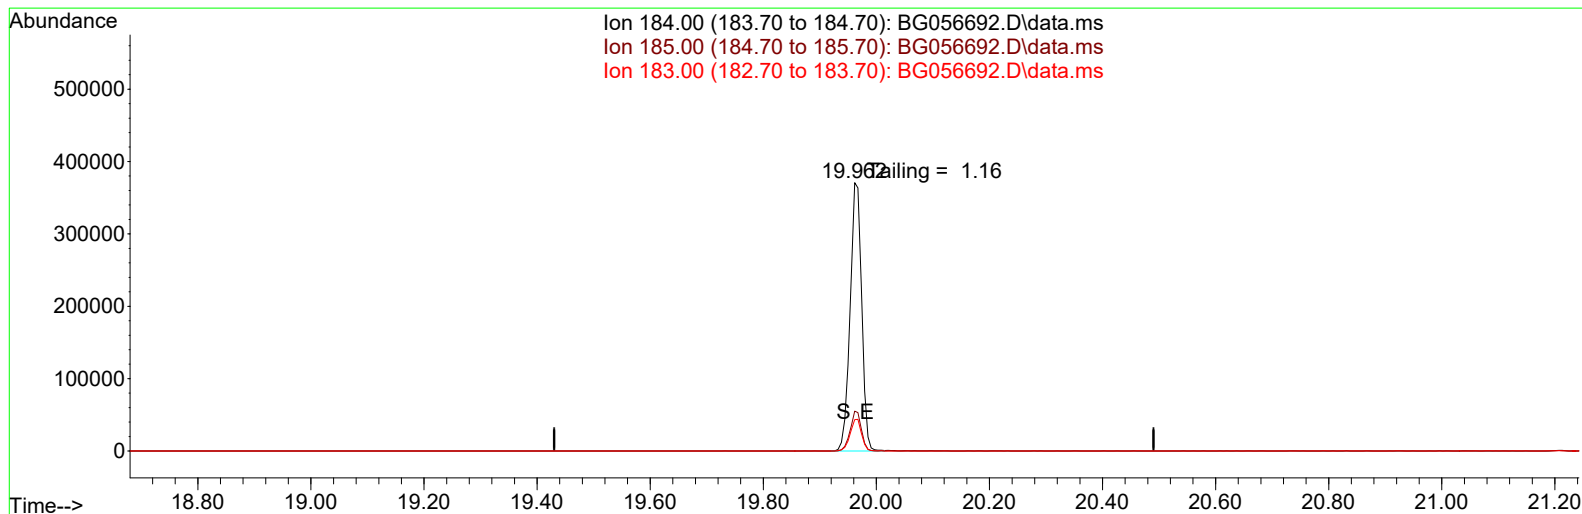

TIC: BG056692.D\data.ms

(77) Benzidine

19.960min (-19.960) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	13.20	0.00#
183.00	11.70	0.00#
0.00	0.00	0.00