


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022223\
Data File : BG056692.D
Acq On : 22 Feb 2023 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 23 01:45:41 2023

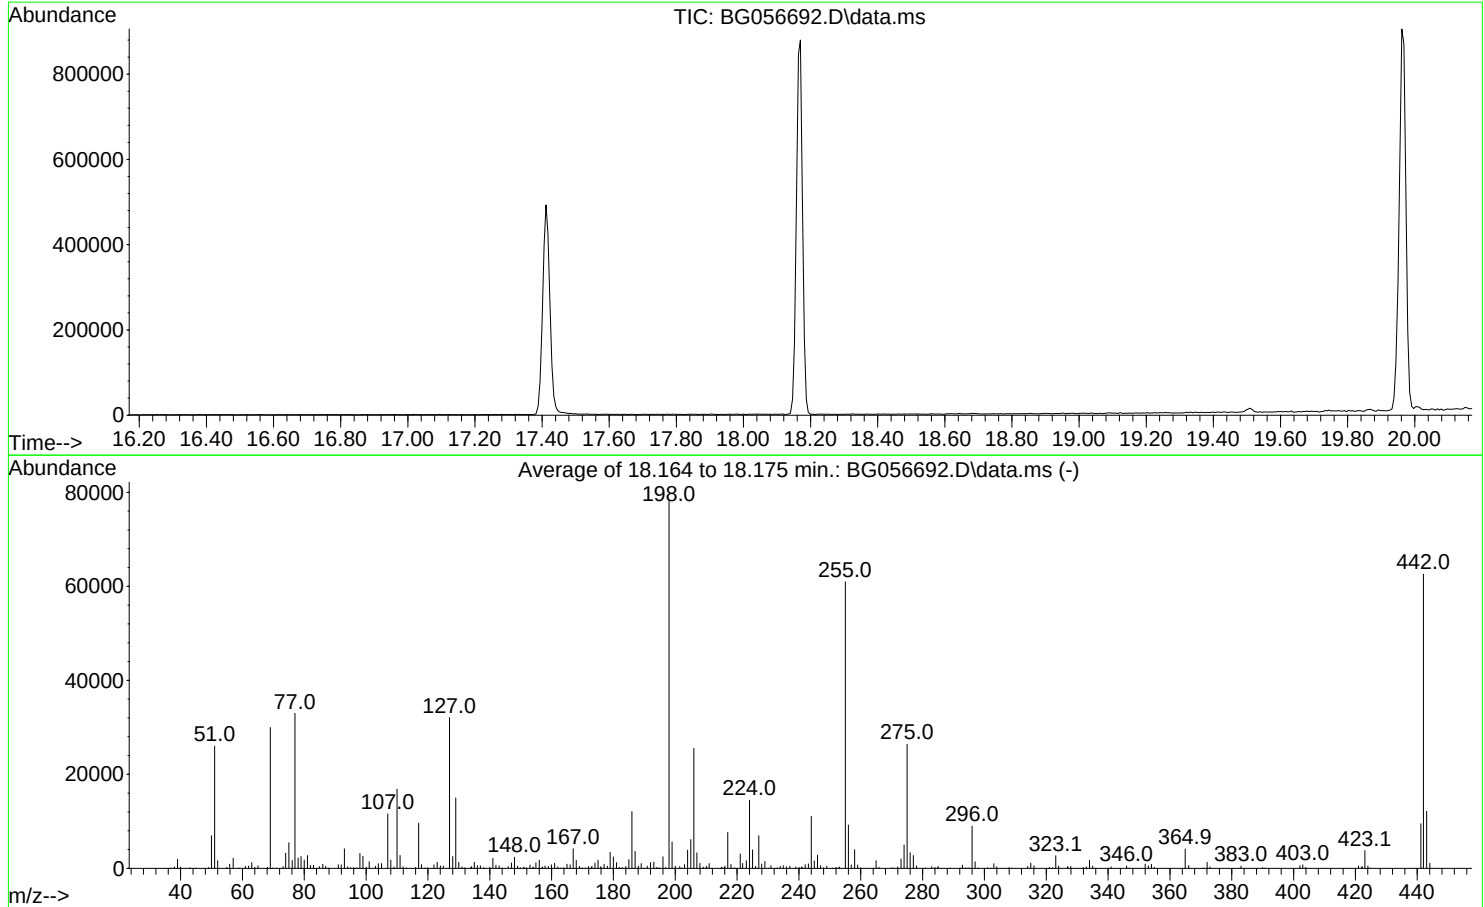




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	25980	PASS
68	69	0.00	2	0.7	217	PASS
69	198	0.00	100	38.3	29949	PASS
70	69	0.00	2	0.2	70	PASS
127	198	10	80	40.9	32040	PASS
197	198	0.00	2	0.3	201	PASS
198	198	100	100	100.0	78275	PASS
199	198	5	9	7.2	5611	PASS
275	198	10	60	33.7	26408	PASS
365	198	1	100	5.2	4109	PASS
441	198	0.01	100	12.1	9491	PASS
442	442	50	100	100.0	62600	PASS
443	442	15	24	19.4	12142	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022223\
 Data File : BG056692.D
 Acq On : 22 Feb 2023 10:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Feb 23 04:22:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 23 01:45:41 2023
 Response via : Initial Calibration

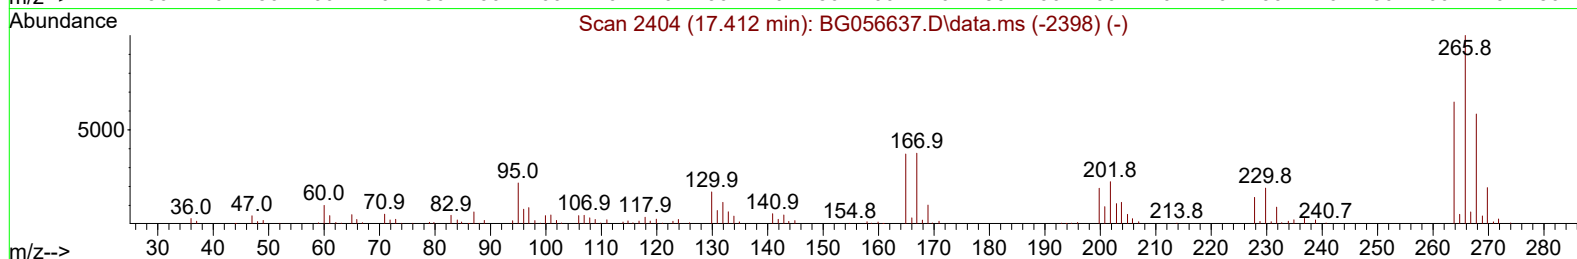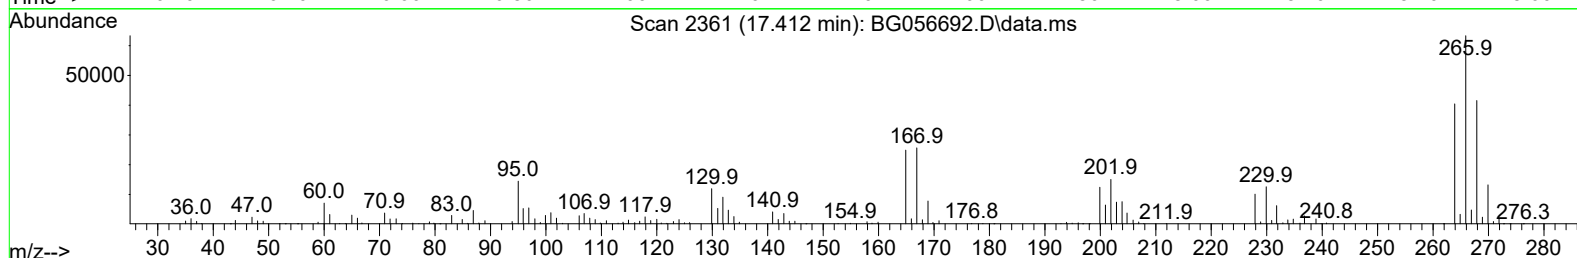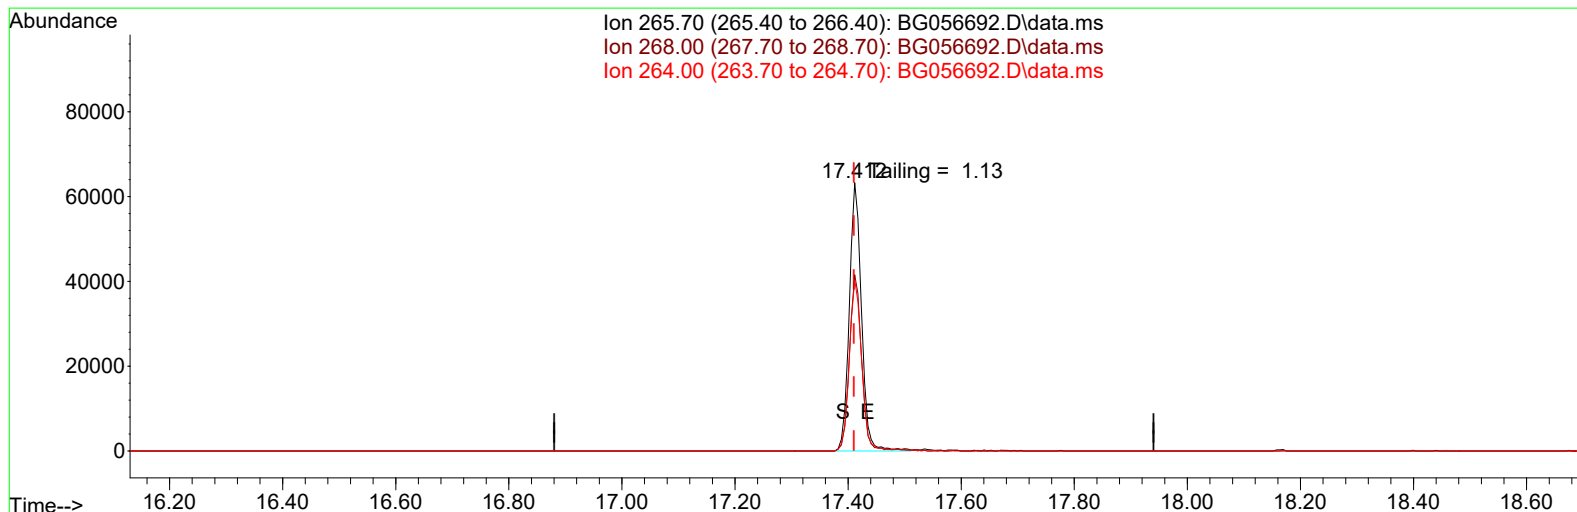

TIC: BG056692.D\data.ms

(70) Pentachlorophenol (C)

17.412min (+ 0.002) 18200.95 ng




response 94601

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	58.40	65.64
264.00	64.70	63.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022223\
Data File : BG056692.D
Acq On : 22 Feb 2023 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 23 04:22:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG021523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 23 01:45:41 2023
Response via : Initial Calibration

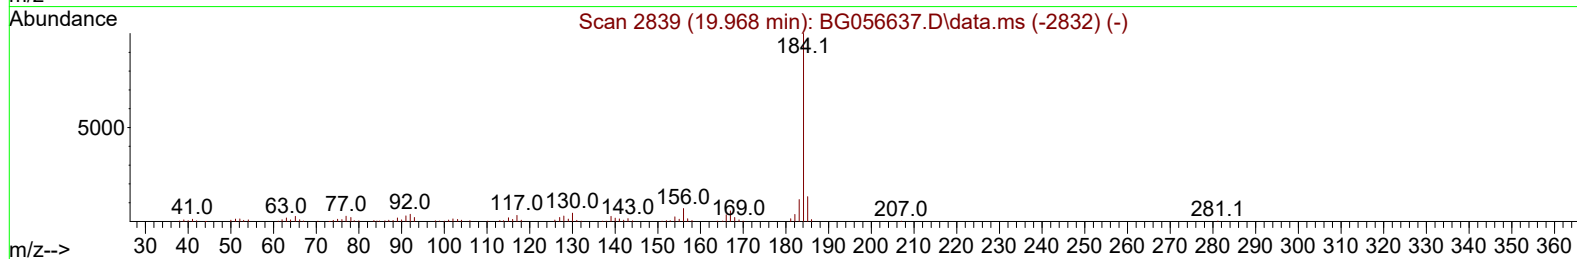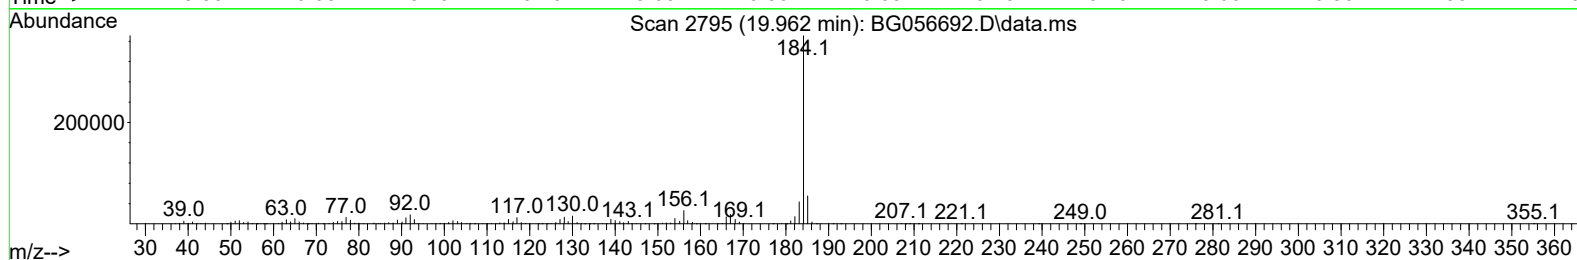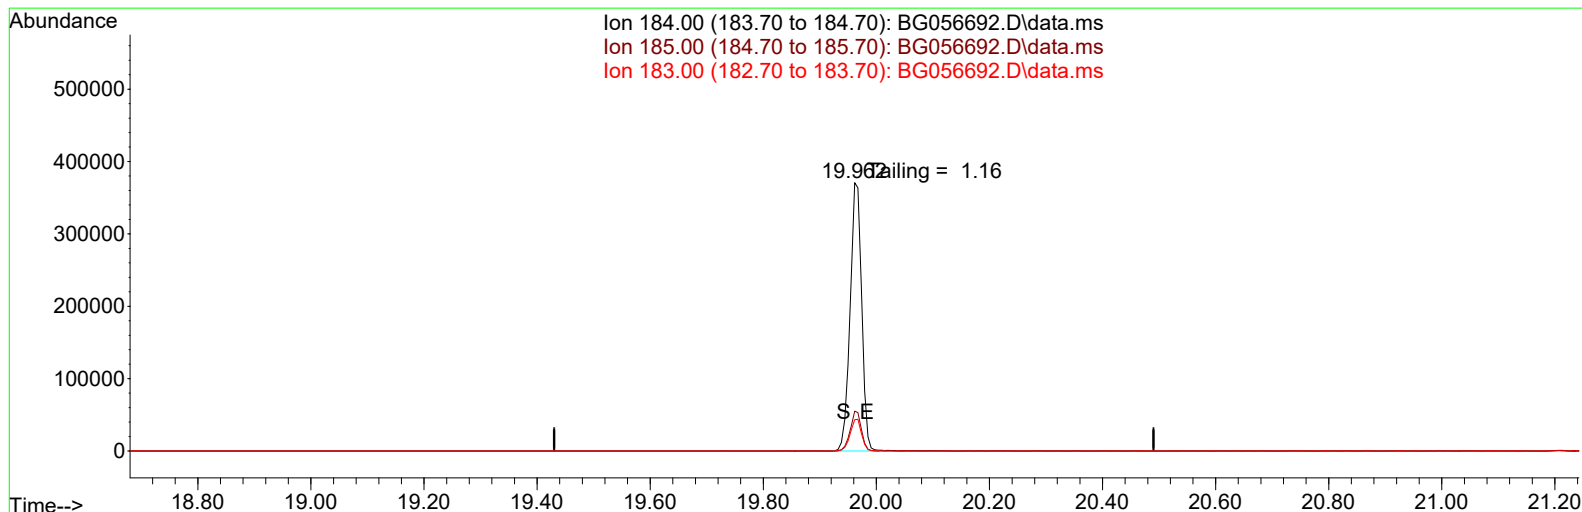

TIC: BG056692.D\data.ms

(77) Benzidine

19.960min (-19.960) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	13.20	0.00#
183.00	11.70	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/22/2023	BNA_G	<u>BG056692.D</u>
Compound Name	Response	Retention Time
DDT	211108	21.207
DDD	7574	20.743
DDE	119	20.244
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7693	218801	3.52

Instrument :
BNA_G
ClientSampleId :
DFTPP