

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022323\
 Data File : BG056708.D
 Acq On : 23 Feb 2023 11:32
 Operator : CG/JU
 Sample : SSTD00559
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD005414

Quant Time: Feb 23 13:53:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 23 13:51:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.426	152	16653	20.000	ng/u1	0.00
20) Naphthalene-d8	11.264	136	72249	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	15.030	164	59367	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.762	188	148744	20.000	ng/u1	0.00
79) Chrysene-d12	22.075	240	117324	20.000	ng/u1	0.00
88) Perylene-d12	25.612	264	128947	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.696	96	356	0.984	ng/uL	-0.01
4) Pyridine-d5	4.149	84	6001	4.567	ng/u1	0.00
7) Phenol-d5	7.545	99	7150	4.475	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.727	67	4499	4.707	ng/u1	0.00
11) 2-Chlorophenol-d4	7.950	132	5076	5.274	ng/u1	0.00
15) 4-Methylphenol-d8	9.113	113	5645	4.755	ng/u1	0.00
21) Nitrobenzene-d5	9.595	128	3003	6.665	ng/u1	0.00
24) 2-Nitrophenol-d4	10.330	143	3237	6.136	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.864	165	6368	5.269	ng/u1	0.00
31) 4-Chloroaniline-d4	11.387	131	8223	4.719	ng/u1	0.00
46) Dimethylphthalate-d6	14.413	166	22726	5.144	ng/u1	0.00
49) Acenaphthylene-d8	14.724	160	25984	5.090	ng/u1	0.00
54) 4-Nitrophenol-d4	15.183	143	3528	5.121	ng/u1	0.00
60) Fluorene-d10	16.011	176	21208	4.876	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	16.111	200	3972	5.567	ng/u1	0.00
73) Anthracene-d10	17.862	188	35627	5.219	ng/u1	0.00
81) Pyrene-d10	20.118	212	38681	5.743	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.365	264	34404	5.198	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.737	88	658	1.482	ng/uL	95
5) Pyridine	4.166	79	5831	4.331	ng/u1	95
6) Benzaldehyde	7.551	77	4724	6.406	ng/u1	97
8) Phenol	7.574	94	7485	4.610	ng/u1	93
10) Bis(2-Chloroethyl)ether	7.821	93	5645	4.833	ng/u1#	92
12) 2-Chlorophenol	7.979	128	5047	5.145	ng/u1	96
13) 2-Methylphenol	8.849	108	5776	4.679	ng/u1	90
14) 2,2'-oxybis(1-Chloropr...	8.943	45	7780	5.015	ng/u1#	91
16) Acetophenone	9.249	105	10272	4.844	ng/u1	98
17) N-Nitroso-di-n-propyla...	9.219	70	6016	5.266	ng/u1#	87
18) 4-Methylphenol	9.178	108	6447	4.903	ng/u1#	73
19) Hexachloroethane	9.519	117	2240	5.824	ng/u1#	79
22) Nitrobenzene	9.642	77	8108	6.442	ng/u1#	82
23) Isophorone	10.165	82	16371	5.066	ng/u1	95
25) 2-Nitrophenol	10.359	139	3390	6.293	ng/u1	92
26) 2,4-Dimethylphenol	10.394	107	7591	5.196	ng/u1	95
27) Bis(2-Chloroethoxy)met...	10.641	93	8318	4.975	ng/u1	98
29) 2,4-Dichlorophenol	10.894	162	6355	5.342	ng/u1	97
30) Naphthalene	11.317	128	19349	5.082	ng/u1#	93
32) 4-Chloroaniline	11.405	127	7603	4.427	ng/u1	96
33) Hexachlorobutadiene	11.587	225	5105	4.923	ng/u1	93
34) Caprolactam	12.139	113	2452	6.000	ng/u1#	67
35) 4-Chloro-3-methylphenol	12.486	107	7517	5.706	ng/u1	93
36) 2-Methylnaphthalene	12.891	142	14262	5.085	ng/u1	97

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022323\
 Data File : BG056708.D
 Acq On : 23 Feb 2023 11:32
 Operator : CG/JU
 Sample : SSTD00559
 Misc :
 ALS Vial : 3 Sample Multiplier: 1


Instrument :
 BNA_G
 ClientSampleId :
 SSTD005414


Quant Time: Feb 23 13:53:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 23 13:51:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	13.103	142	13276	4.617	ng/ul#	89
39) 1,2,4,5-Tetrachloroben...	13.244	216	9687	4.709	ng/ul	95
40) Hexachlorocyclopentadiene	13.220	237	5616	4.480	ng/ul	95
41) 2,4,6-Trichlorophenol	13.473	196	6532	5.567	ng/ul	96
42) 2,4,5-Trichlorophenol	13.473	196	5919	4.359	ng/ul	91
43) 1,1'-Biphenyl	13.867	154	20828	5.031	ng/ul	92
44) 2-Chloronaphthalene	13.920	162	17172	4.974	ng/ul	96
45) 2-Nitroaniline	14.102	65	5692	7.738	ng/ul	90
47) Dimethylphthalate	14.460	163	23759	5.302	ng/ul#	99
48) 2,6-Dinitrotoluene	14.583	165	4432	6.128	ng/ul	94
50) Acenaphthylene	14.754	152	26588	5.069	ng/ul	99
51) 3-Nitroaniline	14.918	138	4571	6.429	ng/ul#	90
52) Acenaphthene	15.095	153	18067	4.964	ng/ul	97
53) 2,4-Dinitrophenol	15.118	184	1884	3.589	ng/ul#	81
55) 4-Nitrophenol	15.200	109	3856	5.829	ng/ul	91
56) Dibenzofuran	15.424	168	28151	5.096	ng/ul	99
57) 2,4-Dinitrotoluene	15.365	165	6818	6.531	ng/ul#	95
58) 2,3,4,6-Tetrachlorophenol	15.641	232	6726	5.724	ng/ul#	92
59) Diethylphthalate	15.806	149	23557	5.460	ng/ul	96
61) Fluorene	16.070	166	21700	4.877	ng/ul	91
62) 4-Chlorophenyl-phenyle...	16.046	204	13178	4.970	ng/ul	93
63) 4-Nitroaniline	16.064	138	4677	6.715	ng/ul	95
66) 4,6-Dinitro-2-methylph...	16.123	198	3977	5.651	ng/ul#	95
67) N-Nitrosodiphenylamine	16.258	169	20164	5.272	ng/ul	96
68) 4-Bromophenyl-phenylether	16.940	248	8997	5.366	ng/ul	95
69) Hexachlorobenzene	17.069	284	10015	5.245	ng/ul	98
70) Atrazine	17.186	200	8807	5.533	ng/ul	97
71) Pentachlorophenol	17.404	266	4549	4.425	ng/ul	92
72) Phenanthrene	17.803	178	39415	5.187	ng/ul	98
74) Anthracene	17.897	178	41250	5.373	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.843	216	10652	5.267	ng/ul	92
76) Pentachlorobenzene	15.341	250	10914	5.142	ng/ul#	89
77) Carbazole	18.156	167	33875	5.203	ng/ul	98
78) Di-n-butylphthalate	18.685	149	39126	5.985	ng/ul	99
80) Fluoranthene	19.789	202	47495	5.979	ng/ul	98
82) Pyrene	20.148	202	48713	6.154	ng/ul#	98
83) Butylbenzylphthalate	21.011	149	14764	6.764	ng/ul	91
84) 3,3'-Dichlorobenzidine	21.945	252	16252	6.396	ng/ul#	83
85) Benzo(a)anthracene	22.051	228	42053	5.201	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.916	149	20472	6.206	ng/ul#	95
87) Chrysene	22.122	228	39334	5.288	ng/ul	98
89) Di-n-octyl phthalate	23.232	149	34777	5.830	ng/ul	100
90) Benzo(b)fluoranthene	24.466	252	42592	5.074	ng/ul#	95
91) Benzo(k)fluoranthene	24.548	252	41362	5.119	ng/ul	99
93) Benzo(a)pyrene	25.441	252	37972	5.309	ng/ul#	98
94) Indeno(1,2,3-cd)pyrene	29.678	276	42760	4.341	ng/ul	95
95) Dibenzo(a,h)anthracene	29.754	278	42674	5.239	ng/ul#	90
96) Benzo(g,h,i)perylene	30.947	276	21464	2.733	ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Feb 23 13:53:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 23 13:51:30 2023
Response via : Initial Calibration









#2
1,4-Dioxane
Concen: 1.482 ng/uL
RT: 3.737 min Scan# 34
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion: 88	Resp: 658
Ion Ratio	Lower Upper
88 100	
43 35.5	28.3 42.5
58 69.2	50.6 75.8



#5
Pyridine
Concen: 4.331 ng/uL
RT: 4.166 min Scan# 107
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion: 79	Resp:	5831	
Ion	Ratio	Lower	Upper
79	100		
52	70.0	60.6	91.0
51	39.3	31.9	47.9









#6
Benzaldehyde
Concen: 6.406 ng/ul
RT: 7.551 min Scan# 682
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion: 77 Resp: 4724
Ion Ratio Lower Upper
77 100
105 95.0 72.2 108.4
106 84.4 67.4 101.2



#8
Phenol
Concen: 4.610 ng/ul
RT: 7.574 min Scan# 687
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion: 94 Resp: 7485
Ion Ratio Lower Upper
94 100
65 35.9 25.7 38.5
66 53.8 38.9 58.3









#10
Bis(2-Chloroethyl)ether
Concen: 4.833 ng/ul
RT: 7.821 min Scan# 710
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion: 93 Resp: 5645
Ion Ratio Lower Upper
93 100
63 80.1 66.6 100.0
95 41.8 25.0 37.4#



#12
2-Chlorophenol
Concen: 5.145 ng/ul
RT: 7.979 min Scan# 756
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:128 Resp: 5047
Ion Ratio Lower Upper
128 100
64 55.1 45.5 68.3
130 30.2 27.7 41.5









#13
2-Methylphenol
Concen: 4.679 ng/ul
RT: 8.849 min Scan# 904
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:108 Resp: 5776
Ion Ratio Lower Upper
108 100
107 81.7 73.4 110.0



#14
2,2'-oxybis(1-Chloropropane)
Concen: 5.015 ng/ul
RT: 8.943 min Scan# 920
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion: 45 Resp: 7780
Ion Ratio Lower Upper
45 100
77 11.6 12.4 18.6#
79 15.9 9.8 14.6#









#16
Acetophenone
Concen: 4.844 ng/ul
RT: 9.249 min Scan# 91
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:105 Resp: 10272
Ion Ratio Lower Upper
105 100
77 87.3 71.4 107.0
51 29.1 23.6 35.4



#17
N-Nitroso-di-n-propylamine
Concen: 5.266 ng/ul
RT: 9.219 min Scan# 967
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion: 70 Resp: 6016
Ion Ratio Lower Upper
70 100
42 45.8 46.6 70.0#
101 5.6 7.3 10.9#
130 17.5 13.7 20.5









#18
4-Methylphenol
Concen: 4.903 ng/ul
RT: 9.178 min Scan# 90
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:108 Resp: 6447
Ion Ratio Lower Upper
108 100
107 86.1 92.1 138.1#



#19
Hexachloroethane
Concen: 5.824 ng/ul
RT: 9.519 min Scan# 1018
Delta R.T. -0.016 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:117 Resp: 2240
Ion Ratio Lower Upper
117 100
201 82.0 95.2 142.8#
199 71.2 57.9 86.9









#22
Nitrobenzene
Concen: 6.442 ng/ul
RT: 9.642 min Scan# 1038
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion: 77 Resp: 8108
Ion Ratio Lower Upper
77 100
123 48.3 27.8 41.6#
65 14.7 10.6 16.0



#23
Isophorone
Concen: 5.066 ng/ul
RT: 10.165 min Scan# 1128
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion: 82 Resp: 16371
Ion Ratio Lower Upper
82 100
95 8.3 7.7 11.5
138 17.8 12.1 18.1









#25
2-Nitrophenol
Concen: 6.293 ng/ul
RT: 10.359 min Scan# 1161
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:139 Resp: 3390
Ion Ratio Lower Upper
139 100
65 54.4 49.4 74.2
109 43.3 31.6 47.4



#26
2,4-Dimethylphenol
Concen: 5.196 ng/ul
RT: 10.394 min Scan# 1167
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:107 Resp: 7591
Ion Ratio Lower Upper
107 100
121 40.9 40.2 60.4
122 78.9 63.1 94.7





#27

Bis(2-Chloroethoxy)methane

Concen: 4.975 ng/ul

RT: 10.641 min Scan# 1209

Delta R.T. 0.002 min

Lab File: BG056708.D

Acq: 23 Feb 2023 11:32

Instrument :

BNA_G

ClientSampleId :

SSTD005414





Tgt Ion: 93 Resp: 8318

Ion Ratio Lower Upper

93 100

95 30.1 24.6 37.0

123 9.7 6.6 10.0



#29

2,4-Dichlorophenol

Concen: 5.342 ng/ul

RT: 10.894 min Scan# 1252

Delta R.T. -0.004 min

Lab File: BG056708.D

Acq: 23 Feb 2023 11:32




Tgt Ion:162 Resp: 6355


Ion Ratio Lower Upper

162 100

164 63.7 53.3 79.9

98 33.1 25.5 38.3









#30
Naphthalene
Concen: 5.082 ng/ul
RT: 11.317 min Scan# 11324
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:128 Resp: 19349
Ion Ratio Lower Upper
128 100
129 8.4 8.6 12.8#
127 15.2 9.8 14.8#



#32
4-Chloroaniline
Concen: 4.427 ng/ul
RT: 11.405 min Scan# 1339
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:127 Resp: 7603
Ion Ratio Lower Upper
127 100
129 31.4 23.4 35.0









#33
Hexachlorobutadiene
Concen: 4.923 ng/ul
RT: 11.587 min Scan# 11
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:225 Resp: 5105
Ion Ratio Lower Upper
225 100
223 59.8 53.5 80.3
227 68.0 58.2 87.2



#34
Caprolactam
Concen: 6.000 ng/ul
RT: 12.139 min Scan# 1464
Delta R.T. -0.010 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:113 Resp: 2452
Ion Ratio Lower Upper
113 100
55 142.6 167.0 250.6#
56 117.3 113.5 170.3









#35
4-Chloro-3-methylphenol
Concen: 5.706 ng/ul
RT: 12.486 min Scan# 1523
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:107 Resp: 7517
Ion Ratio Lower Upper
107 100
144 20.5 20.5 30.7
142 64.4 55.8 83.6



#36
2-Methylnaphthalene
Concen: 5.085 ng/ul
RT: 12.891 min Scan# 1592
Delta R.T. 0.008 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:142 Resp: 14262
Ion Ratio Lower Upper
142 100
141 91.7 71.0 106.6





#37

1-Methylnaphthalene

Concen: 4.617 ng/ul

RT: 13.103 min Scan# 1

Delta R.T. 0.002 min

Lab File: BG056708.D

Acq: 23 Feb 2023 11:32

Instrument :

BNA_G

ClientSampleId :

SSTD005414





Tgt Ion:142 Resp: 13276

Ion Ratio Lower Upper

142 100

141 102.4 73.5 110.3

116 3.9 4.0 6.0#



#39

1,2,4,5-Tetrachlorobenzene

Concen: 4.709 ng/ul

RT: 13.244 min Scan# 1652

Delta R.T. 0.002 min

Lab File: BG056708.D

Acq: 23 Feb 2023 11:32

Tgt Ion:216 Resp: 9687




Ion Ratio Lower Upper


216 100

214 75.8 64.4 96.6

179 18.7 16.9 25.3

108 14.2 11.6 17.4









#40
Hexachlorocyclopentadiene
Concen: 4.480 ng/ul
RT: 13.220 min Scan# 1648
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:237 Resp: 5616
Ion Ratio Lower Upper
237 100
235 55.7 47.8 71.8
272 14.1 9.9 14.9



#41
2,4,6-Trichlorophenol
Concen: 5.567 ng/ul
RT: 13.473 min Scan# 1691
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:196 Resp: 6532
Ion Ratio Lower Upper
196 100
198 90.1 75.0 112.6
200 28.9 22.1 33.1









#42
2,4,5-Trichlorophenol
Concen: 4.359 ng/ul
RT: 13.473 min Scan# 1
Delta R.T. -0.069 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:196 Resp: 5919
Ion Ratio Lower Upper
196 100
198 90.1 80.1 120.1
200 28.9 26.7 40.1



#43
1,1'-Biphenyl
Concen: 5.031 ng/ul
RT: 13.867 min Scan# 1758
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:154 Resp: 20828
Ion Ratio Lower Upper
154 100
153 46.1 32.0 48.0
76 12.5 9.0 13.4









#44
2-Chloronaphthalene
Concen: 4.974 ng/ul
RT: 13.920 min Scan# 1767
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:	162	Resp:	17172
Ion Ratio	Lower	Upper	
162	100		
164	32.8	23.3	34.9
127	33.5	25.8	38.8



#45
2-Nitroaniline
Concen: 7.738 ng/ul
RT: 14.102 min Scan# 1798
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:	65	Resp:	5692
Ion Ratio	Lower	Upper	
65	100		
92	63.3	53.9	80.9
138	78.8	73.8	110.6









#47
Dimethylphthalate
Concen: 5.302 ng/ul
RT: 14.460 min Scan# 1859
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:163 Resp: 23759
Ion Ratio Lower Upper
163 100
194 4.0 2.5 3.7#
164 10.1 8.2 12.4

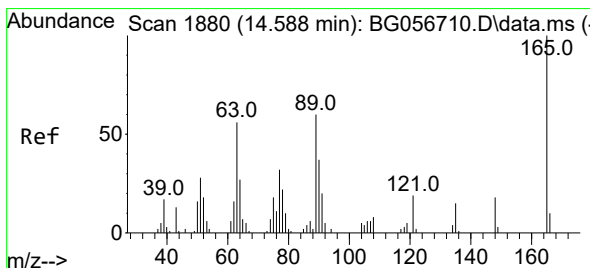

#48
2,6-Dinitrotoluene
Concen: 6.128 ng/ul
RT: 14.583 min Scan# 1880
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:165 Resp: 4432
Ion Ratio Lower Upper
165 100
89 64.6 48.4 72.6
121 16.2 15.5 23.3









#50
Acenaphthylene
Concen: 5.069 ng/ul
RT: 14.754 min Scan# 1909
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:152 Resp: 26588
Ion Ratio Lower Upper
152 100
151 19.2 15.8 23.6
153 13.3 10.6 16.0



#51
3-Nitroaniline
Concen: 6.429 ng/ul
RT: 14.918 min Scan# 1937
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:138 Resp: 4571
Ion Ratio Lower Upper
138 100
108 10.7 6.5 9.7#
92 115.6 102.2 153.2









#52
Acenaphthene
Concen: 4.964 ng/ul
RT: 15.095 min Scan# 1966
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:153 Resp: 18067
Ion Ratio Lower Upper
153 100
152 48.8 38.6 58.0
154 92.0 70.9 106.3



#53
2,4-Dinitrophenol
Concen: 3.589 ng/ul
RT: 15.118 min Scan# 1971
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:184 Resp: 1884
Ion Ratio Lower Upper
184 100
63 50.3 43.8 65.6
154 108.9 66.8 100.2#









#55
4-Nitrophenol
Concen: 5.829 ng/ul
RT: 15.200 min Scan# 1984
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:109 Resp: 3856
Ion Ratio Lower Upper
109 100
139 94.9 71.2 106.8
65 118.7 85.1 127.7



#56
Dibenzofuran
Concen: 5.096 ng/ul
RT: 15.424 min Scan# 2023
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:168 Resp: 28151
Ion Ratio Lower Upper
168 100
139 34.7 28.2 42.2









#57
2,4-Dinitrotoluene
Concen: 6.531 ng/ul
RT: 15.365 min Scan# 2060
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:165 Resp: 6818
Ion Ratio Lower Upper
165 100
63 51.5 38.6 58.0
182 4.6 1.8 2.8#



#58
2,3,4,6-Tetrachlorophenol
Concen: 5.724 ng/ul
RT: 15.641 min Scan# 2060
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:232 Resp: 6726
Ion Ratio Lower Upper
232 100
131 28.0 27.8 41.8
130 0.0 1.8 2.6#
166 24.4 20.2 30.4









#59
Diethylphthalate
Concen: 5.460 ng/ul
RT: 15.806 min Scan# 2088
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:149 Resp: 23557
Ion Ratio Lower Upper
149 100
177 25.9 18.6 28.0
150 13.2 10.7 16.1



#61
Fluorene
Concen: 4.877 ng/ul
RT: 16.070 min Scan# 2133
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:166 Resp: 21700
Ion Ratio Lower Upper
166 100
165 107.0 78.4 117.6
167 15.3 10.5 15.7









#62
4-Chlorophenyl-phenylether
Concen: 4.970 ng/ul
RT: 16.046 min Scan# 2128
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:204 Resp: 13178
Ion Ratio Lower Upper
204 100
206 36.5 26.1 39.1
141 54.4 39.7 59.5



#63
4-Nitroaniline
Concen: 6.715 ng/ul
RT: 16.064 min Scan# 2132
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:138 Resp: 4677
Ion Ratio Lower Upper
138 100
92 61.6 48.6 73.0
108 108.3 93.0 139.6









#66
 4,6-Dinitro-2-methylphenol
 Concen: 5.651 ng/ul
 RT: 16.123 min Scan# 2142
 Delta R.T. -0.004 min
 Lab File: BG056708.D
 Acq: 23 Feb 2023 11:32




Instrument :
 BNA_G
 ClientSampleId :
 SST005414


Tgt Ion:198 Resp: 3977
 Ion Ratio Lower Upper
 198 100
 182 0.0 2.4 3.6#
 77 23.9 21.0 31.6



#67
 N-Nitrosodiphenylamine
 Concen: 5.272 ng/ul
 RT: 16.258 min Scan# 2165
 Delta R.T. 0.002 min
 Lab File: BG056708.D
 Acq: 23 Feb 2023 11:32

Tgt Ion:169 Resp: 20164
 Ion Ratio Lower Upper
 169 100
 168 64.2 55.1 82.7
 167 34.7 28.3 42.5









#68
4-Bromophenyl-phenylether
Concen: 5.366 ng/ul
RT: 16.940 min Scan# 21
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:248 Resp: 8997
Ion Ratio Lower Upper
248 100
250 94.0 80.4 120.6
141 61.3 47.6 71.4



#69
Hexachlorobenzene
Concen: 5.245 ng/ul
RT: 17.069 min Scan# 2303
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:284 Resp: 10015
Ion Ratio Lower Upper
284 100
142 28.7 21.8 32.6
249 32.7 25.9 38.9









#70
 Atrazine
 Concen: 5.533 ng/ul
 RT: 17.186 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BG056708.D
 Acq: 23 Feb 2023 11:32




Instrument :
 BNA_G
 ClientSampleId :
 SST005414


Tgt Ion:200 Resp: 8807
 Ion Ratio Lower Upper
 200 100
 173 22.7 17.4 26.0
 215 54.3 41.7 62.5



#71
 Pentachlorophenol
 Concen: 4.425 ng/ul
 RT: 17.404 min Scan# 2360
 Delta R.T. 0.002 min
 Lab File: BG056708.D
 Acq: 23 Feb 2023 11:32

Tgt Ion:266 Resp: 4549
 Ion Ratio Lower Upper
 266 100
 264 67.4 49.9 74.9
 268 60.3 54.5 81.7









#72
Phenanthrene
Concen: 5.187 ng/ul
RT: 17.803 min Scan# 2428
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:178 Resp: 39415
Ion Ratio Lower Upper
178 100
179 15.8 12.1 18.1
176 16.7 14.4 21.6



#74
Anthracene
Concen: 5.373 ng/ul
RT: 17.897 min Scan# 2444
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:178 Resp: 41250
Ion Ratio Lower Upper
178 100
179 15.7 12.1 18.1
176 17.2 14.1 21.1









#75
1,2,3,4-Tetrachlorobenzene
Concen: 5.267 ng/uL
RT: 13.843 min Scan# 11
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:216 Resp: 10652
Ion Ratio Lower Upper
216 100
214 72.4 64.2 96.2
218 42.1 36.6 54.8



#76
Pentachlorobenzene
Concen: 5.142 ng/uL
RT: 15.341 min Scan# 2009
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:250 Resp: 10914
Ion Ratio Lower Upper
250 100
248 74.5 47.1 70.7#
252 64.4 52.4 78.6









#77
 Carbazole
 Concen: 5.203 ng/ul
 RT: 18.156 min Scan# 2488
 Delta R.T. 0.002 min
 Lab File: BG056708.D
 Acq: 23 Feb 2023 11:32




Instrument :
 BNA_G
 ClientSampleId :
 SSTD005414


Tgt Ion:167 Resp: 33875
 Ion Ratio Lower Upper
 167 100
 166 21.4 18.2 27.2
 139 12.1 9.8 14.8



#78
 Di-n-butylphthalate
 Concen: 5.985 ng/ul
 RT: 18.685 min Scan# 2578
 Delta R.T. 0.002 min
 Lab File: BG056708.D
 Acq: 23 Feb 2023 11:32

Tgt Ion:149 Resp: 39126
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.4 11.0
 104 6.1 5.4 8.2









#80
Fluoranthene
Concen: 5.979 ng/ul
RT: 19.789 min Scan# 2766
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:202 Resp: 47495
Ion Ratio Lower Upper
202 100
101 6.0 4.7 7.1
100 4.5 4.4 6.6



#82
Pyrene
Concen: 6.154 ng/ul
RT: 20.148 min Scan# 2827
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:202 Resp: 48713
Ion Ratio Lower Upper
202 100
101 6.7 5.3 7.9
100 4.5 4.6 7.0#





#83

Butylbenzylphthalate

Concen: 6.764 ng/ul

RT: 21.011 min Scan# 2974

Delta R.T. 0.002 min

Lab File: BG056708.D

Acq: 23 Feb 2023 11:32

Instrument :

BNA_G

ClientSampleId :

SSTD005414





Tgt Ion:149 Resp: 14764

Ion Ratio Lower Upper

149 100

91 81.6 59.3 88.9

206 20.8 19.7 29.5



#84

3,3'-Dichlorobenzidine

Concen: 6.396 ng/ul

RT: 21.945 min Scan# 3133

Delta R.T. -0.004 min

Lab File: BG056708.D

Acq: 23 Feb 2023 11:32




Tgt Ion:252 Resp: 16252


Ion Ratio Lower Upper

252 100

254 50.8 52.6 78.8#

126 4.9 5.0 7.6#









#85
Benzo(a)anthracene
Concen: 5.201 ng/ul
RT: 22.051 min Scan# 3151
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:228 Resp: 42053
Ion Ratio Lower Upper
228 100
229 20.3 16.2 24.4
226 27.8 20.6 31.0



#86
Bis(2-ethylhexyl)phthalate
Concen: 6.206 ng/ul
RT: 21.916 min Scan# 3128
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:149 Resp: 20472
Ion Ratio Lower Upper
149 100
167 24.9 21.8 32.8
279 7.4 4.2 6.2#









#87
Chrysene
Concen: 5.288 ng/ul
RT: 22.122 min Scan# 3163
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:228 Resp: 39334
Ion Ratio Lower Upper
228 100
226 29.1 23.6 35.4
229 17.9 15.4 23.0



#89
Di-n-octyl phthalate
Concen: 5.830 ng/ul
RT: 23.232 min Scan# 3352
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:149 Resp: 34777









#90
Benzo(b)fluoranthene
Concen: 5.074 ng/ul
RT: 24.466 min Scan# 3562
Delta R.T. -0.010 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:252 Resp: 42592
Ion Ratio Lower Upper
252 100
253 24.3 17.4 26.2
125 4.7 3.0 4.6#



#91
Benzo(k)fluoranthene
Concen: 5.119 ng/ul
RT: 24.548 min Scan# 3576
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:252 Resp: 41362
Ion Ratio Lower Upper
252 100
253 23.0 18.2 27.2
125 4.6 3.4 5.2









#93
Benzo(a)pyrene
Concen: 5.309 ng/ul
RT: 25.441 min Scan# 3727
Delta R.T. 0.002 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32




Instrument :
BNA_G
ClientSampleId :
SSTD005414


Tgt Ion:252 Resp: 37972
Ion Ratio Lower Upper
252 100
253 20.6 17.4 26.0
125 5.5 3.6 5.4#



#94
Indeno(1,2,3-cd)pyrene
Concen: 4.341 ng/ul
RT: 29.678 min Scan# 4449
Delta R.T. -0.004 min
Lab File: BG056708.D
Acq: 23 Feb 2023 11:32

Tgt Ion:276 Resp: 42760
Ion Ratio Lower Upper
276 100
138 7.9 5.7 8.5
277 25.2 18.1 27.1









#95
 Dibenzo(a,h)anthracene
 Concen: 5.239 ng/ul
 RT: 29.754 min Scan# 4462
 Delta R.T. -0.004 min
 Lab File: BG056708.D
 Acq: 23 Feb 2023 11:32

Instrument :
 BNA_G
 ClientSampleId :
 SSTD005414

Tgt Ion:278 Resp: 42674
 Ion Ratio Lower Upper
 278 100
 139 8.1 4.3 6.5#
 279 21.8 21.7 32.5



#96
 Benzo(g,h,i)perylene
 Concen: 2.733 ng/ul
 RT: 30.947 min Scan# 4665
 Delta R.T. -0.010 min
 Lab File: BG056708.D
 Acq: 23 Feb 2023 11:32

Tgt Ion:276 Resp: 21464
 Ion Ratio Lower Upper
 276 100
 138 11.0 6.5 9.7#
 277 29.2 20.7 31.1

