

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022323\
 Data File : BG056709.D
 Acq On : 23 Feb 2023 12:14
 Operator : CG/JU
 Sample : SST01060
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST010415

Quant Time: Feb 23 13:54:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 23 13:51:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.427	152	15236	20.000	ng/u1	0.00
20) Naphthalene-d8	11.265	136	66749	20.000	ng/u1	0.00
38) Acenaphthene-d10	15.025	164	53370	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.763	188	136874	20.000	ng/u1	0.00
79) Chrysene-d12	22.076	240	109700	20.000	ng/u1	0.00
88) Perylene-d12	25.607	264	118487	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.709	96	1096	3.311	ng/uL	0.00
4) Pyridine-d5	4.150	84	9608	7.992	ng/u1	0.00
7) Phenol-d5	7.546	99	13947	9.541	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.728	67	8643	9.883	ng/u1	0.00
11) 2-Chlorophenol-d4	7.946	132	9584	10.884	ng/u1	0.00
15) 4-Methylphenol-d8	9.115	113	11003	10.130	ng/u1	0.00
21) Nitrobenzene-d5	9.597	128	5467	13.134	ng/u1	0.00
24) 2-Nitrophenol-d4	10.331	143	6545	13.429	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.872	165	11981	10.731	ng/u1	0.00
31) 4-Chloroaniline-d4	11.383	131	15942	9.904	ng/u1	0.00
46) Dimethylphthalate-d6	14.414	166	42879	10.795	ng/u1	0.00
49) Acenaphthylene-d8	14.726	160	48082	10.477	ng/u1	0.00
54) 4-Nitrophenol-d4	15.178	143	7443	12.018	ng/u1	0.00
60) Fluorene-d10	16.013	176	39031	9.982	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	16.112	200	8287	12.621	ng/u1	0.00
73) Anthracene-d10	17.863	188	65423	10.415	ng/u1	0.00
81) Pyrene-d10	20.119	212	73564	11.682	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.360	264	62262	10.237	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.745	88	1371	3.376	ng/uL	98
5) Pyridine	4.168	79	10759	8.735	ng/u1	96
6) Benzaldehyde	7.546	77	9238	13.692	ng/u1	88
8) Phenol	7.575	94	14877	10.016	ng/u1	95
10) Bis(2-Chloroethyl)ether	7.822	93	10684	9.997	ng/u1	89
12) 2-Chlorophenol	7.981	128	9353	10.420	ng/u1	91
13) 2-Methylphenol	8.850	108	11249	9.960	ng/u1	93
14) 2,2'-oxybis(1-Chloropr...	8.944	45	14496	10.213	ng/u1	97
16) Acetophenone	9.250	105	19748	10.179	ng/u1	90
17) N-Nitroso-di-n-propyla...	9.220	70	11054	10.576	ng/u1	97
18) 4-Methylphenol	9.174	108	12358	10.273	ng/u1	93
19) Hexachloroethane	9.532	117	4090	11.623	ng/u1	93
22) Nitrobenzene	9.638	77	15947	13.714	ng/u1	96
23) Isophorone	10.161	82	31703	10.619	ng/u1	98
25) 2-Nitrophenol	10.360	139	6185	12.428	ng/u1	95
26) 2,4-Dimethylphenol	10.396	107	13972	10.352	ng/u1	95
27) Bis(2-Chloroethoxy)met...	10.637	93	15804	10.232	ng/u1	95
29) 2,4-Dichlorophenol	10.901	162	11604	10.557	ng/u1	88
30) Naphthalene	11.318	128	36311	10.323	ng/u1	99
32) 4-Chloroaniline	11.406	127	16177	10.197	ng/u1	99
33) Hexachlorobutadiene	11.588	225	9454	9.868	ng/u1	91
34) Caprolactam	12.147	113	3883	10.285	ng/u1	91
35) 4-Chloro-3-methylphenol	12.487	107	13413	11.020	ng/u1	95
36) 2-Methylnaphthalene	12.887	142	25217	9.732	ng/u1	95


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022323\
 Data File : BG056709.D
 Acq On : 23 Feb 2023 12:14
 Operator : CG/JU
 Sample : SSTD01060
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD010415

Quant Time: Feb 23 13:54:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 23 13:51:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	13.104	142	25795	9.710	ng/ul	96
39) 1,2,4,5-Tetrachloroben...	13.239	216	18214	9.850	ng/ul	89
40) Hexachlorocyclopentadiene	13.222	237	11495	10.201	ng/ul	94
41) 2,4,6-Trichlorophenol	13.468	196	12277	11.640	ng/ul	91
42) 2,4,5-Trichlorophenol	13.545	196	13291	10.889	ng/ul	93
43) 1,1'-Biphenyl	13.868	154	38451	10.331	ng/ul	98
44) 2-Chloronaphthalene	13.921	162	31131	10.030	ng/ul	96
45) 2-Nitroaniline	14.103	65	10596	16.023	ng/ul	90
47) Dimethylphthalate	14.461	163	43841	10.884	ng/ul#	99
48) 2,6-Dinitrotoluene	14.585	165	8606	13.236	ng/ul#	87
50) Acenaphthylene	14.755	152	48143	10.209	ng/ul	98
51) 3-Nitroaniline	14.914	138	8352	13.066	ng/ul#	96
52) Acenaphthene	15.090	153	33249	10.162	ng/ul	98
53) 2,4-Dinitrophenol	15.119	184	4615	9.780	ng/ul	86
55) 4-Nitrophenol	15.190	109	8112	13.640	ng/ul	89
56) Dibenzofuran	15.419	168	50652	10.199	ng/ul	92
57) 2,4-Dinitrotoluene	15.366	165	12140	12.935	ng/ul	90
58) 2,3,4,6-Tetrachlorophenol	15.637	232	11809	11.179	ng/ul	93
59) Diethylphthalate	15.807	149	45012	11.605	ng/ul	99
61) Fluorene	16.065	166	41780	10.444	ng/ul	93
62) 4-Chlorophenyl-phenyle...	16.048	204	24241	10.170	ng/ul	97
63) 4-Nitroaniline	16.065	138	8336	13.312	ng/ul	97
66) 4,6-Dinitro-2-methylph...	16.124	198	7879	12.167	ng/ul#	99
67) N-Nitrosodiphenylamine	16.259	169	38012	10.801	ng/ul	97
68) 4-Bromophenyl-phenylether	16.941	248	16724	10.839	ng/ul	96
69) Hexachlorobenzene	17.070	284	17690	10.068	ng/ul	94
70) Atrazine	17.188	200	16453	11.232	ng/ul	95
71) Pentachlorophenol	17.405	266	9040	9.556	ng/ul	95
72) Phenanthrene	17.805	178	72582	10.380	ng/ul	97
74) Anthracene	17.893	178	73984	10.473	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.845	216	19744	10.608	ng/ul	98
76) Pentachlorobenzene	15.343	250	20088	10.285	ng/ul	94
77) Carbazole	18.157	167	63933	10.672	ng/ul	96
78) Di-n-butylphthalate	18.680	149	71375	11.866	ng/ul	99
80) Fluoranthene	19.790	202	87560	11.788	ng/ul	98
82) Pyrene	20.149	202	86452	11.681	ng/ul	99
83) Butylbenzylphthalate	21.007	149	26160	12.818	ng/ul	89
84) 3,3'-Dichlorobenzidine	21.947	252	30290	12.748	ng/ul	98
85) Benzo(a)anthracene	22.053	228	77904	10.304	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.917	149	39697	12.871	ng/ul	100
87) Chrysene	22.123	228	72388	10.409	ng/ul	99
89) Di-n-octyl phthalate	23.233	149	63053	11.503	ng/ul	100
90) Benzo(b)fluoranthene	24.473	252	76646	9.937	ng/ul	98
91) Benzo(k)fluoranthene	24.544	252	76599	10.317	ng/ul	98
93) Benzo(a)pyrene	25.437	252	70397	10.712	ng/ul	96
94) Indeno(1,2,3-cd)pyrene	29.673	276	42320	4.675	ng/ul	99
95) Dibenzo(a,h)anthracene	29.749	278	77968	10.417	ng/ul	95
96) Benzo(g,h,i)perylene	30.954	276	73318	10.161	ng/ul#	90





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 3.376 ng/uL
RT: 3.745 min Scan# 31
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion: 88 Resp: 1371
Ion Ratio Lower Upper
88 100
43 35.6 28.3 42.5
58 65.7 50.6 75.8



#5
Pyridine
Concen: 8.735 ng/uL
RT: 4.168 min Scan# 107
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion: 79 Resp: 10759
Ion Ratio Lower Upper
79 100
52 71.3 60.6 91.0
51 41.4 31.9 47.9




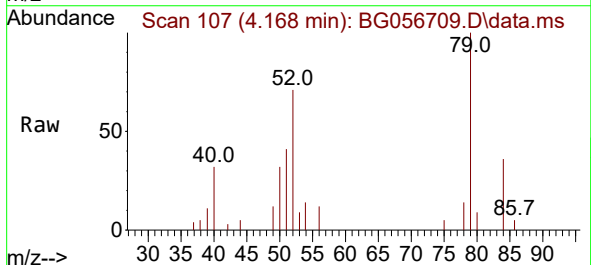




#6
Benzaldehyde
Concen: 13.692 ng/ul
RT: 7.546 min Scan# 682
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion: 77 Resp: 9238
Ion Ratio Lower Upper
77 100
105 103.8 72.2 108.4
106 92.5 67.4 101.2



#8
Phenol
Concen: 10.016 ng/ul
RT: 7.575 min Scan# 687
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion: 94 Resp: 14877
Ion Ratio Lower Upper
94 100
65 29.3 25.7 38.5
66 52.1 38.9 58.3









#10
 Bis(2-Chloroethyl)ether
 Concen: 9.997 ng/ul
 RT: 7.822 min Scan# 710
 Delta R.T. -0.003 min
 Lab File: BG056709.D
 Acq: 23 Feb 2023 12:14

Instrument :
 BNA_G
 ClientSampleId :
 SSTD010415

Tgt Ion: 93 Resp: 10684




Ion	Ratio	Lower	Upper
93	100		
63	95.9	66.6	100.0
95	32.7	25.0	37.4




#12
 2-Chlorophenol
 Concen: 10.420 ng/ul
 RT: 7.981 min Scan# 756
 Delta R.T. 0.003 min
 Lab File: BG056709.D
 Acq: 23 Feb 2023 12:14

Tgt Ion: 128 Resp: 9353

Ion	Ratio	Lower	Upper
128	100		
64	64.5	45.5	68.3
130	38.7	27.7	41.5









#13
2-Methylphenol
Concen: 9.960 ng/ul
RT: 8.850 min Scan# 904
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:108 Resp: 11249
Ion Ratio Lower Upper
108 100
107 84.7 73.4 110.0

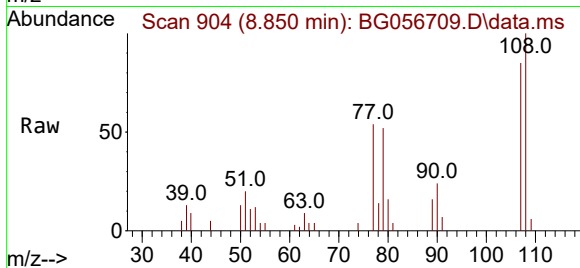

#14
2,2'-oxybis(1-Chloropropane)
Concen: 10.213 ng/ul
RT: 8.944 min Scan# 920
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion: 45 Resp: 14496
Ion Ratio Lower Upper
45 100
77 15.0 12.4 18.6
79 9.8 9.8 14.6




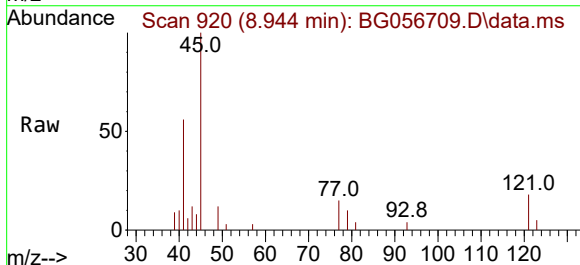




#16
Acetophenone
Concen: 10.179 ng/ul
RT: 9.250 min Scan# 91
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:105 Resp: 19748
Ion Ratio Lower Upper
105 100
77 77.9 71.4 107.0
51 27.7 23.6 35.4



#17
N-Nitroso-di-n-propylamine
Concen: 10.576 ng/ul
RT: 9.220 min Scan# 967
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion: 70 Resp: 11054
Ion Ratio Lower Upper
70 100
42 56.1 46.6 70.0
101 7.3 7.3 10.9
130 18.1 13.7 20.5





#18

4-Methylphenol

Concen: 10.273 ng/ul

RT: 9.174 min Scan# 91

Delta R.T. -0.003 min

Lab File: BG056709.D

Acq: 23 Feb 2023 12:14

Instrument :

BNA_G

ClientSampleId :





SSTD010415

Tgt Ion:108 Resp: 12358

Ion Ratio Lower Upper

108 100

107 107.0 92.1 138.1



#19

Hexachloroethane

Concen: 11.623 ng/ul

RT: 9.532 min Scan# 1020

Delta R.T. -0.003 min

Lab File: BG056709.D

Acq: 23 Feb 2023 12:14




Tgt Ion:117 Resp: 4090


Ion Ratio Lower Upper

117 100

201 125.0 95.2 142.8

199 79.5 57.9 86.9









#22
Nitrobenzene
Concen: 13.714 ng/ul
RT: 9.638 min Scan# 1038
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:	77	Resp:	15947
Ion	Ratio	Lower	Upper
77	100		
123	32.3	27.8	41.6
65	14.3	10.6	16.0

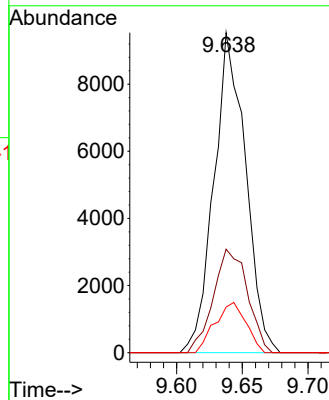

#23
Isophorone
Concen: 10.619 ng/ul
RT: 10.161 min Scan# 1127
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:	82	Resp:	31703
Ion	Ratio	Lower	Upper
82	100		
95	8.9	7.7	11.5
138	15.6	12.1	18.1


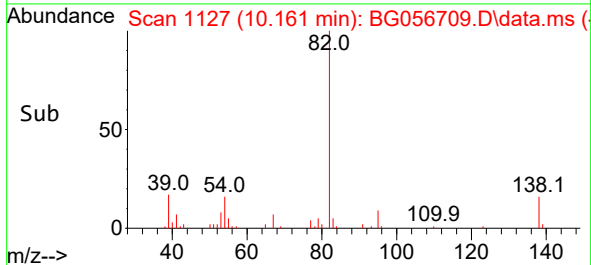
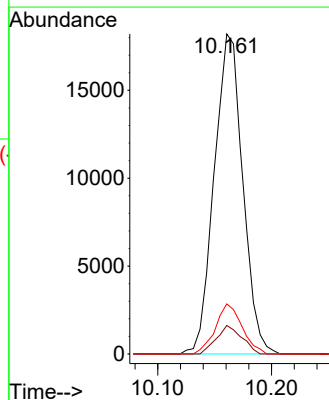





#25
2-Nitrophenol
Concen: 12.428 ng/ul
RT: 10.360 min Scan# 1161
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:139 Resp: 6185
Ion Ratio Lower Upper
139 100
65 58.1 49.4 74.2
109 36.5 31.6 47.4



#26
2,4-Dimethylphenol
Concen: 10.352 ng/ul
RT: 10.396 min Scan# 1167
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:107 Resp: 13972
Ion Ratio Lower Upper
107 100
121 50.7 40.2 60.4
122 71.8 63.1 94.7

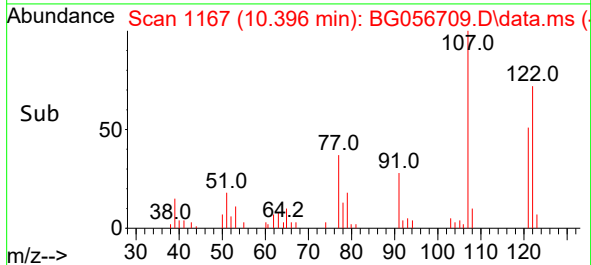



#27

Bis(2-Chloroethoxy)methane

Concen: 10.232 ng/ul

RT: 10.637 min Scan# 1208

Delta R.T. -0.003 min

Lab File: BG056709.D

Acq: 23 Feb 2023 12:14

Instrument :

BNA_G

ClientSampleId :

SSTD010415





Tgt Ion: 93 Resp: 15804

Ion Ratio Lower Upper

93 100

95 28.0 24.6 37.0

123 9.9 6.6 10.0



#29

2,4-Dichlorophenol

Concen: 10.557 ng/ul

RT: 10.901 min Scan# 1253

Delta R.T. 0.003 min

Lab File: BG056709.D

Acq: 23 Feb 2023 12:14




Tgt Ion:162 Resp: 11604


Ion Ratio Lower Upper

162 100

164 54.4 53.3 79.9

98 29.5 25.5 38.3









#30
Naphthalene
Concen: 10.323 ng/ul
RT: 11.318 min Scan# 11
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:128 Resp: 36311
Ion Ratio Lower Upper
128 100
129 10.1 8.6 12.8
127 12.3 9.8 14.8

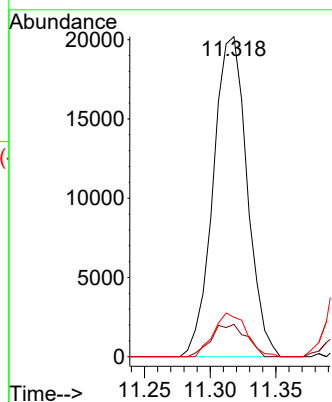

#32
4-Chloroaniline
Concen: 10.197 ng/ul
RT: 11.406 min Scan# 1339
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:127 Resp: 16177
Ion Ratio Lower Upper
127 100
129 28.8 23.4 35.0



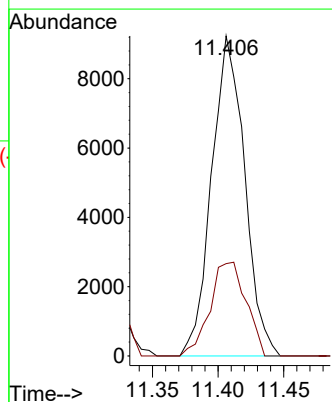





#33
Hexachlorobutadiene
Concen: 9.868 ng/ul
RT: 11.588 min Scan# 11
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:225 Resp: 9454
Ion Ratio Lower Upper
225 100
223 63.1 53.5 80.3
227 62.4 58.2 87.2



#34
Caprolactam
Concen: 10.285 ng/ul
RT: 12.147 min Scan# 1465
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:113 Resp: 3883
Ion Ratio Lower Upper
113 100
55 222.8 167.0 250.6
56 153.8 113.5 170.3




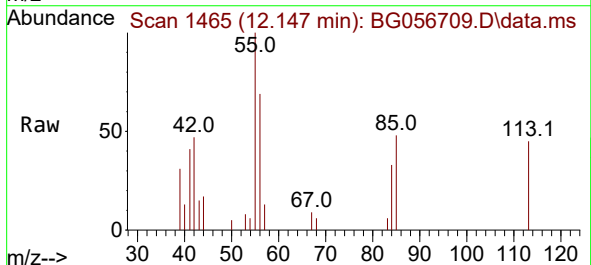




#35
4-Chloro-3-methylphenol
Concen: 11.020 ng/ul
RT: 12.487 min Scan# 1523
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:107 Resp: 13413
Ion Ratio Lower Upper
107 100
144 23.4 20.5 30.7
142 74.1 55.8 83.6



#36
2-Methylnaphthalene
Concen: 9.732 ng/ul
RT: 12.887 min Scan# 1591
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:142 Resp: 25217
Ion Ratio Lower Upper
142 100
141 93.4 71.0 106.6









#37
1-Methylnaphthalene
Concen: 9.710 ng/ul
RT: 13.104 min Scan# 1627
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:142 Resp: 25795
Ion Ratio Lower Upper
142 100
141 95.8 73.5 110.3
116 4.6 4.0 6.0



#39
1,2,4,5-Tetrachlorobenzene
Concen: 9.850 ng/ul
RT: 13.239 min Scan# 1651
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14


Tgt Ion:216 Resp: 18214
Ion Ratio Lower Upper
216 100
214 67.6 64.4 96.6
179 19.4 16.9 25.3
108 14.5 11.6 17.4

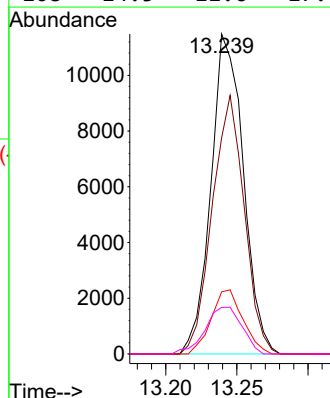






#40
Hexachlorocyclopentadiene
Concen: 10.201 ng/ul
RT: 13.222 min Scan# 1648
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14


Instrument :
BNA_G
ClientSampleId :
SSTD010415





Tgt Ion:237 Resp: 11495
Ion Ratio Lower Upper
237 100
235 54.4 47.8 71.8
272 11.2 9.9 14.9

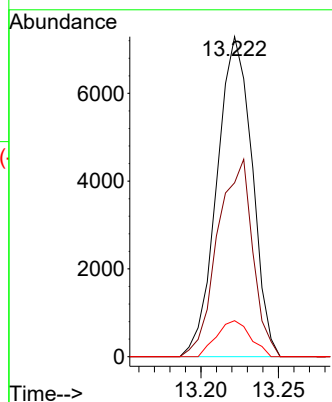


#41
2,4,6-Trichlorophenol
Concen: 11.640 ng/ul
RT: 13.468 min Scan# 1690
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14



Tgt Ion:196 Resp: 12277
Ion Ratio Lower Upper
196 100
198 103.0 75.0 112.6
200 31.2 22.1 33.1



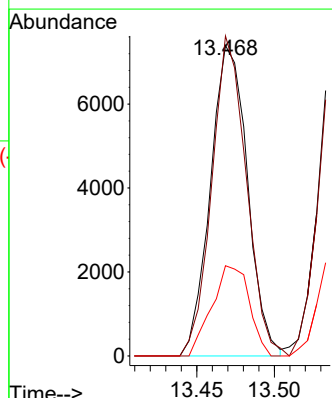





#42
2,4,5-Trichlorophenol
Concen: 10.889 ng/ul
RT: 13.545 min Scan# 1702
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:196 Resp: 13291
Ion Ratio Lower Upper
196 100
198 93.7 80.1 120.1
200 28.5 26.7 40.1

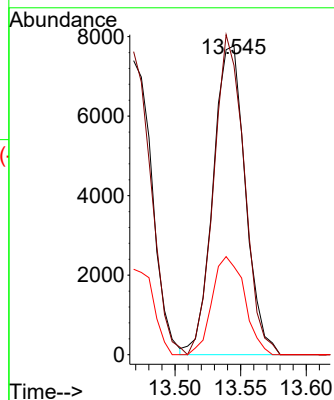

#43
1,1'-Biphenyl
Concen: 10.331 ng/ul
RT: 13.868 min Scan# 1758
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:154 Resp: 38451
Ion Ratio Lower Upper
154 100
153 40.9 32.0 48.0
76 12.4 9.0 13.4



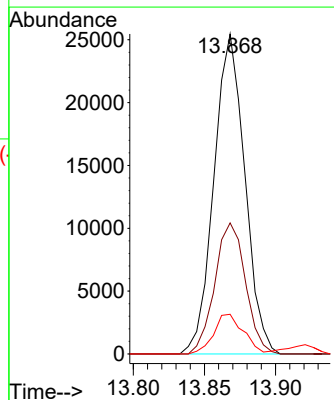





#44
2-Chloronaphthalene
Concen: 10.030 ng/ul
RT: 13.921 min Scan# 1767
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:162 Resp: 31131
Ion Ratio Lower Upper
162 100
164 31.2 23.3 34.9
127 34.9 25.8 38.8



#45
2-Nitroaniline
Concen: 16.023 ng/ul
RT: 14.103 min Scan# 1798
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion: 65 Resp: 10596
Ion Ratio Lower Upper
65 100
92 80.1 53.9 80.9
138 87.0 73.8 110.6




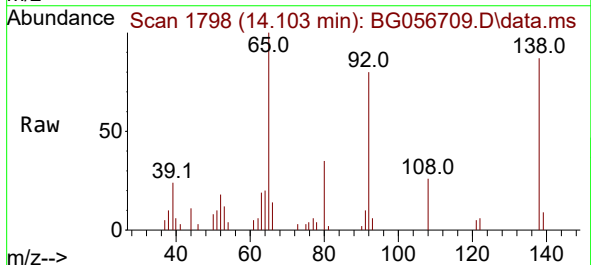




#47
Dimethylphthalate
Concen: 10.884 ng/ul
RT: 14.461 min Scan# 1859
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:163 Resp: 43841
Ion Ratio Lower Upper
163 100
194 4.3 2.5 3.7#
164 10.2 8.2 12.4

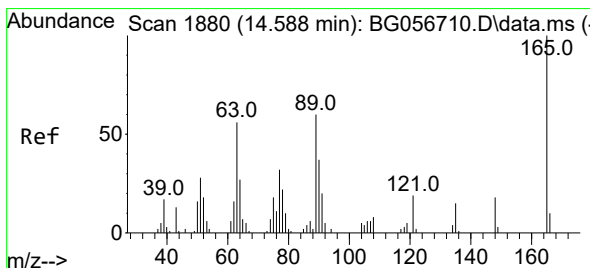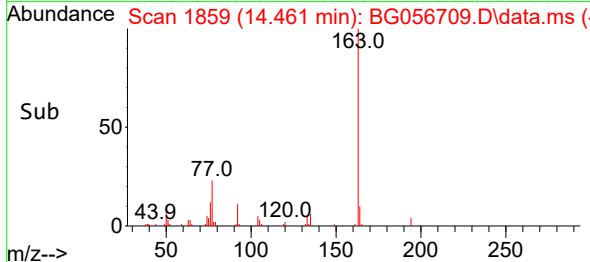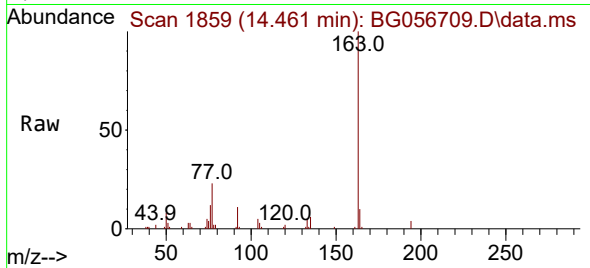

#48
2,6-Dinitrotoluene
Concen: 13.236 ng/ul
RT: 14.585 min Scan# 1880
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:165 Resp: 8606
Ion Ratio Lower Upper
165 100
89 72.8 48.4 72.6#
121 18.6 15.5 23.3


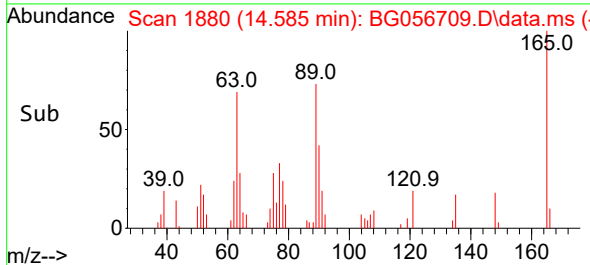

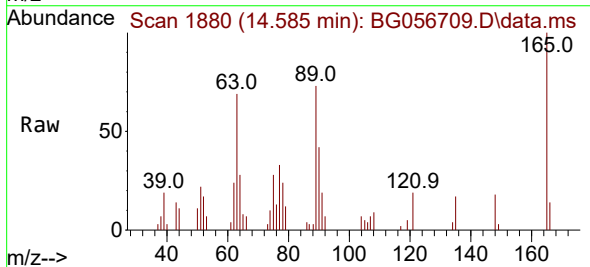




#50
Acenaphthylene
Concen: 10.209 ng/ul
RT: 14.755 min Scan# 1909
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:152 Resp: 48143
Ion Ratio Lower Upper
152 100
151 20.3 15.8 23.6
153 11.8 10.6 16.0



#51
3-Nitroaniline
Concen: 13.066 ng/ul
RT: 14.914 min Scan# 1936
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:138 Resp: 8352
Ion Ratio Lower Upper
138 100
108 12.8 6.5 9.7#
92 132.0 102.2 153.2


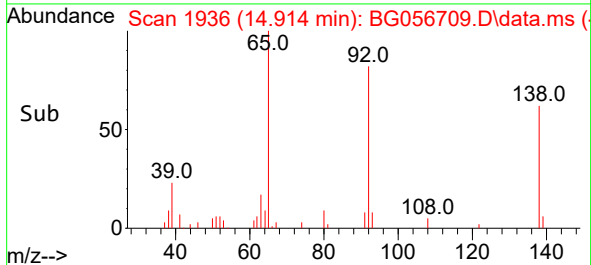






#52
Acenaphthene
Concen: 10.162 ng/ul
RT: 15.090 min Scan# 1966
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:153 Resp: 33249
Ion Ratio Lower Upper
153 100
152 49.7 38.6 58.0
154 86.3 70.9 106.3



#53
2,4-Dinitrophenol
Concen: 9.780 ng/ul
RT: 15.119 min Scan# 1971
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:184 Resp: 4615
Ion Ratio Lower Upper
184 100
63 47.8 43.8 65.6
154 68.5 66.8 100.2


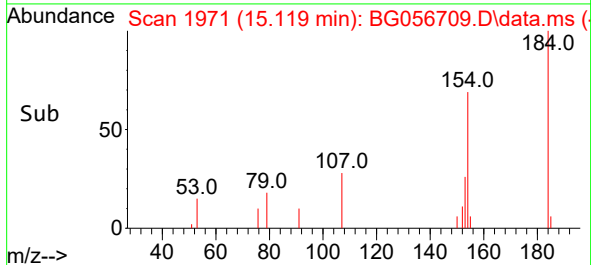






#55
4-Nitrophenol
Concen: 13.640 ng/ul
RT: 15.190 min Scan# 1984
Delta R.T. -0.009 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:109 Resp: 8112
Ion Ratio Lower Upper
109 100
139 72.5 71.2 106.8
65 111.5 85.1 127.7



#56
Dibenzofuran
Concen: 10.199 ng/ul
RT: 15.419 min Scan# 2022
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:168 Resp: 50652
Ion Ratio Lower Upper
168 100
139 39.7 28.2 42.2





#57

2,4-Dinitrotoluene

Concen: 12.935 ng/ul

RT: 15.366 min Scan# 2013

Delta R.T. -0.003 min

Lab File: BG056709.D

Acq: 23 Feb 2023 12:14

Instrument :

BNA_G

ClientSampleId :

SSTD010415





Tgt Ion:165 Resp: 12140

Ion Ratio Lower Upper

165 100

63 55.6 38.6 58.0

182 2.1 1.8 2.8



#58

2,3,4,6-Tetrachlorophenol

Concen: 11.179 ng/ul

RT: 15.637 min Scan# 2059

Delta R.T. -0.003 min

Lab File: BG056709.D

Acq: 23 Feb 2023 12:14

Tgt Ion:232 Resp: 11809




Ion Ratio Lower Upper


232 100

131 38.9 27.8 41.8

130 2.5 1.8 2.6

166 28.5 20.2 30.4

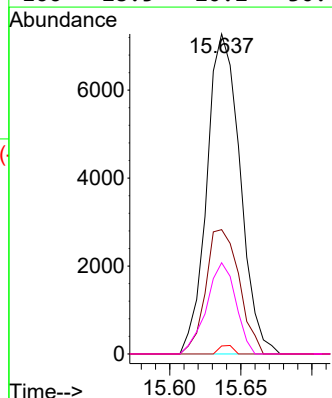



#59
Diethylphthalate
Concen: 11.605 ng/ul
RT: 15.807 min Scan# 2088
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14





Instrument :

BNA_G

ClientSampleId :




SSTD010415


Tgt Ion:149 Resp: 45012
Ion Ratio Lower Upper
149 100
177 23.4 18.6 28.0
150 12.3 10.7 16.1

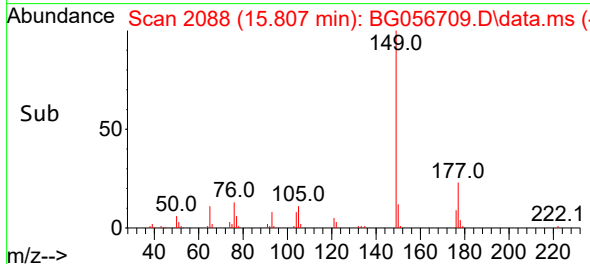

#61
Fluorene
Concen: 10.444 ng/ul
RT: 16.065 min Scan# 2132
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:166 Resp: 41780
Ion Ratio Lower Upper
166 100
165 90.2 78.4 117.6
167 13.6 10.5 15.7


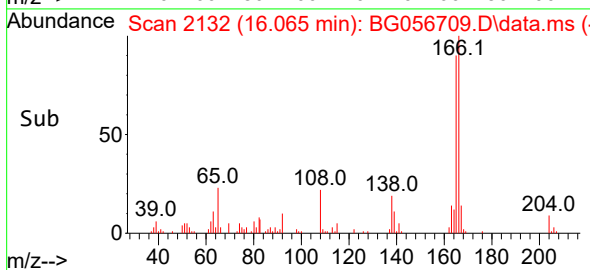

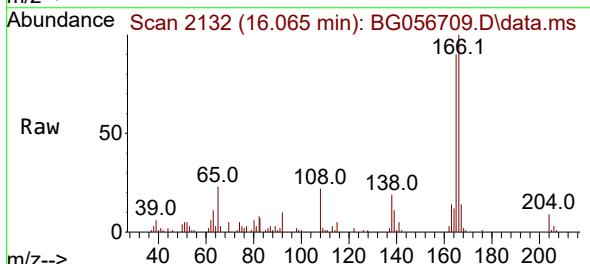




#62
4-Chlorophenyl-phenylether
Concen: 10.170 ng/ul
RT: 16.048 min Scan# 2128
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:204 Resp: 24241
Ion Ratio Lower Upper
204 100
206 34.2 26.1 39.1
141 51.2 39.7 59.5



#63
4-Nitroaniline
Concen: 13.312 ng/ul
RT: 16.065 min Scan# 2132
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:138 Resp: 8336
Ion Ratio Lower Upper
138 100
92 55.3 48.6 73.0
108 116.1 93.0 139.6




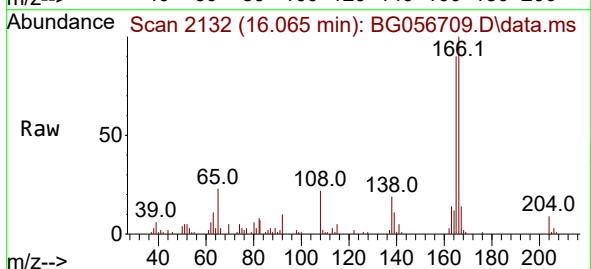




#66
4,6-Dinitro-2-methylphenol
Concen: 12.167 ng/ul
RT: 16.124 min Scan# 2142
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:198 Resp: 7879
Ion Ratio Lower Upper
198 100
182 4.5 2.4 3.6#
77 26.9 21.0 31.6



#67
N-Nitrosodiphenylamine
Concen: 10.801 ng/ul
RT: 16.259 min Scan# 2165
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:169 Resp: 38012
Ion Ratio Lower Upper
169 100
168 67.6 55.1 82.7
167 32.8 28.3 42.5




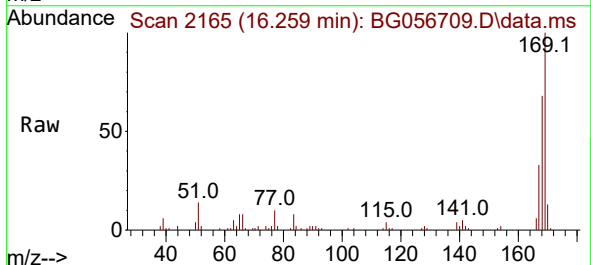




#68
4-Bromophenyl-phenylether
Concen: 10.839 ng/ul
RT: 16.941 min Scan# 21
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:248 Resp: 16724
Ion Ratio Lower Upper
248 100
250 96.9 80.4 120.6
141 63.6 47.6 71.4

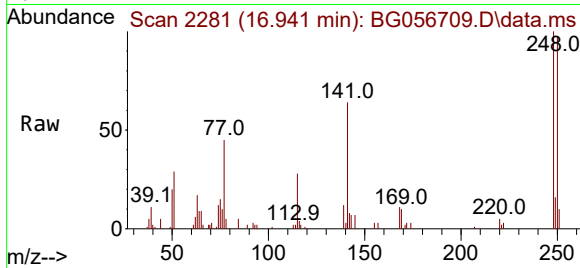

#69
Hexachlorobenzene
Concen: 10.068 ng/ul
RT: 17.070 min Scan# 2303
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:284 Resp: 17690
Ion Ratio Lower Upper
284 100
142 21.8 21.8 32.6
249 33.5 25.9 38.9




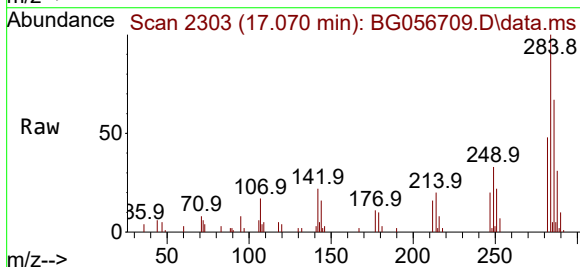




#70
Atrazine
Concen: 11.232 ng/ul
RT: 17.188 min Scan# 21
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:200 Resp: 16453
Ion Ratio Lower Upper
200 100
173 23.2 17.4 26.0
215 48.3 41.7 62.5



#71
Pentachlorophenol
Concen: 9.556 ng/ul
RT: 17.405 min Scan# 2360
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:266 Resp: 9040
Ion Ratio Lower Upper
266 100
264 67.4 49.9 74.9
268 70.8 54.5 81.7









#72
Phenanthrene
Concen: 10.380 ng/ul
RT: 17.805 min Scan# 2428
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:178 Resp: 72582
Ion Ratio Lower Upper
178 100
179 16.7 12.1 18.1
176 19.3 14.4 21.6

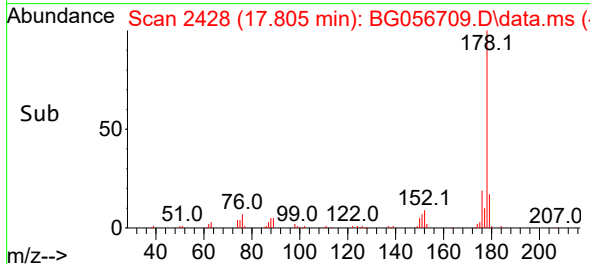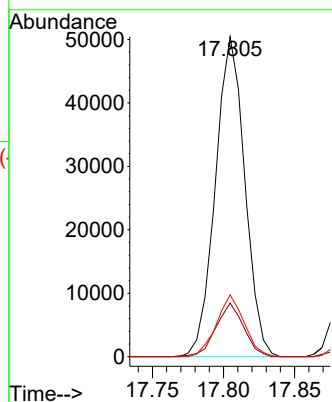

#74
Anthracene
Concen: 10.473 ng/ul
RT: 17.893 min Scan# 2443
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:178 Resp: 73984
Ion Ratio Lower Upper
178 100
179 15.8 12.1 18.1
176 18.2 14.1 21.1


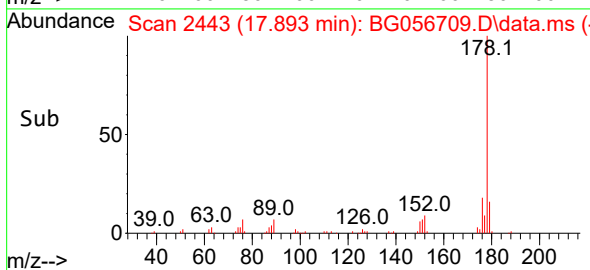

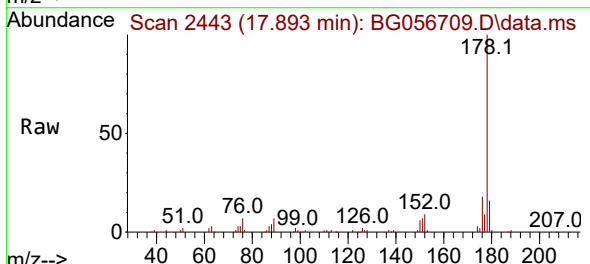




#75
1,2,3,4-Tetrachlorobenzene
Concen: 10.608 ng/uL
RT: 13.845 min Scan# 11
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:216 Resp: 19744
Ion Ratio Lower Upper
216 100
214 78.2 64.2 96.2
218 45.5 36.6 54.8



#76
Pentachlorobenzene
Concen: 10.285 ng/uL
RT: 15.343 min Scan# 2009
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:250 Resp: 20088
Ion Ratio Lower Upper
250 100
248 66.2 47.1 70.7
252 66.9 52.4 78.6



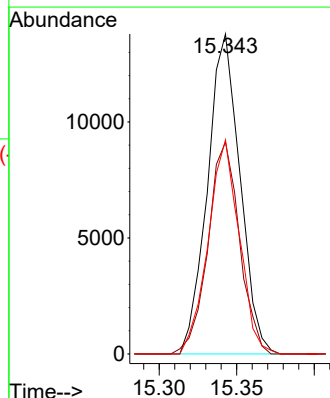





#77
 Carbazole
 Concen: 10.672 ng/ul
 RT: 18.157 min Scan# 2488
 Delta R.T. 0.003 min
 Lab File: BG056709.D
 Acq: 23 Feb 2023 12:14




Instrument :
 BNA_G
 ClientSampleId :
 SSTD010415


Tgt Ion:167 Resp: 63933
 Ion Ratio Lower Upper
 167 100
 166 20.7 18.2 27.2
 139 13.4 9.8 14.8

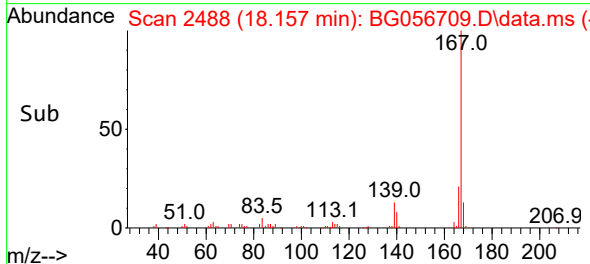

#78
 Di-n-butylphthalate
 Concen: 11.866 ng/ul
 RT: 18.680 min Scan# 2577
 Delta R.T. -0.003 min
 Lab File: BG056709.D
 Acq: 23 Feb 2023 12:14

Tgt Ion:149 Resp: 71375
 Ion Ratio Lower Upper
 149 100
 150 8.9 7.4 11.0
 104 6.6 5.4 8.2


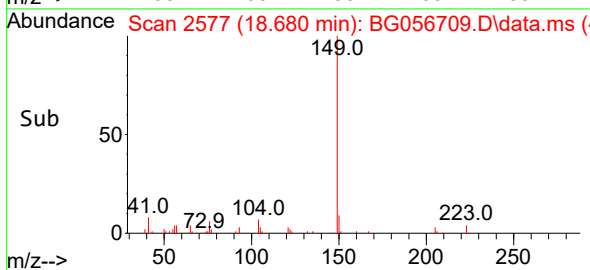

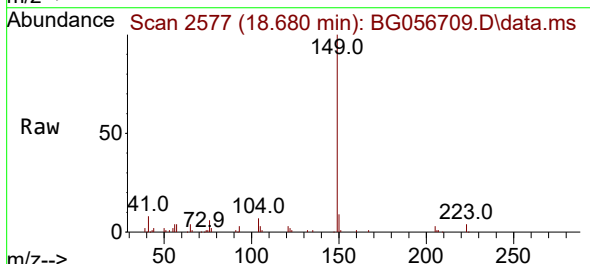




#80
 Fluoranthene
 Concen: 11.788 ng/ul
 RT: 19.790 min Scan# 21
 Delta R.T. 0.003 min
 Lab File: BG056709.D
 Acq: 23 Feb 2023 12:14




Instrument :
 BNA_G
 ClientSampleId :
 SSTD010415


Tgt Ion:202 Resp: 87560
 Ion Ratio Lower Upper
 202 100
 101 5.3 4.7 7.1
 100 4.7 4.4 6.6



#82
 Pyrene
 Concen: 11.681 ng/ul
 RT: 20.149 min Scan# 2827
 Delta R.T. -0.003 min
 Lab File: BG056709.D
 Acq: 23 Feb 2023 12:14

Tgt Ion:202 Resp: 86452
 Ion Ratio Lower Upper
 202 100
 101 6.7 5.3 7.9
 100 6.2 4.6 7.0









#83
 Butylbenzylphthalate
 Concen: 12.818 ng/ul
 RT: 21.007 min Scan# 2973
 Delta R.T. -0.003 min
 Lab File: BG056709.D
 Acq: 23 Feb 2023 12:14




Instrument :
 BNA_G
 ClientSampleId :
 SSTD010415


Tgt Ion:	149	Resp:	26160
Ion Ratio	Lower	Upper	
149	100		
91	84.8	59.3	88.9
206	26.7	19.7	29.5

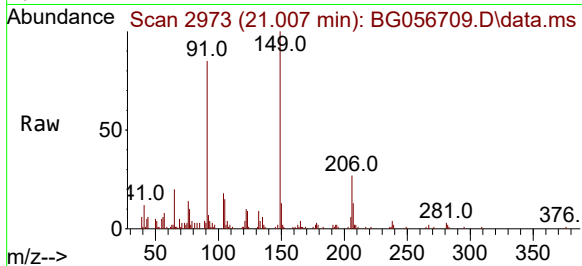

#84
 3,3'-Dichlorobenzidine
 Concen: 12.748 ng/ul
 RT: 21.947 min Scan# 3133
 Delta R.T. -0.003 min
 Lab File: BG056709.D
 Acq: 23 Feb 2023 12:14

Tgt Ion:	252	Resp:	30290
Ion Ratio	Lower	Upper	
252	100		
254	64.1	52.6	78.8
126	6.6	5.0	7.6




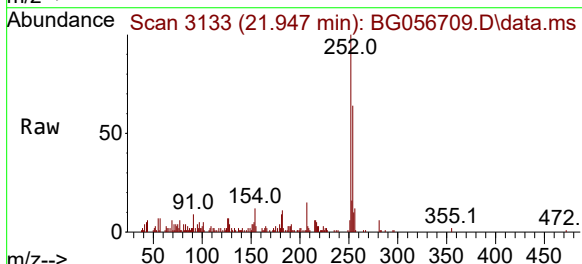




#85
Benzo(a)anthracene
Concen: 10.304 ng/ul
RT: 22.053 min Scan# 3151
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:228 Resp: 77904
Ion Ratio Lower Upper
228 100
229 19.9 16.2 24.4
226 25.2 20.6 31.0

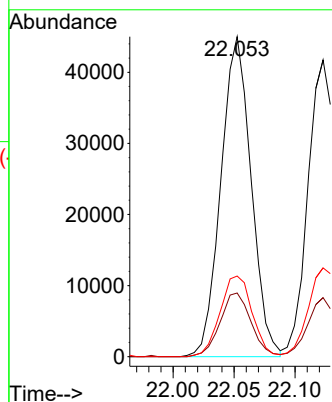

#86
Bis(2-ethylhexyl)phthalate
Concen: 12.871 ng/ul
RT: 21.917 min Scan# 3128
Delta R.T. 0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:149 Resp: 39697
Ion Ratio Lower Upper
149 100
167 27.5 21.8 32.8
279 5.2 4.2 6.2



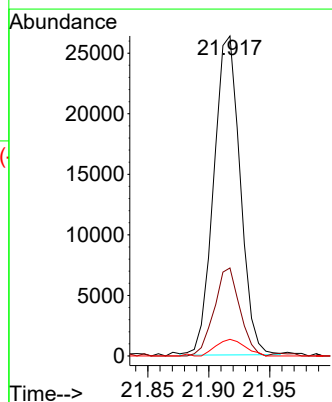





#87
Chrysene
Concen: 10.409 ng/ul
RT: 22.123 min Scan# 3163
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:228 Resp: 72388
Ion Ratio Lower Upper
228 100
226 29.9 23.6 35.4
229 19.9 15.4 23.0



#89
Di-n-octyl phthalate
Concen: 11.503 ng/ul
RT: 23.233 min Scan# 3352
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:149 Resp: 63053









#90
Benzo(b)fluoranthene
Concen: 9.937 ng/ul
RT: 24.473 min Scan# 3563
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:252 Resp: 76646
Ion Ratio Lower Upper
252 100
253 22.9 17.4 26.2
125 4.4 3.0 4.6

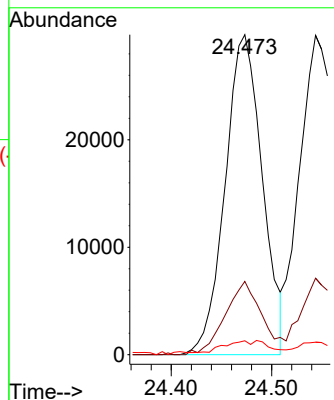

#91
Benzo(k)fluoranthene
Concen: 10.317 ng/ul
RT: 24.544 min Scan# 3575
Delta R.T. -0.009 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:252 Resp: 76599
Ion Ratio Lower Upper
252 100
253 23.9 18.2 27.2
125 3.9 3.4 5.2



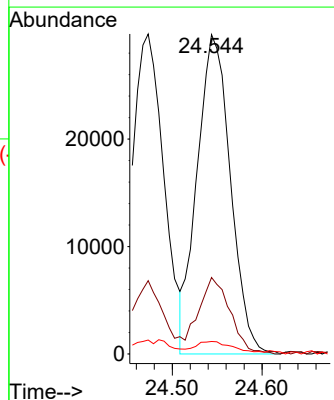
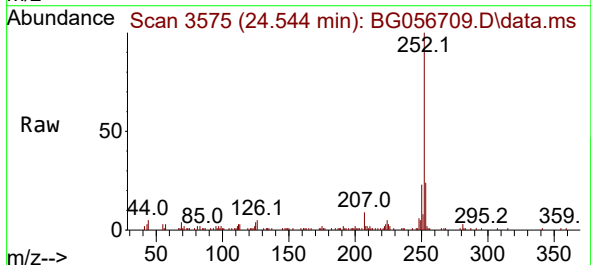




#93
Benzo(a)pyrene
Concen: 10.712 ng/ul
RT: 25.437 min Scan# 31
Delta R.T. -0.003 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14




Instrument :
BNA_G
ClientSampleId :
SSTD010415


Tgt Ion:252 Resp: 70397
Ion Ratio Lower Upper
252 100
253 19.7 17.4 26.0
125 4.8 3.6 5.4



#94
Indeno(1,2,3-cd)pyrene
Concen: 4.675 ng/ul
RT: 29.673 min Scan# 4448
Delta R.T. -0.009 min
Lab File: BG056709.D
Acq: 23 Feb 2023 12:14

Tgt Ion:276 Resp: 42320
Ion Ratio Lower Upper
276 100
138 8.2 5.7 8.5
277 22.5 18.1 27.1









#95
 Dibenzo(a,h)anthracene
 Concen: 10.417 ng/ul
 RT: 29.749 min Scan# 4461
 Delta R.T. -0.009 min
 Lab File: BG056709.D
 Acq: 23 Feb 2023 12:14

Instrument :
 BNA_G
 ClientSampleId :
 SSTD010415

Tgt Ion:278 Resp: 77968
 Ion Ratio Lower Upper
 278 100
 139 6.2 4.3 6.5
 279 24.1 21.7 32.5



#96
 Benzo(g,h,i)perylene
 Concen: 10.161 ng/ul
 RT: 30.954 min Scan# 4666
 Delta R.T. -0.003 min
 Lab File: BG056709.D
 Acq: 23 Feb 2023 12:14

Tgt Ion:276 Resp: 73318
 Ion Ratio Lower Upper
 276 100
 138 6.6 6.5 9.7
 277 20.0 20.7 31.1#

