
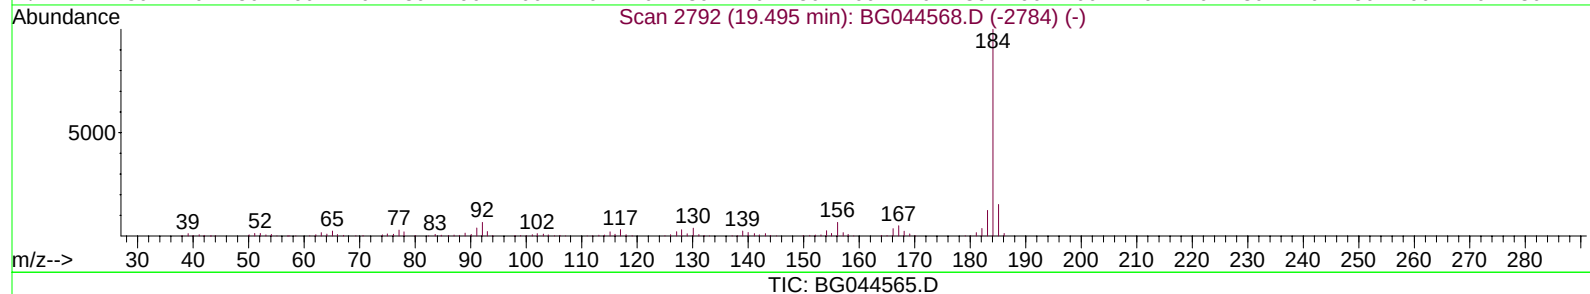
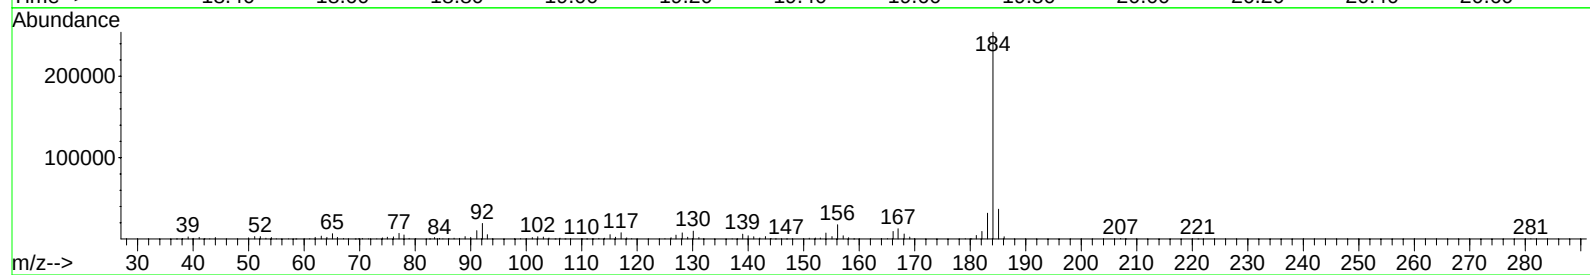


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG022420\
Data File : BG044565.D
Acq On : 24 Feb 2020 10:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 17:50:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 24 16:11:23 2020
Response via : Initial Calibration

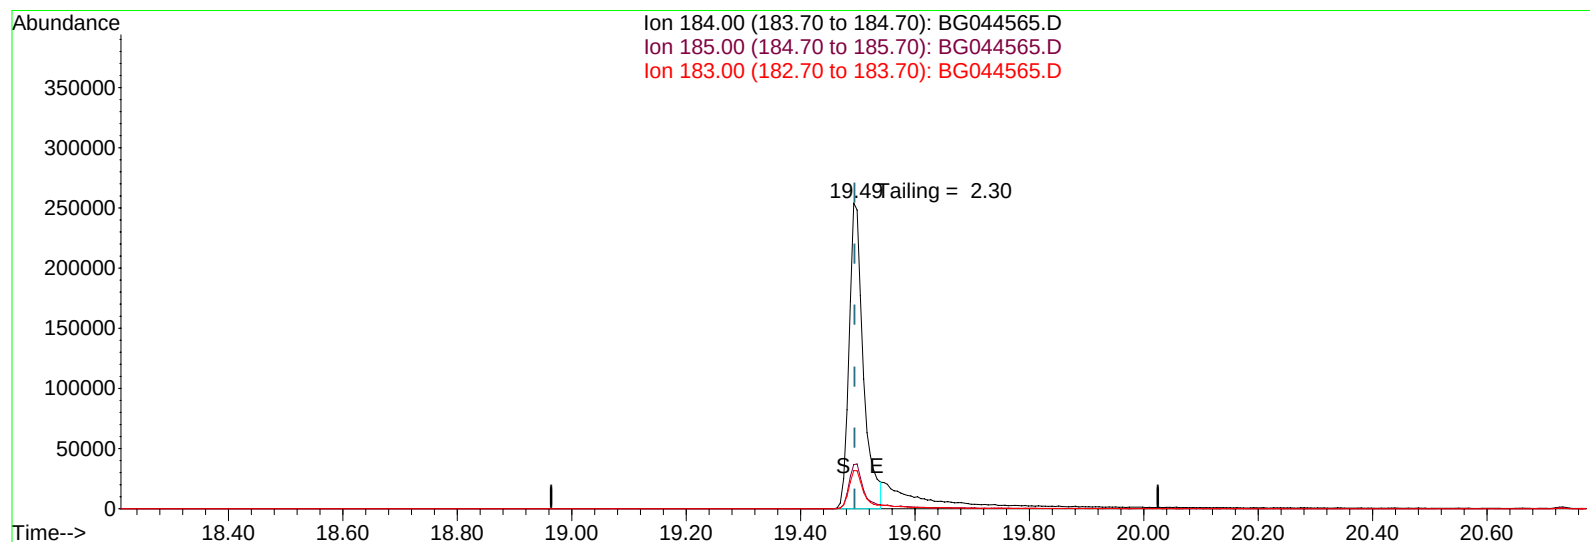

(77) Benzidine




19.493min (-0.002) 0.00ng

response 543819

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.43
183.00	12.40	12.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG022420\
Data File : BG044565.D
Acq On : 24 Feb 2020 10:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 17:50:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 24 16:11:23 2020
Response via : Initial Calibration

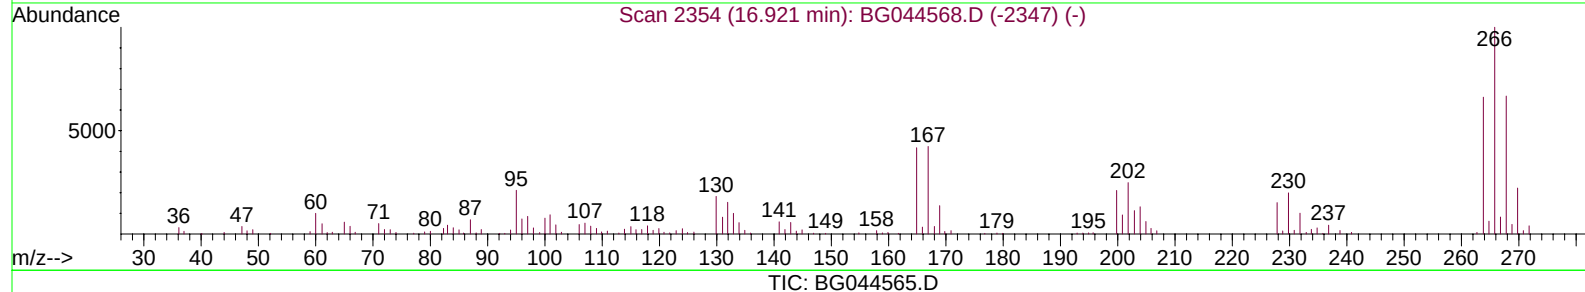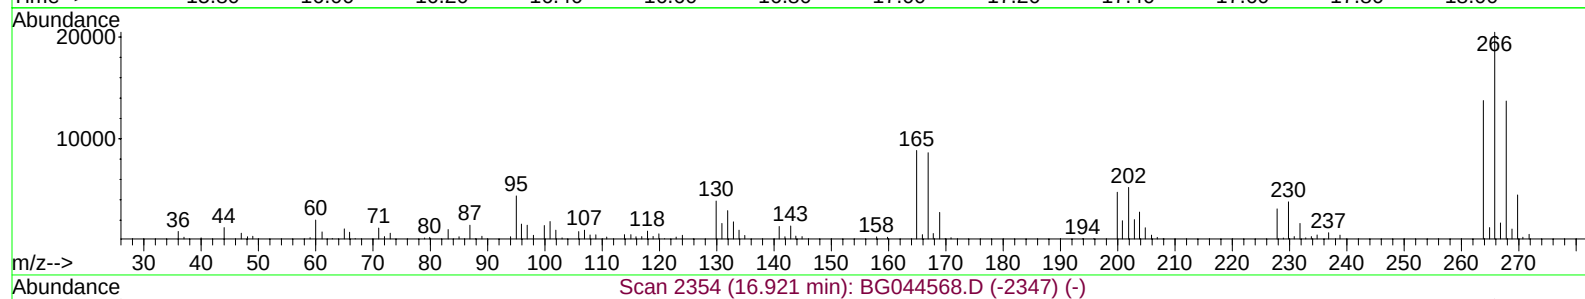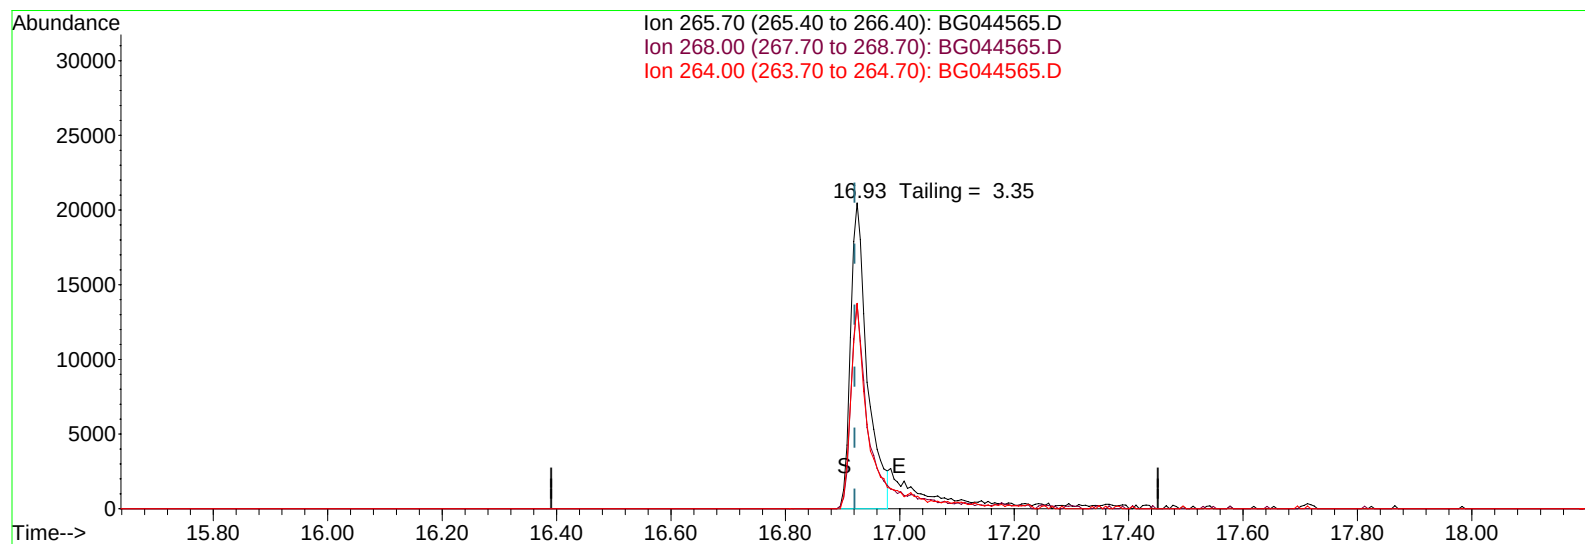

(70) Pentachlorophenol (C)

16.925min (+0.004) 14634.32ng

response 50607

Ion	Exp%	Act%
265.70	100	100
268.00	66.70	66.96
264.00	66.20	67.19
0.00	0.00	0.00