

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022422\
 Data File : BG052482.D
 Acq On : 24 Feb 2022 17:49
 Operator : CG/JU
 Sample : N1616-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052482.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.535	6	8	10	rVB2	1184	961	0.21%	0.049%
2	3.558	10	12	13	rBV2	773	631	0.14%	0.032%
3	3.646	25	27	31	rVB2	1332	1405	0.30%	0.071%
4	3.699	34	36	37	rBV2	670	663	0.14%	0.034%
5	3.723	39	40	43	rBV3	830	697	0.15%	0.035%
6	3.746	43	44	46	rBV2	707	555	0.12%	0.028%
7	4.116	106	107	110	rVB2	1010	612	0.13%	0.031%
8	4.146	110	112	115	rVB2	1208	692	0.15%	0.035%
9	4.234	124	127	128	rBV	900	947	0.20%	0.048%
10	4.322	141	142	147	rVB3	1544	1902	0.41%	0.096%
11	4.481	165	169	171	rBV4	675	1055	0.23%	0.054%
12	4.516	173	175	179	rBV2	796	1046	0.23%	0.053%
13	4.645	196	197	200	rBV2	662	667	0.14%	0.034%
14	4.774	217	219	220	rBV2	750	542	0.12%	0.027%
15	4.880	235	237	238	rBV	895	529	0.11%	0.027%
16	4.962	249	251	253	rVB	784	610	0.13%	0.031%
17	4.998	255	257	259	rVV3	997	820	0.18%	0.042%
18	5.021	259	261	262	rVB2	849	555	0.12%	0.028%
19	5.280	303	305	308	rBV2	633	997	0.22%	0.051%
20	5.344	314	316	319	rVB	574	673	0.15%	0.034%
21	5.456	332	335	339	rBV2	771	892	0.19%	0.045%
22	5.585	352	357	358	rBV2	551	745	0.16%	0.038%
23	5.855	398	403	405	rBV2	929	1252	0.27%	0.064%
24	6.031	431	433	435	rBV2	540	587	0.13%	0.030%
25	6.137	449	451	453	rVB	653	522	0.11%	0.026%
26	6.155	453	454	457	rVB	942	565	0.12%	0.029%
27	6.231	464	467	473	rBV	688	1302	0.28%	0.066%
28	6.519	514	516	517	rVB	1148	582	0.13%	0.030%
29	6.636	533	536	538	rBV2	603	755	0.16%	0.038%
30	6.948	586	589	590	rBV	798	697	0.15%	0.035%
31	7.189	628	630	632	rBV	887	740	0.16%	0.038%
32	7.289	645	647	650	rVB	725	528	0.11%	0.027%
33	7.465	674	677	678	rBV	670	613	0.13%	0.031%
34	7.676	710	713	714	rBV	733	617	0.13%	0.031%
35	7.788	729	732	733	rBV2	614	550	0.12%	0.028%
36	8.117	785	788	789	rBV	552	679	0.15%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022422\
 Data File : BG052482.D
 Acq On : 24 Feb 2022 17:49
 Operator : CG/JU
 Sample : N1616-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

37	8.217	798	805	813	rBV	74797	125440	27.10%	6.363%
38	8.358	828	829	832	rBV	625	631	0.14%	0.032%
39	8.399	834	836	839	rVB	812	662	0.14%	0.034%
40	8.493	849	852	857	rVB2	495	945	0.20%	0.048%
41	8.540	857	860	861	rBV	476	537	0.12%	0.027%
42	8.728	889	892	894	rBV	461	630	0.14%	0.032%
43	8.969	930	933	934	rBV2	671	533	0.12%	0.027%
44	9.480	1018	1020	1022	rVB	793	606	0.13%	0.031%
45	9.950	1099	1100	1103	rBV	543	545	0.12%	0.028%
46	11.060	1280	1289	1297	rBV	96396	180245	38.94%	9.143%
47	11.154	1303	1305	1307	rVB	722	562	0.12%	0.029%
48	11.189	1307	1311	1312	rBV2	676	661	0.14%	0.034%
49	11.671	1391	1393	1396	rVB	538	544	0.12%	0.028%
50	11.694	1396	1397	1400	rBV2	525	569	0.12%	0.029%
51	12.247	1488	1491	1494	rVB	471	588	0.13%	0.030%
52	12.576	1544	1547	1550	rVB	545	611	0.13%	0.031%
53	12.787	1582	1583	1586	rBV2	575	573	0.12%	0.029%
54	13.251	1660	1662	1664	rVB2	726	537	0.12%	0.027%
55	13.698	1736	1738	1743	rVB	634	699	0.15%	0.035%
56	14.038	1795	1796	1800	rBV	548	562	0.12%	0.029%
57	14.297	1838	1840	1842	rVB2	581	525	0.11%	0.027%
58	14.867	1929	1937	1945	rBV	169472	281094	60.73%	14.258%
59	15.501	2044	2045	2049	rBV2	692	887	0.19%	0.045%
60	15.671	2071	2074	2076	rVB	533	534	0.12%	0.027%
61	15.748	2084	2087	2089	rBV2	426	552	0.12%	0.028%
62	15.924	2115	2117	2122	rBV2	459	531	0.11%	0.027%
63	16.723	2251	2253	2255	rBV2	500	622	0.13%	0.032%
64	17.240	2338	2341	2343	rBV	805	1011	0.22%	0.051%
65	17.293	2346	2350	2353	rBV2	870	1452	0.31%	0.074%
66	17.575	2395	2398	2399	rBV	1149	991	0.21%	0.050%
67	17.616	2399	2405	2414	rBV	242666	394529	85.23%	20.012%
68	17.716	2419	2422	2428	rVB2	2021	3741	0.81%	0.190%
69	17.839	2442	2443	2446	rVB2	759	645	0.14%	0.033%
70	18.050	2477	2479	2481	rBV2	816	647	0.14%	0.033%
71	18.086	2483	2485	2487	rVB2	876	768	0.17%	0.039%
72	18.103	2487	2488	2490	rBV	852	594	0.13%	0.030%
73	18.233	2508	2510	2511	rBV	673	551	0.12%	0.028%
74	18.726	2592	2594	2597	rVB2	789	760	0.16%	0.039%
75	18.902	2622	2624	2626	rBV2	886	743	0.16%	0.038%
76	19.102	2657	2658	2661	rBV2	983	977	0.21%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022422\
 Data File : BG052482.D
 Acq On : 24 Feb 2022 17:49
 Operator : CG/JU
 Sample : N1616-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

77	19.137	2663	2664	2667	rVB	1059	814	0.18%	0.041%
78	19.172	2667	2670	2671	rBV2	923	802	0.17%	0.041%
79	19.190	2671	2673	2677	rBV2	1015	1001	0.22%	0.051%
80	19.313	2692	2694	2695	rBV	672	551	0.12%	0.028%
81	19.419	2711	2712	2714	rVB	823	570	0.12%	0.029%
82	19.449	2714	2717	2718	rBV2	683	730	0.16%	0.037%
83	19.525	2727	2730	2731	rBV3	859	1021	0.22%	0.052%
84	19.760	2769	2770	2772	rBV2	798	670	0.14%	0.034%
85	19.960	2800	2804	2805	rBV3	1416	1482	0.32%	0.075%
86	19.983	2807	2808	2810	rVB	1560	786	0.17%	0.040%
87	20.482	2891	2893	2896	rVB3	2214	1911	0.41%	0.097%
88	21.928	3132	3139	3150	rVB	264938	462873	100.00%	23.479%
89	25.388	3719	3728	3745	rVB2	146995	461189	99.64%	23.394%




Sum of corrected areas: 1971419

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022422\
Data File : BG052482.D
Acq On : 24 Feb 2022 17:49
Operator : CG/JU
Sample : N1616-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

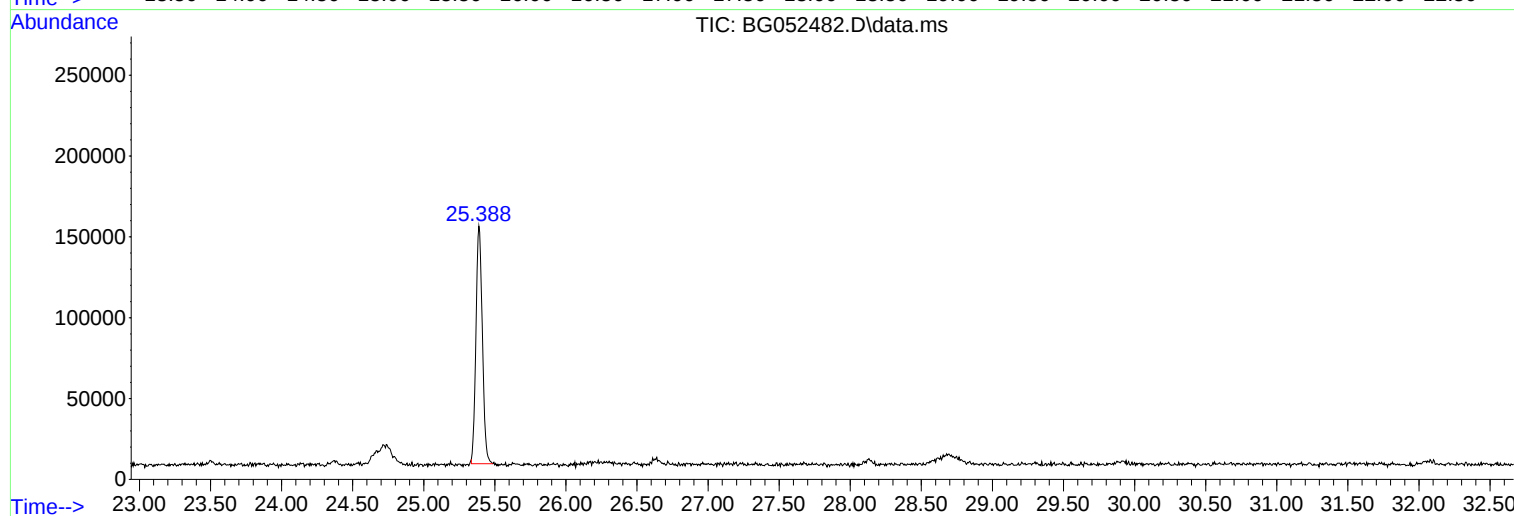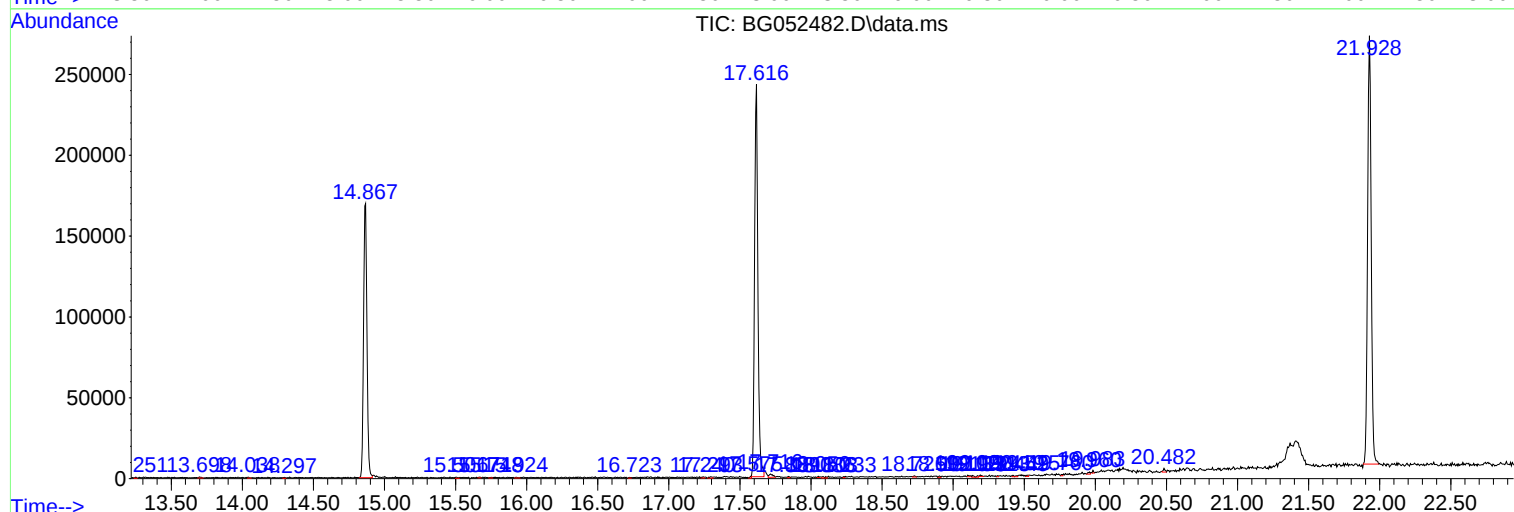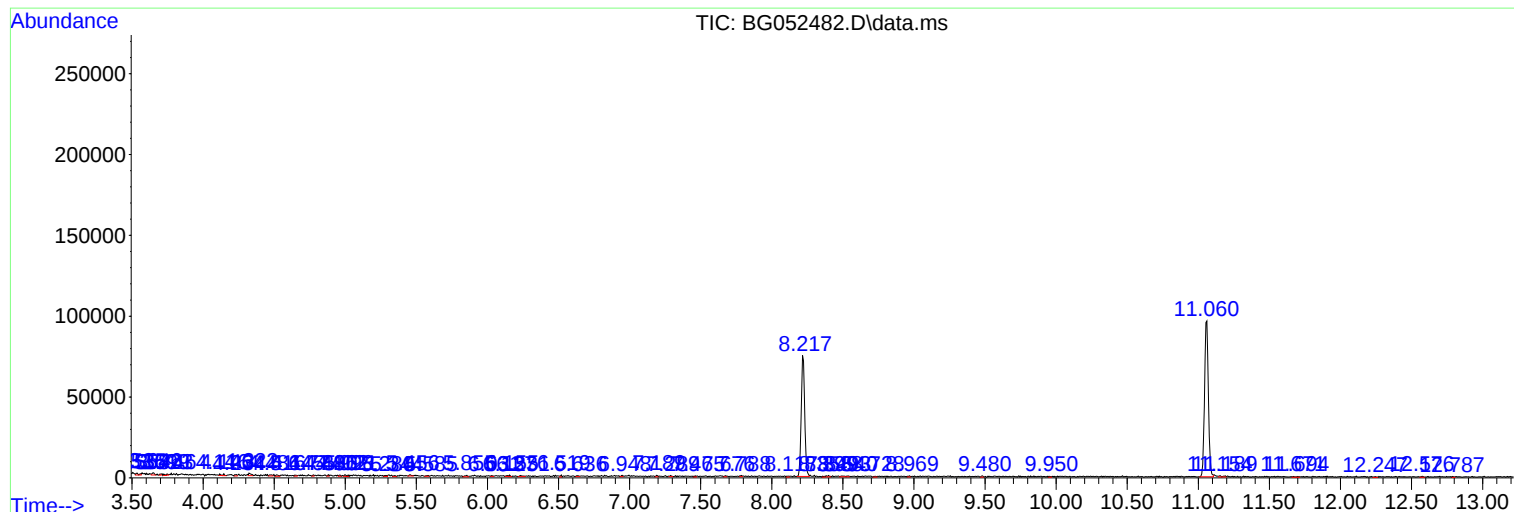

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022422\
Data File : BG052482.D
Acq On : 24 Feb 2022 17:49
Operator : CG/JU
Sample : N1616-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022422\
Data File : BG052482.D
Acq On : 24 Feb 2022 17:49
Operator : CG/JU
Sample : N1616-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------