

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022620\
 Data File : BG044601.D
 Acq On : 26 Feb 2020 13:13
 Operator : CG/JU
 Sample : PB127061BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB127061BL

Quant Time: Feb 27 07:02:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 24 16:11:23 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	62493	20.00	ng	0.00
21) Naphthalene-d8	10.67	136	261853	20.00	ng	0.00
39) Acenaphthene-d10	14.51	164	177308	20.00	ng	0.00
64) Phenanthrene-d10	17.26	188	415819	20.00	ng	0.00
76) Chrysene-d12	21.50	240	403821	20.00	ng	0.00
87) Perylene-d12	24.57	264	416246	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	237763	61.04	ng	0.00
7) Phenol-d6	7.04	99	186554	34.99	ng	0.00
23) Nitrobenzene-d5	9.03	82	431534	84.90	ng	0.00
42) 2,4,6-Tribromophenol	16.00	330	325923	129.64	ng	0.00
45) 2-Fluorobiphenyl	13.14	172	1021764	82.52	ng	0.00
79) Terphenyl-d14	19.88	244	1741841	81.66	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.97	163	32829	2.294	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022620\
Data File : BG044601.D
Acq On : 26 Feb 2020 13:13
Operator : CG/JU
Sample : PB127061BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB127061BL

Quant Time: Feb 27 07:02:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 24 16:11:23 2020
Response via : Initial Calibration

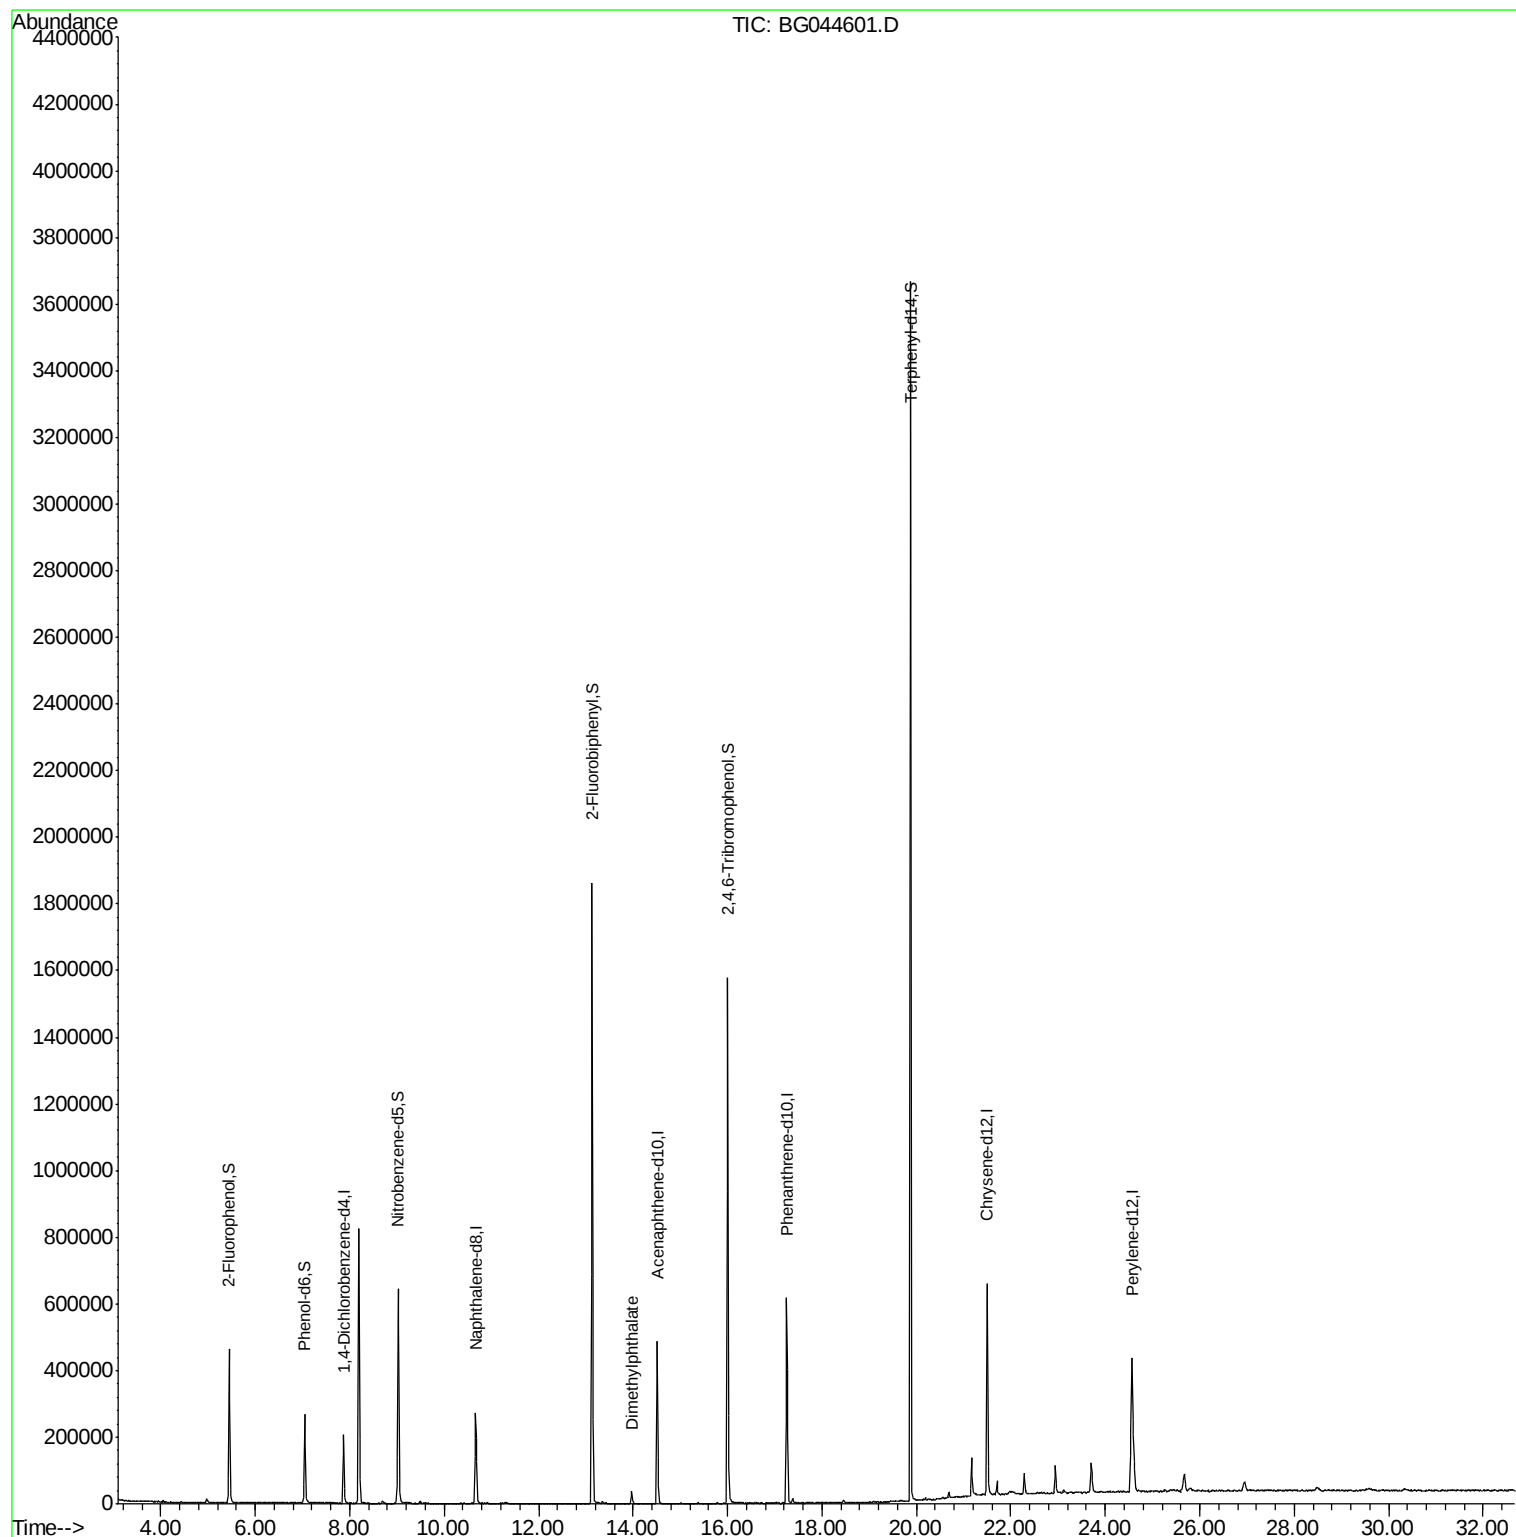

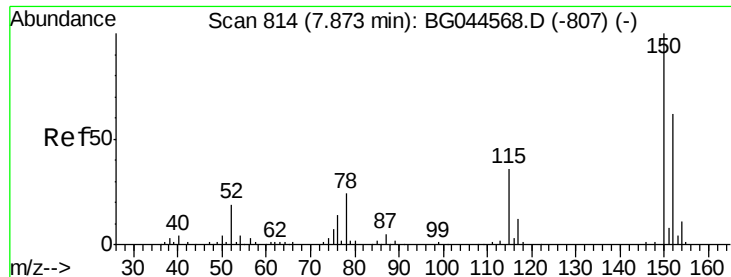


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.87 min Scan# 814
Delta R.T. 0.00 min
Lab File: BG044601.D
Acq: 26 Feb 2020 13:13

Instrument :
BNA_G
ClientSampleId :
PB127061BL

Tot Ion:152 Resp: 62493
Ion Ratio Lower Upper
152 100
150 156.9 128.9 193.3
115 55.5 47.0 70.4

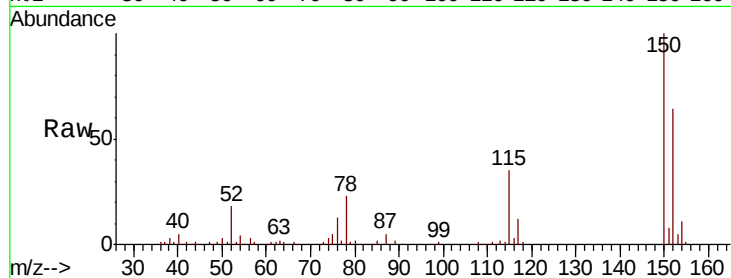


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

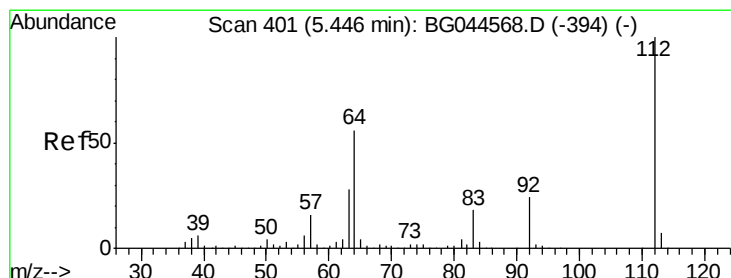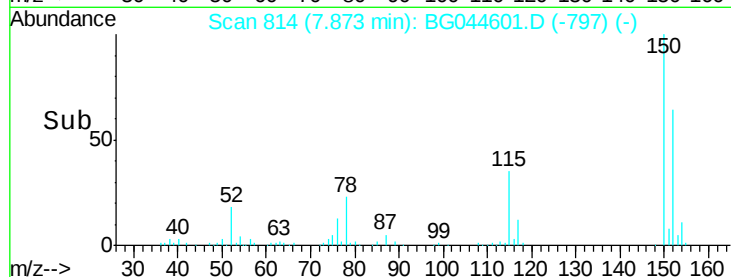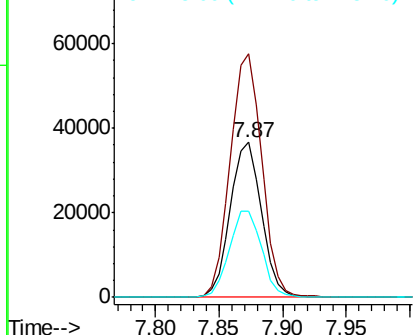



#5

2-Fluorophenol
Concen: 61.044 ng
RT: 5.45 min Scan# 401
Delta R.T. 0.00 min
Lab File: BG044601.D
Acq: 26 Feb 2020 13:13

Tgt Ion:112 Resp: 237763
Ion Ratio Lower Upper
112 100
64 55.4 44.8 67.2
63 27.5 22.3 33.5

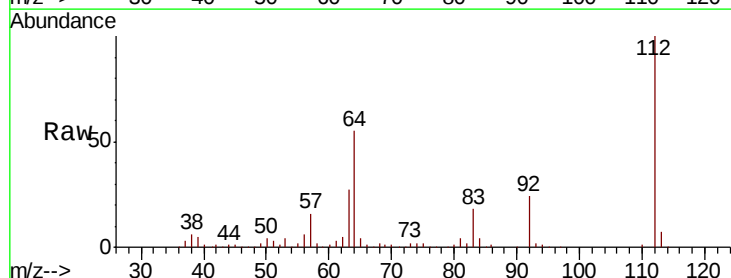

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

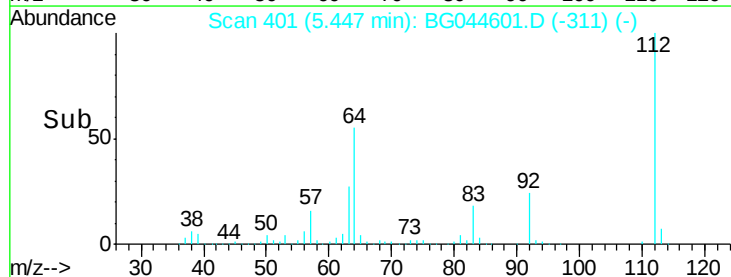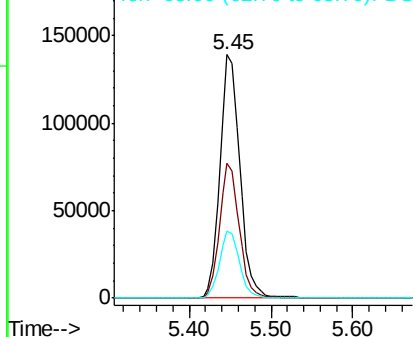



#7

Phenol-d6

Concen: 34.991 ng

RT: 7.04 min Scan# 673

Delta R.T. -0.01 min

Lab File: BG044601.D

Acq: 26 Feb 2020 13:13

Instrument :

BNA_G

ClientSampled :

PB127061BL


Tot Ion: 99 Resp: 186554

Ion Ratio Lower Upper




99 100

42 16.2 12.8 19.2

71 30.1 24.4 36.6

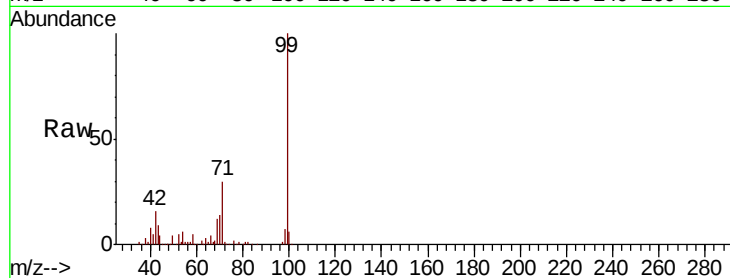

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

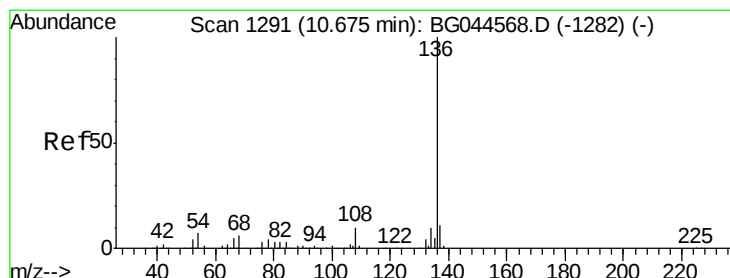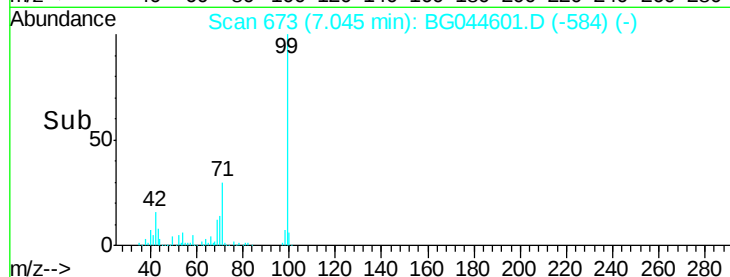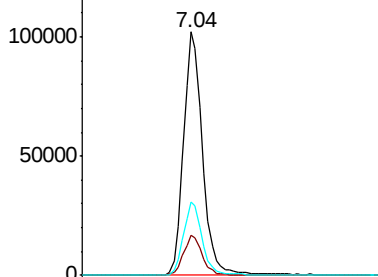

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.67 min Scan# 1290

Delta R.T. -0.01 min

Lab File: BG044601.D

Acq: 26 Feb 2020 13:13

Tgt Ion: 136 Resp: 261853


Ion Ratio Lower Upper

136 100



137 10.4 8.8 13.2


54 7.2 5.7 8.5

68 5.6 4.5 6.7

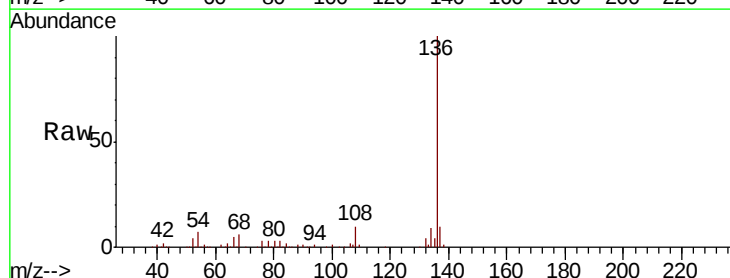

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

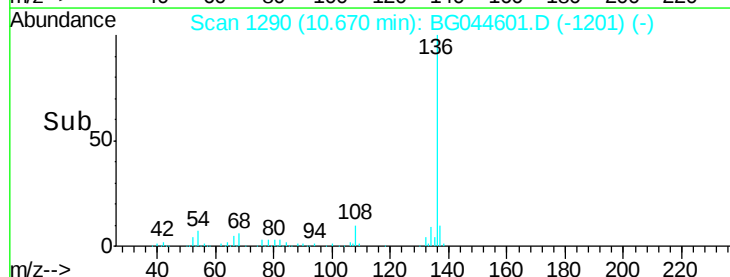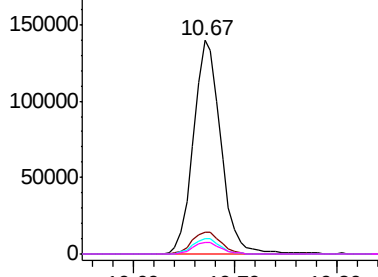


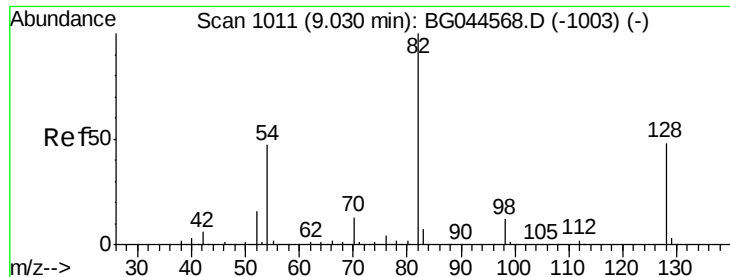




#23
 Nitrobenzene-d5
 Concen: 84.902 ng
 RT: 9.03 min Scan# 1011
 Delta R.T. 0.00 min
 Lab File: BG044601.D
 Acq: 26 Feb 2020 13:13

Instrument :
 BNA_G
 ClientSampleId :
 PB127061BL

Tot Ion	82	Resp	431534
Ion Ratio	100	Lower	Upper
128	46.2	38.1	57.1
54	45.5	37.5	56.3

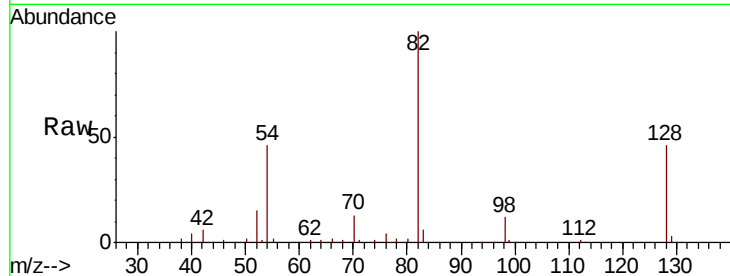


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

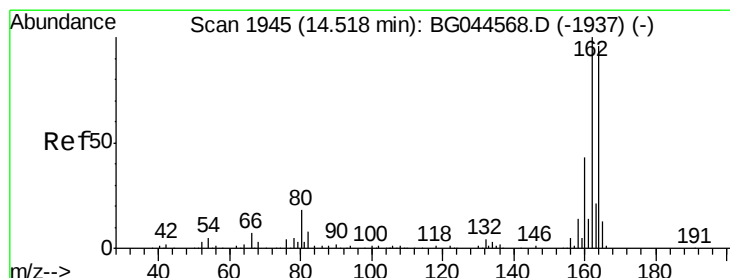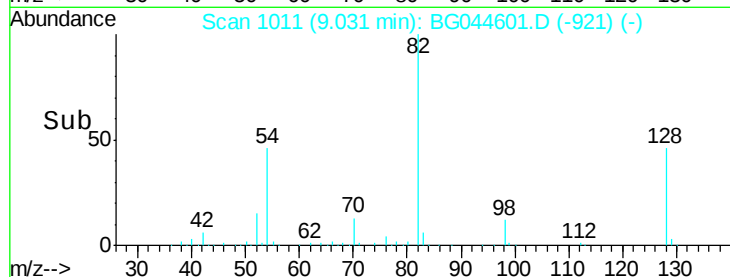
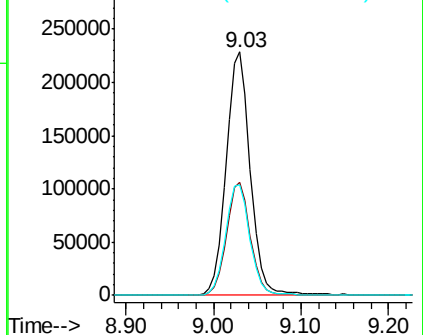



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.51 min Scan# 1944
 Delta R.T. -0.01 min
 Lab File: BG044601.D
 Acq: 26 Feb 2020 13:13

Tgt Ion	164	Resp	177308
Ion Ratio	100	Lower	Upper
162	101.3	83.6	125.4
160	43.7	36.2	54.4

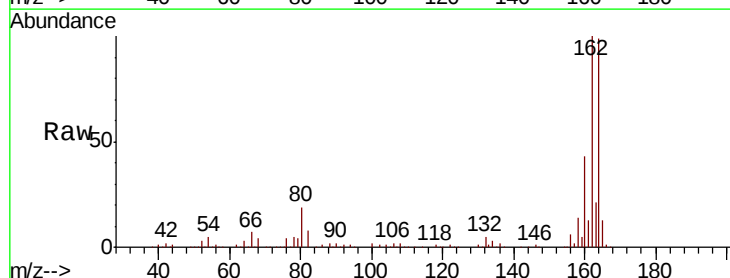

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

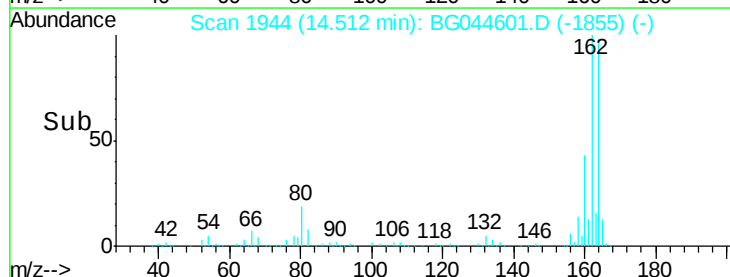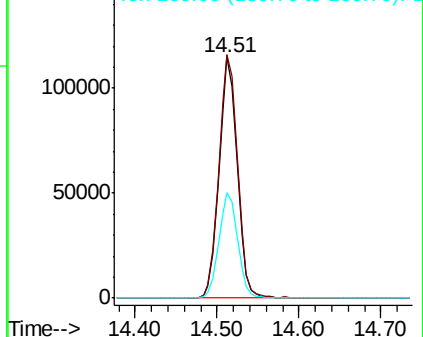


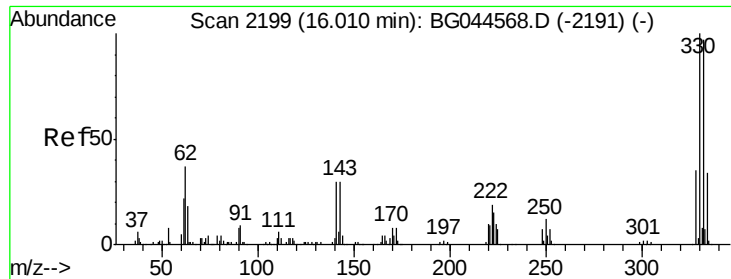




#42
 2,4,6-Tribromophenol
 Concen: 129.639 ng
 RT: 16.00 min Scan# 2198
 Delta R.T. -0.01 min
 Lab File: BG044601.D
 Acq: 26 Feb 2020 13:13

Instrument :
 BNA_G
 ClientSampled :
 PB127061BL

Tot Ion:330 Resp: 325923
 Ion Ratio Lower Upper
 330 100
 332 97.1 77.4 116.0
 141 33.4 26.1 39.1

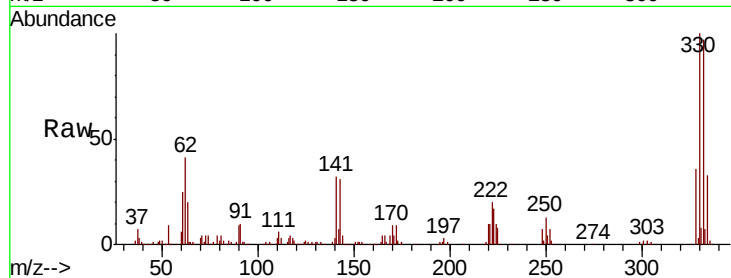


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

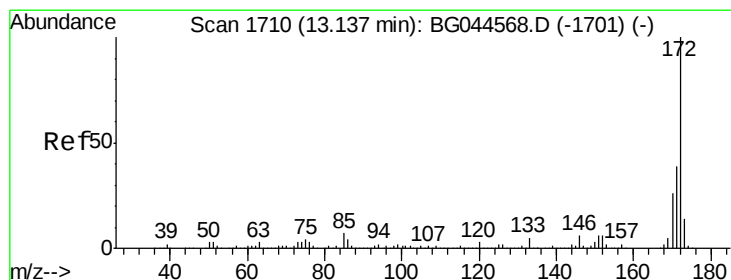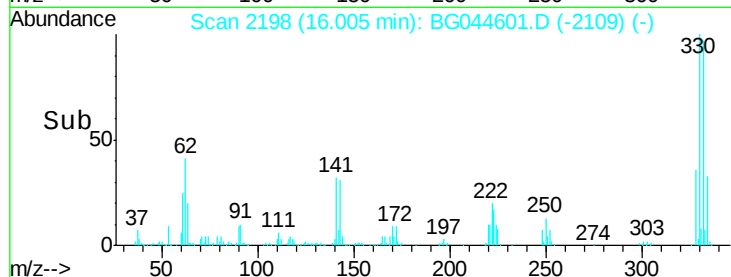
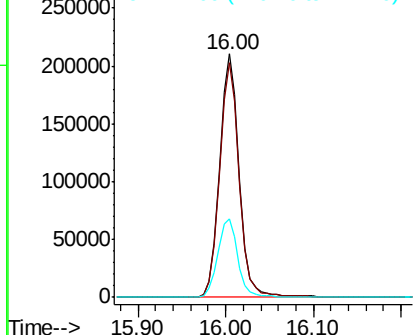



#45
 2-Fluorobiphenyl
 Concen: 82.521 ng
 RT: 13.14 min Scan# 1710
 Delta R.T. 0.00 min
 Lab File: BG044601.D
 Acq: 26 Feb 2020 13:13

Tgt Ion:172 Resp: 1021764
 Ion Ratio Lower Upper
 172 100
 171 38.5 31.3 46.9
 170 25.9 21.0 31.4

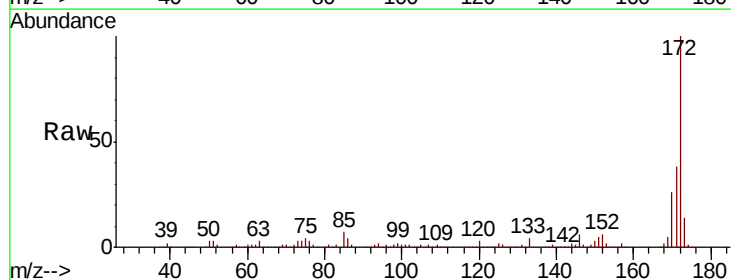

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

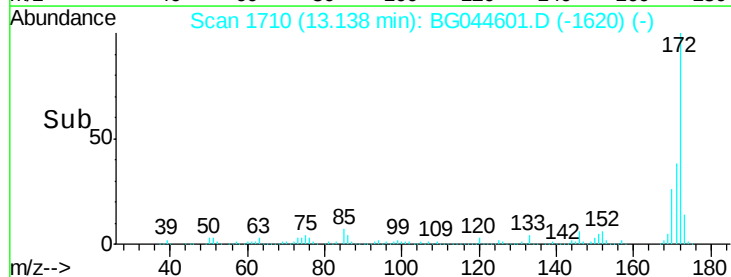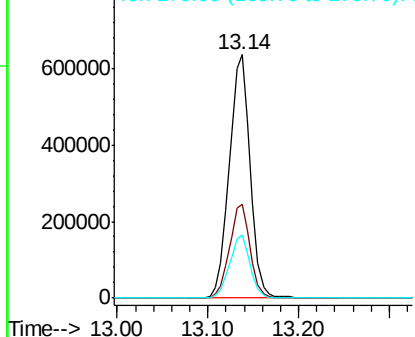

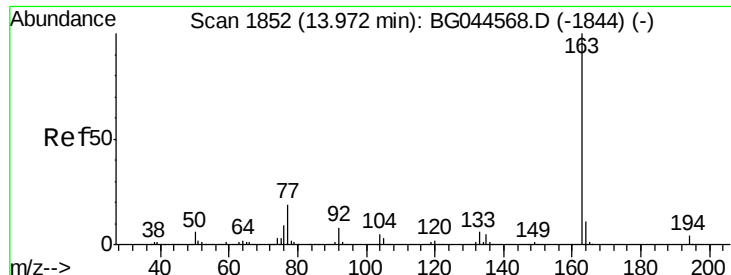

#50

Dimethylphthalate

Concen: 2.294 ng

RT: 13.97 min Scan# 1852

Delta R.T. 0.00 min

Lab File: BG044601.D

Acq: 26 Feb 2020 13:13

Instrument :

BNA_G

ClientSampleId :

PB127061BL


Tot Ion:163 Resp: 32829

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0




164 9.6 8.7 13.1

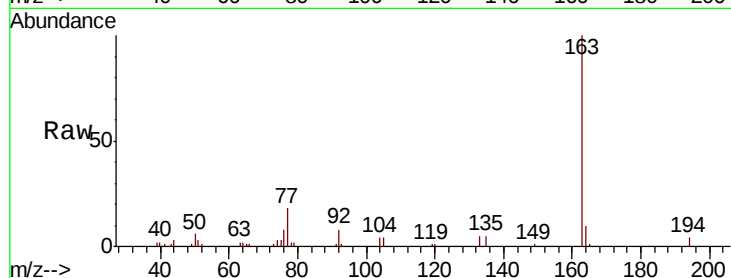

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

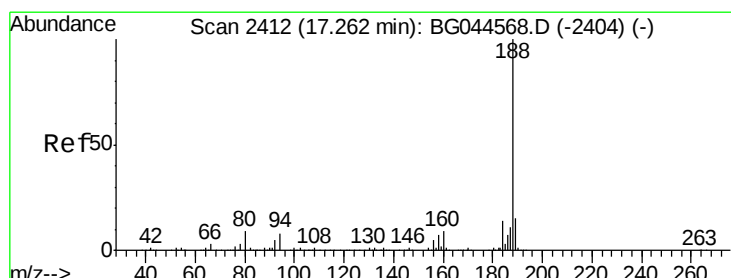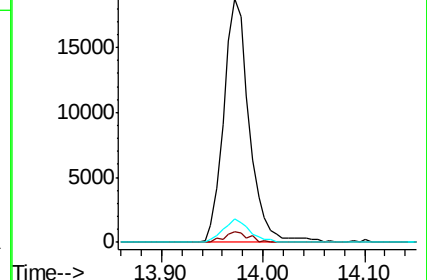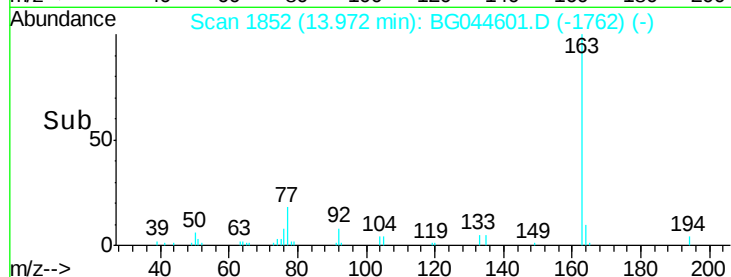

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.26 min Scan# 2411

Delta R.T. -0.01 min

Lab File: BG044601.D

Acq: 26 Feb 2020 13:13


Tgt Ion:188 Resp: 415819

Ion Ratio Lower Upper

188 100

94 8.5 6.7 10.1



80 9.4 7.6 11.4

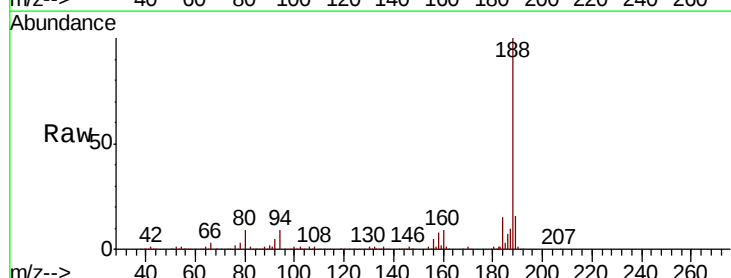


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC



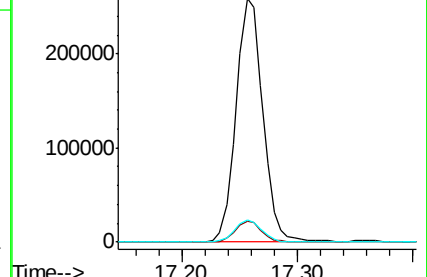
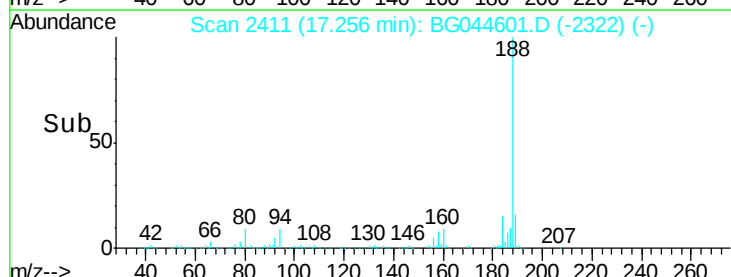


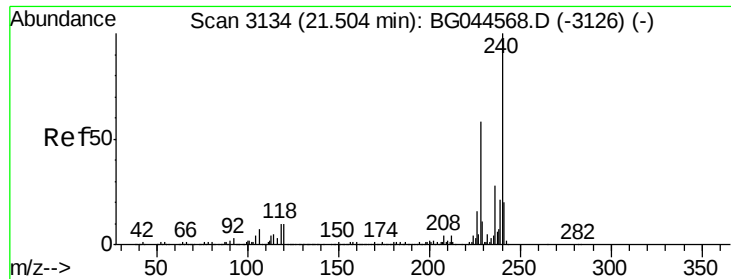

#76
 Chrvsene-d12
 Concen: 20.000 ng
 RT: 21.50 min Scan# 3133
 Delta R.T. -0.01 min
 Lab File: BG044601.D
 Acq: 26 Feb 2020 13:13




Instrument :
 BNA_G
 ClientSampleId :
 PB127061BL


Tot Ion:240 Resp: 403821
 Ion Ratio Lower Upper
 240 100
 120 10.1 8.3 12.5
 236 26.9 22.3 33.5

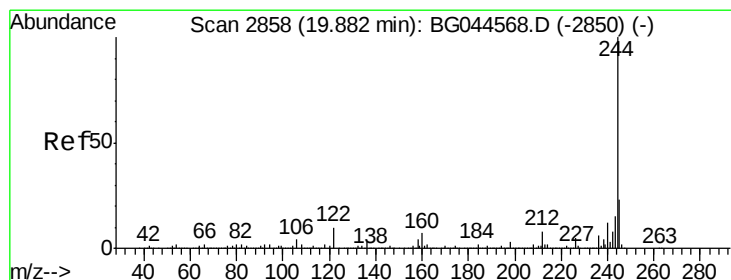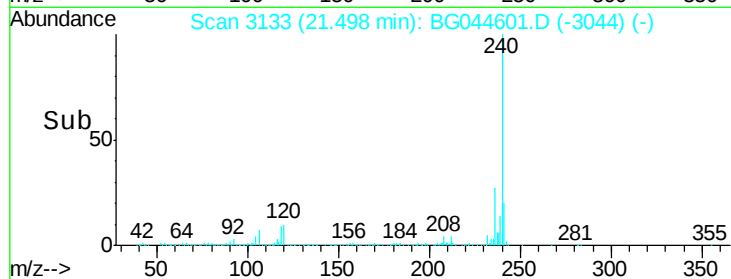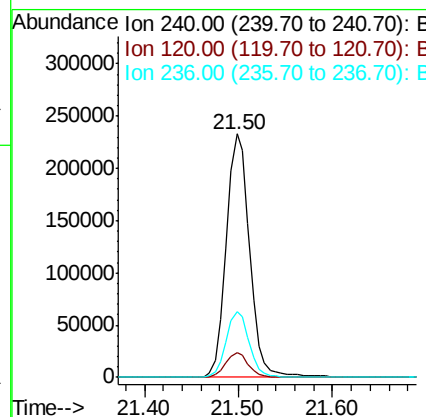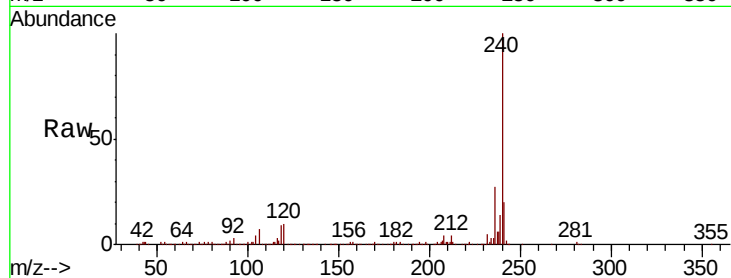

#79
 Terphenyl-d14
 Concen: 81.656 ng
 RT: 19.88 min Scan# 2857
 Delta R.T. -0.01 min
 Lab File: BG044601.D
 Acq: 26 Feb 2020 13:13

Tgt Ion:244 Resp: 1741841
 Ion Ratio Lower Upper
 244 100
 212 8.7 6.5 9.7
 122 12.0 8.2 12.4

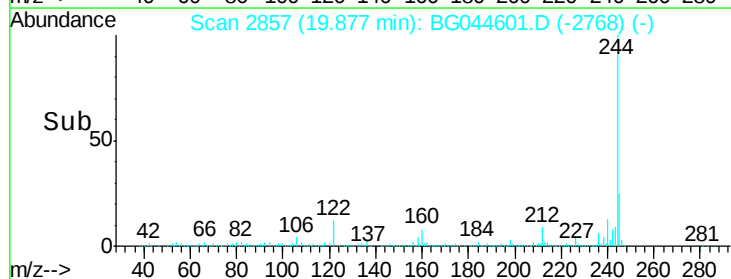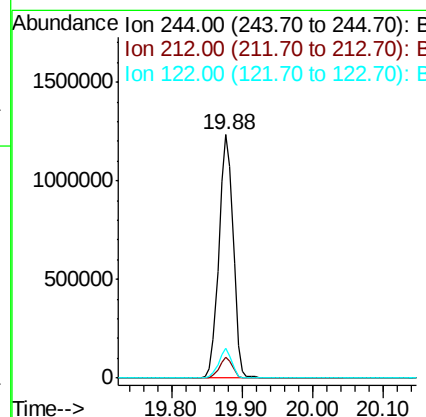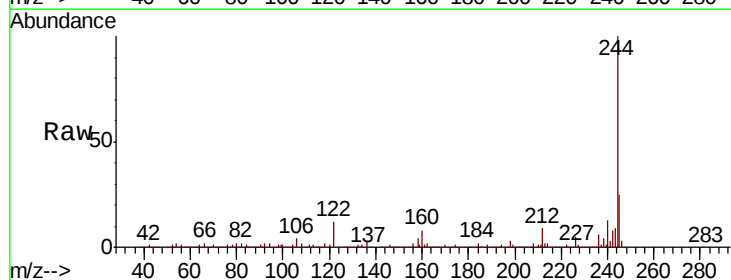

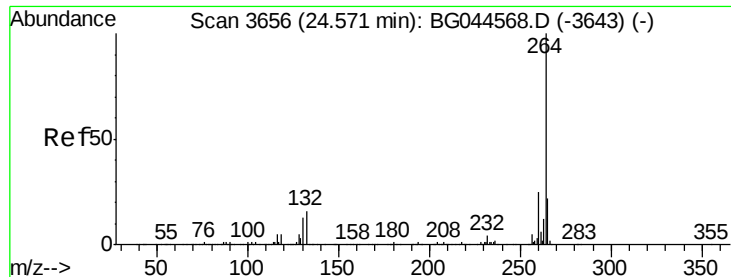

#87
Pervlene-d12
Concen: 20.000 ng
RT: 24.57 min Scan# 3655
Delta R.T. -0.01 min
Lab File: BG044601.D
Acq: 26 Feb 2020 13:13

Instrument :
BNA_G
ClientSampleId :
PB127061BL

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.7	29.5
265	22.1	17.8	26.8

