
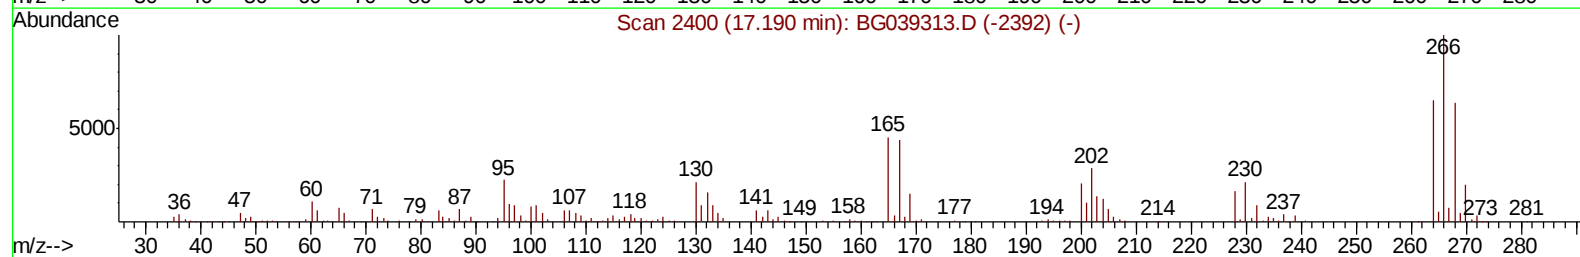
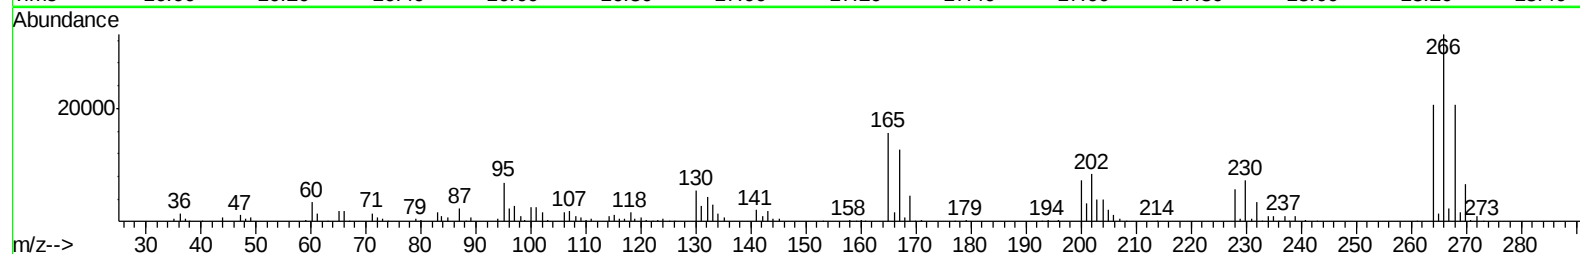


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG022719\
Data File : BG039629.D
Acq On : 27 Feb 2019 11:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 08:26:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

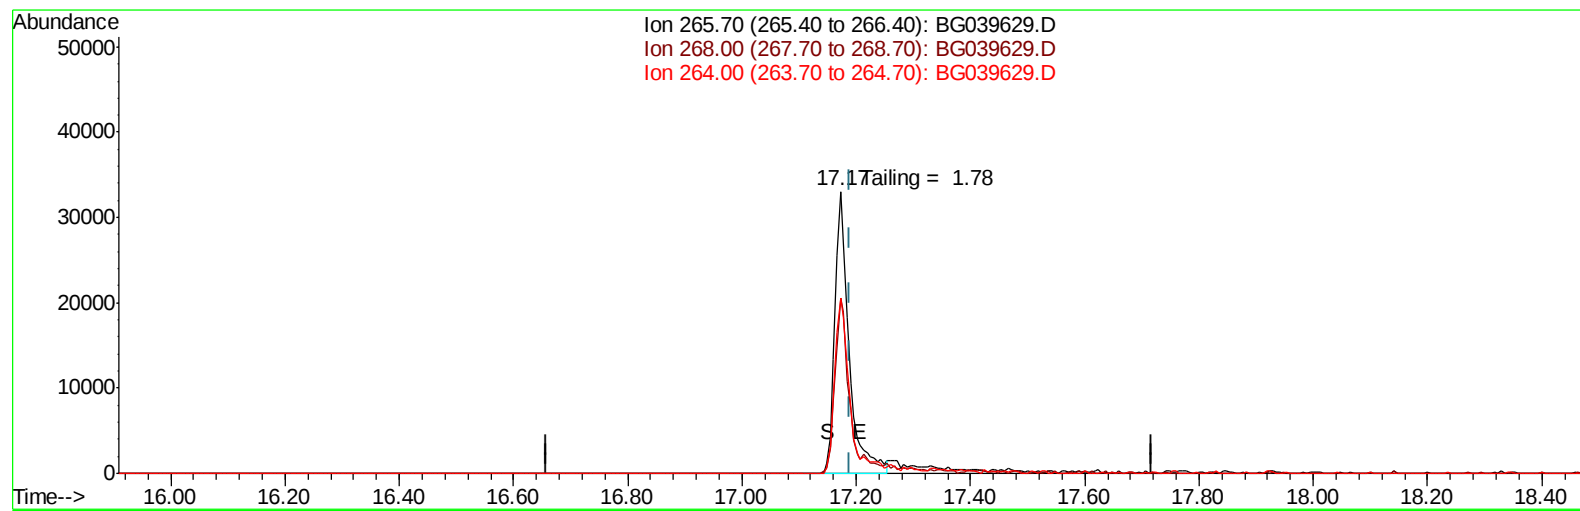

TIC: BG039629.D

(70) Pentachlorophenol (C)




17.172min (-0.018) 20703.31ng

response 56536

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.32
264.00	65.10	62.27
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG022719\
 Data File : BG039629.D
 Acq On : 27 Feb 2019 11:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 08:26:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

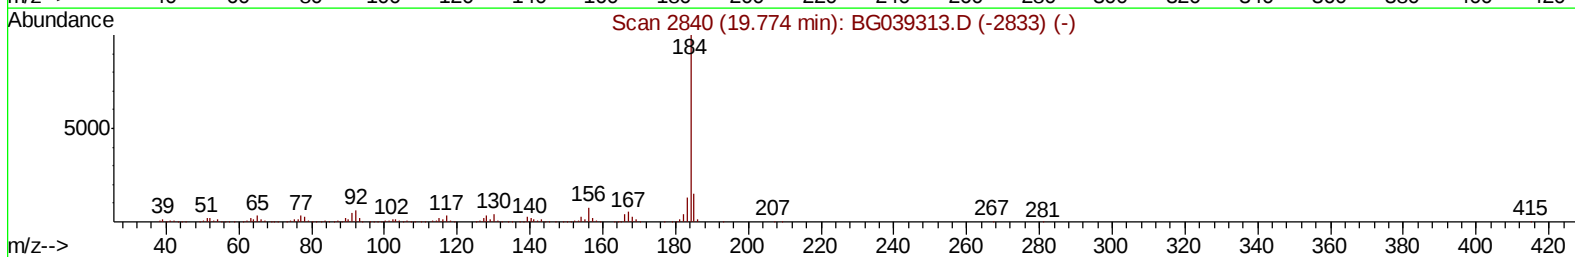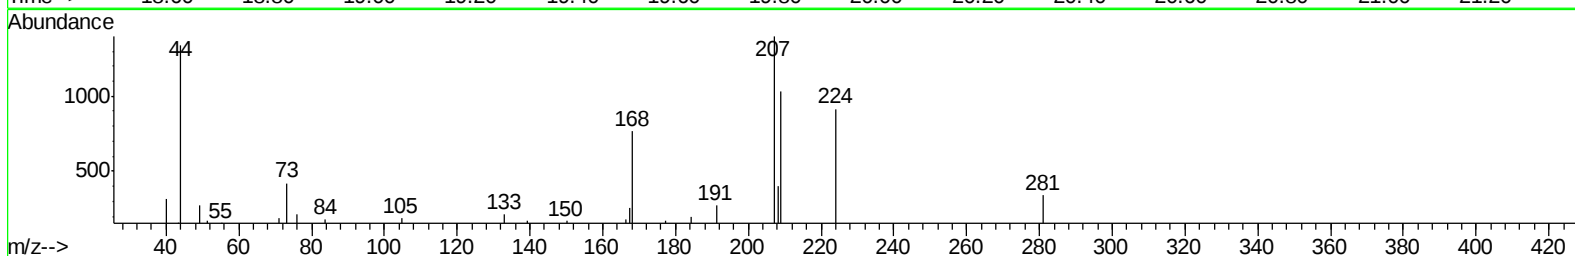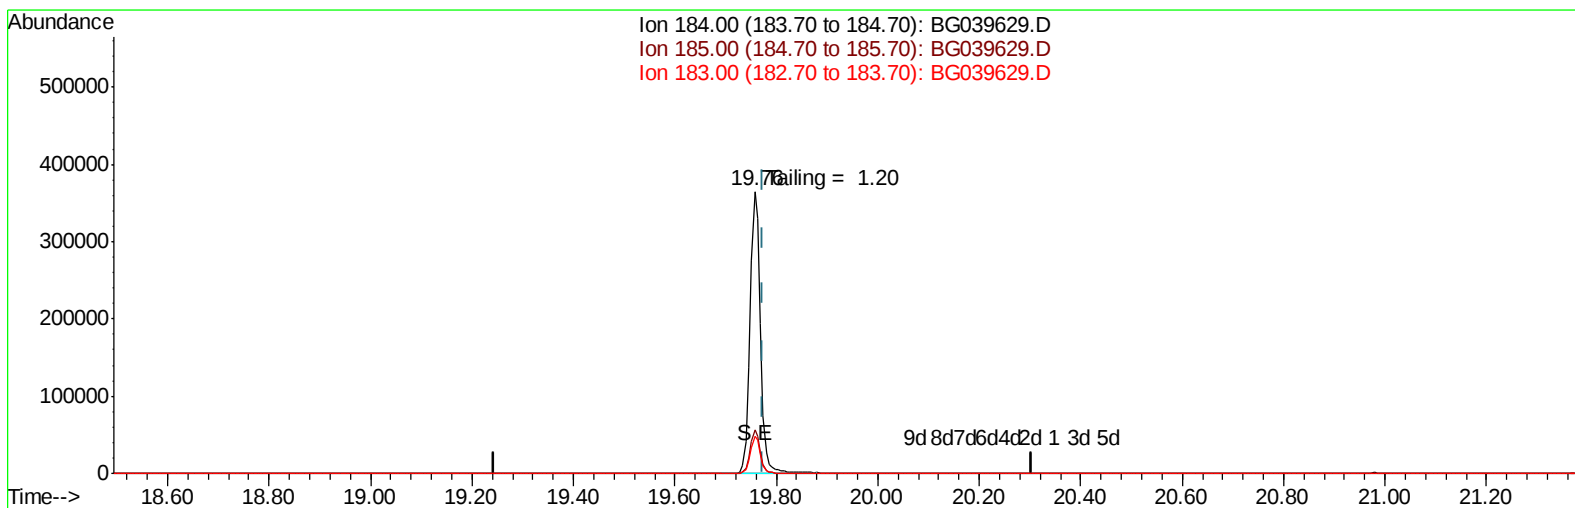

TIC: BG039629.D

(77) Benzidine

20.350min (+0.576) 99.34ng

response 241

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	0.00#
183.00	13.20	0.00#
0.00	0.00	0.00