
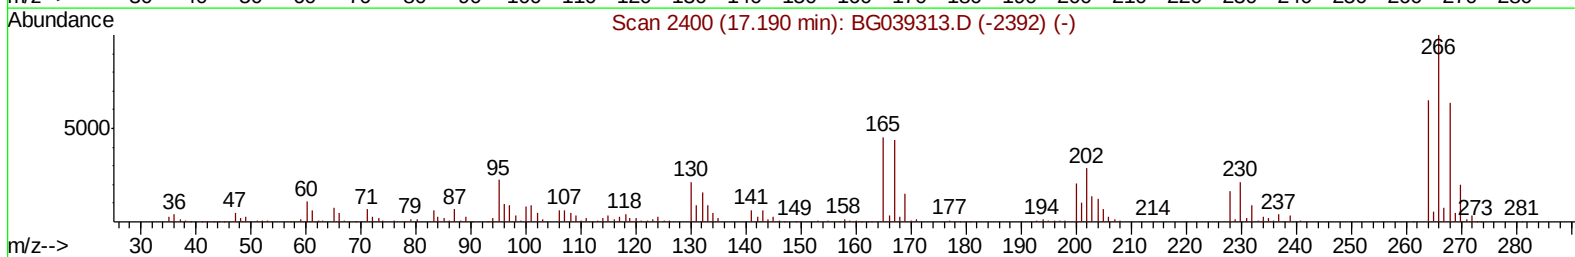
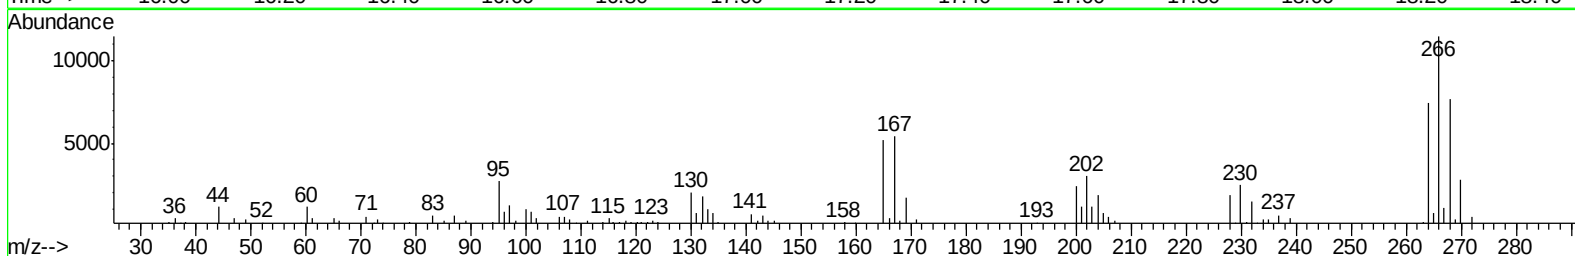


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG022719\
Data File : BG039648.D
Acq On : 28 Feb 2019 00:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 08:24:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

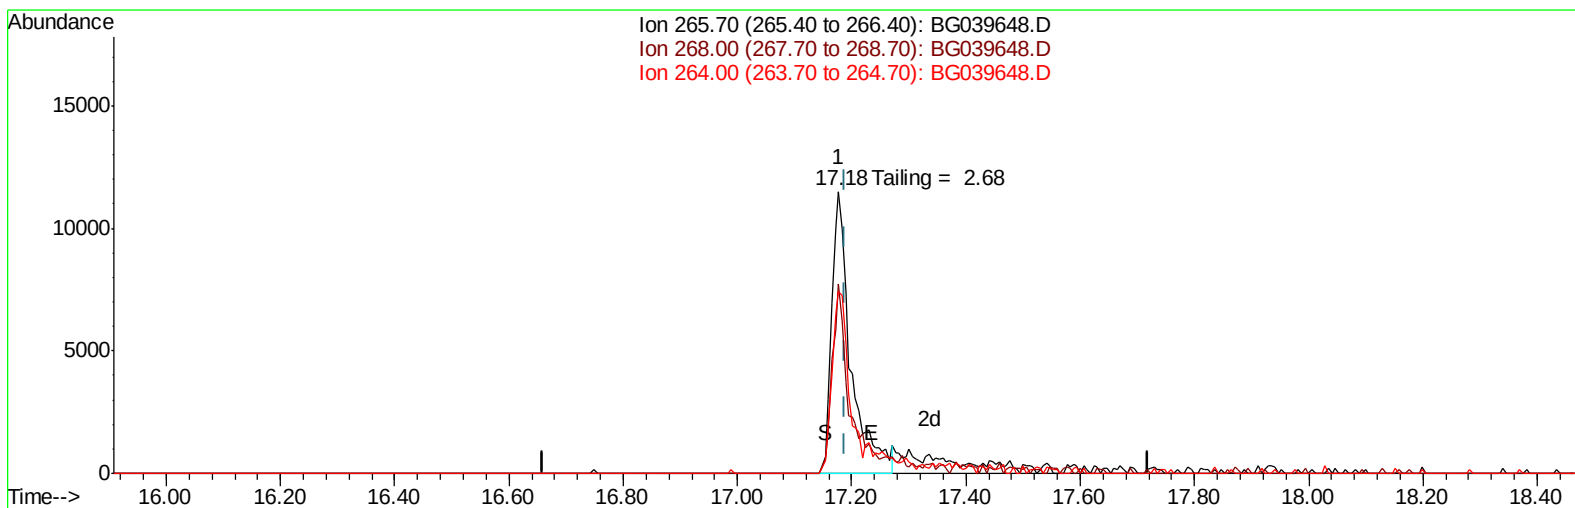

TIC: BG039648.D

(70) Pentachlorophenol (C)




17.177min (-0.013) 9694.32ng

response 26248

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.23
264.00	65.10	64.60
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG022719\
 Data File : BG039648.D
 Acq On : 28 Feb 2019 00:34
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 08:24:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

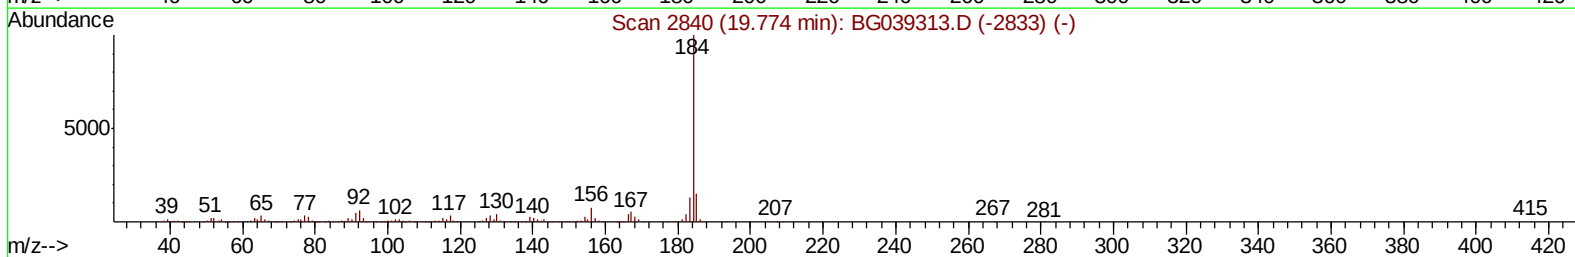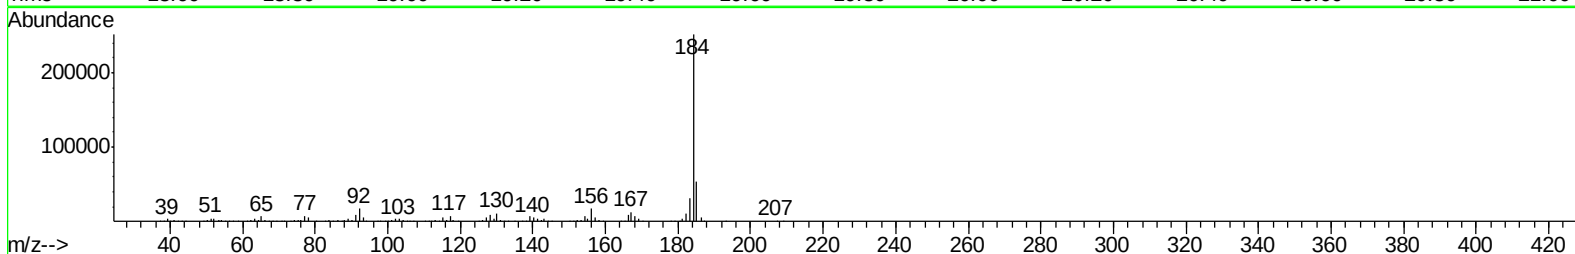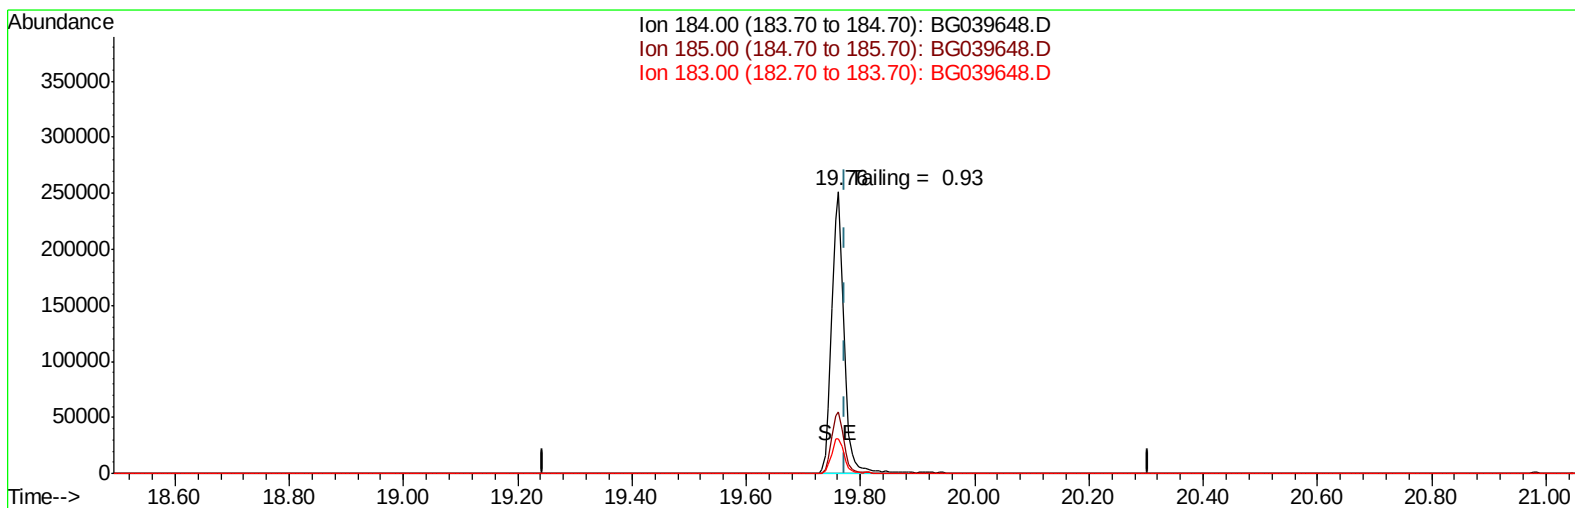

TIC: BG039648.D

(77) Benzidine




19.762min (-0.013) 0.00ng

response 370984

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	21.62#
183.00	13.20	12.45
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG022719\
Data File : BG039648.D
Acq On : 28 Feb 2019 00:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 08:24:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

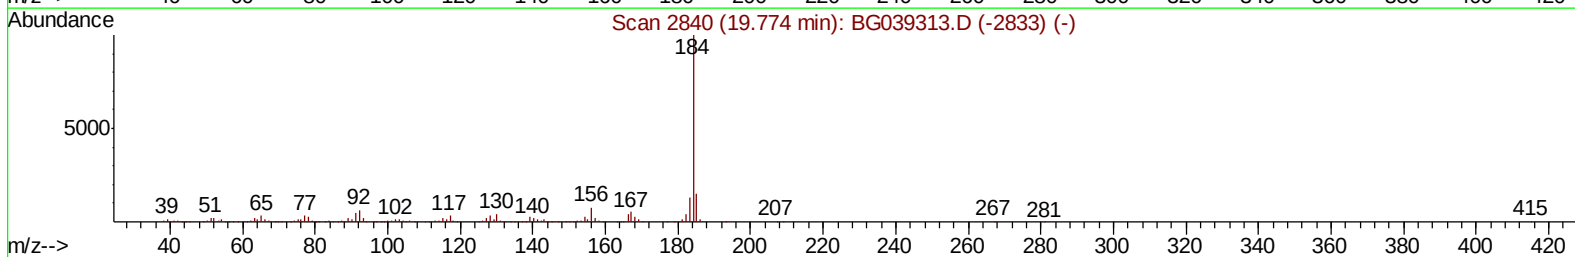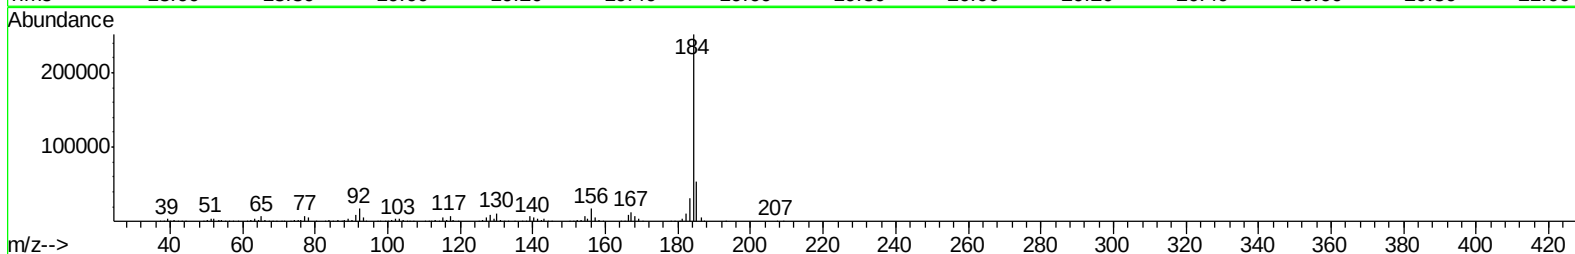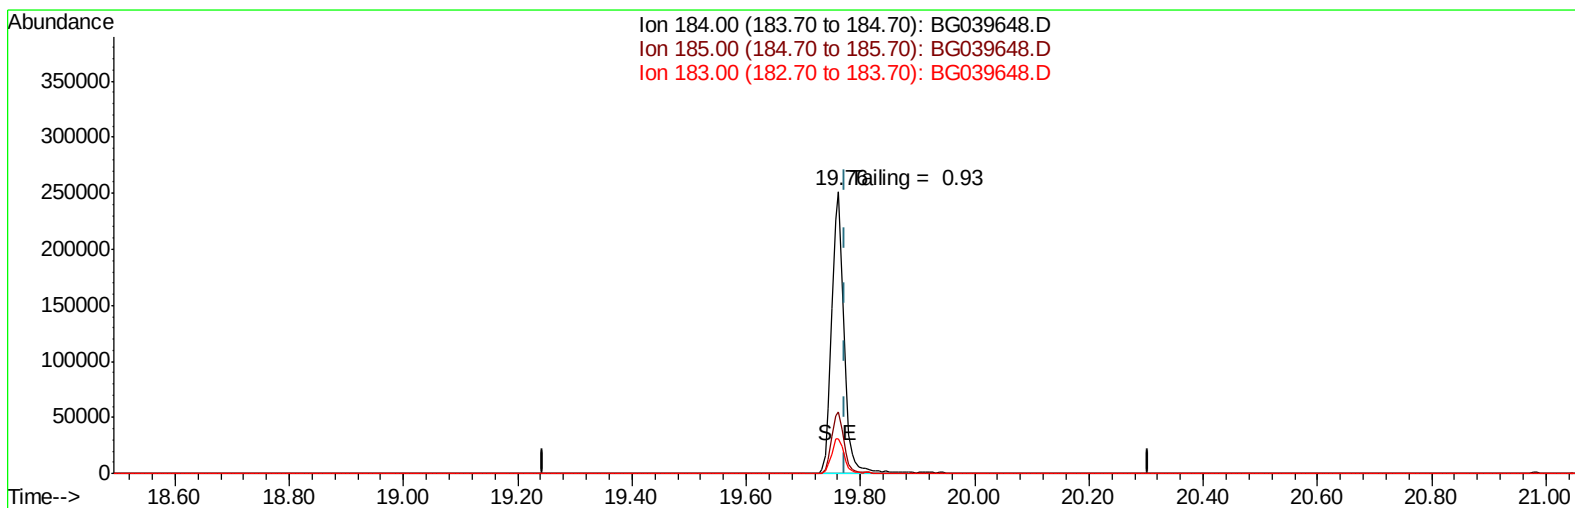

TIC: BG039648.D

(77) Benzidine

19.762min (-0.013) 0.00ng

response 370984

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	21.62#
183.00	13.20	12.45
0.00	0.00	0.00