

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022719\
 Data File : BG039654.D
 Acq On : 28 Feb 2019 4:33
 Operator : JU/SJ
 Sample : K1353-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PL-02-022619-B

Quant Time: Feb 28 07:56:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	52660	20.00	ng	-0.02
21) Naphthalene-d8	10.99	136	242085	20.00	ng	-0.02
39) Acenaphthene-d10	14.79	164	169085	20.00	ng	-0.02
64) Phenanthrene-d10	17.54	188	412773	20.00	ng	-0.02
76) Chrysene-d12	21.82	240	372620	20.00	ng	-0.02
87) Perylene-d12	25.20	264	365020	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	407702	132.51	ng	0.00
7) Phenol-d6	7.31	99	544740	120.28	ng	0.00
23) Nitrobenzene-d5	9.35	82	407152	105.07	ng	-0.02
42) 2,4,6-Tribromophenol	16.28	330	234857	128.99	ng	-0.01
45) 2-Fluorobiphenyl	13.42	172	985374	83.60	ng	-0.02
79) Terphenyl-d14	20.13	244	1463991	83.16	ng	-0.02


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022719\
Data File : BG039654.D
Acq On : 28 Feb 2019 4:33
Operator : JU/SJ
Sample : K1353-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PL-02-022619-B

Quant Time: Feb 28 07:56:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

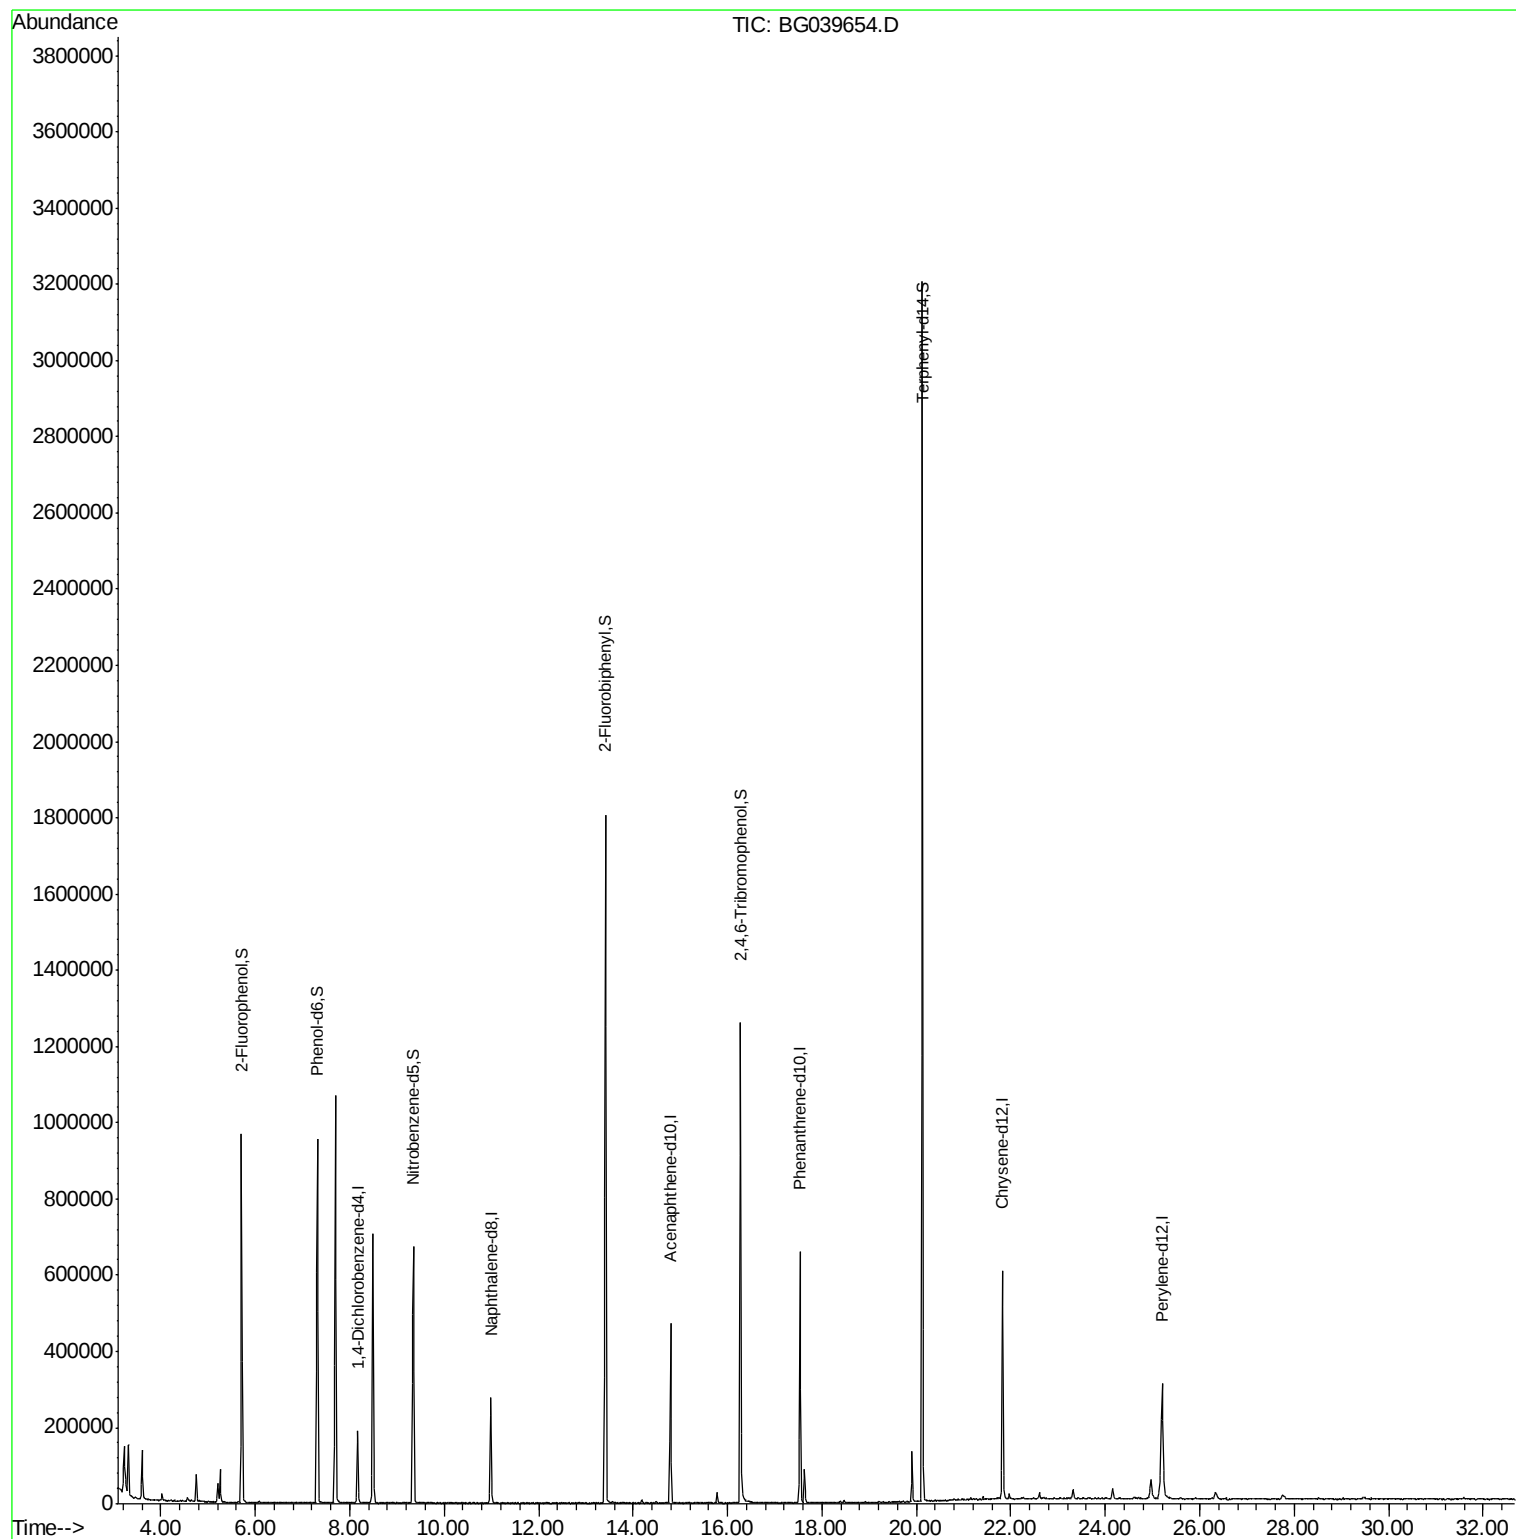




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.17 min Scan# 864
Delta R.T. -0.02 min
Lab File: BG039654.D
Acq: 28 Feb 2019 4:33

Instrument :
BNA_G
ClientSampleId :
PL-02-022619-B

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.5	123.7	185.5
115	56.7	45.9	68.9



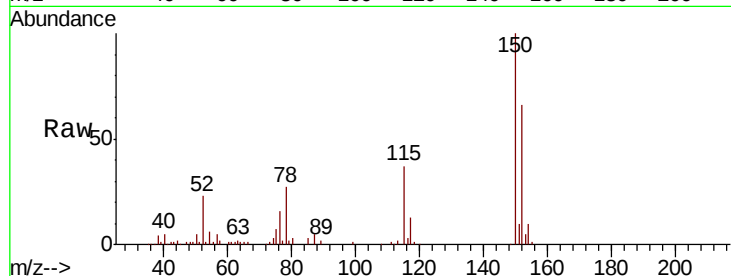


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

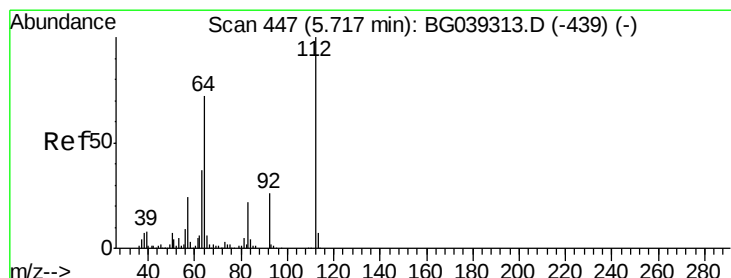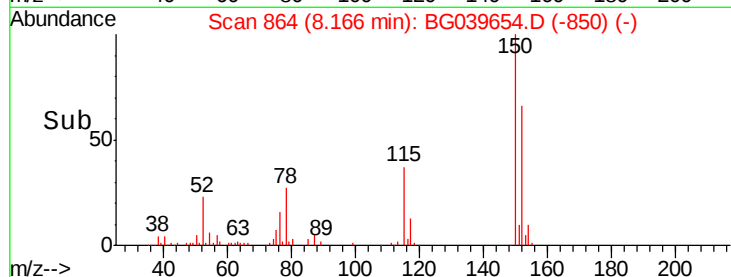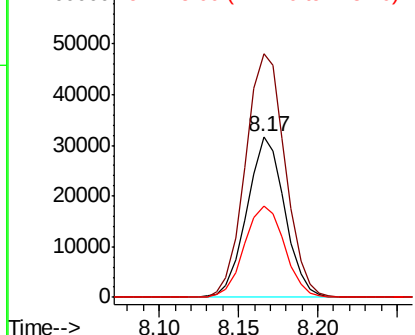

#5

2-Fluorophenol
Concen: 132.508 ng
RT: 5.72 min Scan# 447
Delta R.T. -0.00 min
Lab File: BG039654.D
Acq: 28 Feb 2019 4:33

Tgt Ion	Ratio	Lower	Upper
112	100		
64	68.8	57.8	86.8
63	35.3	29.8	44.6


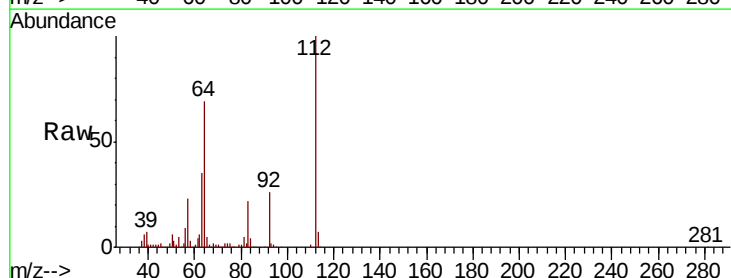


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

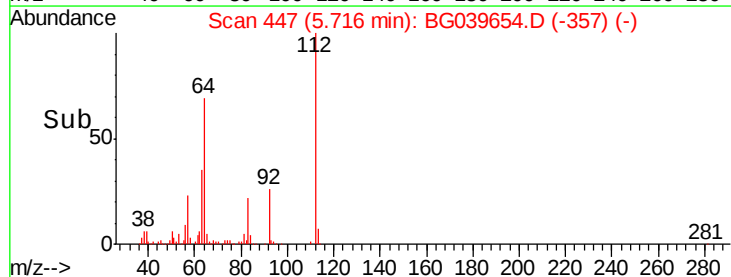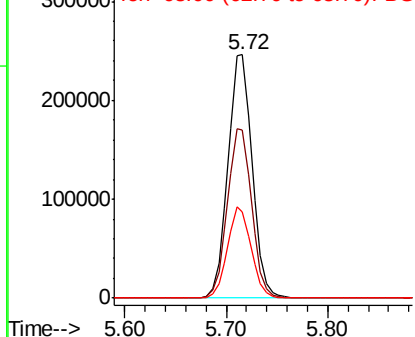



#7

Phenol-d6

Concen: 120.278 ng

RT: 7.31 min Scan# 719

Delta R.T. -0.01 min

Lab File: BG039654.D

Acq: 28 Feb 2019 4:33

Instrument :

BNA_G

ClientSampleId :

PL-02-022619-B


Tot Ion: 99 Resp: 544740

Ion Ratio Lower Upper

99 100

42 20.4 18.2 27.2

71 35.6 28.0 42.0



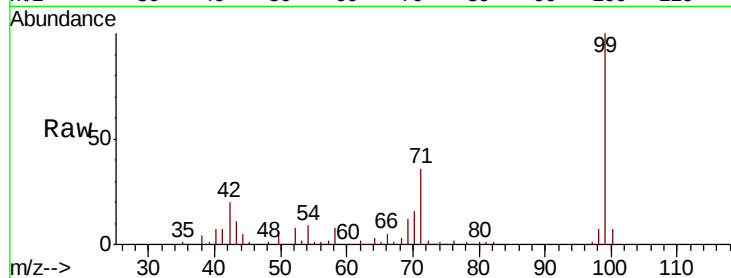


Abundance

Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

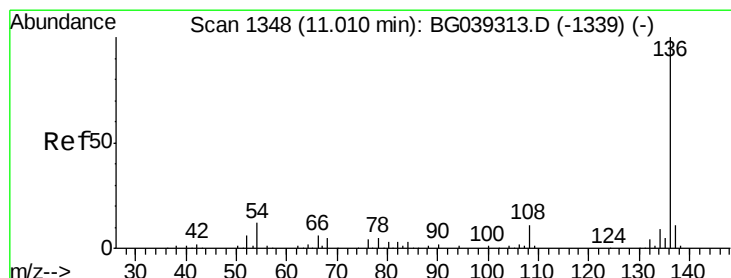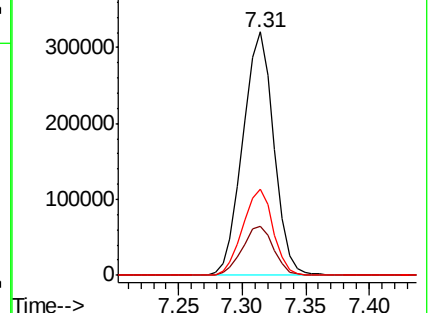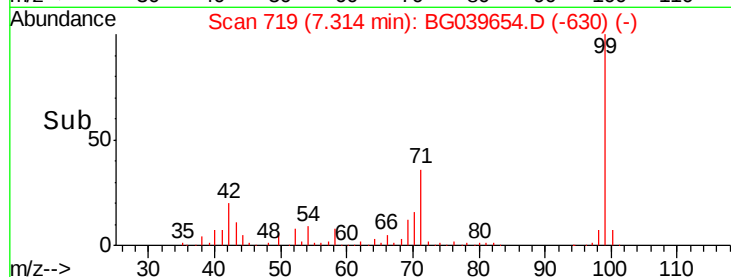

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.99 min Scan# 1344

Delta R.T. -0.02 min

Lab File: BG039654.D

Acq: 28 Feb 2019 4:33

Tgt Ion: 136 Resp: 242085


Ion Ratio Lower Upper

136 100

137 10.8 9.1 13.7

54 10.7 9.4 14.2

68 5.9 4.2 6.4

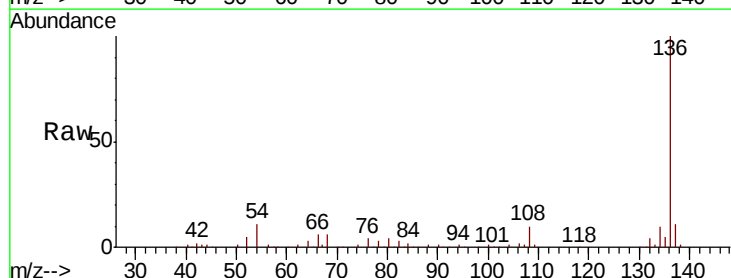



Abundance

Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC

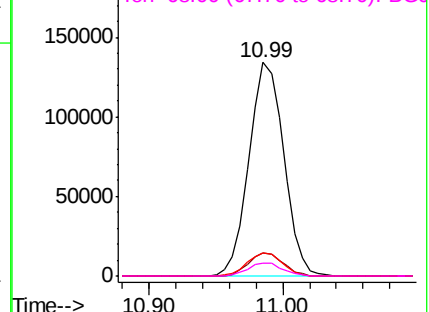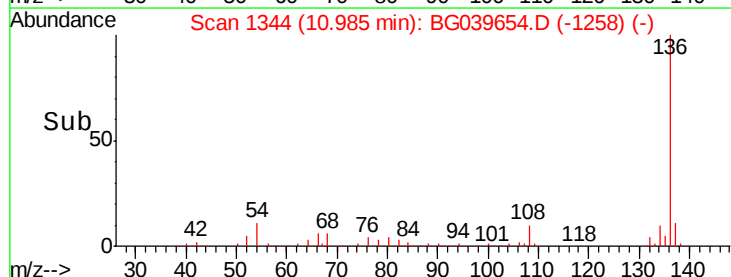




#23
Nitrobenzene-d5
Concen: 105.068 ng
RT: 9.35 min Scan# 1065
Delta R.T. -0.02 min
Lab File: BG039654.D
Acq: 28 Feb 2019 4:33

Instrument :
BNA_G
ClientSampleId :
PL-02-022619-B

Tot Ion	Ratio	Lower	Upper
82	100		
128	43.7	31.3	46.9
54	59.9	50.9	76.3



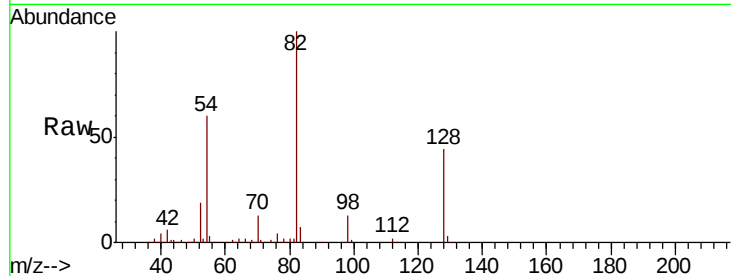


Abundance

Ion 82.00 (81.70 to 82.70): BGC


Ion 128.00 (127.70 to 128.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

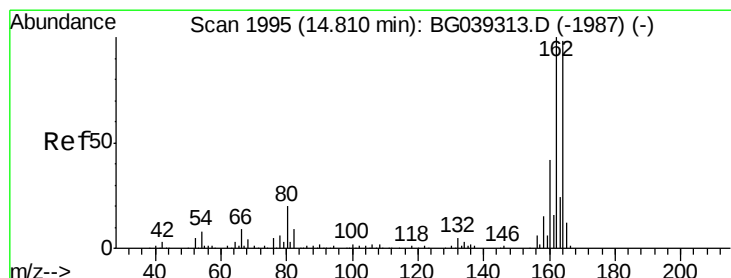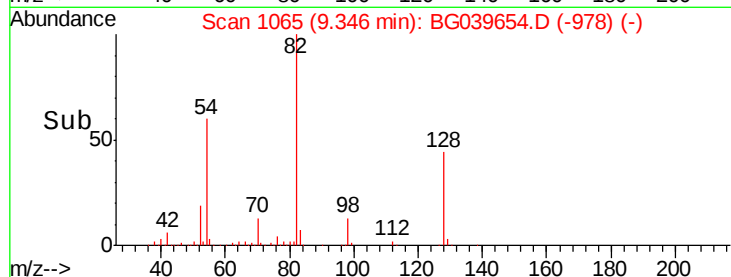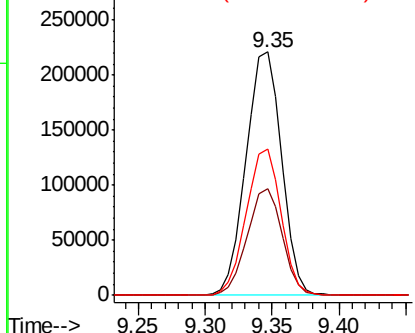

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.79 min Scan# 1992
Delta R.T. -0.02 min
Lab File: BG039654.D
Acq: 28 Feb 2019 4:33

Tgt Ion	Ratio	Lower	Upper
164	100		
162	101.8	81.6	122.4
160	42.8	34.2	51.2


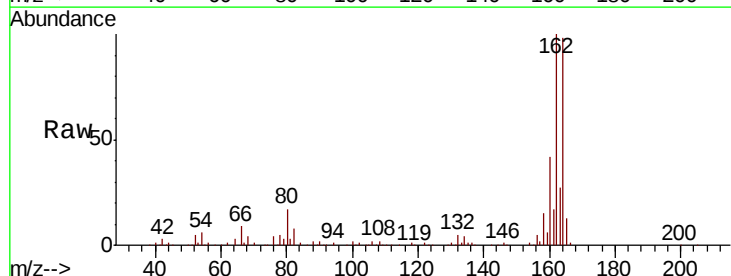


Abundance

Ion 164.00 (163.70 to 164.70): BGC

Ion 162.00 (161.70 to 162.70): BGC

Ion 160.00 (159.70 to 160.70): BGC

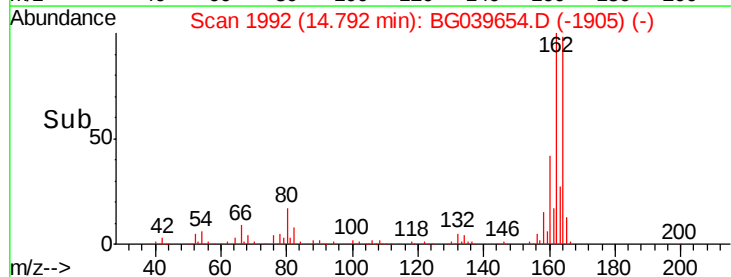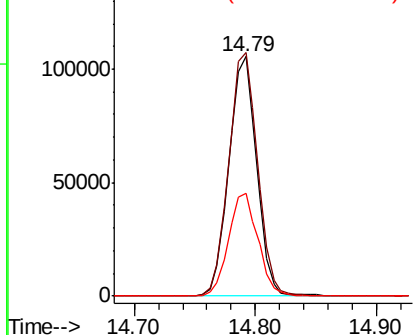



#42

2,4,6-Tribromophenol

Concen: 128.989 ng

RT: 16.28 min Scan# 2245

Delta R.T. -0.01 min

Lab File: BG039654.D

Acq: 28 Feb 2019 4:33

Instrument :

BNA_G

ClientSampleId :

PL-02-022619-B


Tot Ion:330 Resp: 234857

Ion Ratio Lower Upper

330 100

332 95.1 75.7 113.5




141 42.2 35.6 53.4

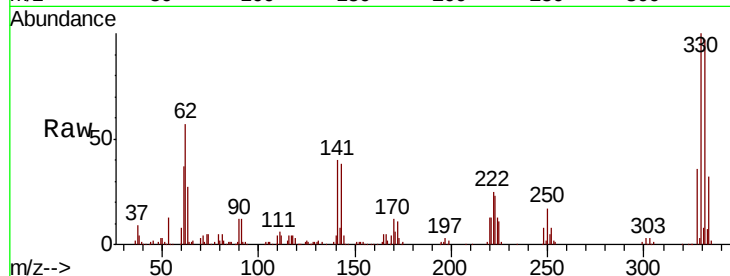

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

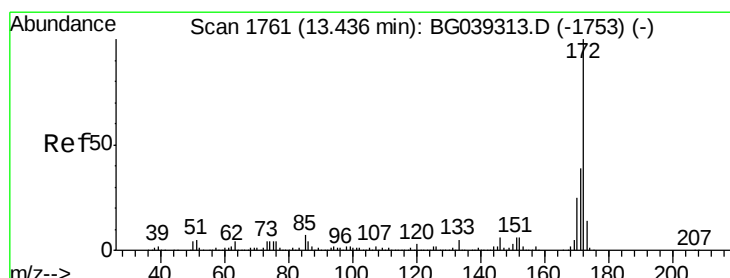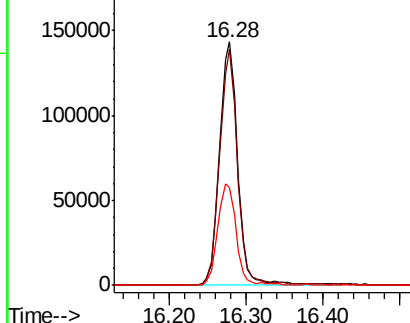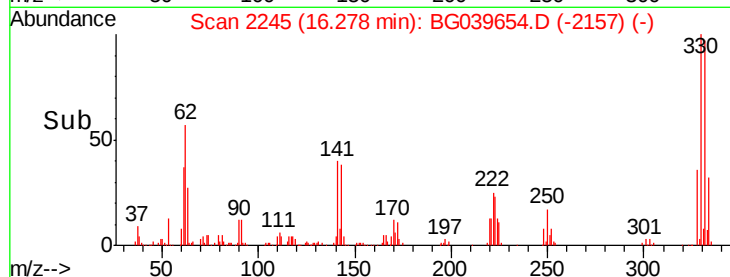

#45

2-Fluorobiphenyl

Concen: 83.601 ng

RT: 13.42 min Scan# 1758

Delta R.T. -0.02 min

Lab File: BG039654.D

Acq: 28 Feb 2019 4:33


Tgt Ion:172 Resp: 985374

Ion Ratio Lower Upper

172 100

171 38.3 30.8 46.2



170 25.4 20.2 30.4

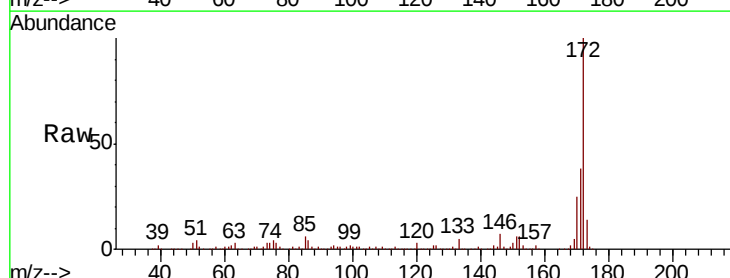

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

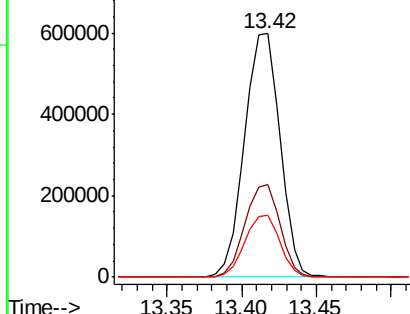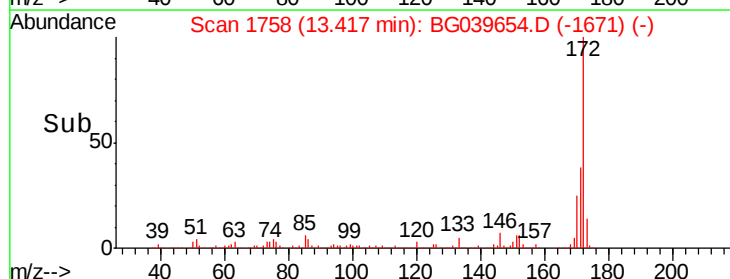



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.54 min Scan# 2459

Delta R.T. -0.02 min

Lab File: BG039654.D

Acq: 28 Feb 2019 4:33

Instrument :

BNA_G

ClientSampleId :

PL-02-022619-B


Tot Ion:188 Resp: 412773

Ion Ratio Lower Upper

188 100

94 8.1 6.9 10.3




80 9.1 8.1 12.1

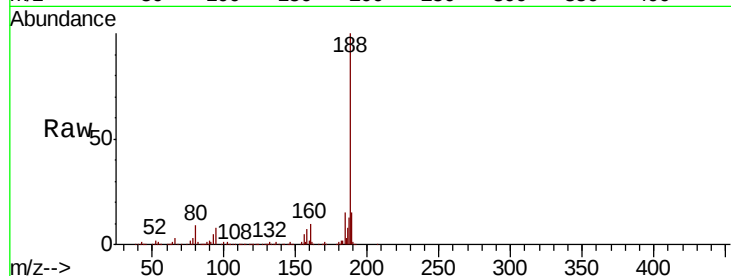

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

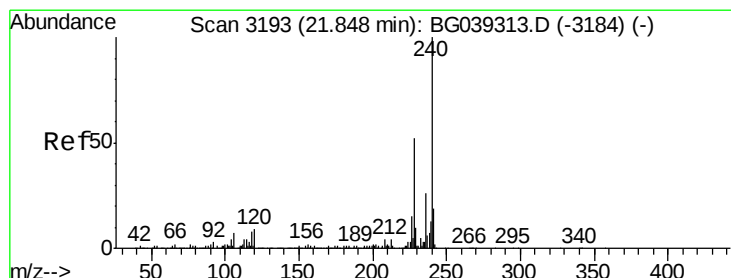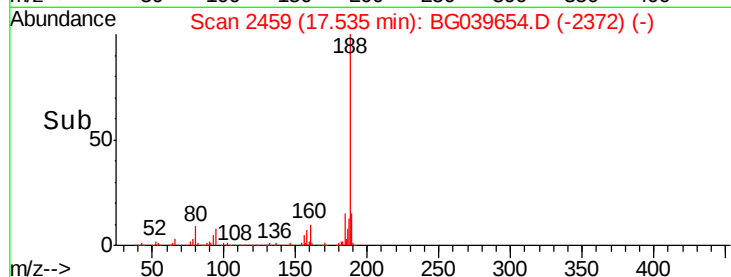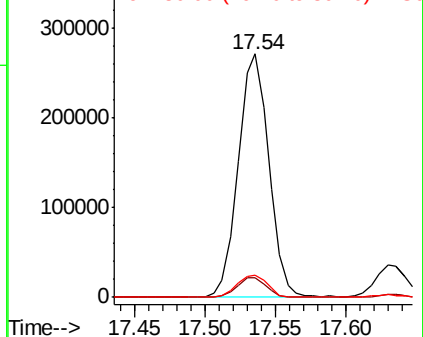

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.82 min Scan# 3189

Delta R.T. -0.02 min

Lab File: BG039654.D

Acq: 28 Feb 2019 4:33


Tgt Ion:240 Resp: 372620

Ion Ratio Lower Upper

240 100

120 9.7 7.0 10.6



236 25.5 21.0 31.4

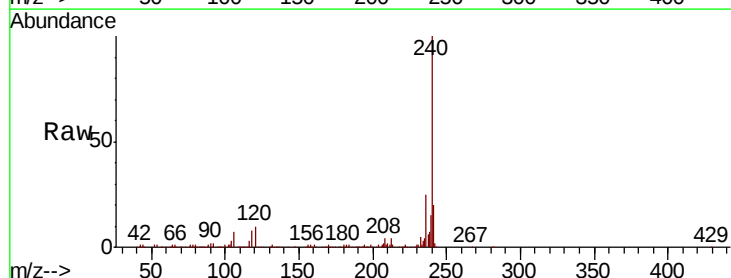

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

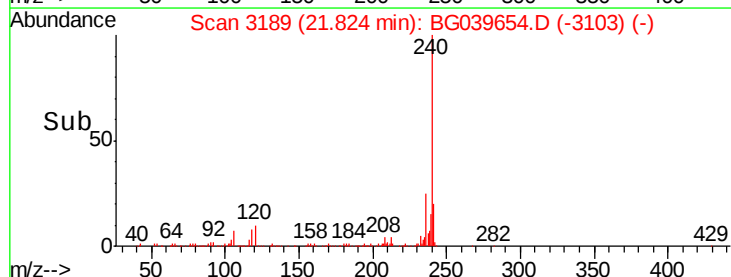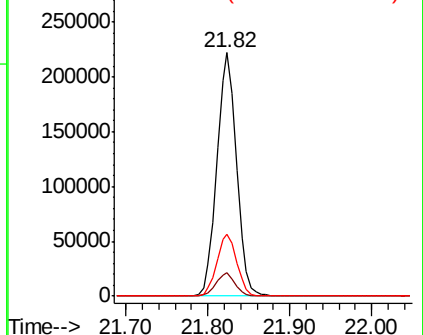



#79

Terphenyl-d14

Concen: 83.163 ng

RT: 20.13 min Scan# 2900

Delta R.T. -0.02 min

Lab File: BG039654.D

Acq: 28 Feb 2019 4:33

Instrument :

BNA_G

ClientSampleId :

PL-02-022619-B


Tot Ion:244 Resp: 1463991

Ion Ratio Lower Upper

244 100

212 9.3 7.3 10.9



122 10.2 8.4 12.6

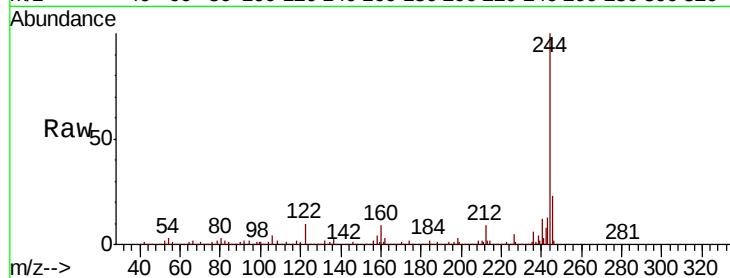

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

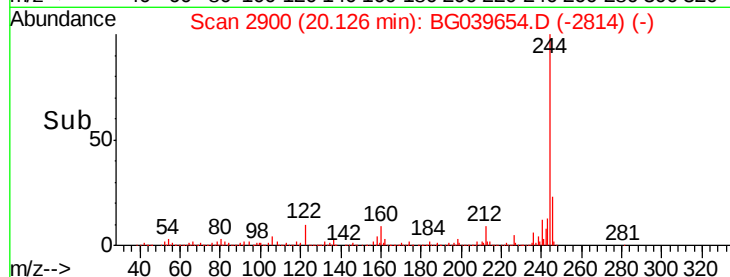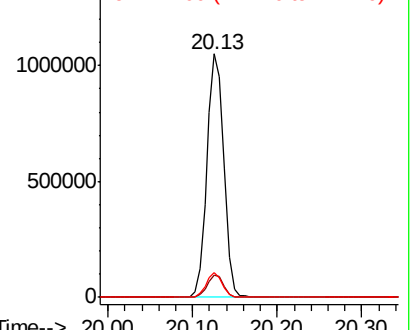

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.20 min Scan# 3764

Delta R.T. -0.04 min

Lab File: BG039654.D

Acq: 28 Feb 2019 4:33


Tgt Ion:264 Resp: 365020

Ion Ratio Lower Upper

264 100

260 25.3 18.2 27.4

265 22.6 18.5 27.7

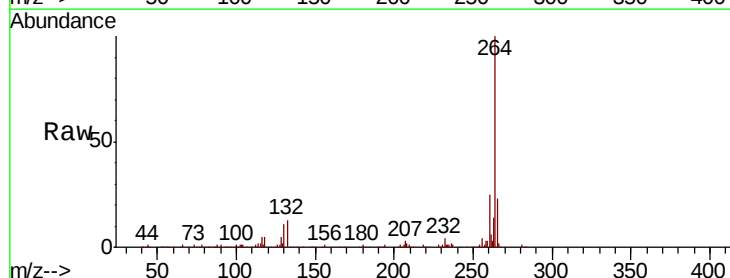

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

