

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022719\
 Data File : BG039656.D
 Acq On : 28 Feb 2019 5:51
 Operator : JU/SJ
 Sample : K1353-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PL-02-022619-D

Quant Time: Feb 28 07:58:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	50484	20.00	ng	-0.02
21) Naphthalene-d8	10.99	136	229391	20.00	ng	-0.02
39) Acenaphthene-d10	14.79	164	169237	20.00	ng	-0.02
64) Phenanthrene-d10	17.53	188	425958	20.00	ng	-0.02
76) Chrysene-d12	21.82	240	380181	20.00	ng	-0.03
87) Perylene-d12	25.20	264	374064	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.71	112	425952	144.41	ng	0.00
7) Phenol-d6	7.31	99	583601	134.41	ng	0.00
23) Nitrobenzene-d5	9.34	82	407059	110.86	ng	-0.02
42) 2,4,6-Tribromophenol	16.28	330	263077	144.36	ng	-0.01
45) 2-Fluorobiphenyl	13.42	172	1039839	88.14	ng	-0.02
79) Terphenyl-d14	20.12	244	1585945	88.30	ng	-0.03


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022719\
Data File : BG039656.D
Acq On : 28 Feb 2019 5:51
Operator : JU/SJ
Sample : K1353-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PL-02-022619-D

Quant Time: Feb 28 07:58:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

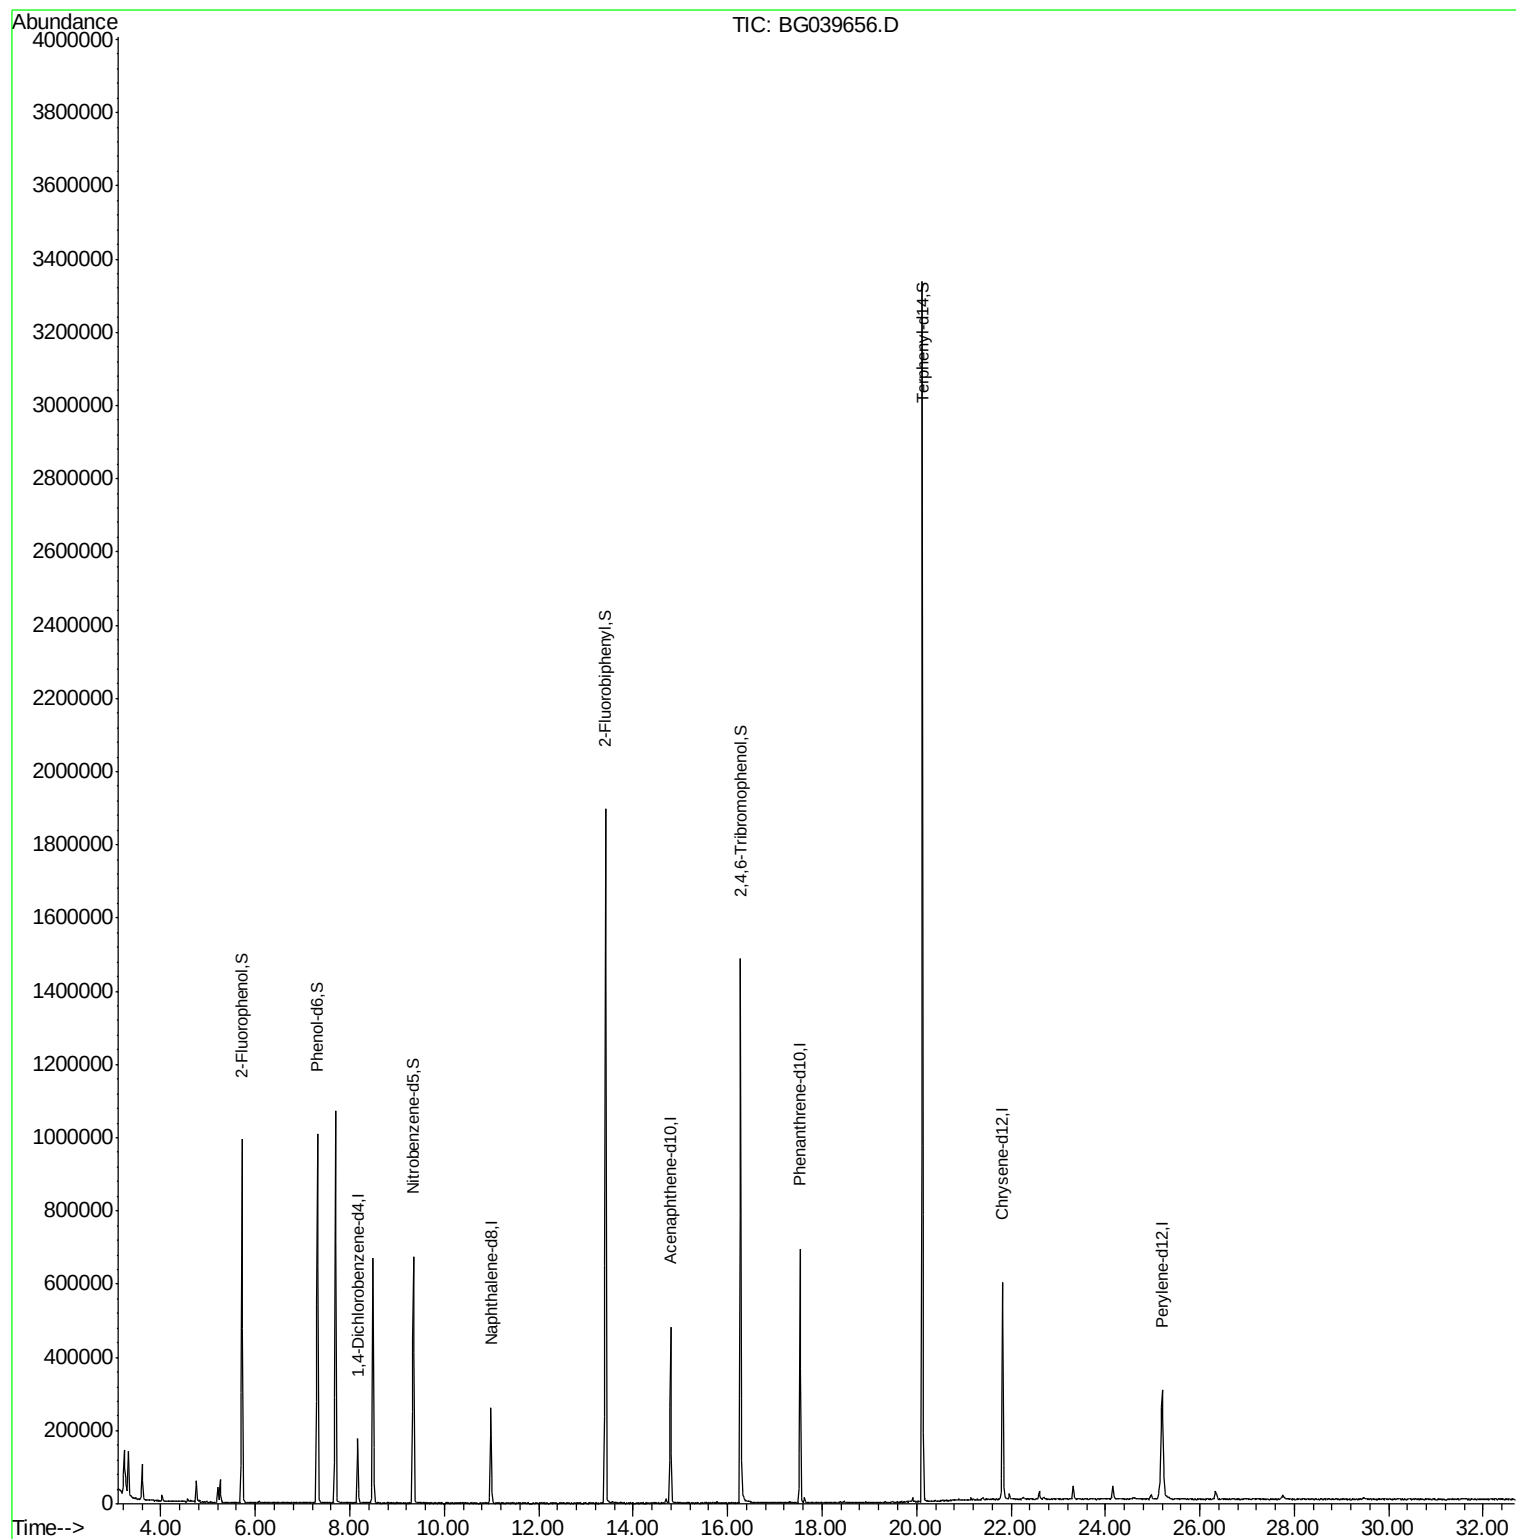




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.16 min Scan# 864
Delta R.T. -0.02 min
Lab File: BG039656.D
Acq: 28 Feb 2019 5:51

Instrument :
BNA_G
ClientSampleId :
PL-02-022619-D

Tot Ion:152 Resp: 50484
Ion Ratio Lower Upper
152 100
150 149.9 123.7 185.5
115 59.8 45.9 68.9

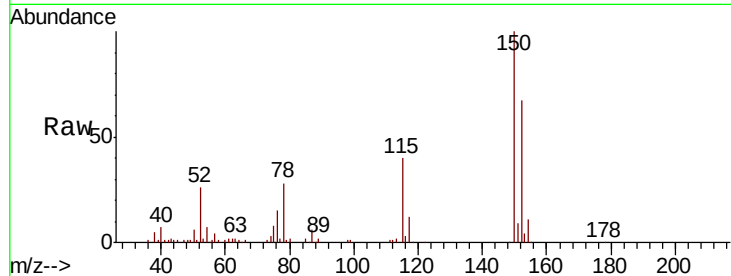


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

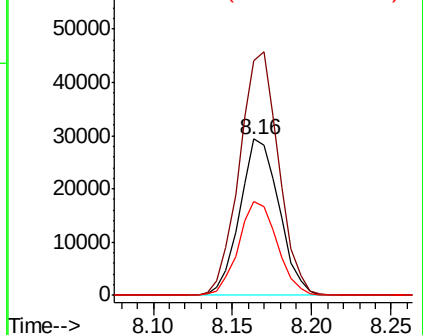



#5


2-Fluorophenol
Concen: 144.406 ng
RT: 5.71 min Scan# 447
Delta R.T. -0.00 min
Lab File: BG039656.D
Acq: 28 Feb 2019 5:51

Tgt Ion:112 Resp: 425952
Ion Ratio Lower Upper
112 100
64 65.8 57.8 86.8
63 36.1 29.8 44.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

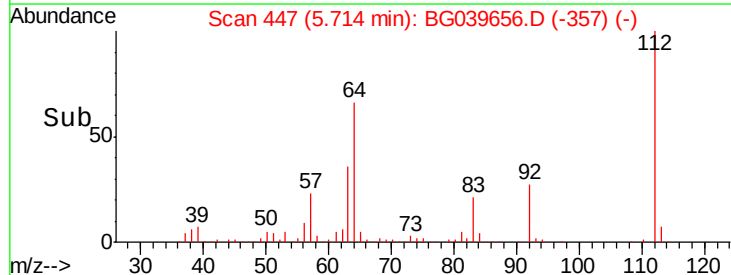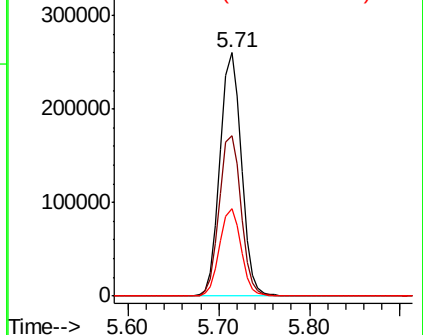

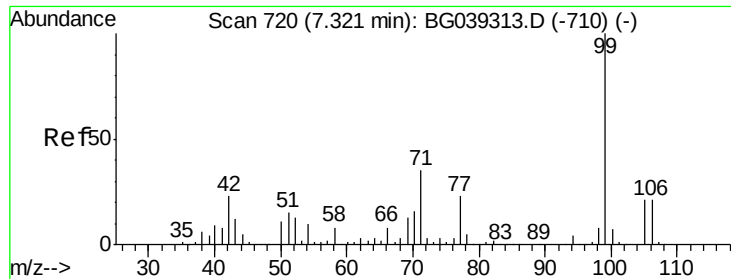

#7

Phenol-d6

Concen: 134.413 ng

RT: 7.31 min Scan# 719

Delta R.T. -0.01 min

Lab File: BG039656.D

Acq: 28 Feb 2019 5:51

Instrument :

BNA_G

ClientSampleId :

PL-02-022619-D


Tot Ion: 99 Resp: 583601

Ion Ratio Lower Upper




99 100

42 20.2 18.2 27.2

71 35.2 28.0 42.0

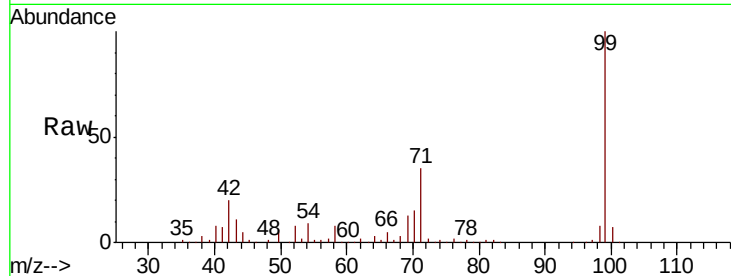

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

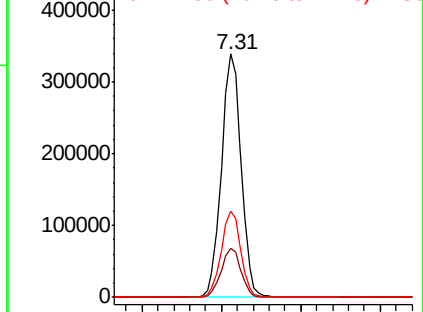

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.99 min Scan# 1345

Delta R.T. -0.02 min

Lab File: BG039656.D

Acq: 28 Feb 2019 5:51

Tgt Ion: 136 Resp: 229391


Ion Ratio Lower Upper

136 100



137 12.1 9.1 13.7


54 9.6 9.4 14.2

68 5.7 4.2 6.4



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




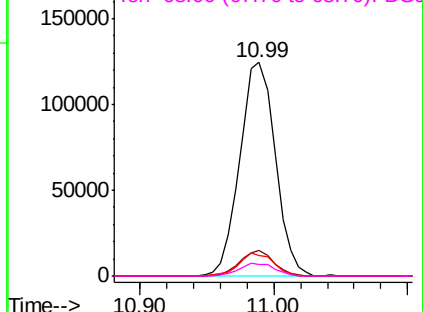




#23
 Nitrobenzene-d5
 Concen: 110.857 ng
 RT: 9.34 min Scan# 1065
 Delta R.T. -0.02 min
 Lab File: BG039656.D
 Acq: 28 Feb 2019 5:51




Instrument :
 BNA_G
 ClientSampleId :
 PL-02-022619-D


Tot Ion	82	Resp	407059
Ion Ratio	100	Lower	Upper
128	44.4	31.3	46.9
54	60.3	50.9	76.3

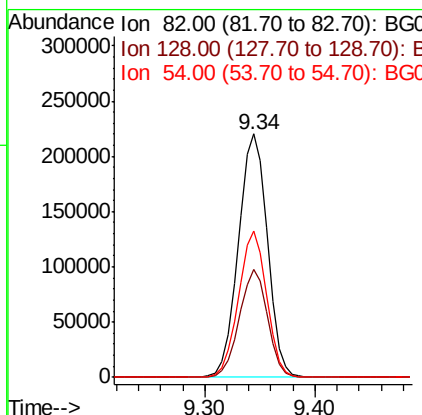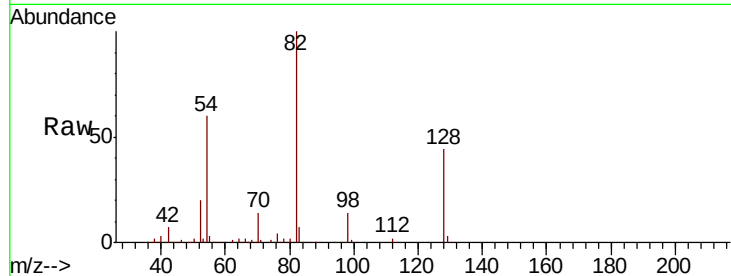

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.79 min Scan# 1992
 Delta R.T. -0.02 min
 Lab File: BG039656.D
 Acq: 28 Feb 2019 5:51

Tgt Ion	164	Resp	169237
Ion Ratio	100	Lower	Upper
162	102.7	81.6	122.4
160	45.5	34.2	51.2

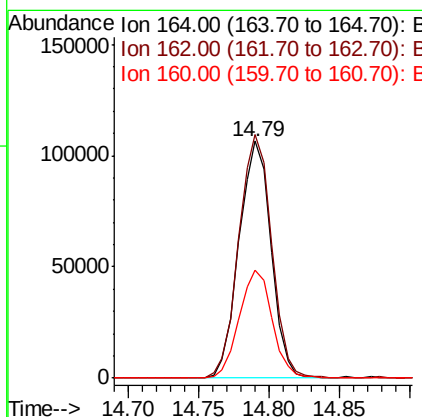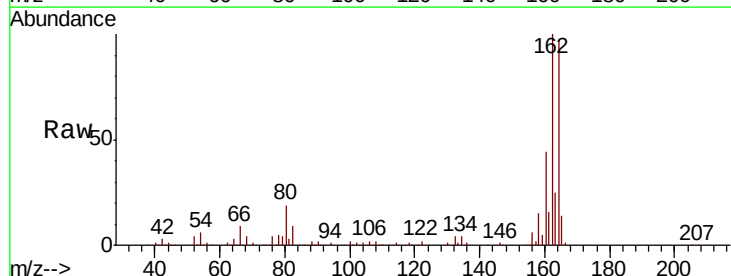







#42
 2,4,6-Tribromophenol
 Concen: 144.358 ng
 RT: 16.28 min Scan# 2245
 Delta R.T. -0.01 min
 Lab File: BG039656.D
 Acq: 28 Feb 2019 5:51

Instrument :
 BNA_G
 ClientSampleId :
 PL-02-022619-D

Tot Ion:330 Resp: 263077
 Ion Ratio Lower Upper
 330 100
 332 95.6 75.7 113.5
 141 41.4 35.6 53.4




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


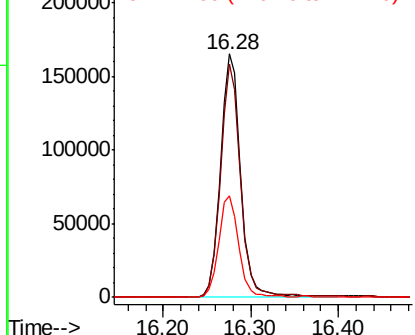



#45
 2-Fluorobiphenyl
 Concen: 88.143 ng
 RT: 13.42 min Scan# 1758
 Delta R.T. -0.02 min
 Lab File: BG039656.D
 Acq: 28 Feb 2019 5:51

Tgt Ion:172 Resp: 1039839
 Ion Ratio Lower Upper
 172 100
 171 38.4 30.8 46.2
 170 25.0 20.2 30.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

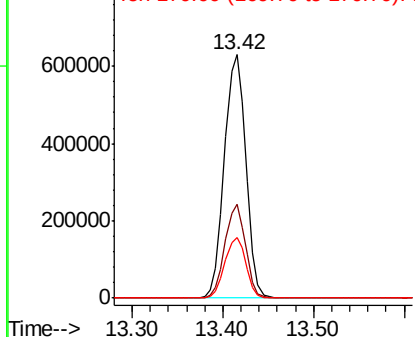



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.53 min Scan# 2459

Delta R.T. -0.02 min

Lab File: BG039656.D

Acq: 28 Feb 2019 5:51

Instrument :

BNA_G

ClientSampleId :

PL-02-022619-D


Tot Ion:188 Resp: 425958

Ion Ratio Lower Upper

188 100

94 8.2 6.9 10.3




80 8.5 8.1 12.1

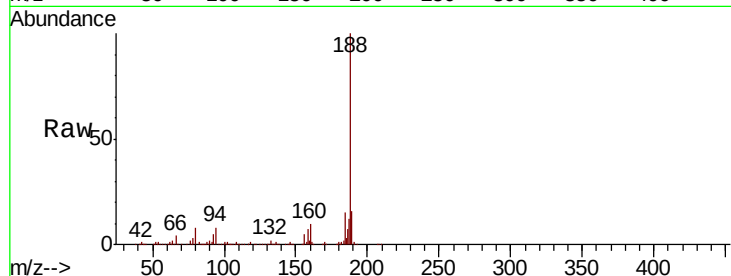

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

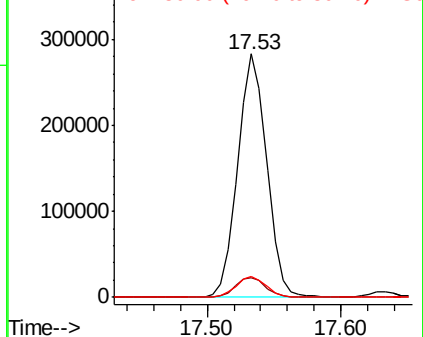

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.82 min Scan# 3189

Delta R.T. -0.03 min

Lab File: BG039656.D

Acq: 28 Feb 2019 5:51


Tgt Ion:240 Resp: 380181

Ion Ratio Lower Upper

240 100

120 8.7 7.0 10.6



236 26.1 21.0 31.4




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

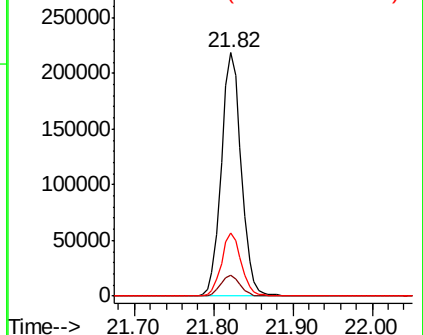

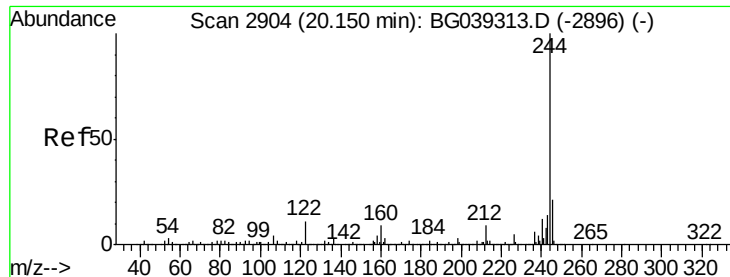

#79

Terphenyl-d14

Concen: 88.299 ng

RT: 20.12 min Scan# 2900

Delta R.T. -0.03 min

Lab File: BG039656.D

Acq: 28 Feb 2019 5:51

Instrument :

BNA_G

ClientSampleId :

PL-02-022619-D


Tot Ion:244 Resp: 1585945

Ion Ratio Lower Upper

244 100

212 9.7 7.3 10.9




122 10.7 8.4 12.6

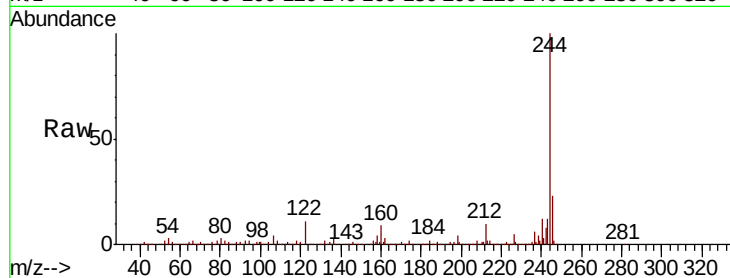

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

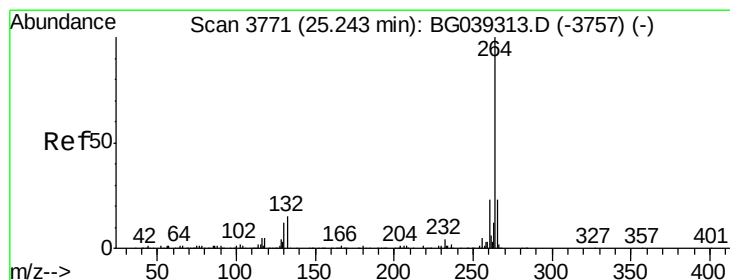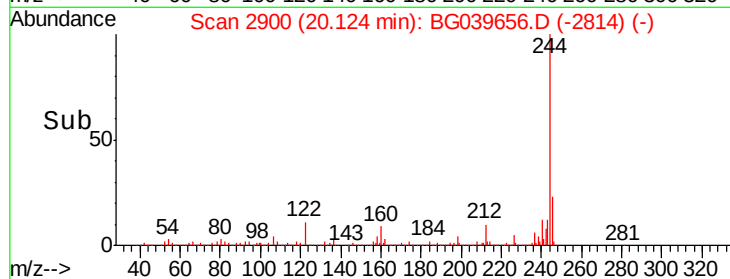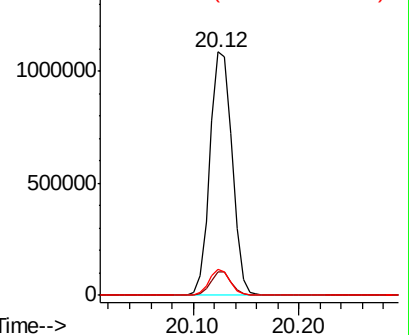

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.20 min Scan# 3764

Delta R.T. -0.04 min

Lab File: BG039656.D

Acq: 28 Feb 2019 5:51


Tgt Ion:264 Resp: 374064

Ion Ratio Lower Upper

264 100

260 24.8 18.2 27.4

265 20.7 18.5 27.7

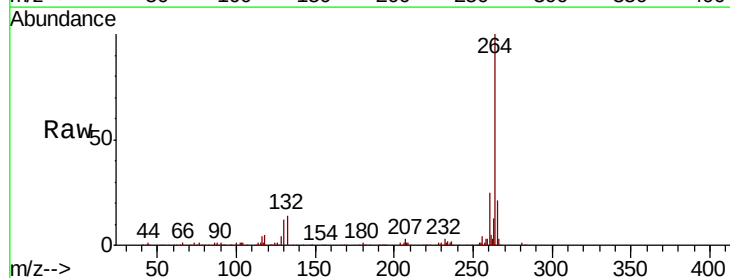

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

