


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022719\
Data File : BG039648.D
Acq On : 28 Feb 2019 00:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 29 15:41:51 2019

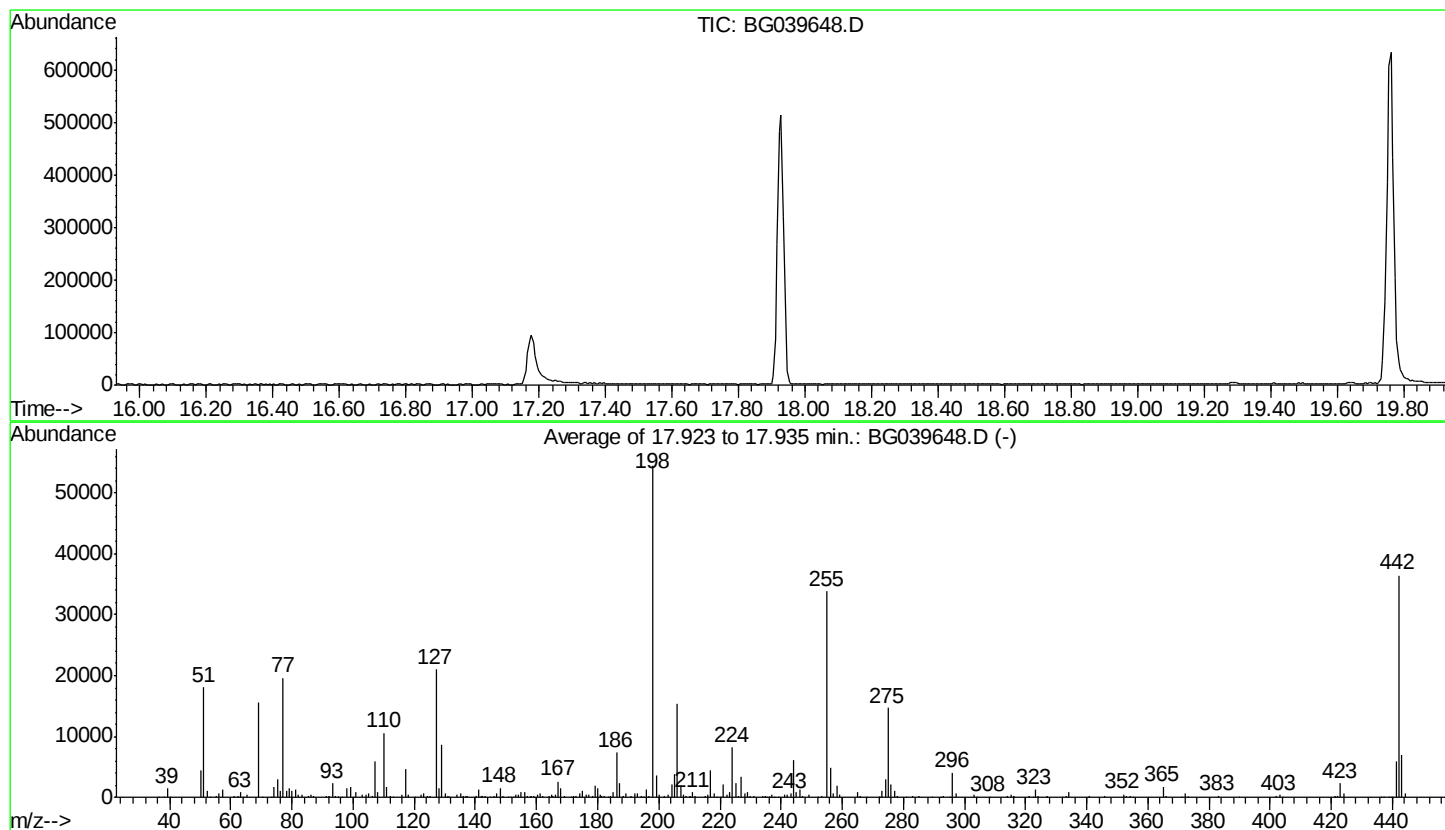

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	18070	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.6	15610	PASS
70	69	0.00	2	0.3	51	PASS
127	198	10	80	38.5	20992	PASS
197	198	0.00	2	0.3	168	PASS
198	198	100	100	100.0	54520	PASS
199	198	5	9	6.7	3656	PASS
275	198	10	60	26.9	14672	PASS
365	198	1	100	3.2	1758	PASS
441	198	0.01	100	11.0	5975	PASS
442	198	50	100	66.9	36469	PASS
443	442	15	24	19.0	6918	PASS