

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022723\
 Data File : BG056740.D
 Acq On : 27 Feb 2023 21:35
 Operator : CG/JU
 Sample : 01648-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZU2

Quant Time: Feb 28 00:32:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 00:23:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.420	152	13907	20.000	ng/ul	0.00
20) Naphthalene-d8	11.258	136	58542	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.024	164	46878	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.756	188	123298	20.000	ng/ul	0.00
79) Chrysene-d12	22.069	240	116256	20.000	ng/ul	0.00
88) Perylene-d12	25.600	264	125460	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.696	96	927	3.698	ng/uL	0.00
4) Pyridine-d5	4.143	84	7113	7.029	ng/ul	0.00
7) Phenol-d5	7.539	99	22988	16.518	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.721	67	13324	15.696	ng/ul	0.00
11) 2-Chlorophenol-d4	7.944	132	15014	16.246	ng/ul	0.00
15) 4-Methylphenol-d8	9.102	113	16661	15.668	ng/ul	0.00
21) Nitrobenzene-d5	9.589	128	8197	16.708	ng/ul	0.00
24) 2-Nitrophenol-d4	10.318	143	9662	16.545	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.858	165	18400	16.724	ng/ul	0.00
31) 4-Chloroaniline-d4	11.381	131	17660	12.307	ng/ul	0.00
46) Dimethylphthalate-d6	14.407	166	67619	17.878	ng/ul	0.00
49) Acenaphthylene-d8	14.724	160	73094	17.004	ng/ul	0.00
54) 4-Nitrophenol-d4	15.171	143	11168	17.126	ng/ul	0.00
60) Fluorene-d10	16.005	176	61843	17.676	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.099	200	12740	15.444	ng/ul	0.00
73) Anthracene-d10	17.856	188	107700	18.005	ng/ul	0.00
81) Pyrene-d10	20.112	212	134741	17.128	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.347	264	125619	18.550	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	9.248	105	4079	2.240	ng/ul	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022723\
Data File : BG056740.D
Acq On : 27 Feb 2023 21:35
Operator : CG/JU
Sample : 01648-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZU2

Quant Time: Feb 28 00:32:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 28 00:23:23 2023
Response via : Initial Calibration

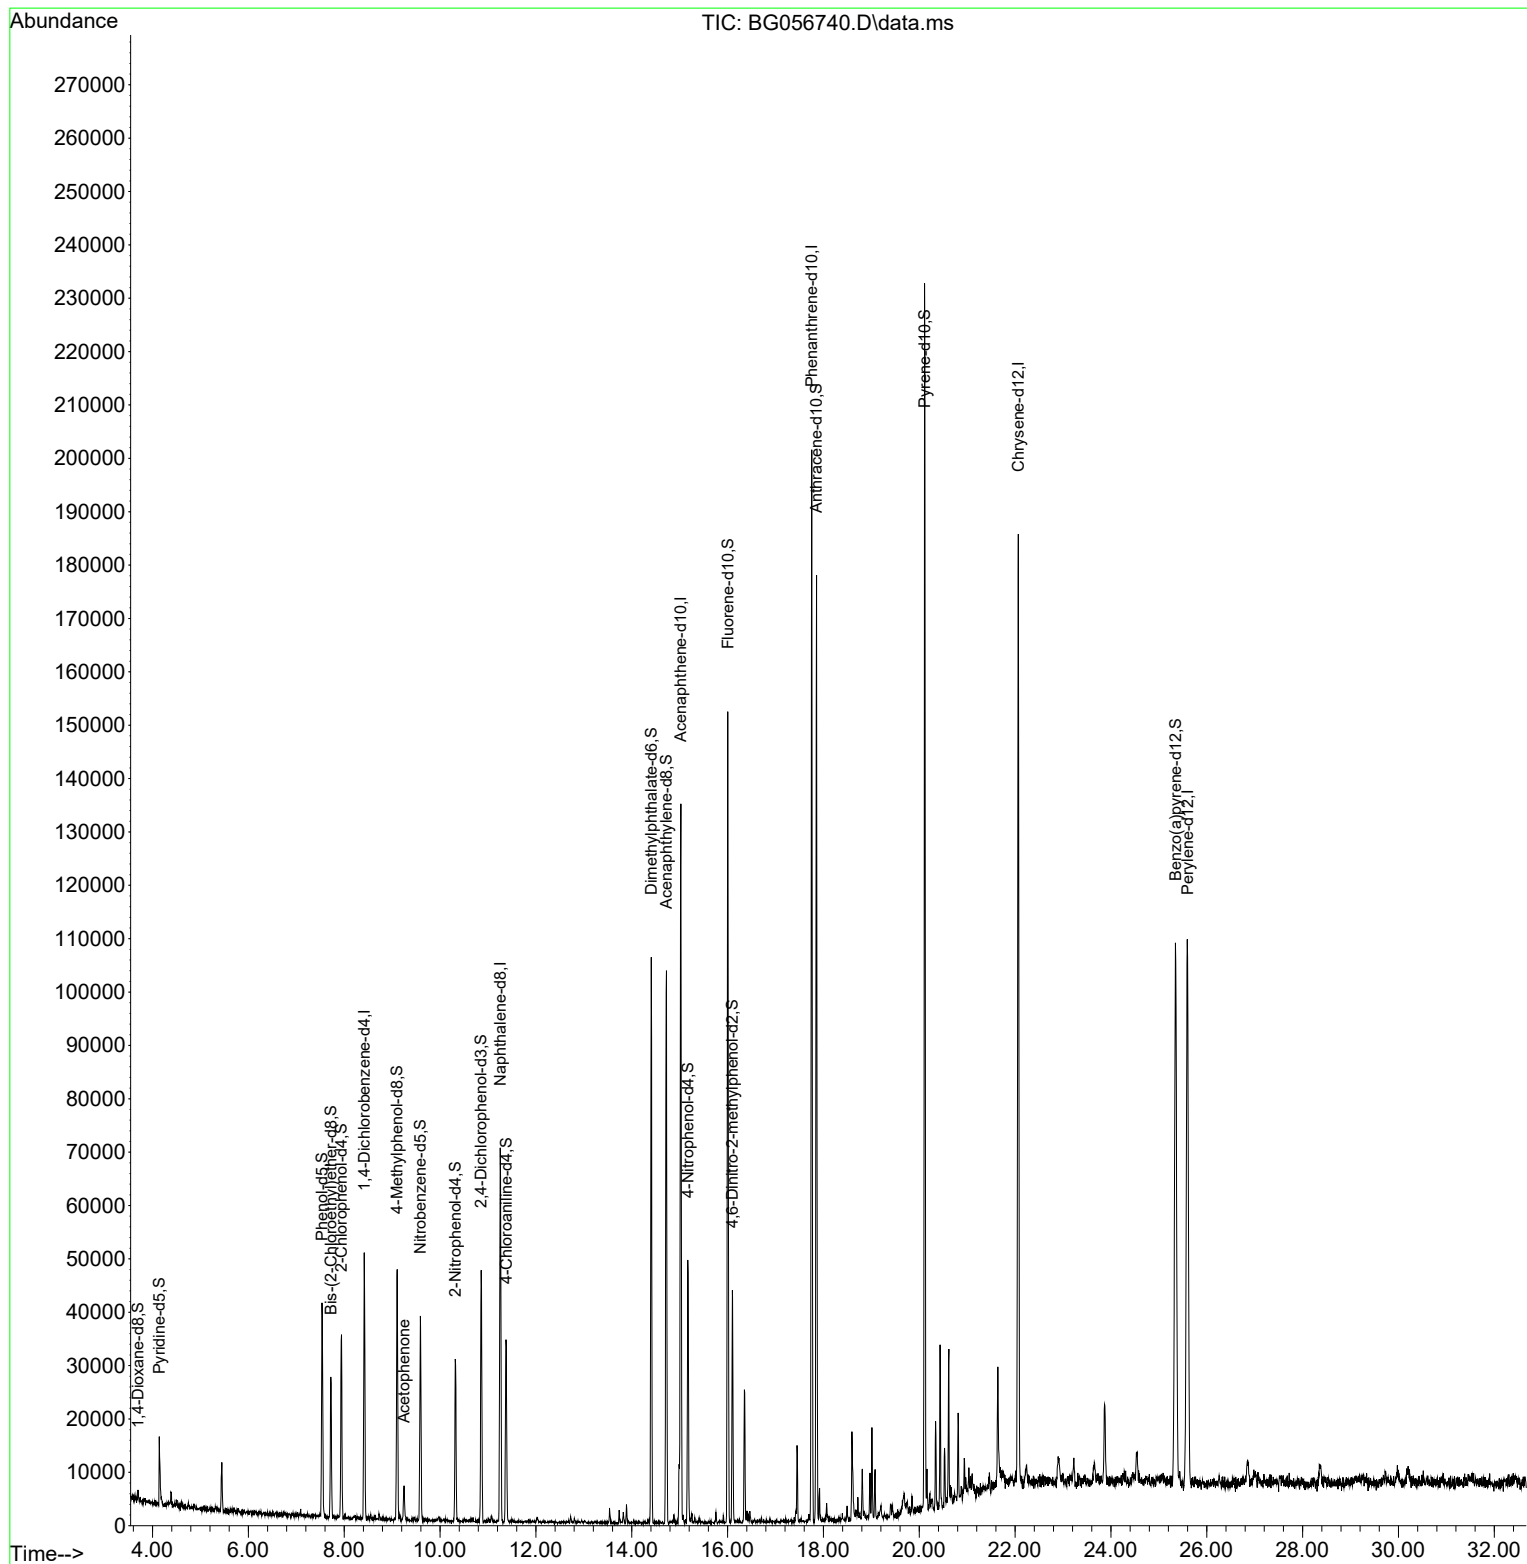

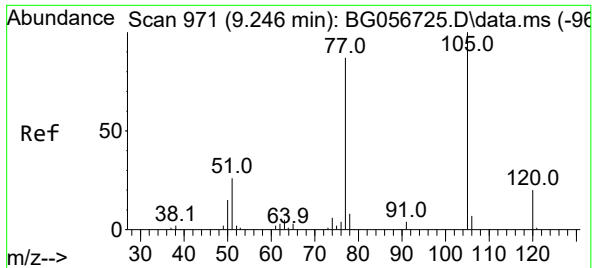

#16
 Acetophenone
 Concen: 2.240 ng/ul
 RT: 9.248 min Scan# 91
 Delta R.T. 0.003 min
 Lab File: BG056740.D
 Acq: 27 Feb 2023 21:35

Instrument :
 BNA_G
 ClientSampleId :
 DBZU2

Tgt Ion:	105	Resp:	4079
Ion	Ratio	Lower	Upper
105	100		
77	97.5	71.4	107.0
51	33.9	23.6	35.4

