

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022723\
 Data File : BG056742.D
 Acq On : 27 Feb 2023 22:57
 Operator : CG/JU
 Sample : 01648-16
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZU4

Quant Time: Feb 28 00:32:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 00:23:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.419	152	16697	20.000	ng/ul	0.00
20) Naphthalene-d8	11.257	136	69875	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	15.023	164	56436	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.755	188	146578	20.000	ng/ul	0.00
79) Chrysene-d12	22.068	240	138666	20.000	ng/ul	0.00
88) Perylene-d12	25.593	264	147219	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.701	96	963	3.199	ng/uL	0.00
4) Pyridine-d5	4.148	84	6770	5.572	ng/ul	0.01
7) Phenol-d5	7.538	99	25907	15.505	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.720	67	15927	15.627	ng/ul	0.00
11) 2-Chlorophenol-d4	7.943	132	16771	15.115	ng/ul	0.00
15) 4-Methylphenol-d8	9.107	113	19570	15.329	ng/ul	0.00
21) Nitrobenzene-d5	9.594	128	9423	16.092	ng/ul	0.00
24) 2-Nitrophenol-d4	10.317	143	11063	15.871	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.858	165	20056	15.273	ng/ul	0.00
31) 4-Chloroaniline-d4	11.381	131	21898	12.785	ng/ul	0.00
46) Dimethylphthalate-d6	14.406	166	78025	17.136	ng/ul	0.00
49) Acenaphthylene-d8	14.724	160	84605	16.348	ng/ul	0.00
54) 4-Nitrophenol-d4	15.176	143	11938	15.207	ng/ul	0.00
60) Fluorene-d10	16.010	176	68523	16.268	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.104	200	12633	12.882	ng/ul	0.00
73) Anthracene-d10	17.855	188	119552	16.812	ng/ul	0.00
81) Pyrene-d10	20.117	212	147162	15.683	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.347	264	136886	17.226	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	9.242	105	3469	1.587	ng/ul	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022723\
Data File : BG056742.D
Acq On : 27 Feb 2023 22:57
Operator : CG/JU
Sample : 01648-16
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZU4

Quant Time: Feb 28 00:32:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 28 00:23:23 2023
Response via : Initial Calibration

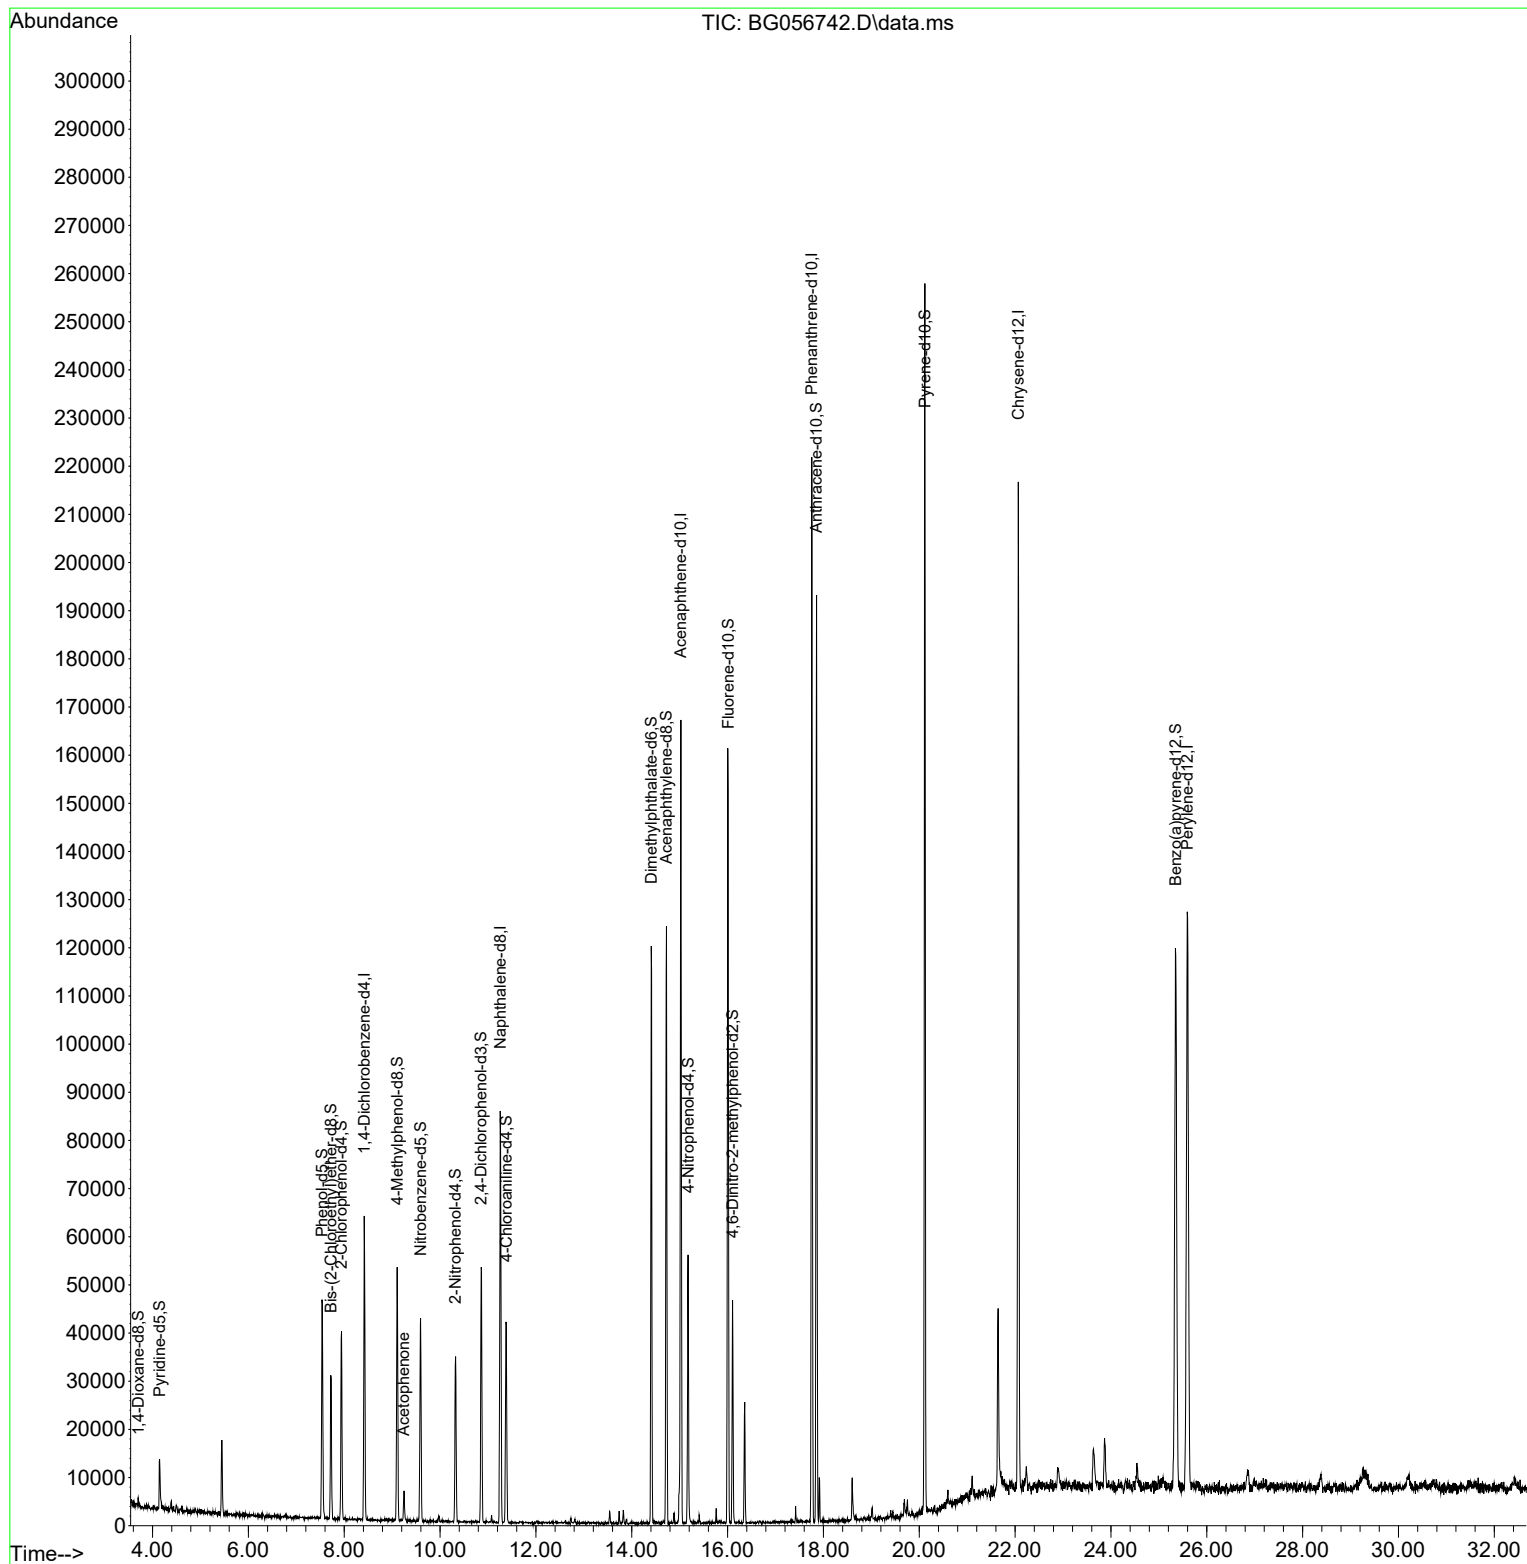

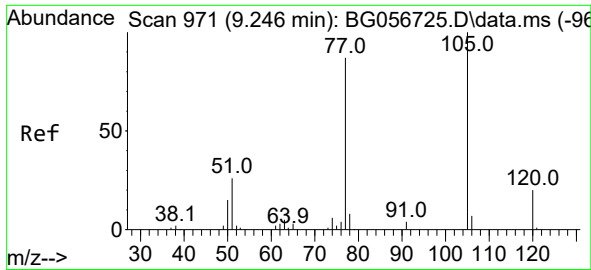

#16
 Acetophenone
 Concen: 1.587 ng/ul
 RT: 9.242 min Scan# 91
 Delta R.T. -0.004 min
 Lab File: BG056742.D
 Acq: 27 Feb 2023 22:57

Instrument :
 BNA_G
 ClientSampleId :
 DBZU4

Tgt Ion:	105	Resp:	3469
Ion	Ratio	Lower	Upper
105	100		
77	81.9	71.4	107.0
51	25.7	23.6	35.4

