




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022723\
Data File : BG056726.D
Acq On : 27 Feb 2023 11:29
Operator : CG/JU
Sample : PB150979BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK979

Manual IntegrationsAPPROVED

Quant Time: Feb 27 12:03:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 23 15:40:42 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/28/2023
Supervised By :Jagrut Upadhyay 02/28/2023

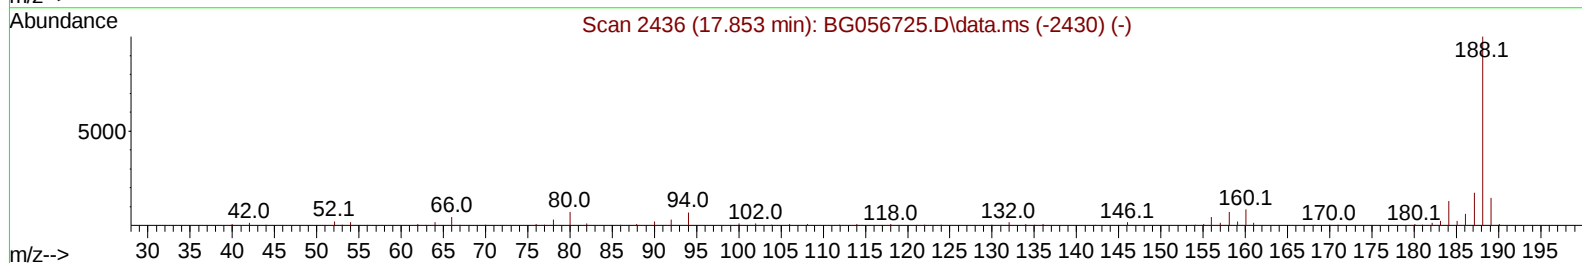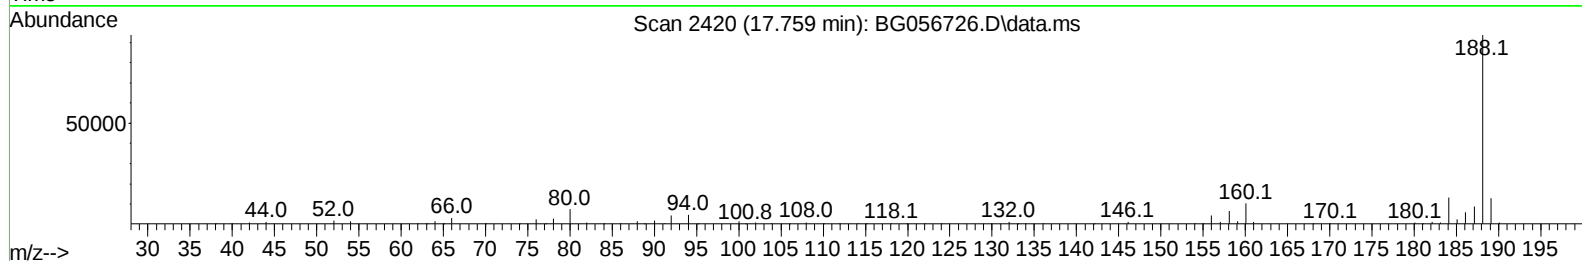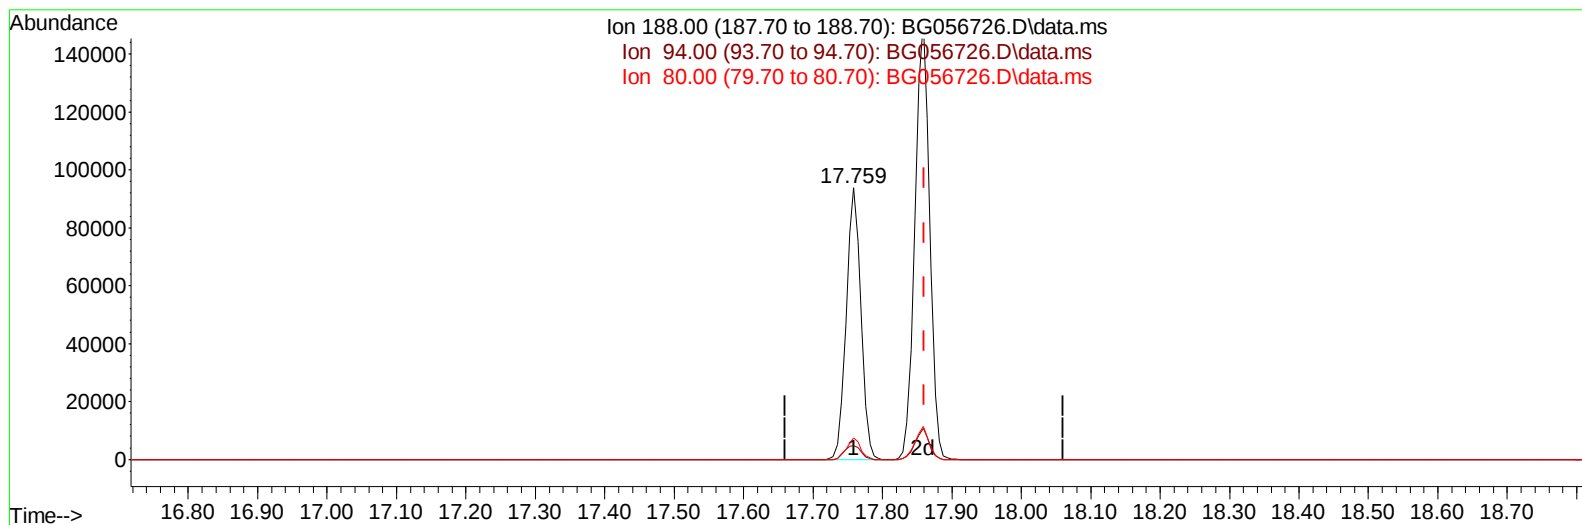

TIC: BG056726.D\data.ms

(73) Anthracene-d10 (S)

17.759min (-0.102) 20.61 ng/u1

response 137264

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	5.90	5.00
80.00	7.20	7.82
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022723\
 Data File : BG056726.D
 Acq On : 27 Feb 2023 11:29
 Operator : CG/JU
 Sample : PB150979BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK979

Manual IntegrationsAPPROVED

Quant Time: Feb 27 12:03:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 23 15:40:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/28/2023
 Supervised By :Jagrut Upadhyay 02/28/2023

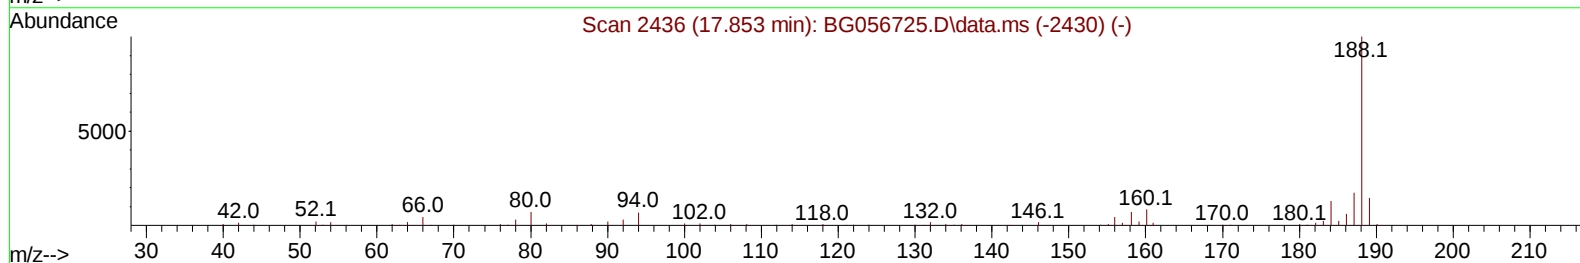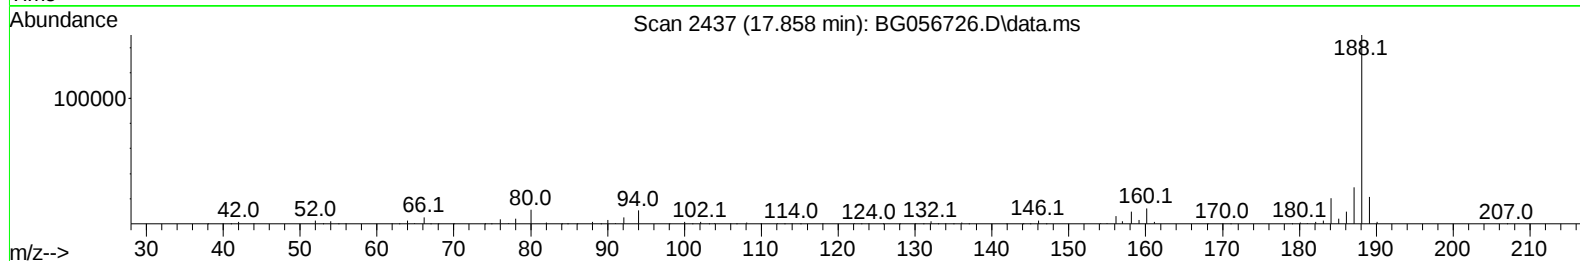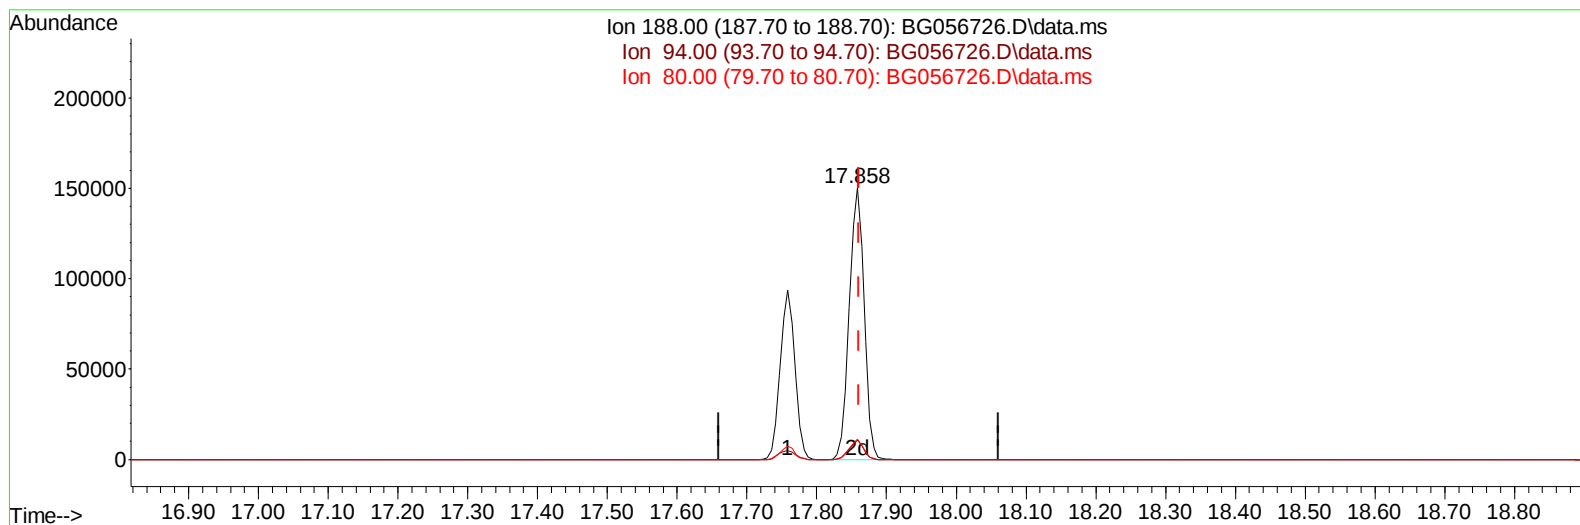

TIC: BG056726.D\data.ms

(73) Anthracene-d10 (S)

17.858min (-0.002) 33.42 ng/ul m

response 222530

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	5.90	7.11#
80.00	7.20	7.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022723\
 Data File : BG056726.D
 Acq On : 27 Feb 2023 11:29
 Operator : CG/JU
 Sample : PB150979BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK979

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/28/2023
 Supervised By :Jagrut Upadhyay 02/28/2023

Quant Time: Feb 27 12:03:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 23 15:40:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.417	152	14942	20.000	ng/ul	0.00
20) Naphthalene-d8	11.260	136	64074	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	15.027	164	51358	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.759	188	137264	20.000	ng/ul	0.00
79) Chrysene-d12	22.071	240	126542	20.000	ng/ul	0.00
88) Perylene-d12	25.602	264	133242	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.699	96	2168	8.049	ng/uL	0.00
4) Pyridine-d5	4.133	84	37260	34.270	ng/ul	0.00
7) Phenol-d5	7.541	99	45077	30.147	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.723	67	28352	31.085	ng/ul	0.00
11) 2-Chlorophenol-d4	7.941	132	30701	30.919	ng/ul	0.00
15) 4-Methylphenol-d8	9.104	113	33210	29.068	ng/ul	-0.01
21) Nitrobenzene-d5	9.592	128	17526	32.639	ng/ul	0.00
24) 2-Nitrophenol-d4	10.320	143	18293	28.620	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.861	165	34213	28.413	ng/ul	0.00
31) 4-Chloroaniline-d4	11.378	131	49794	31.705	ng/ul	0.00
46) Dimethylphthalate-d6	14.410	166	138617	33.453	ng/ul	0.00
49) Acenaphthylene-d8	14.727	160	155672	33.055	ng/ul	0.00
54) 4-Nitrophenol-d4	15.179	143	20837	29.166	ng/ul	0.00
60) Fluorene-d10	16.008	176	127370	33.230	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.102	200	22425	24.419	ng/ul	-0.01
73) Anthracene-d10	17.858	188	222530m	33.417	ng/ul	0.00
81) Pyrene-d10	20.115	212	262679	30.677	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.361	264	233717	32.497	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022723\
Data File : BG056726.D
Acq On : 27 Feb 2023 11:29
Operator : CG/JU
Sample : PB150979BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK979

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/28/2023
Supervised By :Jagrut Upadhyay 02/28/2023

Quant Time: Feb 27 12:03:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 23 15:40:42 2023
Response via : Initial Calibration

