




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022723\
Data File : BG056733.D
Acq On : 27 Feb 2023 16:45
Operator : CG/JU
Sample : PB151019BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK019

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/28/2023
Supervised By :Jagrut Upadhyay 02/28/2023

Quant Time: Feb 28 00:28:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 28 00:23:23 2023
Response via : Initial Calibration

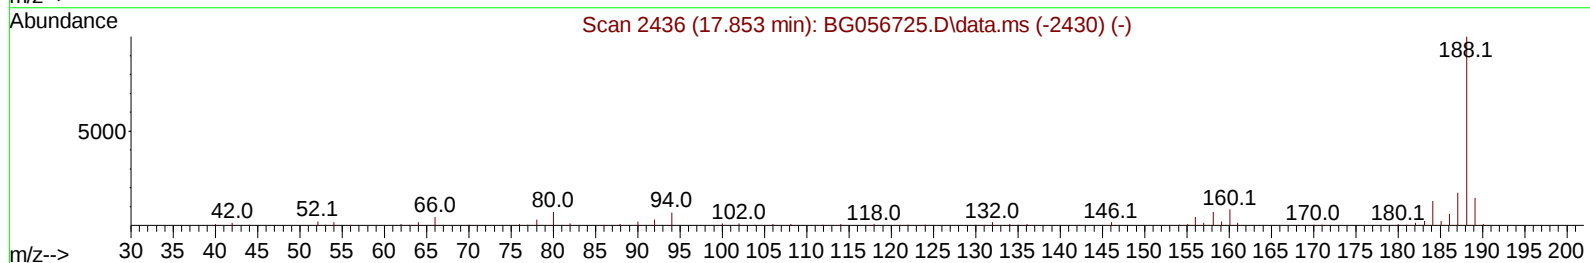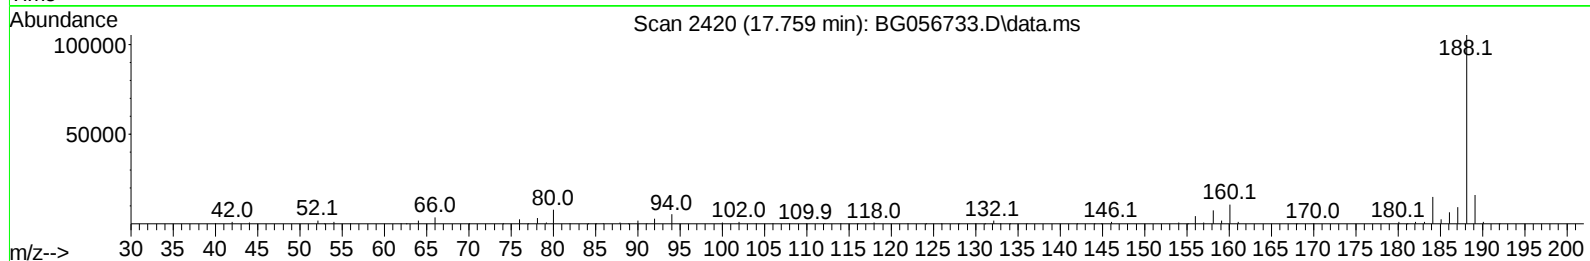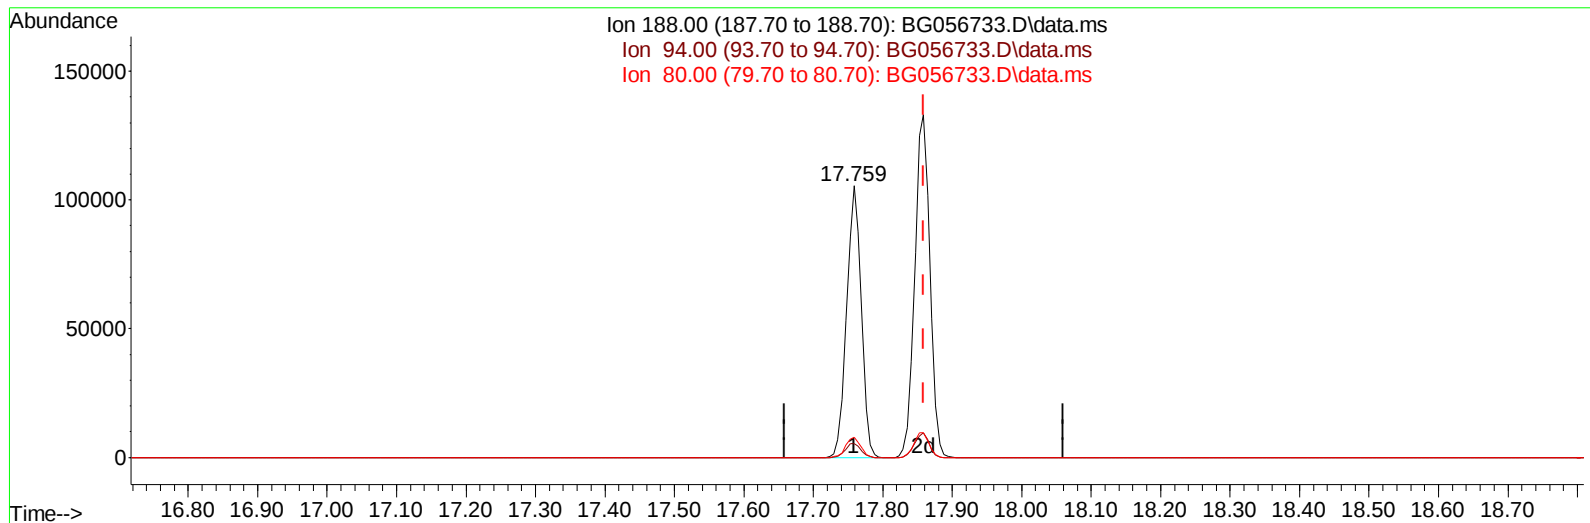

TIC: BG056733.D\data.ms

(73) Anthracene-d10 (S)

17.759min (-0.100) 20.61 ng/u1

response 154220

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	5.90	5.21
80.00	7.20	7.52
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022723\
 Data File : BG056733.D
 Acq On : 27 Feb 2023 16:45
 Operator : CG/JU
 Sample : PB151019BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK019

Manual IntegrationsAPPROVED

Quant Time: Feb 28 00:28:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 00:23:23 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/28/2023
 Supervised By :Jagrut Upadhyay 02/28/2023

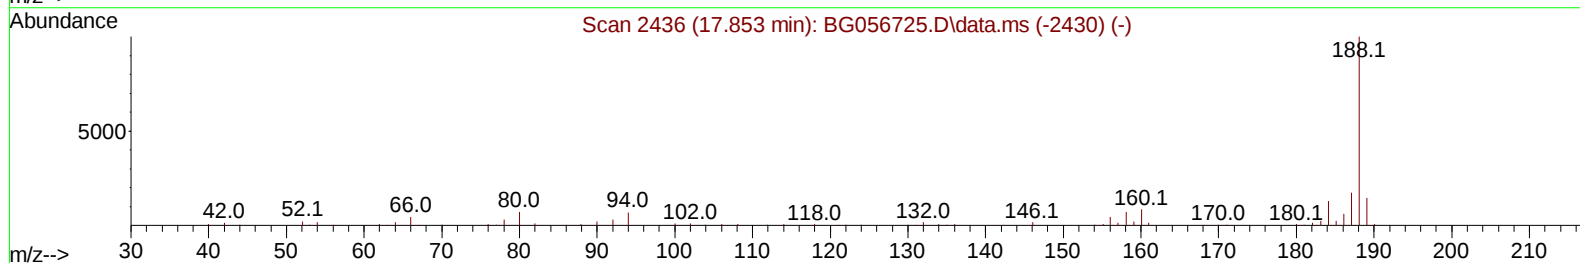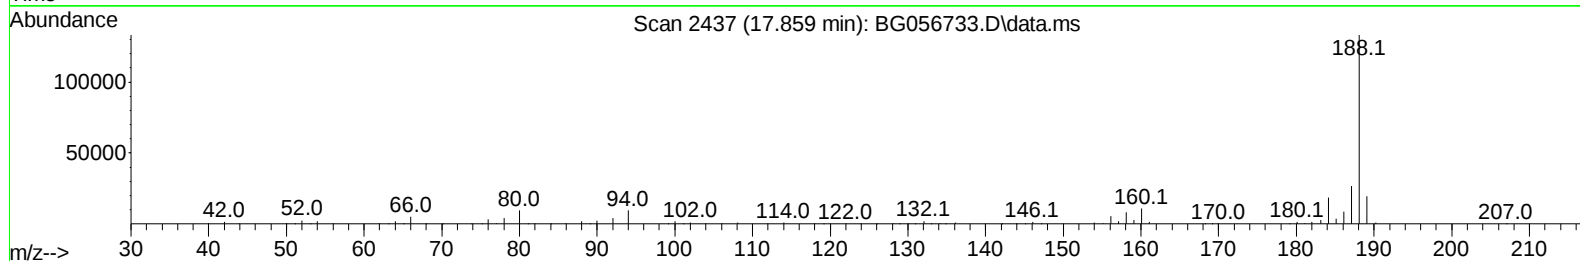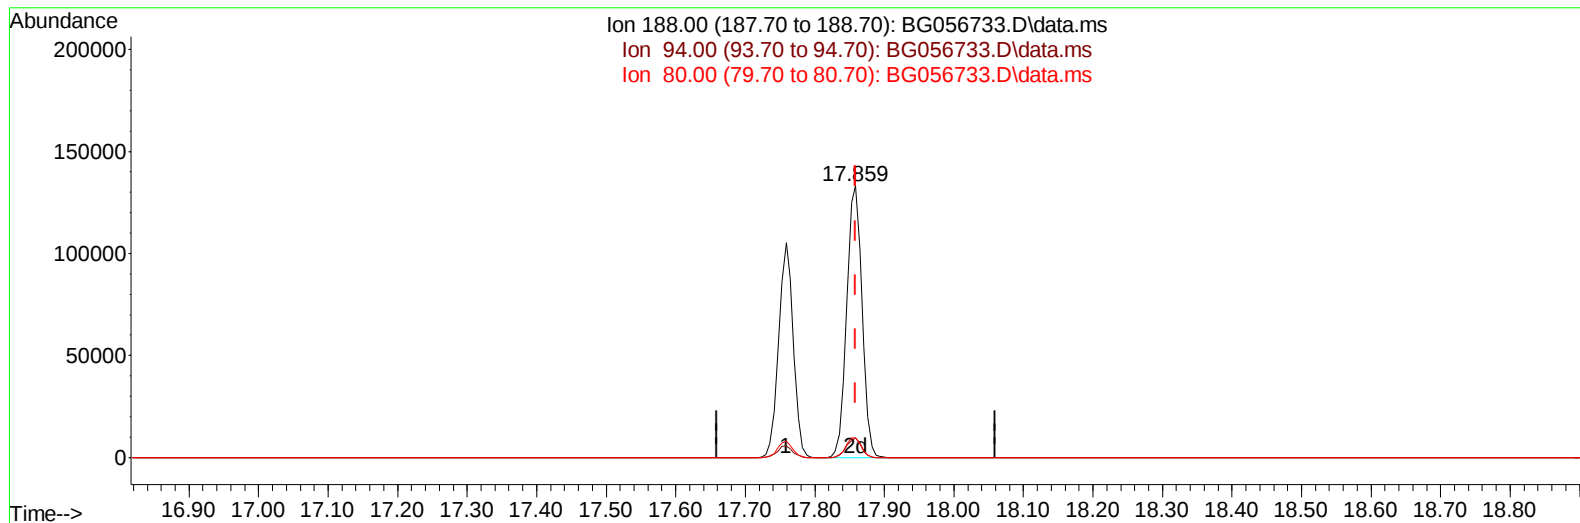

TIC: BG056733.D\data.ms

(73) Anthracene-d10 (S)

17.859min (-0.001) 27.01 ng/ul m

response 202048

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	5.90	7.14#
80.00	7.20	7.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022723\
 Data File : BG056733.D
 Acq On : 27 Feb 2023 16:45
 Operator : CG/JU
 Sample : PB151019BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK019

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/28/2023
 Supervised By :Jagrut Upadhyay 02/28/2023

Quant Time: Feb 28 00:28:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 00:23:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.423	152	16972	20.000	ng/ul	0.00
20) Naphthalene-d8	11.260	136	71152	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.027	164	59150	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.759	188	154220	20.000	ng/ul	0.00
79) Chrysene-d12	22.065	240	147669	20.000	ng/ul	0.00
88) Perylene-d12	25.597	264	153247	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.699	96	2113	6.906	ng/uL	0.00
4) Pyridine-d5	4.139	84	31870	25.807	ng/ul	0.00
7) Phenol-d5	7.541	99	41879	24.658	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.723	67	27291	26.343	ng/ul	0.00
11) 2-Chlorophenol-d4	7.941	132	28660	25.411	ng/ul	0.00
15) 4-Methylphenol-d8	9.104	113	32273	24.869	ng/ul	0.00
21) Nitrobenzene-d5	9.592	128	16663	27.945	ng/ul	0.00
24) 2-Nitrophenol-d4	10.320	143	18817	26.511	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.861	165	33230	24.851	ng/ul	0.00
31) 4-Chloroaniline-d4	11.378	131	46105	26.436	ng/ul	0.00
46) Dimethylphthalate-d6	14.410	166	130938	27.437	ng/ul	0.00
49) Acenaphthylene-d8	14.721	160	143896	26.529	ng/ul	0.00
54) 4-Nitrophenol-d4	15.174	143	20305	24.678	ng/ul	0.00
60) Fluorene-d10	16.008	176	117628	26.645	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.102	200	22185	21.501	ng/ul	0.00
73) Anthracene-d10	17.859	188	202048m	27.005	ng/ul	0.00
81) Pyrene-d10	20.115	212	247296	24.748	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.356	264	220136	26.613	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022723\
Data File : BG056733.D
Acq On : 27 Feb 2023 16:45
Operator : CG/JU
Sample : PB151019BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK019

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/28/2023
Supervised By :Jagrut Upadhyay 02/28/2023

Quant Time: Feb 28 00:28:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 28 00:23:23 2023
Response via : Initial Calibration

