

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022819\
 Data File : BG039671.D
 Acq On : 28 Feb 2019 22:14
 Operator : JU/SJ
 Sample : K1628-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Mar 01 06:06:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	48889	20.00	ng	-0.02
21) Naphthalene-d8	10.99	136	211385	20.00	ng	-0.02
39) Acenaphthene-d10	14.79	164	141142	20.00	ng	-0.02
64) Phenanthrene-d10	17.53	188	335096	20.00	ng	-0.02
76) Chrysene-d12	21.82	240	330322	20.00	ng	-0.03
87) Perylene-d12	25.20	264	327711	20.00	ng	-0.05

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.71	112	445212	155.86	ng	0.00
7) Phenol-d6	7.31	99	649379	154.44	ng	-0.01
23) Nitrobenzene-d5	9.34	82	389606	115.14	ng	-0.02
42) 2,4,6-Tribromophenol	16.27	330	241855	159.13	ng	-0.02
45) 2-Fluorobiphenyl	13.41	172	888384	90.29	ng	-0.02
79) Terphenyl-d14	20.13	244	1249045	80.04	ng	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	7.31	77	1236	Below Cal		# 4
10) Phenol	7.34	94	10009	2.284	ng	# 86
19) n-Nitroso-di-n-propylamine	9.34	70	51448	17.240	ng	# 65
48) 2-Nitroaniline	14.23	65	351	8.411	ng	# 1
50) Dimethylphthalate	14.23	163	62856	5.514	ng	# 98
51) 2,6-Dinitrotoluene	14.23	165	590	6.798	ng	# 21
57) 2,4-Dinitrotoluene	14.79	165	18558	13.517	ng	# 19
62) 4-Nitroaniline	15.44	138	73	4.230	ng	# 10
65) 4,6-Dinitro-2-methylphenol	16.27	198	895	5.031	ng	# 11
67) 4-Bromophenyl-phenylether	16.27	248	18861	5.074	ng	# 1
77) Benzidine	20.13	184	21706	2.004	ng	# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022819\
Data File : BG039671.D
Acq On : 28 Feb 2019 22:14
Operator : JU/SJ
Sample : K1628-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Mar 01 06:06:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

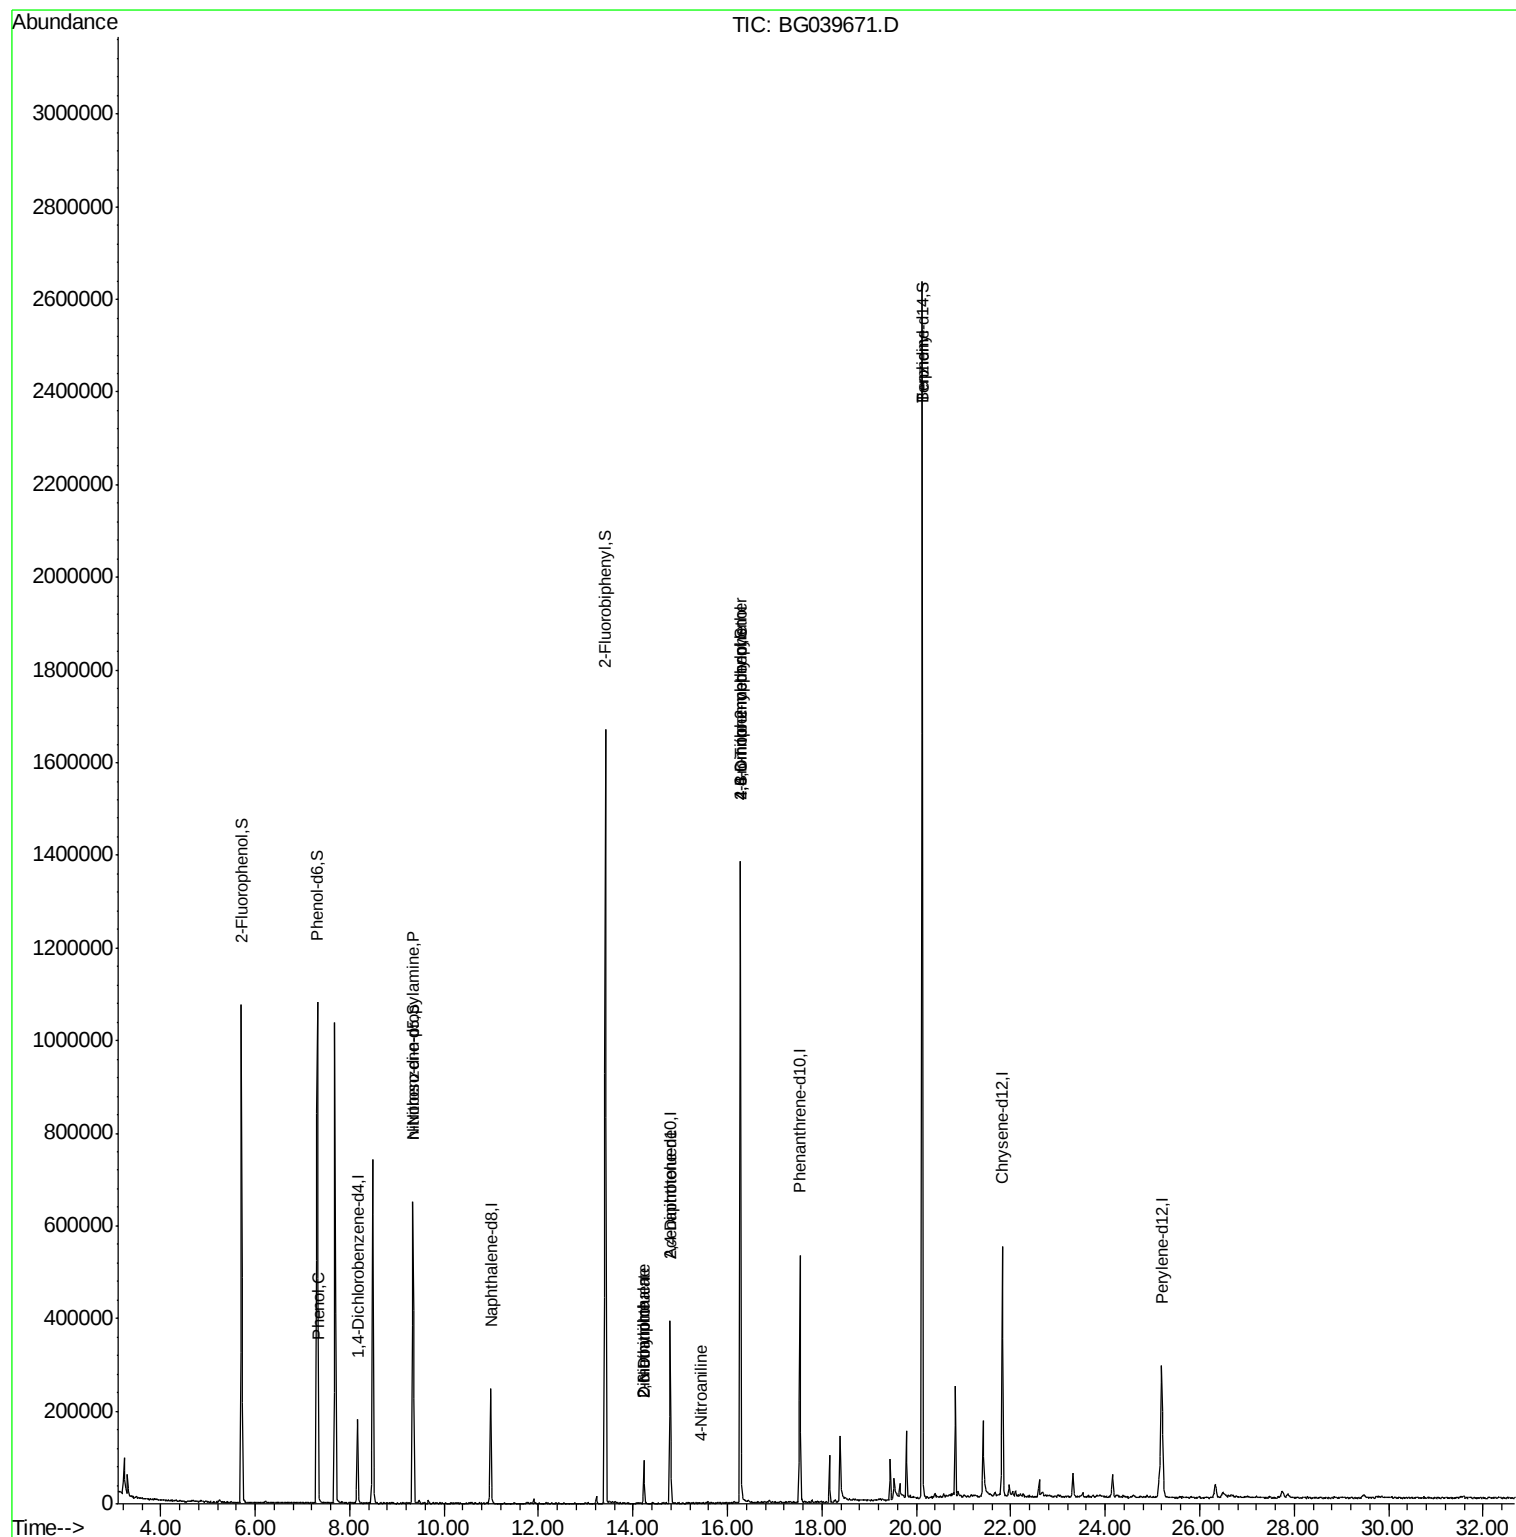




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.17 min Scan# 864
Delta R.T. -0.02 min
Lab File: BG039671.D
Acq: 28 Feb 2019 22:14

Instrument :
BNA_G
ClientSampled :

Tot Ion:152 Resp: 48889
Ion Ratio Lower Upper
152 100
150 150.3 123.7 185.5
115 62.1 45.9 68.9




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

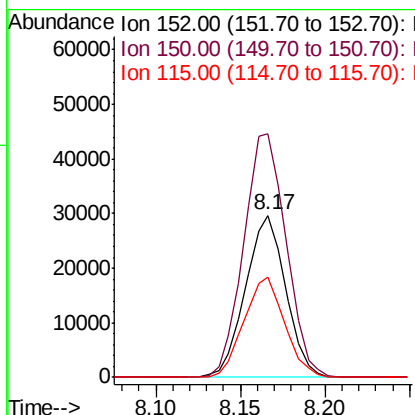



#5


2-Fluorophenol
Concen: 155.860 ng
RT: 5.71 min Scan# 446
Delta R.T. -0.01 min
Lab File: BG039671.D
Acq: 28 Feb 2019 22:14

Tgt Ion:112 Resp: 445212
Ion Ratio Lower Upper
112 100
64 68.1 57.8 86.8
63 35.9 29.8 44.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

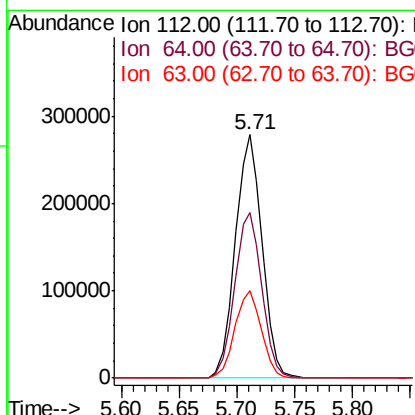

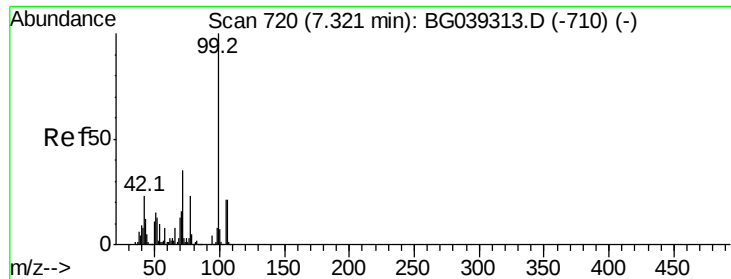

#7

Phenol-d6

Concen: 154.442 ng

RT: 7.31 min Scan# 718

Delta R.T. -0.01 min

Lab File: BG039671.D

Acq: 28 Feb 2019 22:14

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 649379

Ion Ratio Lower Upper




99 100

42 20.2 18.2 27.2

71 36.2 28.0 42.0

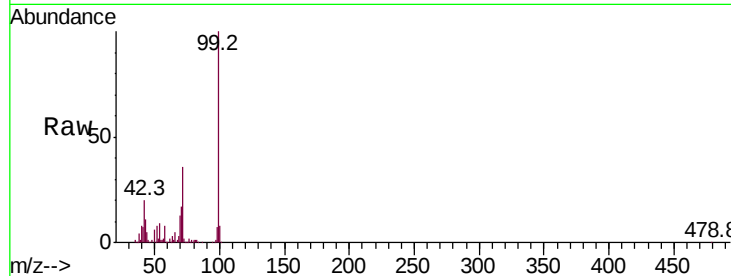

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

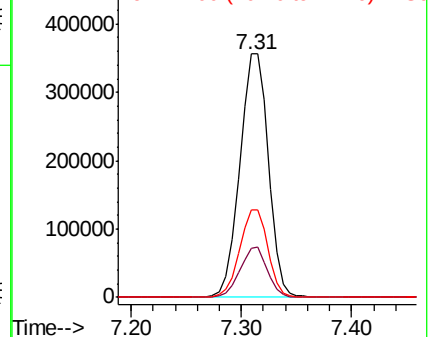

#10

Phenol

Concen: 2.284 ng

RT: 7.34 min Scan# 723

Delta R.T. -0.01 min

Lab File: BG039671.D

Acq: 28 Feb 2019 22:14


Tgt Ion: 94 Resp: 10009

Ion Ratio Lower Upper



94 100


65 33.0 11.7 51.7

66 58.2 23.7 63.7



Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

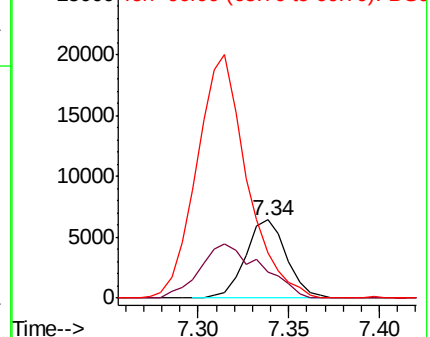

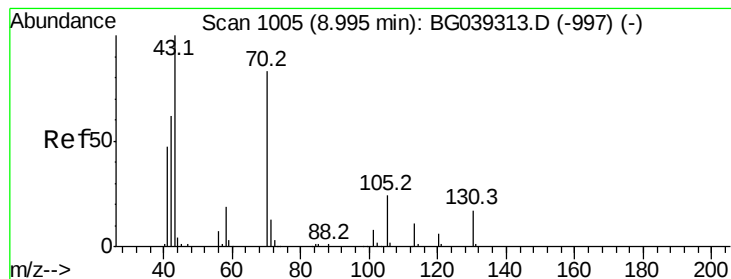

#19

n-Nitroso-di-n-propylamine

Concen: 17.240 ng

RT: 9.34 min Scan# 1064

Delta R.T. 0.35 min

Lab File: BG039671.D

Acq: 28 Feb 2019 22:14

Instrument :

BNA_G

ClientSampleId :

Tot Ion: 70 Resp: 51448





Ion Ratio Lower Upper

70 100

42 45.3 60.4 90.6#

101 0.0 7.5 11.3#

130 2.3 16.9 25.3#

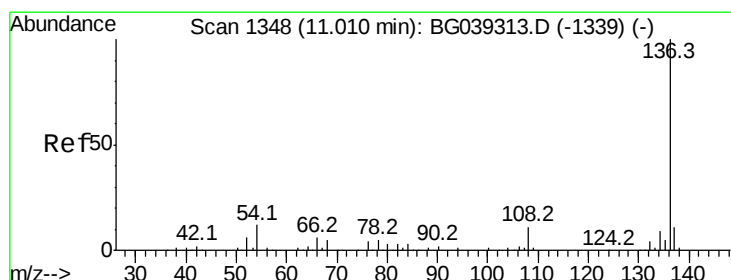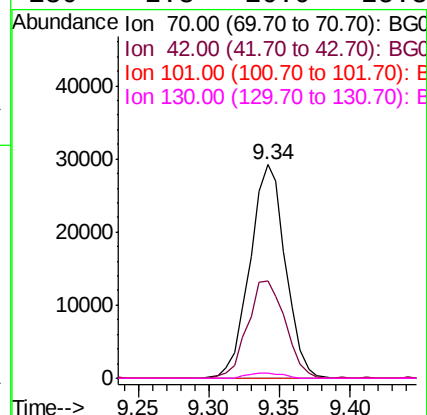

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.99 min Scan# 1344

Delta R.T. -0.02 min

Lab File: BG039671.D

Acq: 28 Feb 2019 22:14

Tgt Ion: 136 Resp: 211385




Ion Ratio Lower Upper


136 100

137 11.2 9.1 13.7

54 10.7 9.4 14.2

68 5.9 4.2 6.4


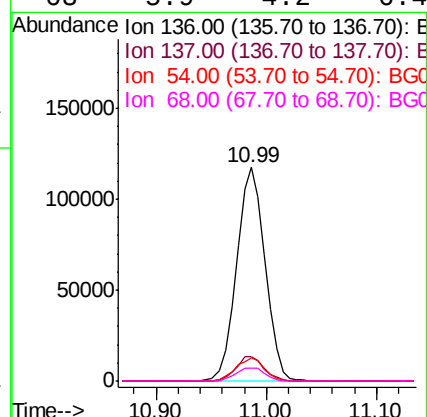






#23
 Nitrobenzene-d5
 Concen: 115.142 ng
 RT: 9.34 min Scan# 1064
 Delta R.T. -0.02 min
 Lab File: BG039671.D
 Acq: 28 Feb 2019 22:14




Instrument :
 BNA_G
 ClientSampled :


Tot Ion	82	Resp	389606
Ion Ratio	Lower	Upper	
82	100		
128	43.1	31.3	46.9
54	56.2	50.9	76.3

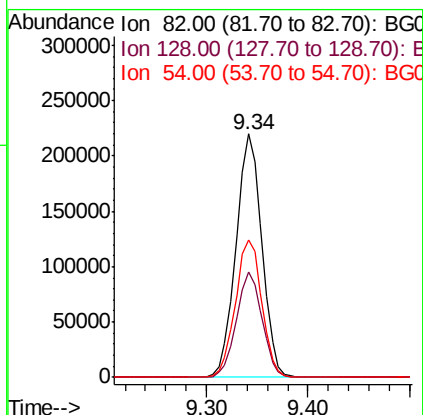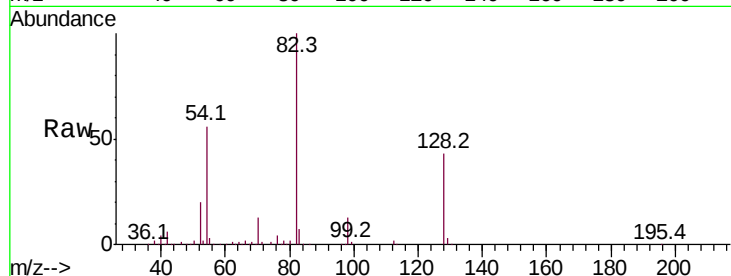

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.79 min Scan# 1991
 Delta R.T. -0.02 min
 Lab File: BG039671.D
 Acq: 28 Feb 2019 22:14

Tgt Ion	164	Resp	141142
Ion Ratio	Lower	Upper	
164	100		
162	100.1	81.6	122.4
160	45.3	34.2	51.2

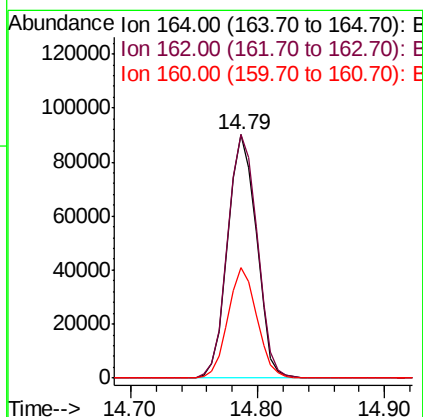


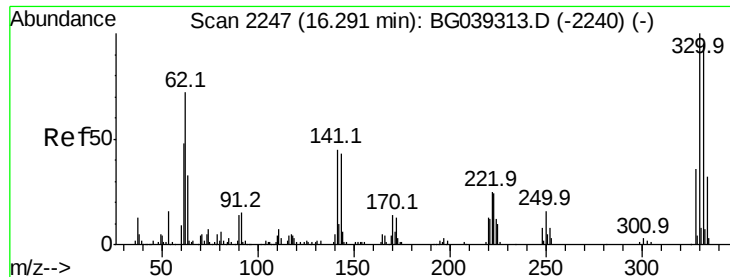




#42
 2,4,6-Tribromophenol
 Concen: 159.130 ng
 RT: 16.27 min Scan# 2244
 Delta R.T. -0.02 min
 Lab File: BG039671.D
 Acq: 28 Feb 2019 22:14

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:330 Resp: 241855
 Ion Ratio Lower Upper
 330 100
 332 97.2 75.7 113.5
 141 40.8 35.6 53.4

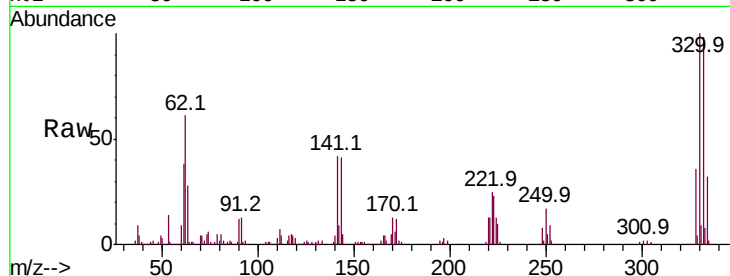


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

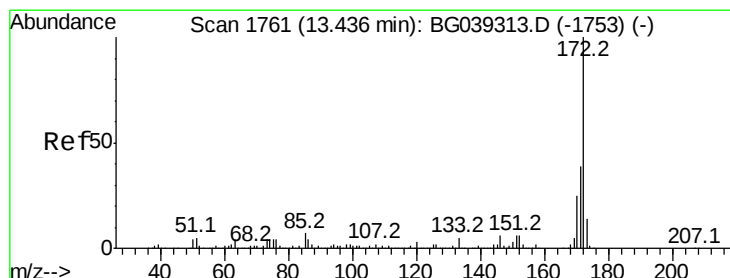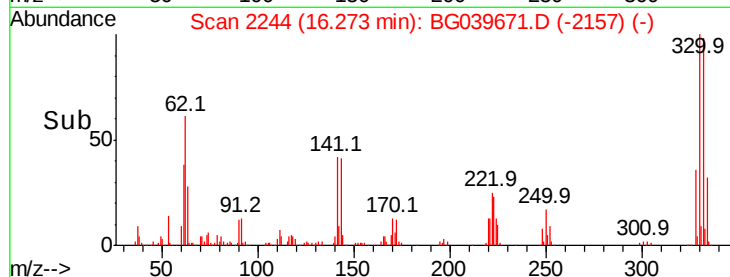
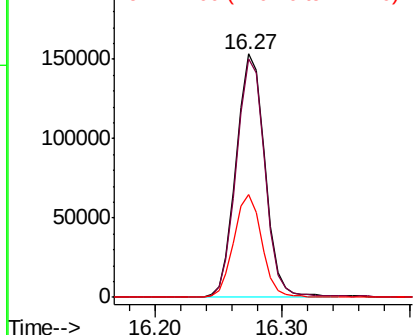



#45
 2-Fluorobiphenyl
 Concen: 90.294 ng
 RT: 13.41 min Scan# 1757
 Delta R.T. -0.02 min
 Lab File: BG039671.D
 Acq: 28 Feb 2019 22:14

Tgt Ion:172 Resp: 888384
 Ion Ratio Lower Upper
 172 100
 171 36.7 30.8 46.2
 170 24.4 20.2 30.4

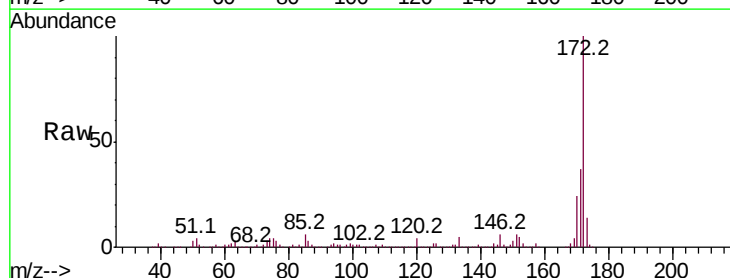

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

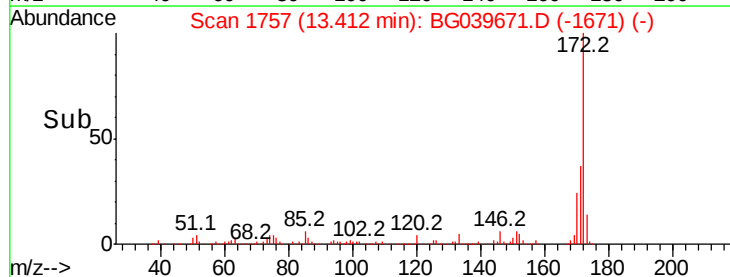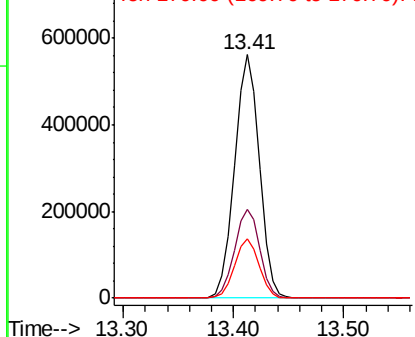

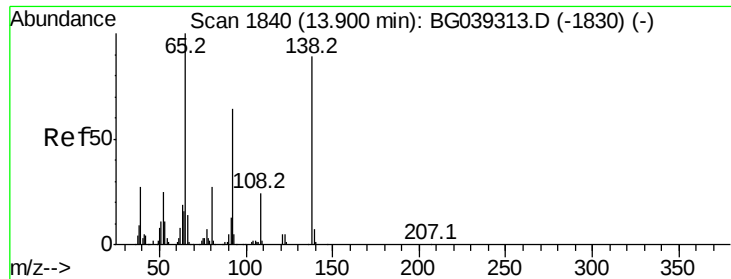

#48

2-Nitroaniline

Concen: 8.411 ng

RT: 14.23 min Scan# 1896

Delta R.T. 0.33 min

Lab File: BG039671.D

Acq: 28 Feb 2019 22:14

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 65 Resp: 351

Ion Ratio Lower Upper

65 100

92 695.2 51.4 77.2#




138 0.0 71.4 107.2#



Abundance Ion 65.00 (64.70 to 65.70): BG039671.D (-1830) (-)

Ion 92.00 (91.70 to 92.70): BG039671.D (-1830) (-)

Ion 138.00 (137.70 to 138.70): BG039671.D (-1830) (-)

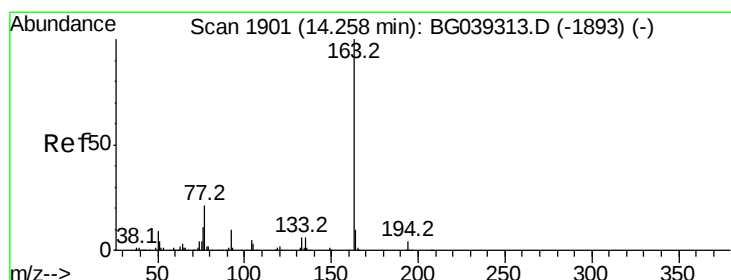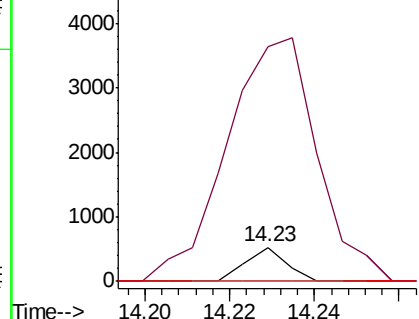

#50

Dimethylphthalate

Concen: 5.514 ng

RT: 14.23 min Scan# 1896

Delta R.T. -0.03 min

Lab File: BG039671.D

Acq: 28 Feb 2019 22:14


Tgt Ion:163 Resp: 62856

Ion Ratio Lower Upper

163 100

194 4.6 3.6 5.4



164 9.7 8.4 12.6




Abundance Ion 163.00 (162.70 to 163.70): BG039671.D (-1811) (-)

Ion 194.00 (193.70 to 194.70): BG039671.D (-1811) (-)

Ion 164.00 (163.70 to 164.70): BG039671.D (-1811) (-)

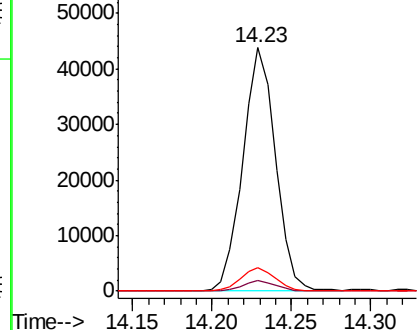

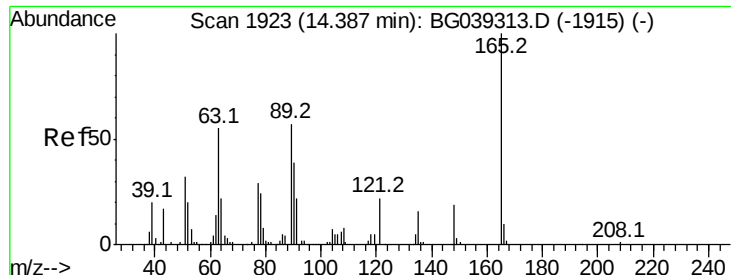

#51

2,6-Dinitrotoluene

Concen: 6.798 ng

RT: 14.23 min Scan# 1897

Delta R.T. -0.15 min

Lab File: BG039671.D

Acq: 28 Feb 2019 22:14

Instrument :

BNA_G

ClientSampleId :


Tot Ion:165 Resp: 590

Ion Ratio Lower Upper

165 100

63 119.0 47.0 70.6#




89 0.0 45.8 68.8#

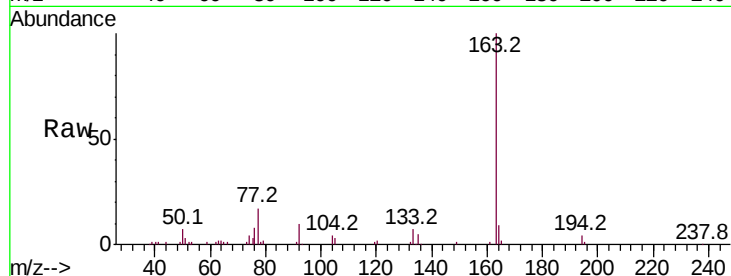

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

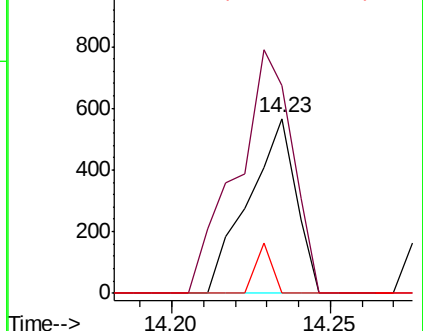

#57

2,4-Dinitrotoluene

Concen: 13.517 ng

RT: 14.79 min Scan# 1991

Delta R.T. -0.38 min

Lab File: BG039671.D

Acq: 28 Feb 2019 22:14

Tgt Ion:165 Resp: 18558


Ion Ratio Lower Upper

165 100

63 0.0 41.0 61.6#

89 2.2 64.6 96.8#

182 0.0 2.0 3.0#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E




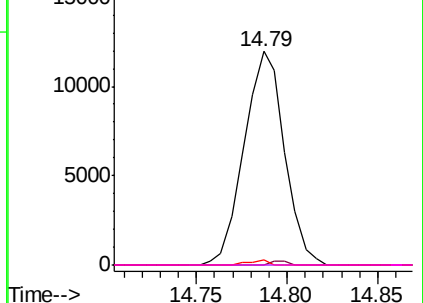




#62
 4-Nitroaniline
 Concen: 4.230 ng
 RT: 15.44 min Scan# 2102
 Delta R.T. -0.44 min
 Lab File: BG039671.D
 Acq: 28 Feb 2019 22:14




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
138	100		
92	0.0	38.7	78.7#
108	0.0	74.6	114.6#

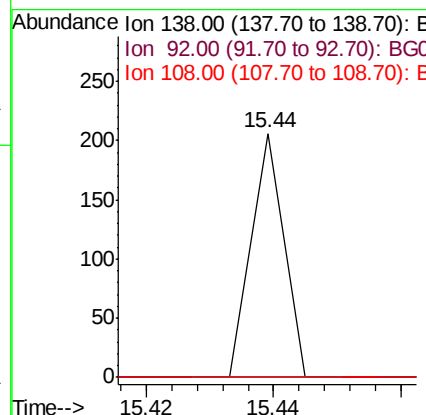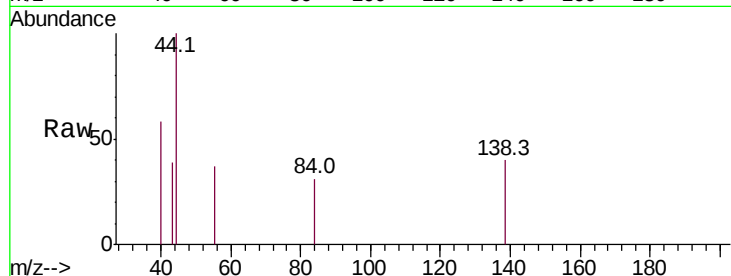

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.53 min Scan# 2458
 Delta R.T. -0.02 min
 Lab File: BG039671.D
 Acq: 28 Feb 2019 22:14

Tgt Ion	Ratio	Lower	Upper
188	100		
94	7.4	6.9	10.3
80	9.6	8.1	12.1

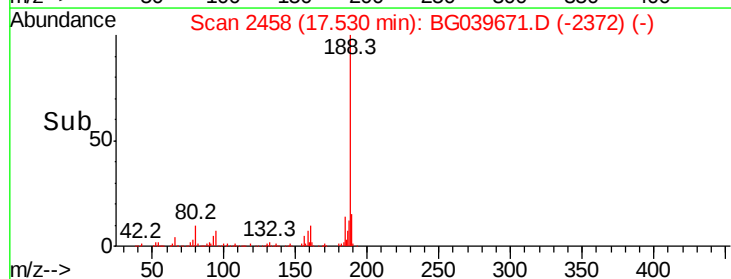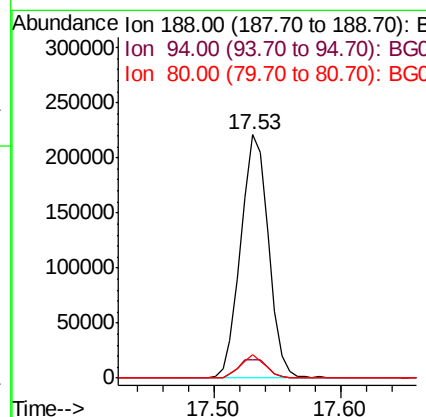

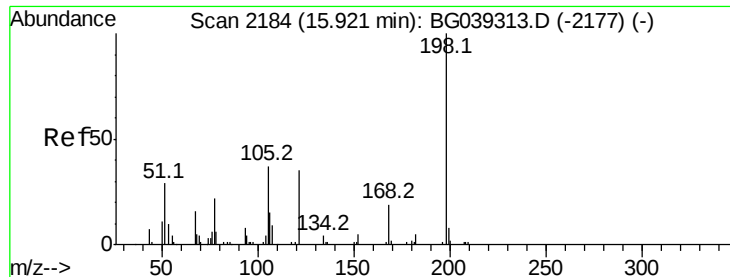

#65

4,6-Dinitro-2-methylphenol

Concen: 5.031 ng

RT: 16.27 min Scan# 2244

Delta R.T. 0.35 min

Lab File: BG039671.D

Acq: 28 Feb 2019 22:14

Instrument :

BNA_G

ClientSampled :


Tot Ion:198 Resp: 895

Ion Ratio Lower Upper

198 100

51 71.7 27.4 67.4#



105 133.3 19.7 59.7#

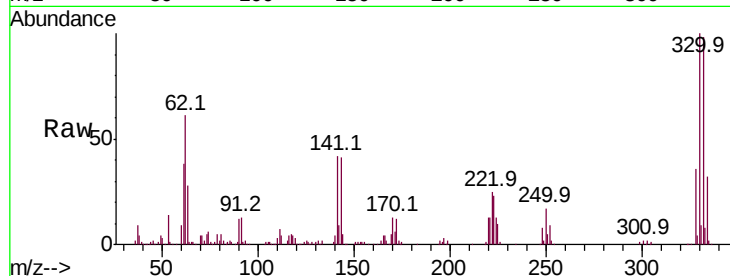

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BG0

Ion 105.00 (104.70 to 105.70): E

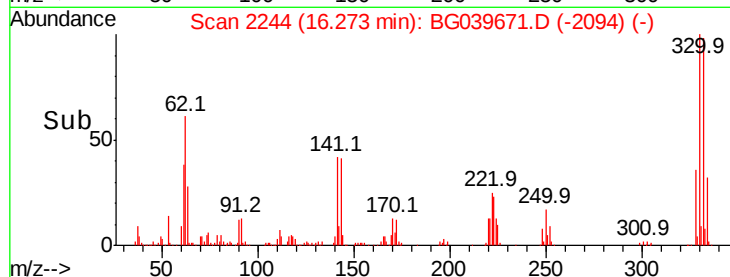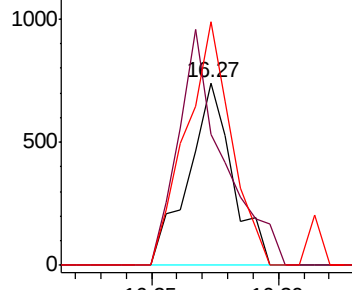

#67

4-Bromophenyl-phenylether

Concen: 5.074 ng

RT: 16.27 min Scan# 2244

Delta R.T. -0.46 min

Lab File: BG039671.D

Acq: 28 Feb 2019 22:14



Tgt Ion:248 Resp: 18861

Ion Ratio Lower Upper

248 100

250 198.2 77.6 116.4#



141 503.7 63.9 95.9#

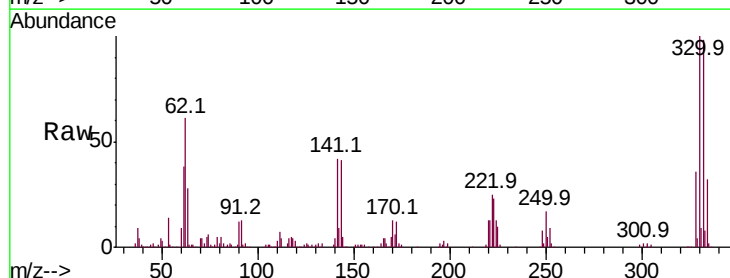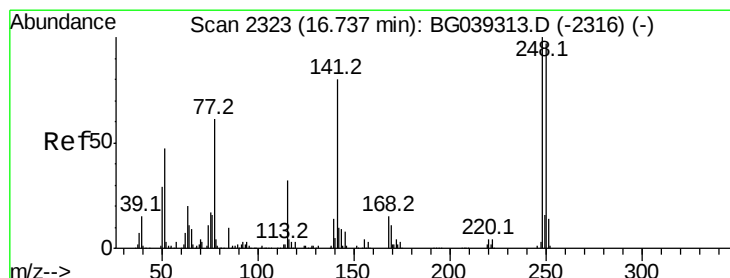


Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E



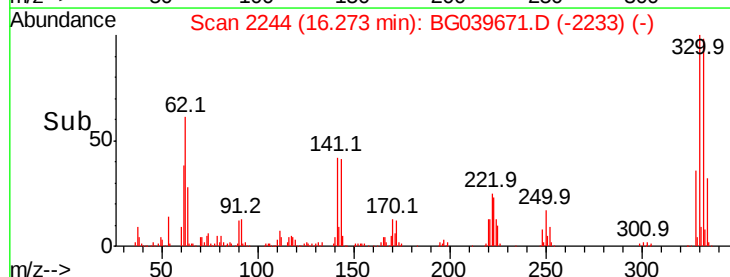
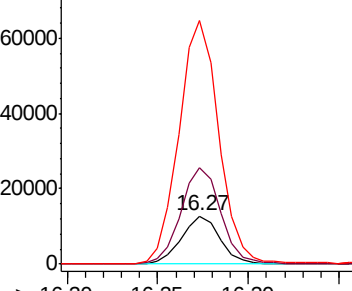


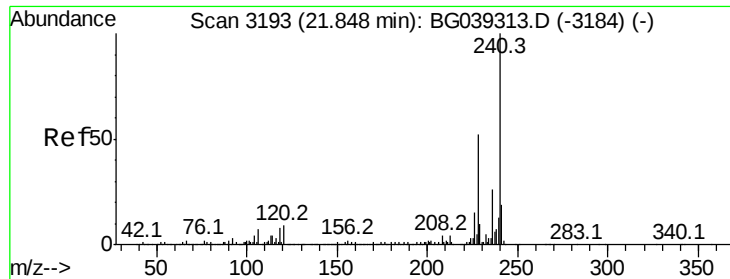

#76
 Chrvsene-d12
 Concen: 20.000 ng
 RT: 21.82 min Scan# 3188
 Delta R.T. -0.03 min
 Lab File: BG039671.D
 Acq: 28 Feb 2019 22:14




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion:240 Resp: 330322
 Ion Ratio Lower Upper
 240 100
 120 9.2 7.0 10.6
 236 25.9 21.0 31.4

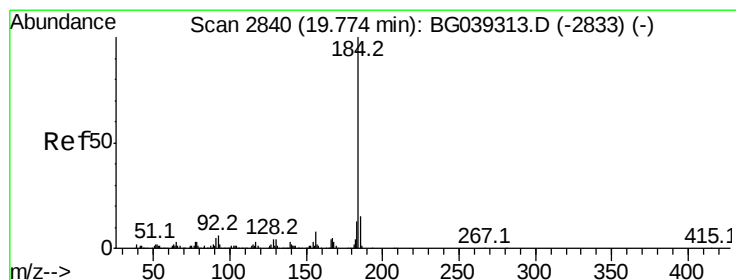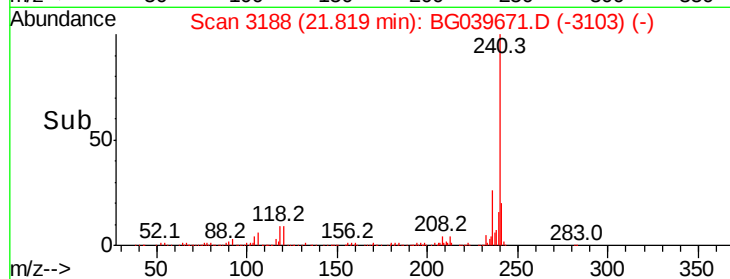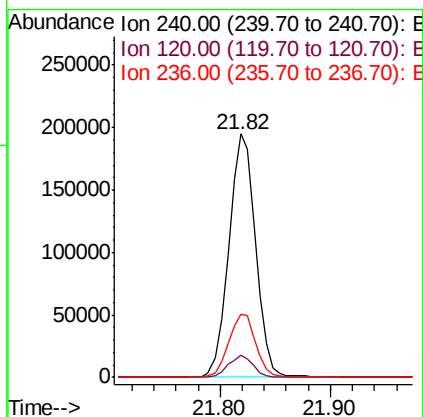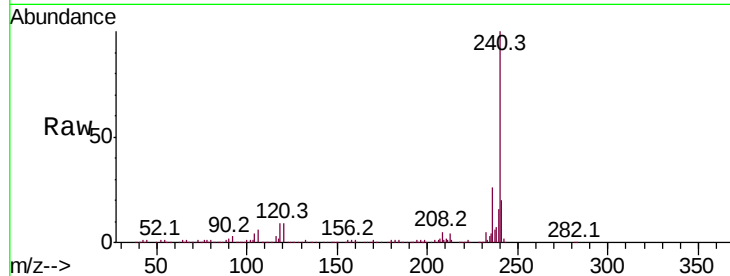

#77
 Benzidine
 Concen: 2.004 ng
 RT: 20.13 min Scan# 2900
 Delta R.T. 0.35 min
 Lab File: BG039671.D
 Acq: 28 Feb 2019 22:14

Tgt Ion:184 Resp: 21706
 Ion Ratio Lower Upper
 184 100
 185 18.9 12.2 18.2#
 183 9.5 10.6 15.8#


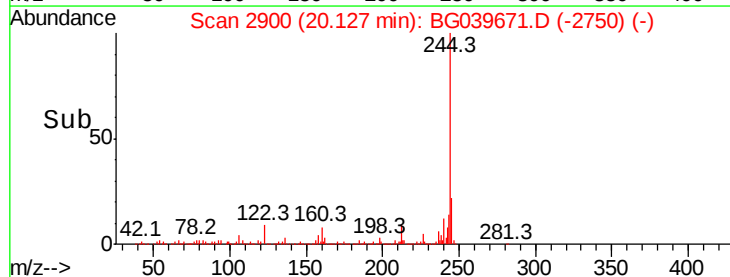
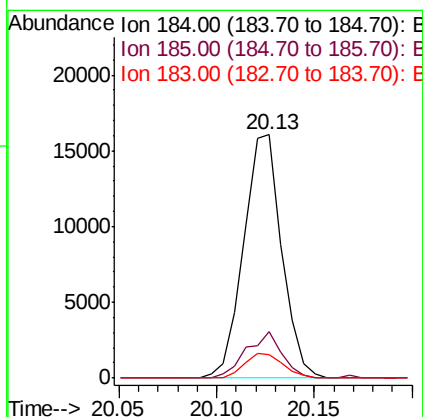
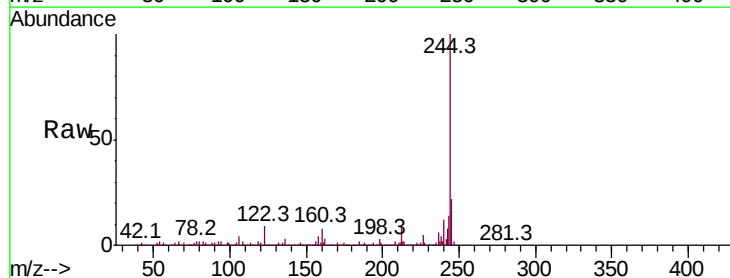


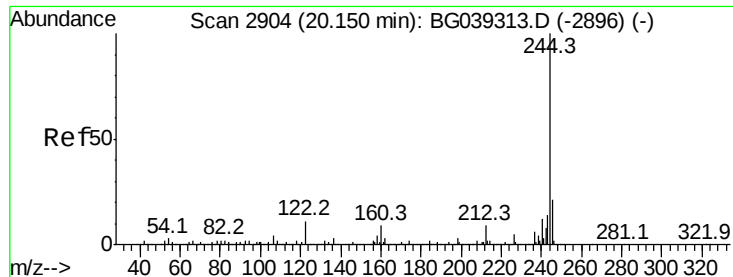

#79
 Terphenyl-d14
 Concen: 80.038 ng
 RT: 20.13 min Scan# 2900
 Delta R.T. -0.02 min
 Lab File: BG039671.D
 Acq: 28 Feb 2019 22:14

Instrument :
 BNA_G
 ClientSampled :

Tot Ion:244 Resp: 1249045
 Ion Ratio Lower Upper
 244 100
 212 9.1 7.3 10.9
 122 9.2 8.4 12.6

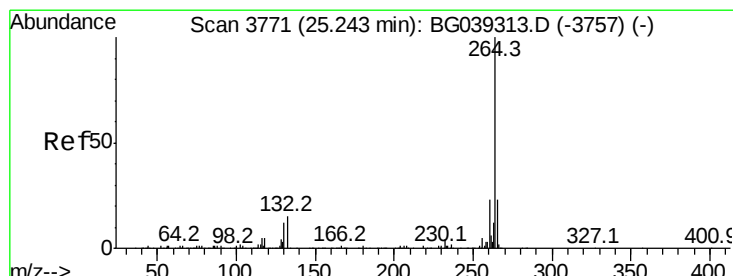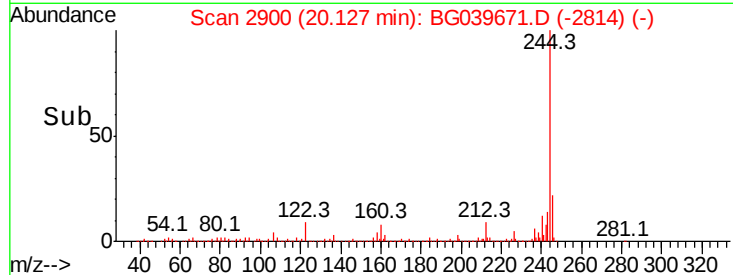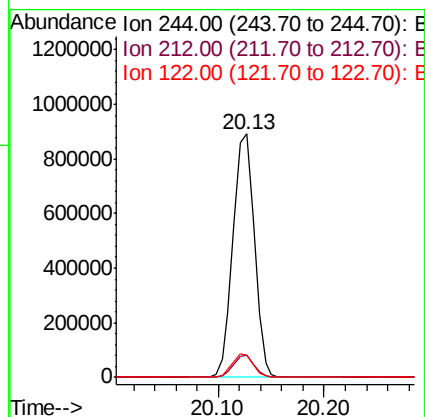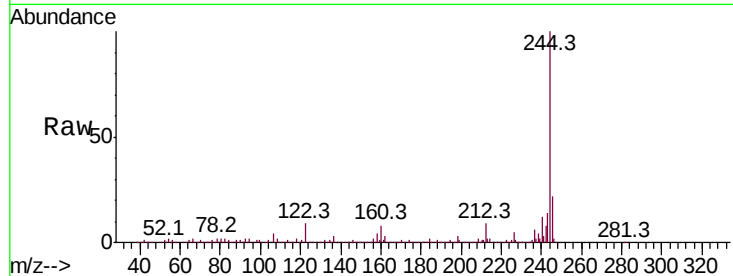

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.20 min Scan# 3763
 Delta R.T. -0.05 min
 Lab File: BG039671.D
 Acq: 28 Feb 2019 22:14

Tgt Ion:264 Resp: 327711
 Ion Ratio Lower Upper
 264 100
 260 23.4 18.2 27.4
 265 21.4 18.5 27.7

