
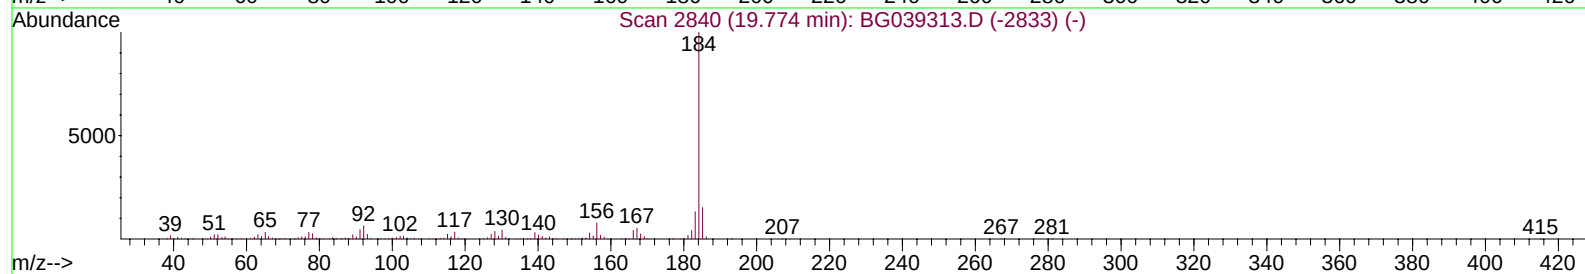
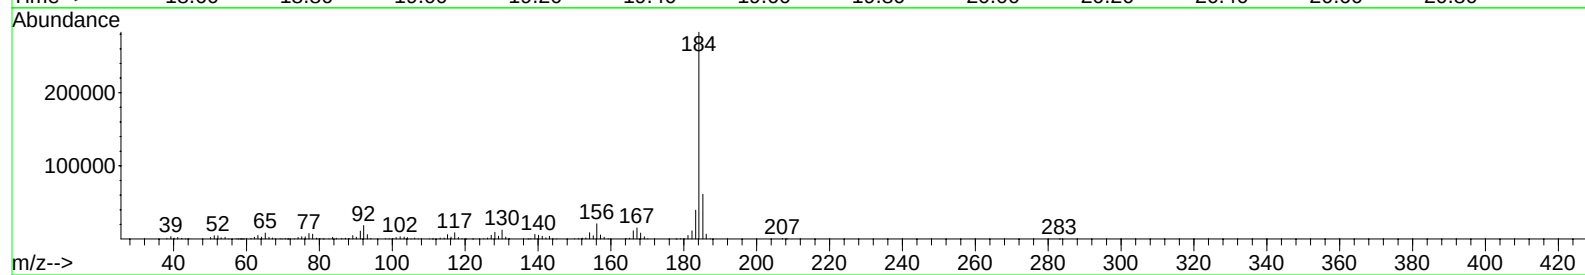


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG022819\
Data File : BG039659.D
Acq On : 28 Feb 2019 13:03
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 18:11:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 06:15:02 2019
Response via : Initial Calibration

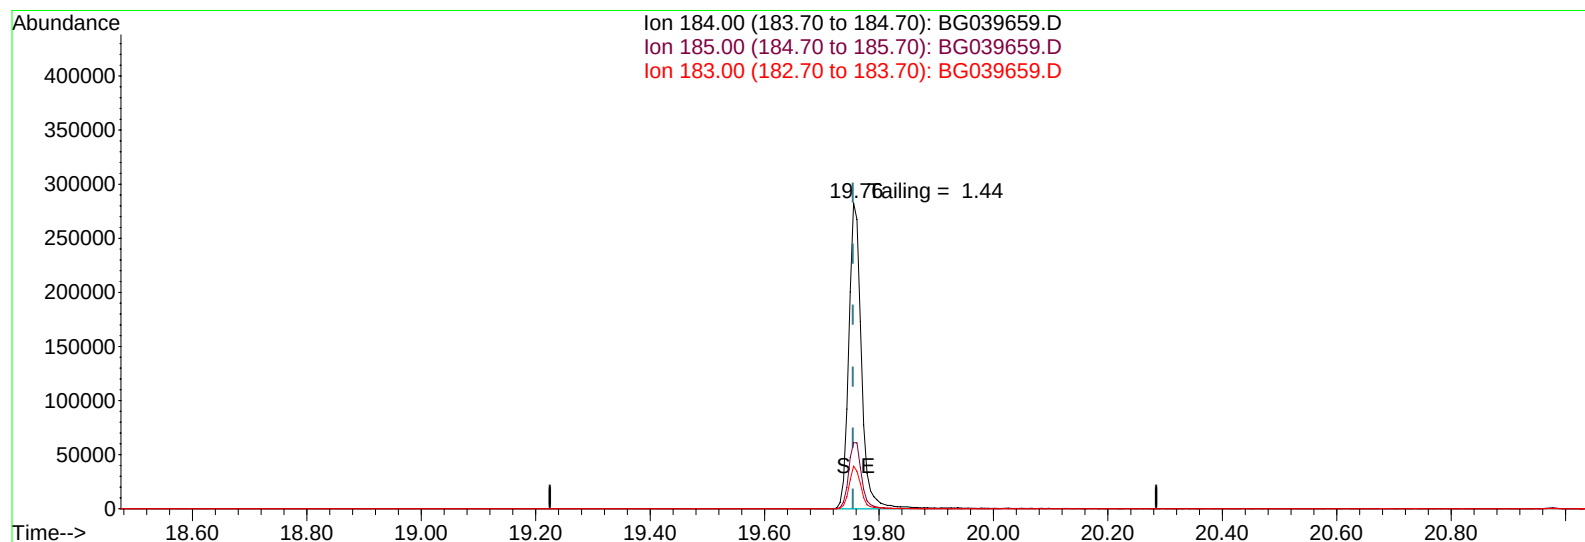

TIC: BG039659.D

(77) Benzidine




19.756min (+0.001) 0.00ng

response 432649

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	21.60#
183.00	13.20	13.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG022819\
Data File : BG039659.D
Acq On : 28 Feb 2019 13:03
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 18:11:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 06:15:02 2019
Response via : Initial Calibration

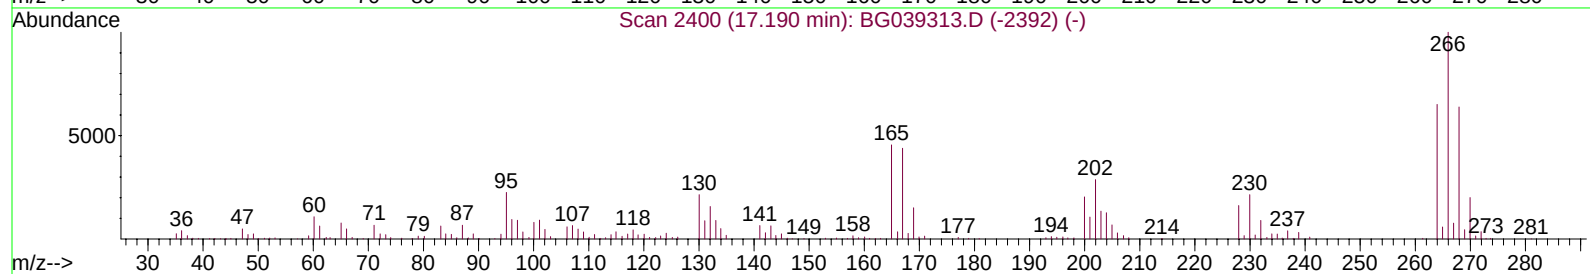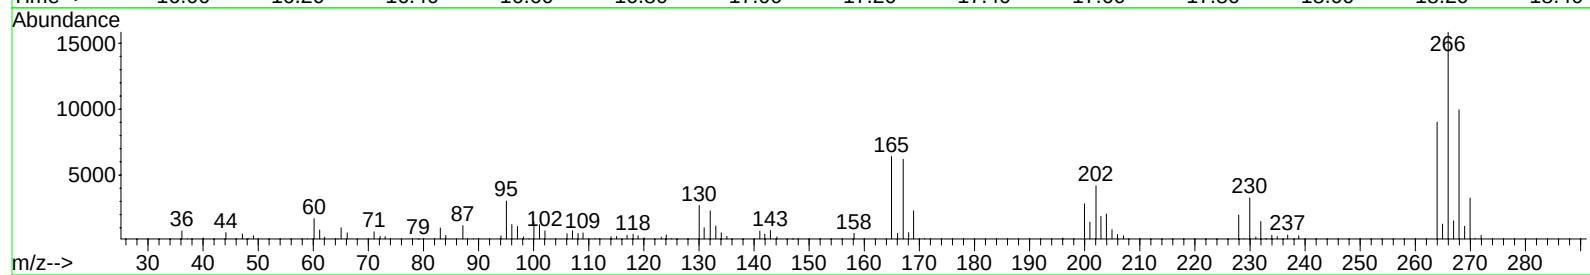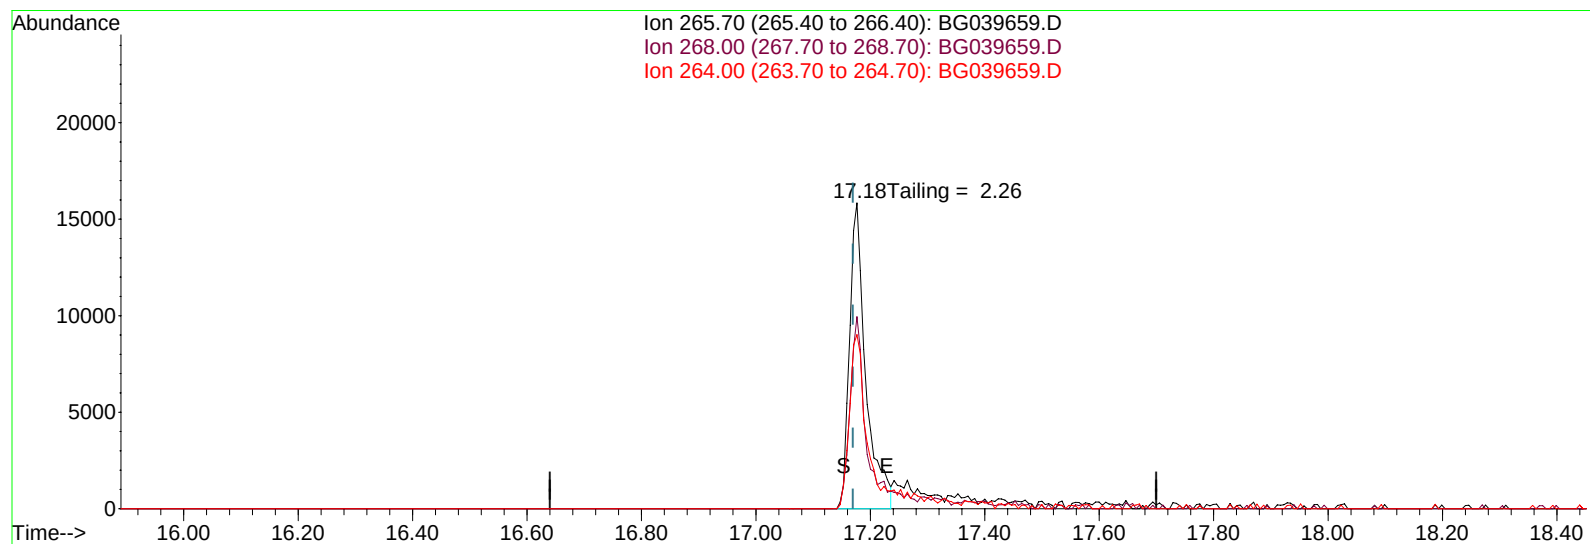

TIC: BG039659.D

(70) Pentachlorophenol (C)

17.177min (+0.007) 9970.20ng

response 31237

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.81
264.00	65.10	56.94
0.00	0.00	0.00