


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022819\
 Data File : BG039659.D
 Acq On : 28 Feb 2019 13:03
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 01 06:15:02 2019

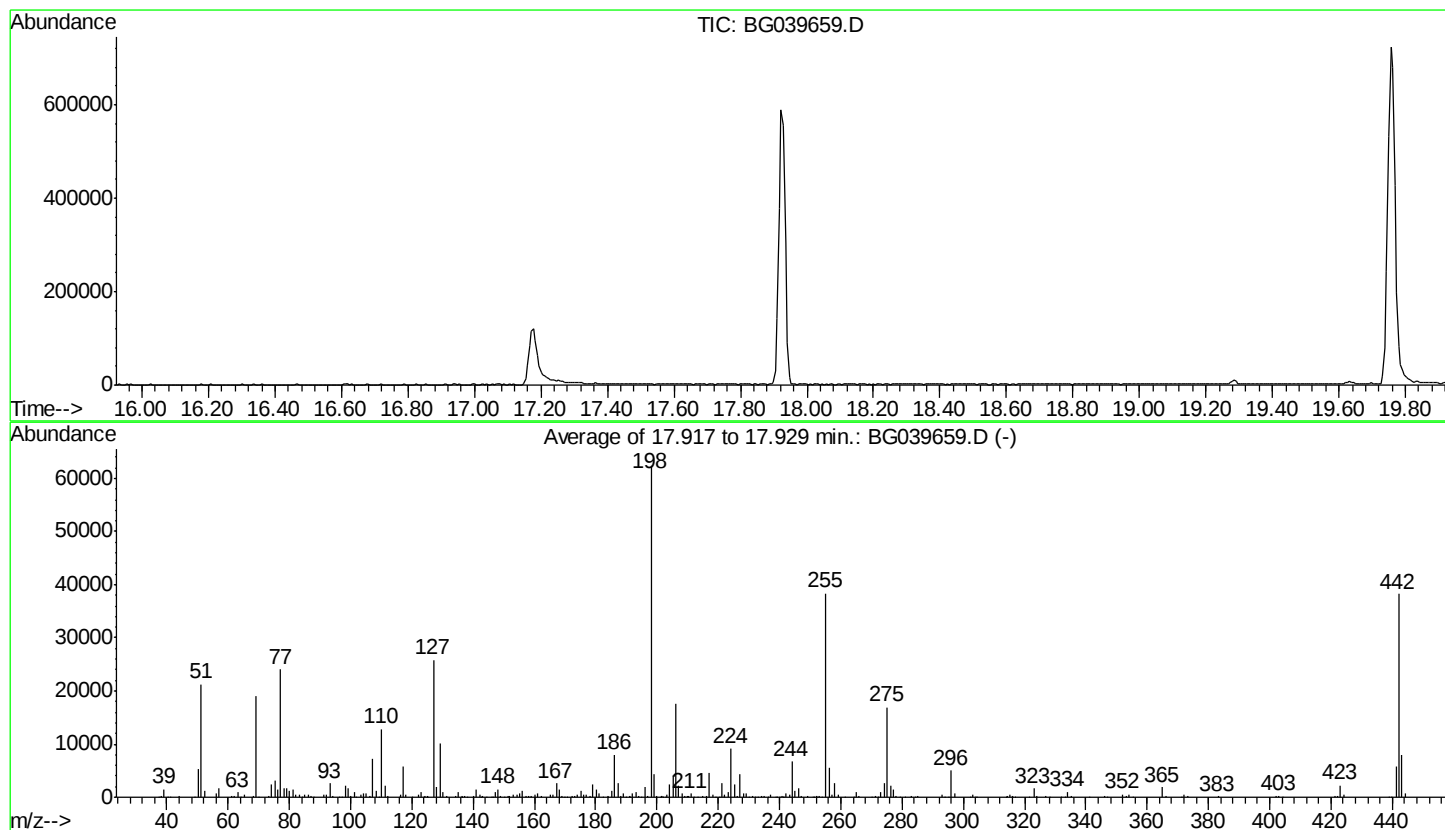

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	21317	PASS
68	69	0.00	2	1.0	183	PASS
69	198	0.00	100	30.6	19077	PASS
70	69	0.00	2	0.3	55	PASS
127	198	10	80	41.4	25805	PASS
197	198	0.00	2	0.4	224	PASS
198	198	100	100	100.0	62397	PASS
199	198	5	9	6.8	4224	PASS
275	198	10	60	27.1	16900	PASS
365	198	1	100	3.0	1876	PASS
441	198	0.01	100	9.3	5785	PASS
442	198	50	100	61.2	38189	PASS
443	442	15	24	20.6	7868	PASS