
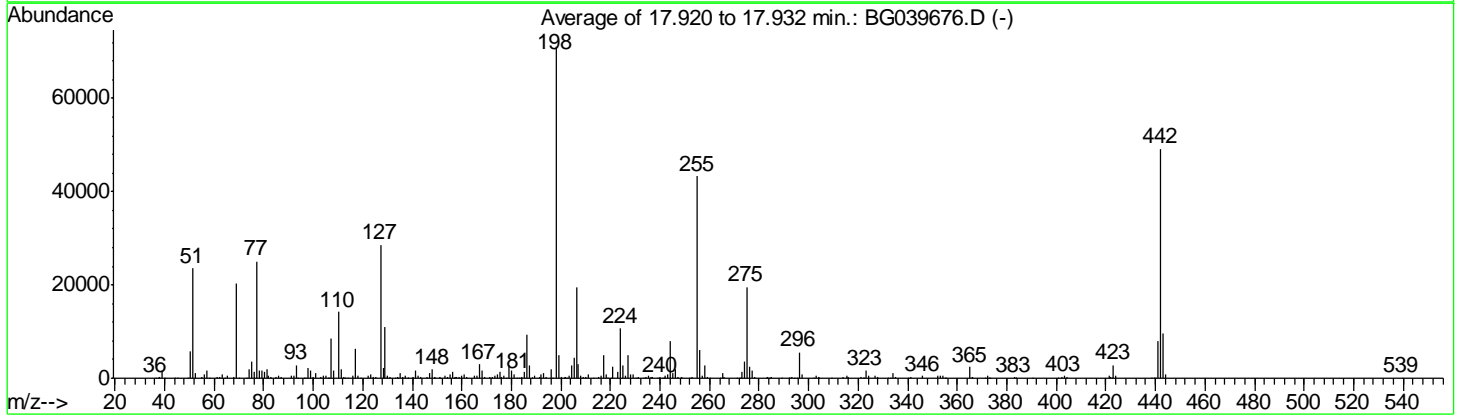


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022819\
 Data File : BG039676.D
 Acq On : 1 Mar 2019 2:08
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 01 06:15:02 2019

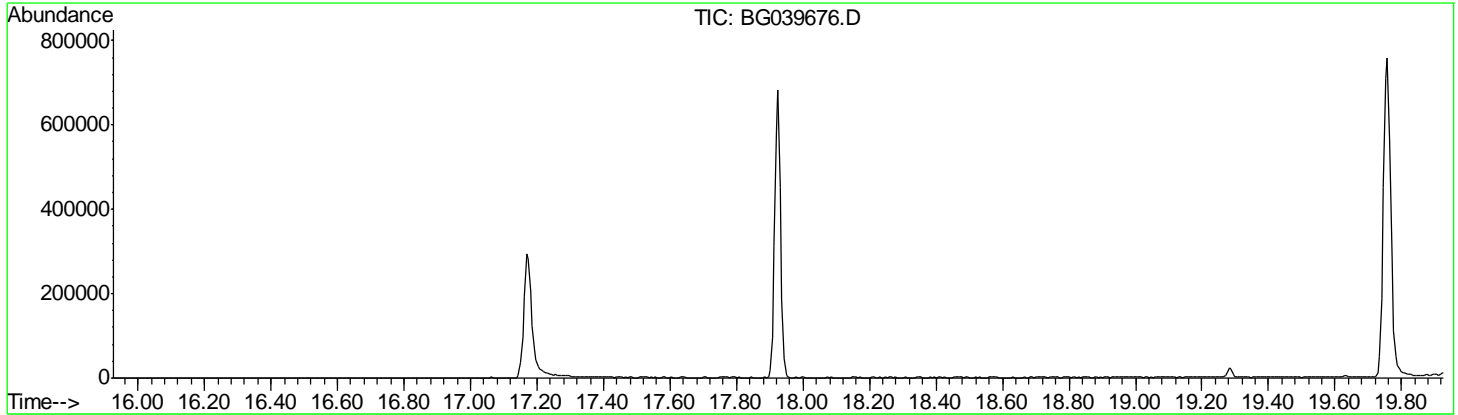

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	23609	PASS
68	69	0.00	2	1.3	262	PASS
69	198	0.00	100	28.5	20259	PASS
70	69	0.00	2	0.3	65	PASS
127	198	10	80	40.3	28661	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71122	PASS
199	198	5	9	7.0	4959	PASS
275	198	10	60	27.5	19545	PASS
365	198	1	100	3.5	2464	PASS
441	198	0.01	100	11.2	7941	PASS
442	198	50	100	69.3	49272	PASS
443	442	15	24	19.5	9585	PASS