

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
 Data File : BG056756.D
 Acq On : 28 Feb 2023 15:40
 Operator : CG/JU
 Sample : 01648-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZT4

Quant Time: Mar 01 00:01:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 23:55:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.421	152	15104	20.000	ng/ul	0.00
20) Naphthalene-d8	11.259	136	64040	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.020	164	51651	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.757	188	132551	20.000	ng/ul	0.00
79) Chrysene-d12	22.064	240	123146	20.000	ng/ul	0.00
88) Perylene-d12	25.584	264	132848	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.697	96	768	2.821	ng/uL	0.00
4) Pyridine-d5	4.138	84	127	0.116	ng/ul	0.00
7) Phenol-d5	7.540	99	17514	11.588	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.722	67	10944	11.870	ng/ul	0.00
11) 2-Chlorophenol-d4	7.940	132	12503	12.457	ng/ul	0.00
15) 4-Methylphenol-d8	9.103	113	13085	11.330	ng/ul	0.00
21) Nitrobenzene-d5	9.591	128	6796	12.663	ng/ul	0.00
24) 2-Nitrophenol-d4	10.319	143	7855	12.296	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.860	165	15485	12.867	ng/ul	0.00
31) 4-Chloroaniline-d4	11.377	131	9557	6.088	ng/ul	0.00
46) Dimethylphthalate-d6	14.408	166	57045	13.689	ng/ul	0.00
49) Acenaphthylene-d8	14.720	160	62483	13.192	ng/ul	0.00
54) 4-Nitrophenol-d4	15.172	143	7443	10.359	ng/ul	0.00
60) Fluorene-d10	16.001	176	52842	13.708	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.101	200	10867	12.254	ng/ul	0.00
73) Anthracene-d10	17.851	188	91480	14.226	ng/ul	0.00
81) Pyrene-d10	20.108	212	109714	13.166	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.343	264	100400	14.002	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	9.250	105	5189	2.624	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
Data File : BG056756.D
Acq On : 28 Feb 2023 15:40
Operator : CG/JU
Sample : 01648-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZT4

Quant Time: Mar 01 00:01:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 28 23:55:08 2023
Response via : Initial Calibration

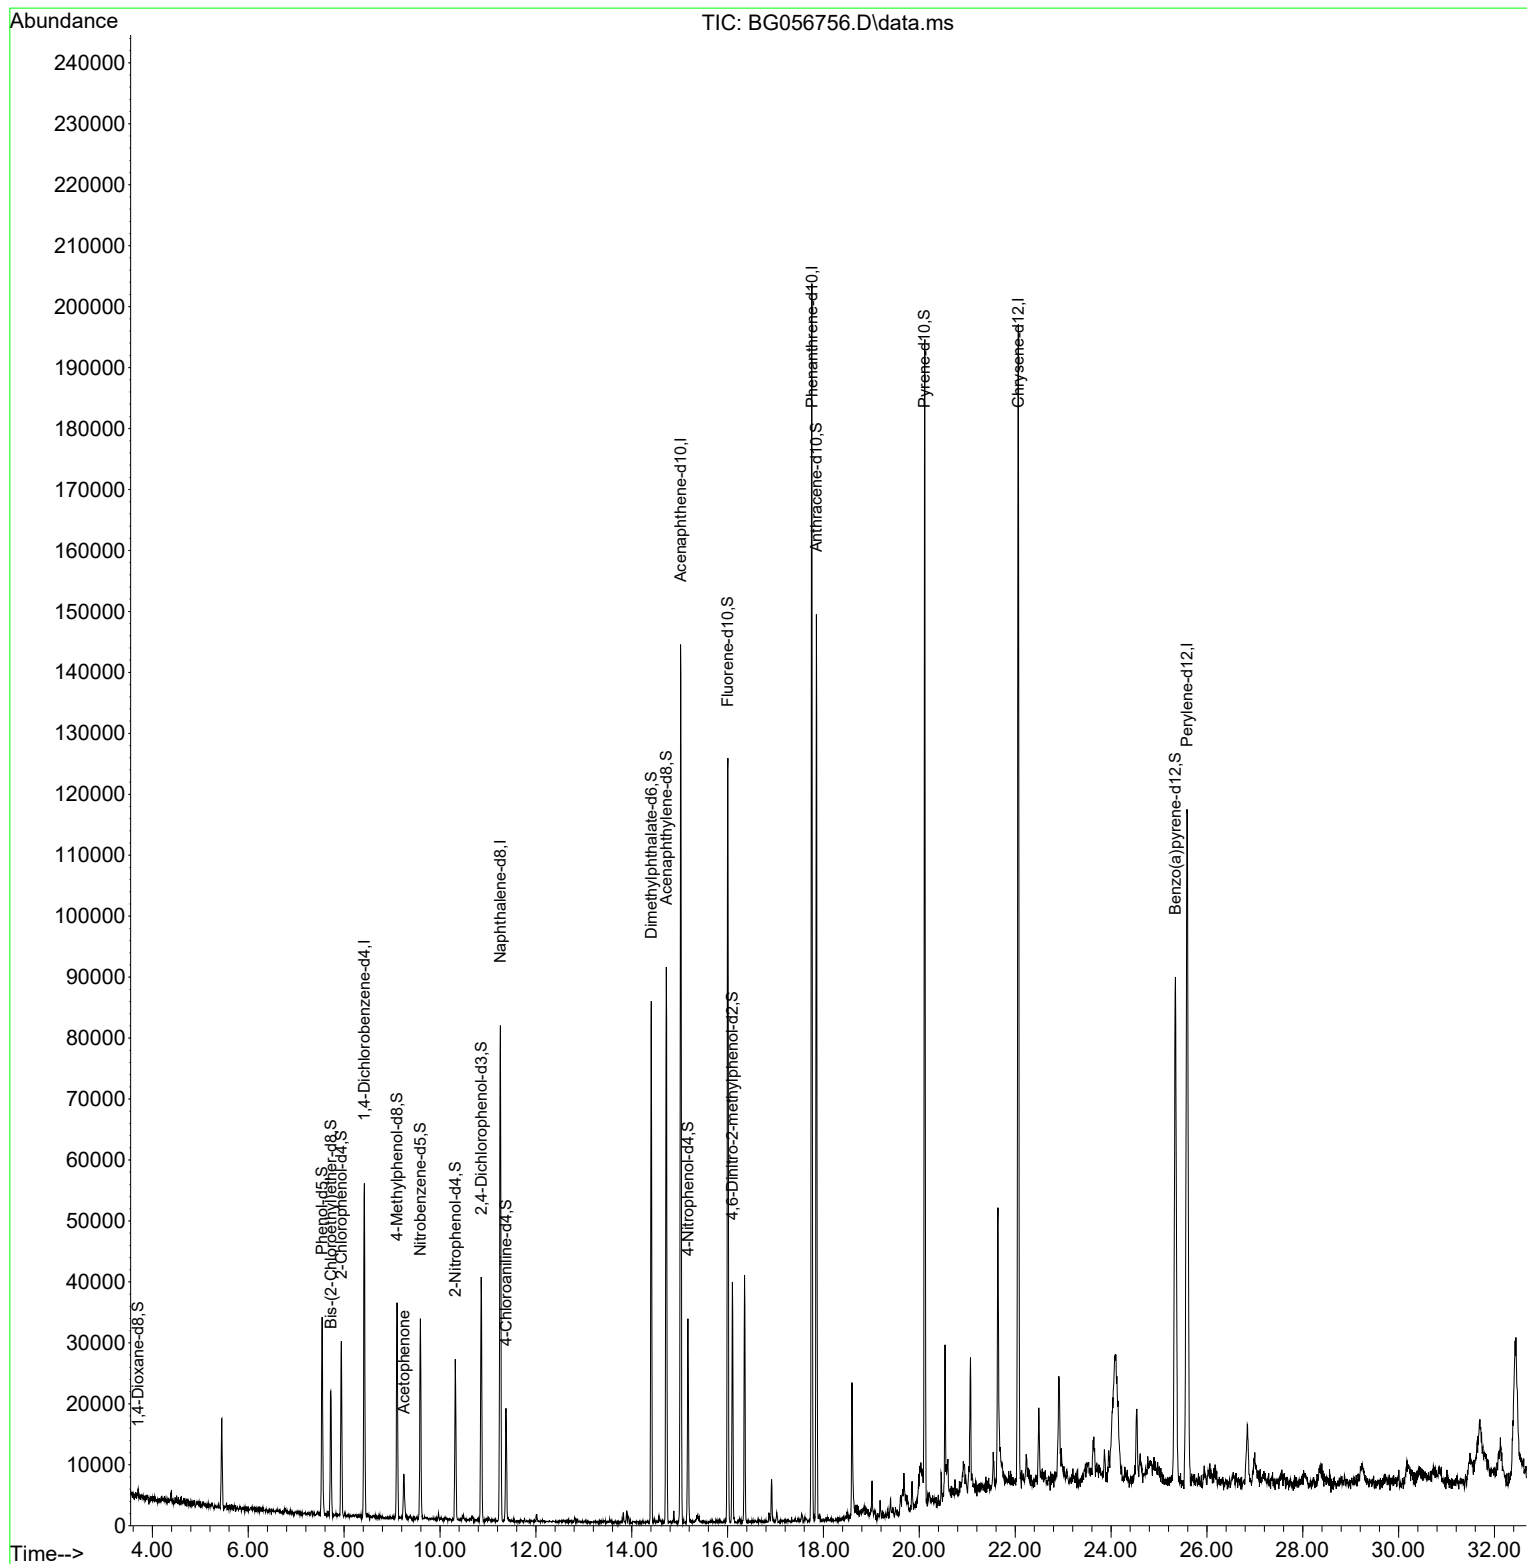

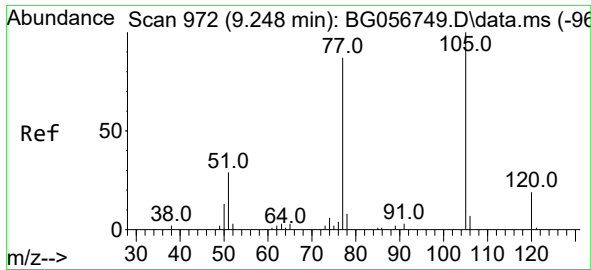

#16
 Acetophenone
 Concen: 2.624 ng/ul
 RT: 9.250 min Scan# 91
 Delta R.T. 0.002 min
 Lab File: BG056756.D
 Acq: 28 Feb 2023 15:40

Instrument :
 BNA_G
 ClientSampleId :
 DBZT4

Tgt Ion:105 Resp: 5189
 Ion Ratio Lower Upper
 105 100
 77 82.0 71.4 107.0
 51 19.7 23.6 35.4#

