




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
 Data File : BG056750.D
 Acq On : 28 Feb 2023 10:01
 Operator : CG/JU
 Sample : PB151019BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK019

Manual IntegrationsAPPROVED

Quant Time: Mar 01 00:00:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 23:55:08 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/01/2023
 Supervised By :Jagrut Upadhyay 03/01/2023

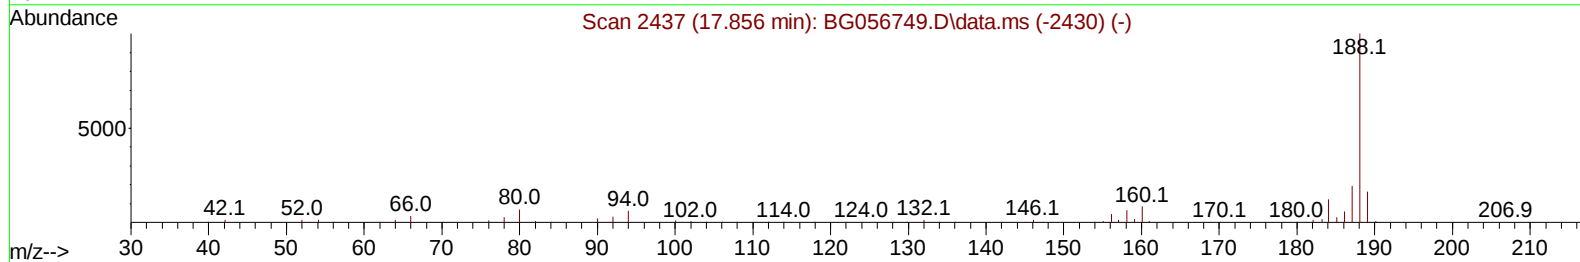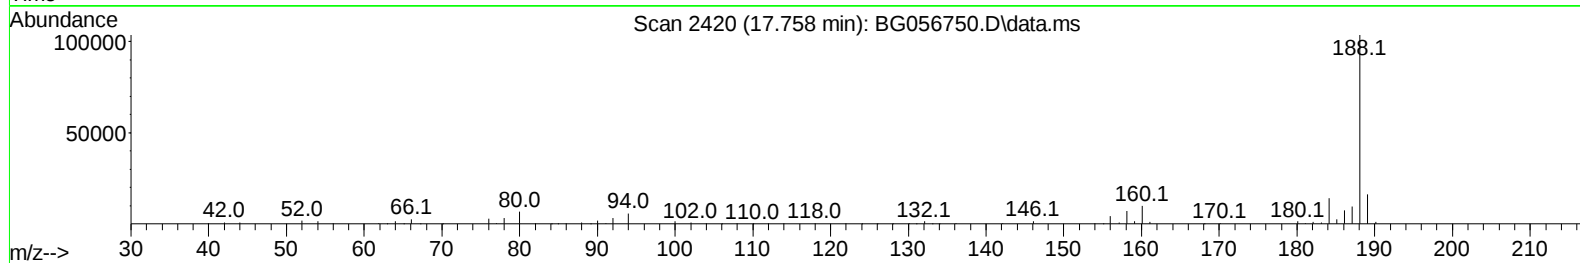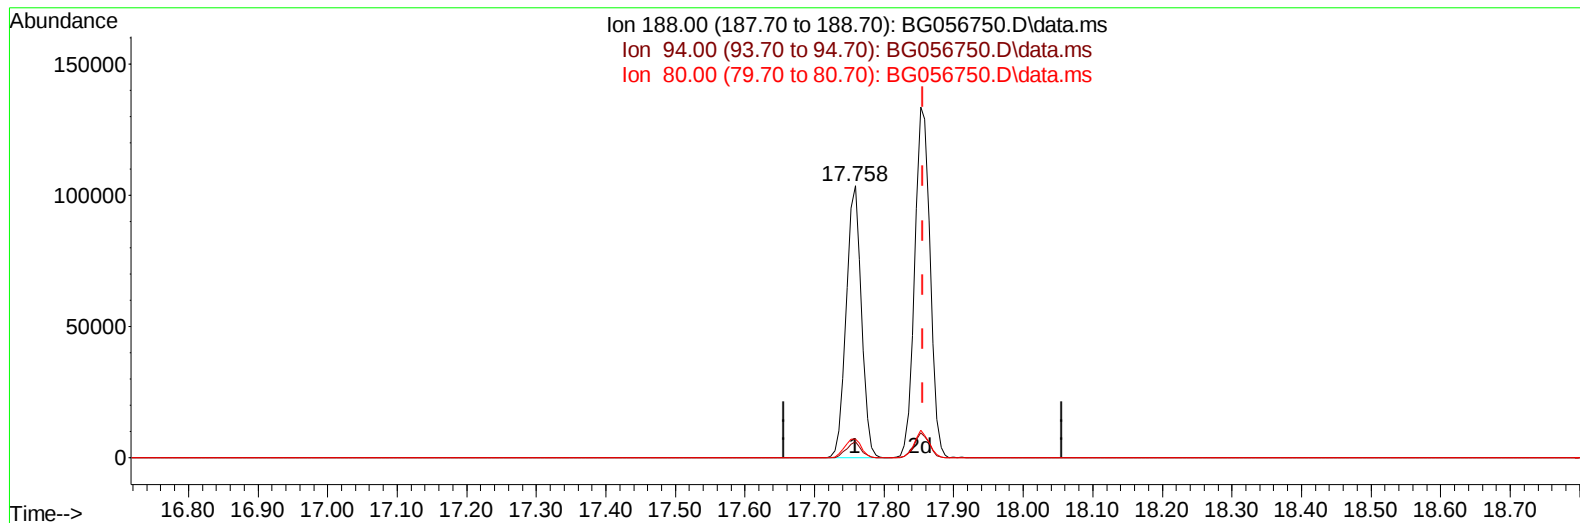

TIC: BG056750.D\data.ms

(73) Anthracene-d10 (S)

17.758min (-0.097) 20.61 ng/u1

response 156058

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	5.90	5.73
80.00	7.20	6.74
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
 Data File : BG056750.D
 Acq On : 28 Feb 2023 10:01
 Operator : CG/JU
 Sample : PB151019BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK019

Manual IntegrationsAPPROVED

Quant Time: Mar 01 00:00:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 23:55:08 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/01/2023
 Supervised By :Jagrut Upadhyay 03/01/2023

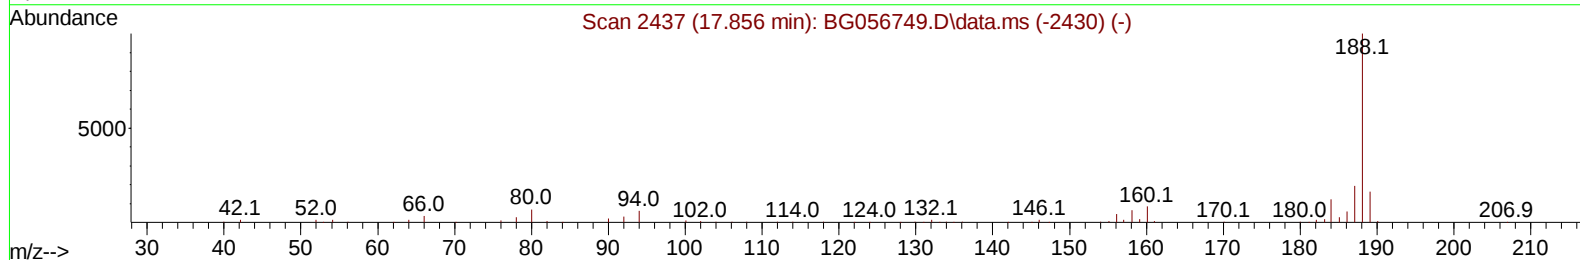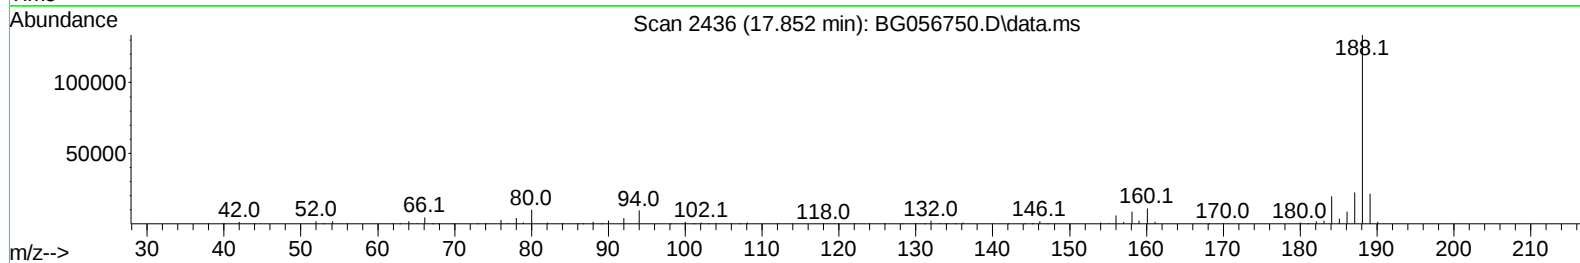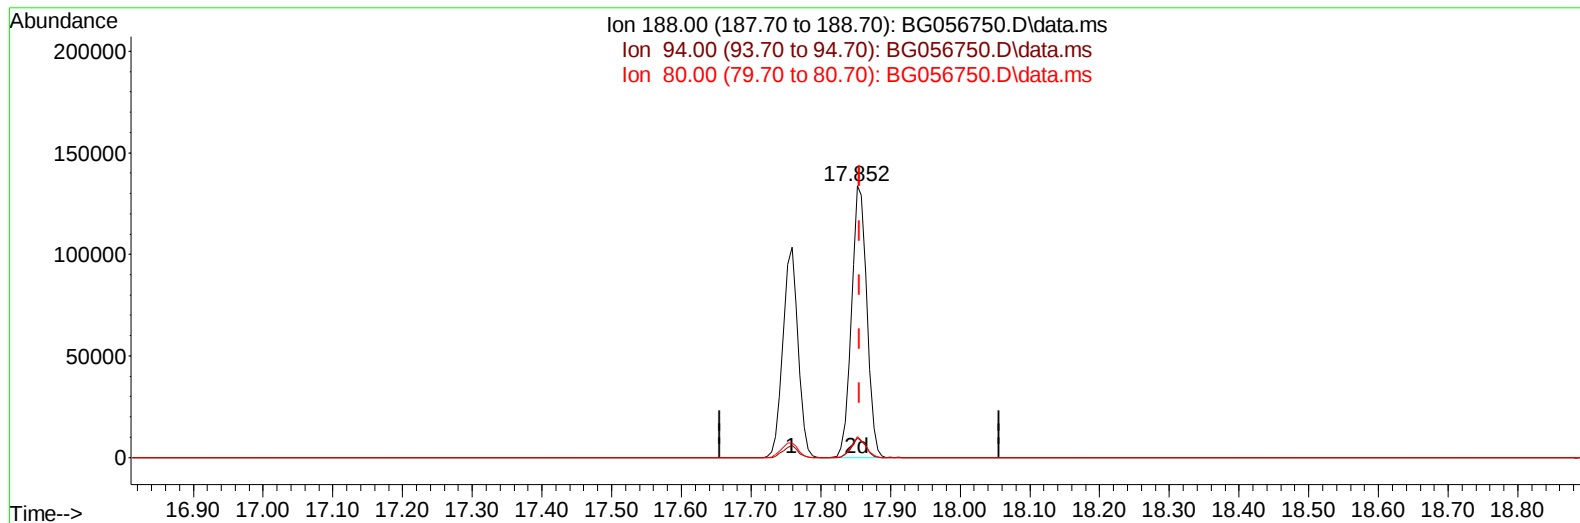

TIC: BG056750.D\data.ms

(73) Anthracene-d10 (S)

17.852min (-0.003) 26.97 ng/ul m

response 204159

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	5.90	7.12#
80.00	7.20	7.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
 Data File : BG056750.D
 Acq On : 28 Feb 2023 10:01
 Operator : CG/JU
 Sample : PB151019BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK019

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/01/2023
 Supervised By :Jagrut Upadhyay 03/01/2023

Quant Time: Mar 01 00:00:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 23:55:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.422	152	17018	20.000	ng/ul	0.00
20) Naphthalene-d8	11.260	136	75163	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	15.020	164	60043	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.758	188	156058	20.000	ng/ul	0.00
79) Chrysene-d12	22.065	240	153471	20.000	ng/ul	0.00
88) Perylene-d12	25.590	264	161122	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.698	96	2174	7.086	ng/uL	0.00
4) Pyridine-d5	4.139	84	33988	27.447	ng/ul	0.00
7) Phenol-d5	7.541	99	43528	25.560	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.723	67	28737	27.664	ng/ul	0.00
11) 2-Chlorophenol-d4	7.941	132	29468	26.057	ng/ul	0.00
15) 4-Methylphenol-d8	9.104	113	32790	25.199	ng/ul	0.00
21) Nitrobenzene-d5	9.592	128	16055	25.488	ng/ul	0.00
24) 2-Nitrophenol-d4	10.320	143	19862	26.490	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.861	165	35104	24.852	ng/ul	0.00
31) 4-Chloroaniline-d4	11.378	131	46189	25.071	ng/ul	0.00
46) Dimethylphthalate-d6	14.409	166	133768	27.613	ng/ul	0.00
49) Acenaphthylene-d8	14.721	160	146958	26.691	ng/ul	0.00
54) 4-Nitrophenol-d4	15.173	143	21451	25.683	ng/ul	0.00
60) Fluorene-d10	16.008	176	121871	27.196	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.107	200	23703	22.702	ng/ul	0.00
73) Anthracene-d10	17.852	188	204159m	26.966	ng/ul	0.00
81) Pyrene-d10	20.115	212	246826	23.767	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.350	264	230812	26.540	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
Data File : BG056750.D
Acq On : 28 Feb 2023 10:01
Operator : CG/JU
Sample : PB151019BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK019

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/01/2023
Supervised By :Jagrut Upadhyay 03/01/2023

Quant Time: Mar 01 00:00:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 28 23:55:08 2023
Response via : Initial Calibration

