




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
 Data File : BG056755.D
 Acq On : 28 Feb 2023 14:58
 Operator : CG/JU
 Sample : 01648-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZT1

Manual IntegrationsAPPROVED

Quant Time: Mar 01 00:01:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 23:55:08 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/01/2023
 Supervised By :Jagrut Upadhyay 03/01/2023

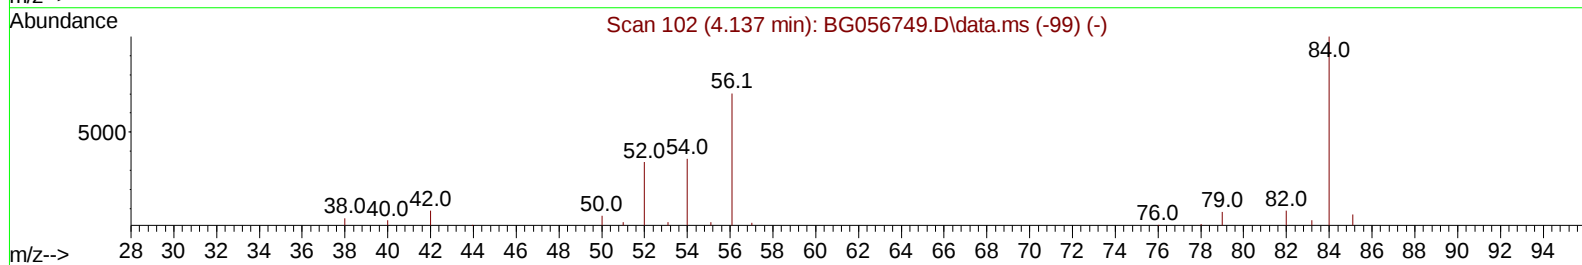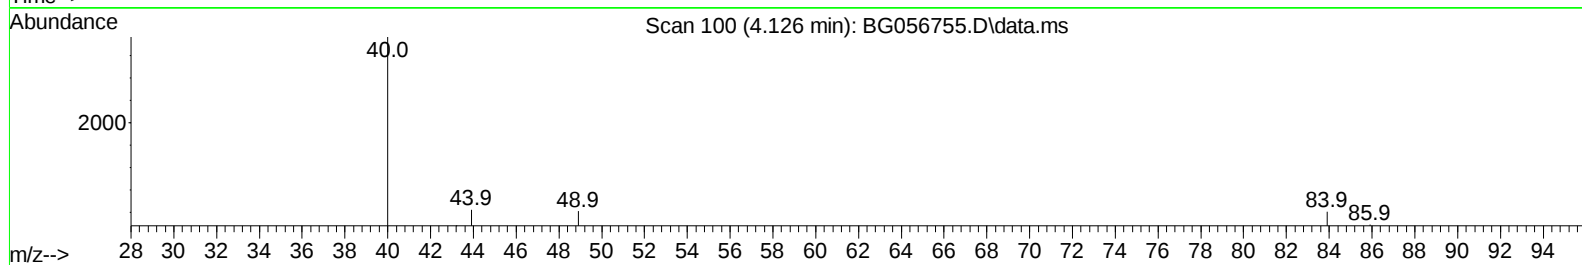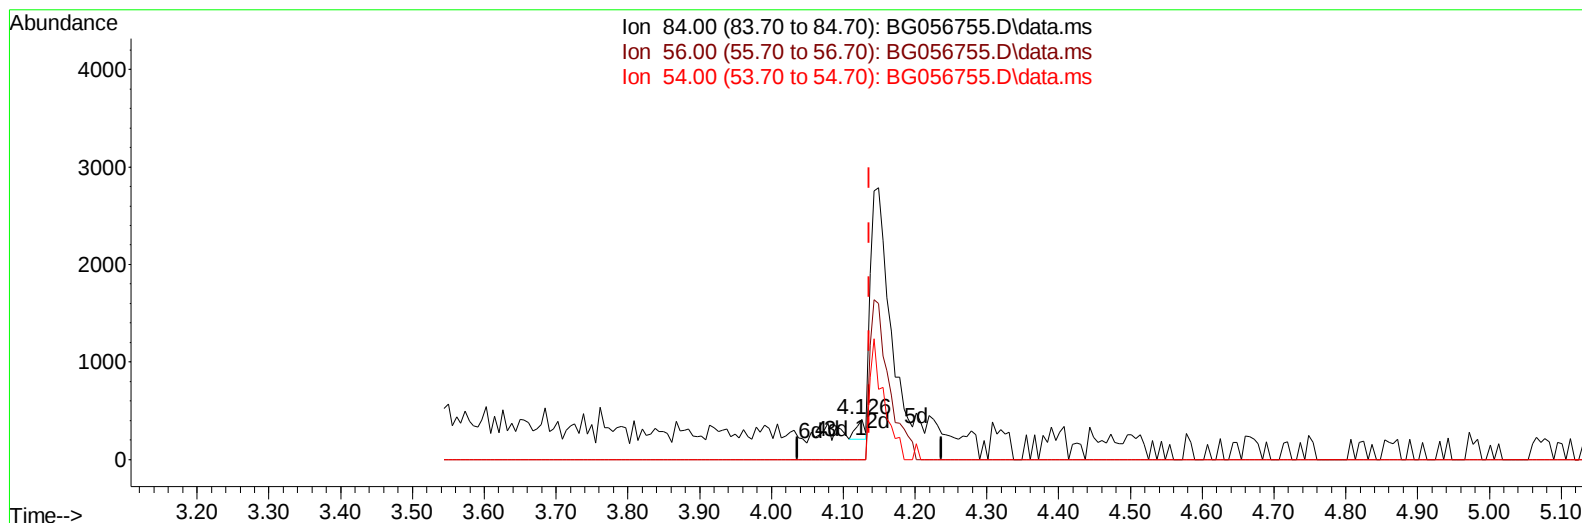

TIC: BG056755.D\data.ms

(4) Pyridine-d5 (S)

4.126min (-0.011) 0.14 ng/u1

response 171

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	67.40	0.00#
54.00	38.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
 Data File : BG056755.D
 Acq On : 28 Feb 2023 14:58
 Operator : CG/JU
 Sample : 01648-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZT1

Manual IntegrationsAPPROVED

Quant Time: Mar 01 00:01:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 23:55:08 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/01/2023
 Supervised By :Jagrut Upadhyay 03/01/2023

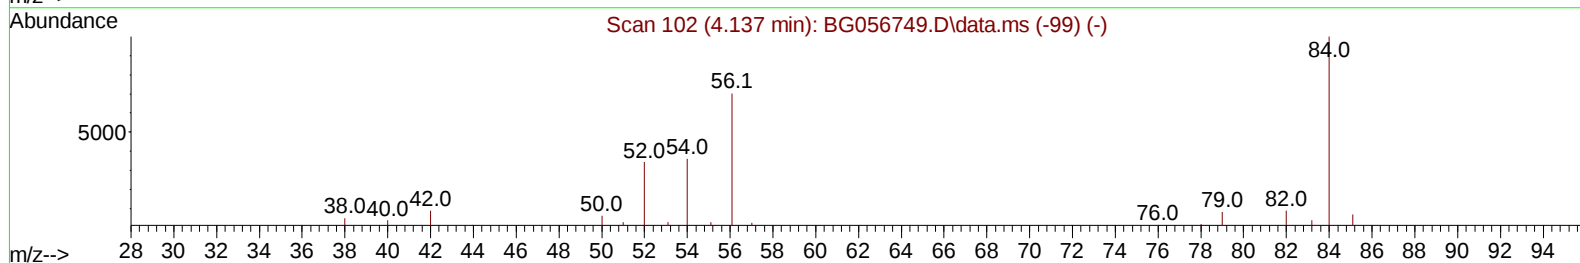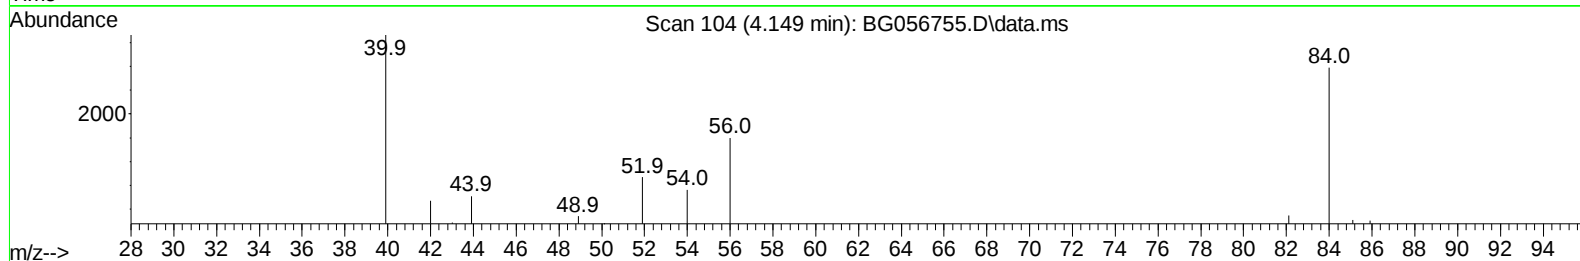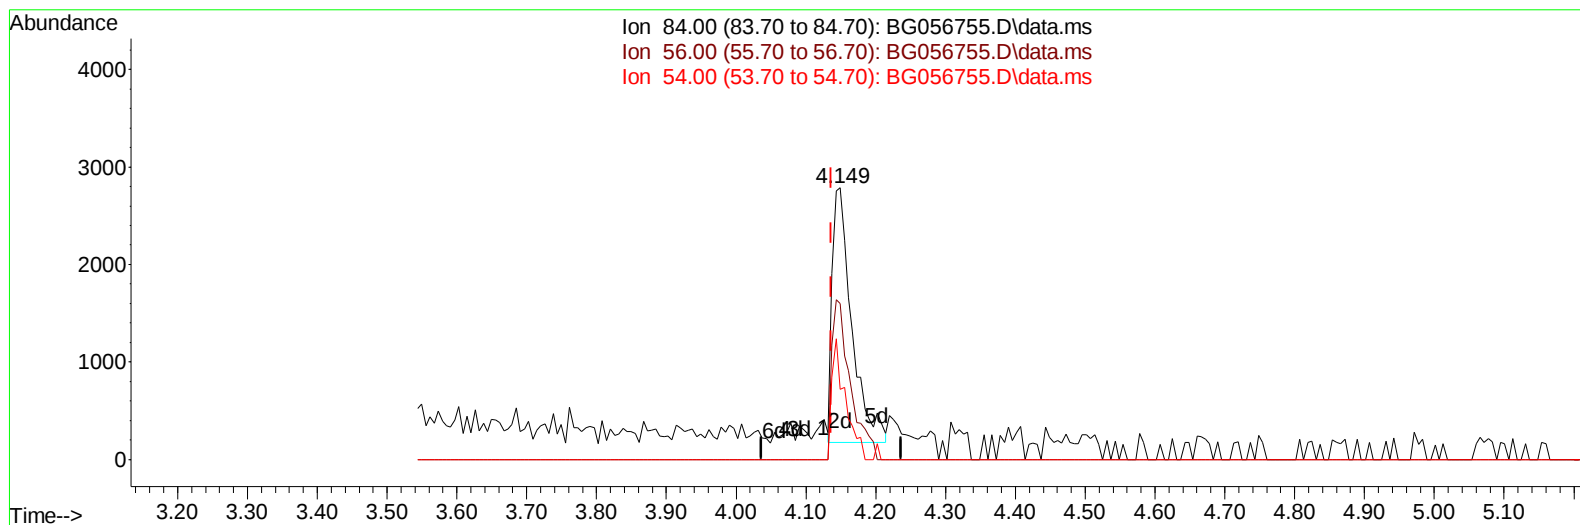

TIC: BG056755.D\data.ms

(4) Pyridine-d5 (S)

4.149min (+ 0.013) 4.19 ng/u1 m

response 5033

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	67.40	57.41
54.00	38.20	25.85#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
 Data File : BG056755.D
 Acq On : 28 Feb 2023 14:58
 Operator : CG/JU
 Sample : 01648-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZT1

Manual IntegrationsAPPROVED

Quant Time: Mar 01 00:01:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 23:55:08 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/01/2023
 Supervised By :Jagrut Upadhyay 03/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.421	152	16499	20.000	ng/ul	0.00
20) Naphthalene-d8	11.258	136	69845	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.025	164	55653	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.757	188	145010	20.000	ng/ul	0.00
79) Chrysene-d12	22.063	240	137413	20.000	ng/ul	0.00
88) Perylene-d12	25.589	264	146031	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.703	96	978	3.288	ng/uL	0.00
4) Pyridine-d5	4.149	84	5033m	4.192	ng/ul	0.01
7) Phenol-d5	7.539	99	27763	16.815	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.721	67	17046	16.926	ng/ul	0.00
11) 2-Chlorophenol-d4	7.939	132	18336	16.723	ng/ul	0.00
15) 4-Methylphenol-d8	9.108	113	21547	17.080	ng/ul	0.00
21) Nitrobenzene-d5	9.590	128	10099	17.254	ng/ul	0.00
24) 2-Nitrophenol-d4	10.318	143	12077	17.333	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.859	165	24582	18.728	ng/ul	0.00
31) 4-Chloroaniline-d4	11.376	131	16269	9.503	ng/ul	0.00
46) Dimethylphthalate-d6	14.408	166	88064	19.612	ng/ul	0.00
49) Acenaphthylene-d8	14.719	160	95270	18.668	ng/ul	0.00
54) 4-Nitrophenol-d4	15.172	143	14136	18.260	ng/ul	0.00
60) Fluorene-d10	16.006	176	79873	19.230	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.100	200	16759	17.274	ng/ul	0.00
73) Anthracene-d10	17.851	188	129726	18.440	ng/ul	0.00
81) Pyrene-d10	20.113	212	164584	17.700	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.342	264	148462	18.835	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
Data File : BG056755.D
Acq On : 28 Feb 2023 14:58
Operator : CG/JU
Sample : 01648-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZT1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/01/2023
Supervised By :Jagrut Upadhyay 03/01/2023

Quant Time: Mar 01 00:01:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 28 23:55:08 2023
Response via : Initial Calibration

