




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
 Data File : BG056757.D
 Acq On : 28 Feb 2023 16:21
 Operator : CG/JU
 Sample : 01648-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZT7

Manual IntegrationsAPPROVED

Quant Time: Mar 01 00:29:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 23:55:08 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/01/2023
 Supervised By :Jagrut Upadhyay 03/01/2023

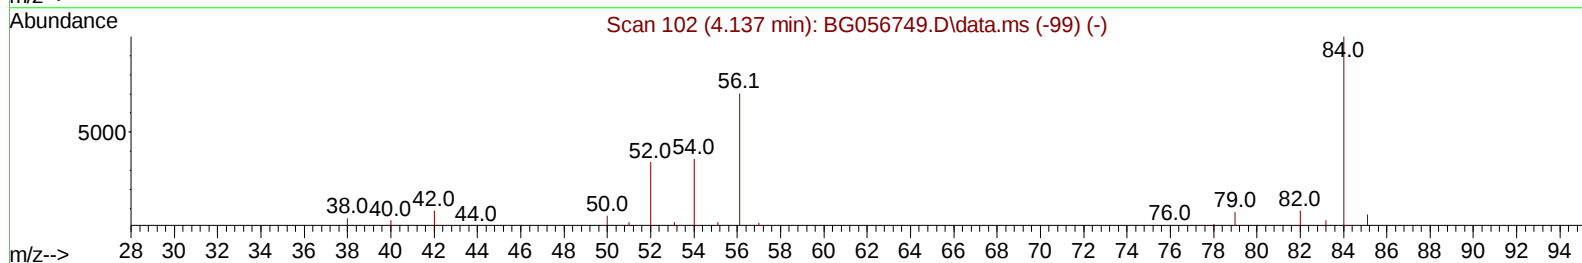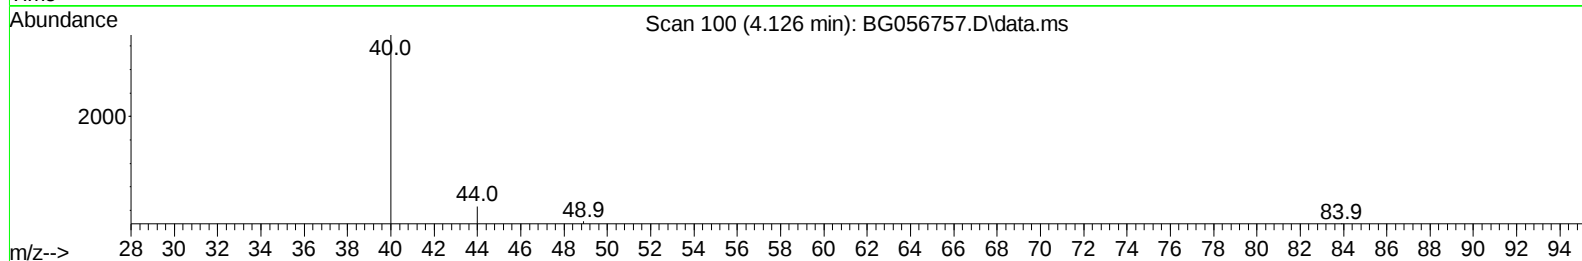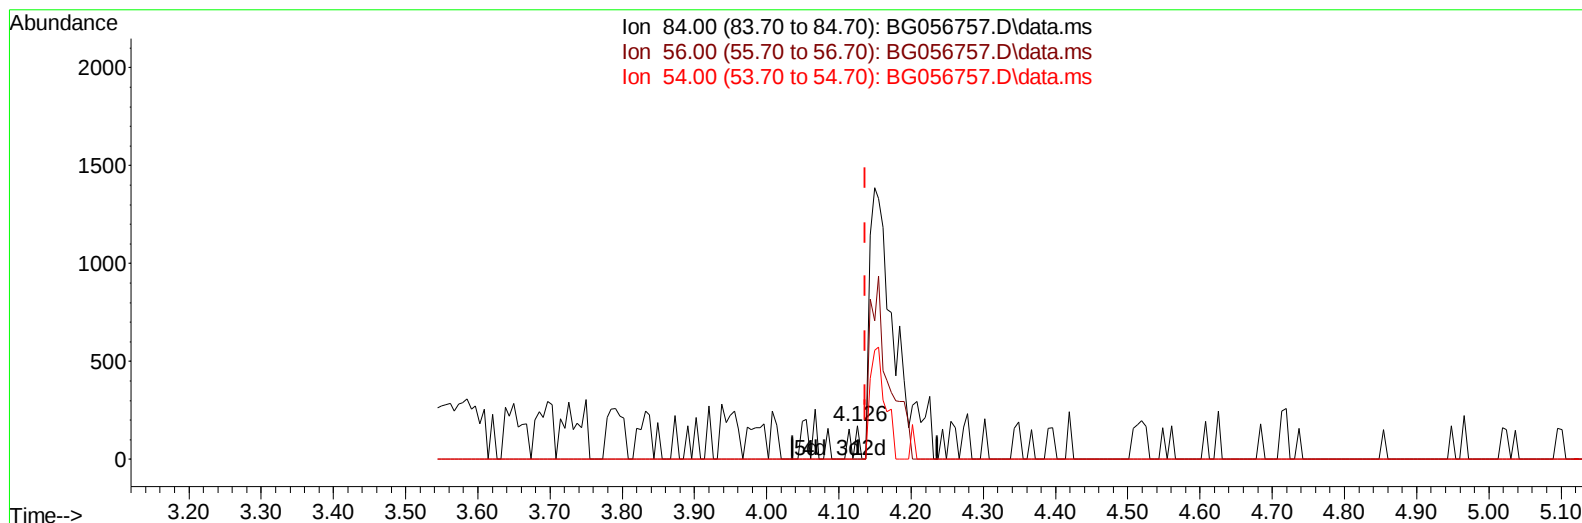

TIC: BG056757.D\data.ms

(4) Pyridine-d5 (S)

4.126min (-0.011) 0.05 ng/u1

response 60

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	67.40	0.00#
54.00	38.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
 Data File : BG056757.D
 Acq On : 28 Feb 2023 16:21
 Operator : CG/JU
 Sample : 01648-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZT7

Manual IntegrationsAPPROVED

Quant Time: Mar 01 00:29:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 23:55:08 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/01/2023
 Supervised By :Jagrut Upadhyay 03/01/2023

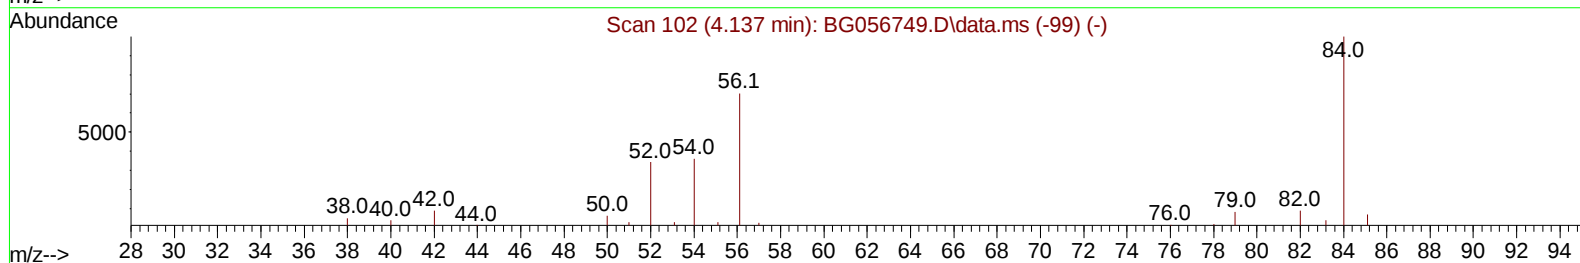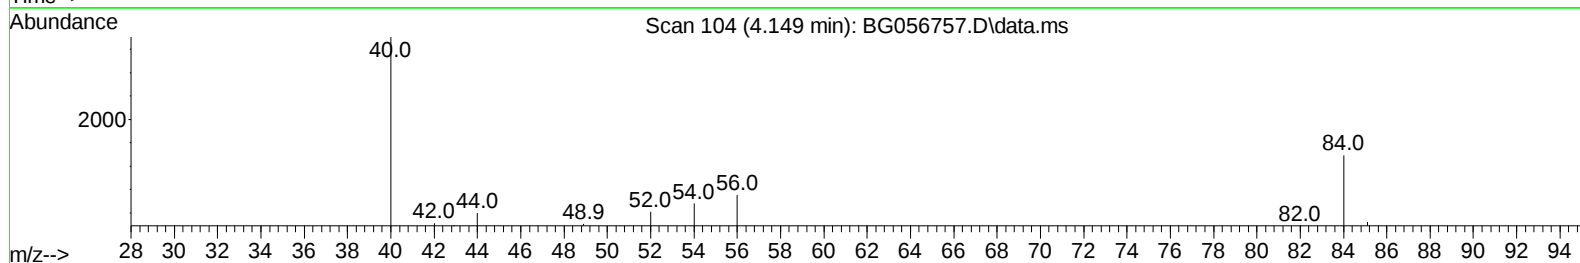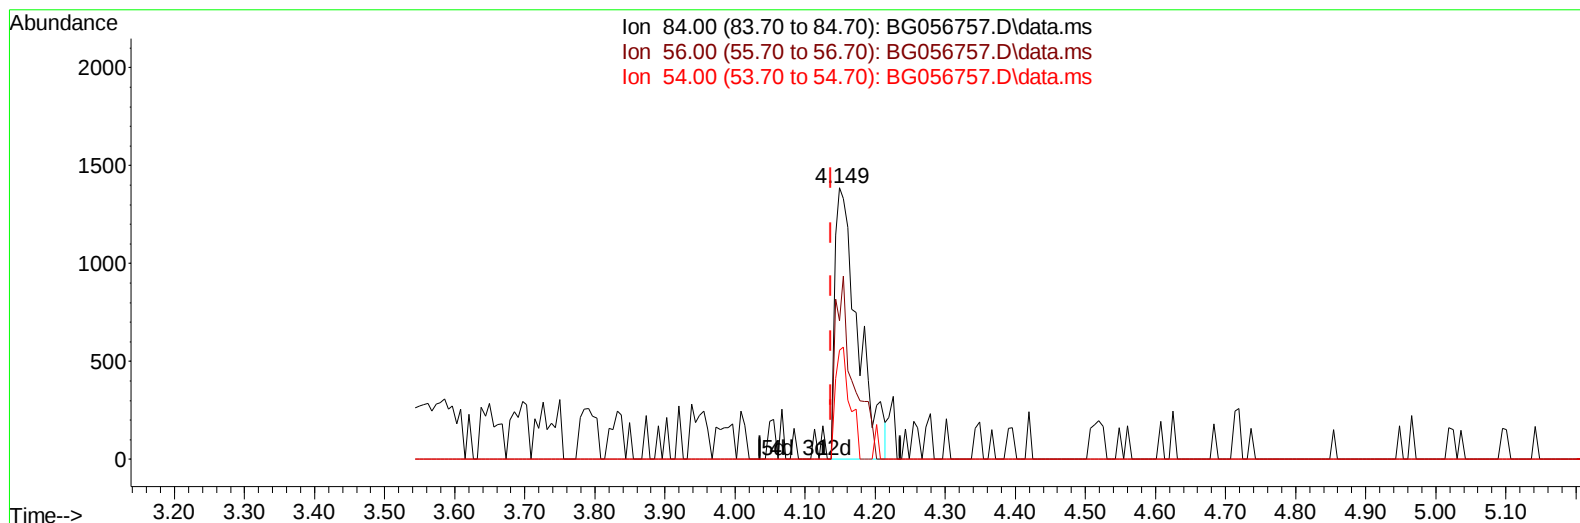

TIC: BG056757.D\data.ms

(4) Pyridine-d5 (S)

4.149min (+ 0.012) 2.81 ng/ul m

response 3171

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	67.40	51.08#
54.00	38.20	40.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
 Data File : BG056757.D
 Acq On : 28 Feb 2023 16:21
 Operator : CG/JU
 Sample : 01648-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZT7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/01/2023
 Supervised By :Jagrut Upadhyay 03/01/2023

Quant Time: Mar 01 00:29:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 23:55:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.421	152	15508	20.000	ng/ul	0.00
20) Naphthalene-d8	11.253	136	65421	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	15.019	164	52004	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.757	188	135824	20.000	ng/ul	0.00
79) Chrysene-d12	22.063	240	125620	20.000	ng/ul	0.00
88) Perylene-d12	25.583	264	132941	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.691	96	1030	3.684	ng/uL	0.00
4) Pyridine-d5	4.149	84	3171m	2.810	ng/ul	0.01
7) Phenol-d5	7.539	99	22455	14.470	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.721	67	13672	14.443	ng/ul	0.00
11) 2-Chlorophenol-d4	7.939	132	15752	15.285	ng/ul	0.00
15) 4-Methylphenol-d8	9.102	113	15710	13.249	ng/ul	0.00
21) Nitrobenzene-d5	9.590	128	8511	15.524	ng/ul	0.00
24) 2-Nitrophenol-d4	10.318	143	10611	16.259	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.859	165	18649	15.168	ng/ul	0.00
31) 4-Chloroaniline-d4	11.382	131	15164	9.456	ng/ul	0.00
46) Dimethylphthalate-d6	14.408	166	72973	17.392	ng/ul	0.00
49) Acenaphthylene-d8	14.719	160	78690	16.501	ng/ul	0.00
54) 4-Nitrophenol-d4	15.171	143	10339	14.292	ng/ul	0.00
60) Fluorene-d10	16.006	176	65439	16.860	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.100	200	13450	14.801	ng/ul	0.00
73) Anthracene-d10	17.851	188	110616	16.787	ng/ul	0.00
81) Pyrene-d10	20.113	212	137901	16.223	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.342	264	127940	17.830	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
Data File : BG056757.D
Acq On : 28 Feb 2023 16:21
Operator : CG/JU
Sample : 01648-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZT7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/01/2023
Supervised By :Jagrut Upadhyay 03/01/2023

Quant Time: Mar 01 00:29:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 28 23:55:08 2023
Response via : Initial Calibration

