

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
 Data File : BG056751.D
 Acq On : 28 Feb 2023 12:02
 Operator : CG/JU
 Sample : 01648-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBAF5

Quant Time: Mar 01 00:14:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 28 23:55:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.419	152	14135	20.000	ng/u1	0.00
20) Naphthalene-d8	11.257	136	58647	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	15.023	164	47697	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.755	188	115610	20.000	ng/u1	0.00
79) Chrysene-d12	22.068	240	106323	20.000	ng/u1	0.00
88) Perylene-d12	25.593	264	117654	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.689	96	1334	5.235	ng/uL	0.00
4) Pyridine-d5	0.000	84	0	0.000	ng/u1	
7) Phenol-d5	7.538	99	35984	25.440	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.720	67	22319	25.868	ng/u1	0.00
11) 2-Chlorophenol-d4	7.937	132	23843	25.383	ng/u1	0.00
15) 4-Methylphenol-d8	9.106	113	27013	24.994	ng/u1	0.00
21) Nitrobenzene-d5	9.588	128	12916	26.280	ng/u1	0.00
24) 2-Nitrophenol-d4	10.317	143	14347	24.523	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.857	165	29682	26.931	ng/u1	0.00
31) 4-Chloroaniline-d4	11.374	131	18527	12.888	ng/u1	0.00
46) Dimethylphthalate-d6	14.406	166	106802	27.753	ng/u1	0.00
49) Acenaphthylene-d8	14.723	160	114815	26.251	ng/u1	0.00
54) 4-Nitrophenol-d4	15.176	143	17297	26.070	ng/u1	0.00
60) Fluorene-d10	16.004	176	97621	27.423	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	16.104	200	14858	19.209	ng/u1	0.00
73) Anthracene-d10	17.855	188	183966	32.800	ng/u1	0.00
81) Pyrene-d10	20.111	212	226471	31.478	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.352	264	211016	33.228	ng/u1	0.00
Target Compounds						
71) Pentachlorophenol	17.397	266	27260	30.501	ng/u1	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
Data File : BG056751.D
Acq On : 28 Feb 2023 12:02
Operator : CG/JU
Sample : 01648-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBAF5

Quant Time: Mar 01 00:14:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 28 23:55:08 2023
Response via : Initial Calibration

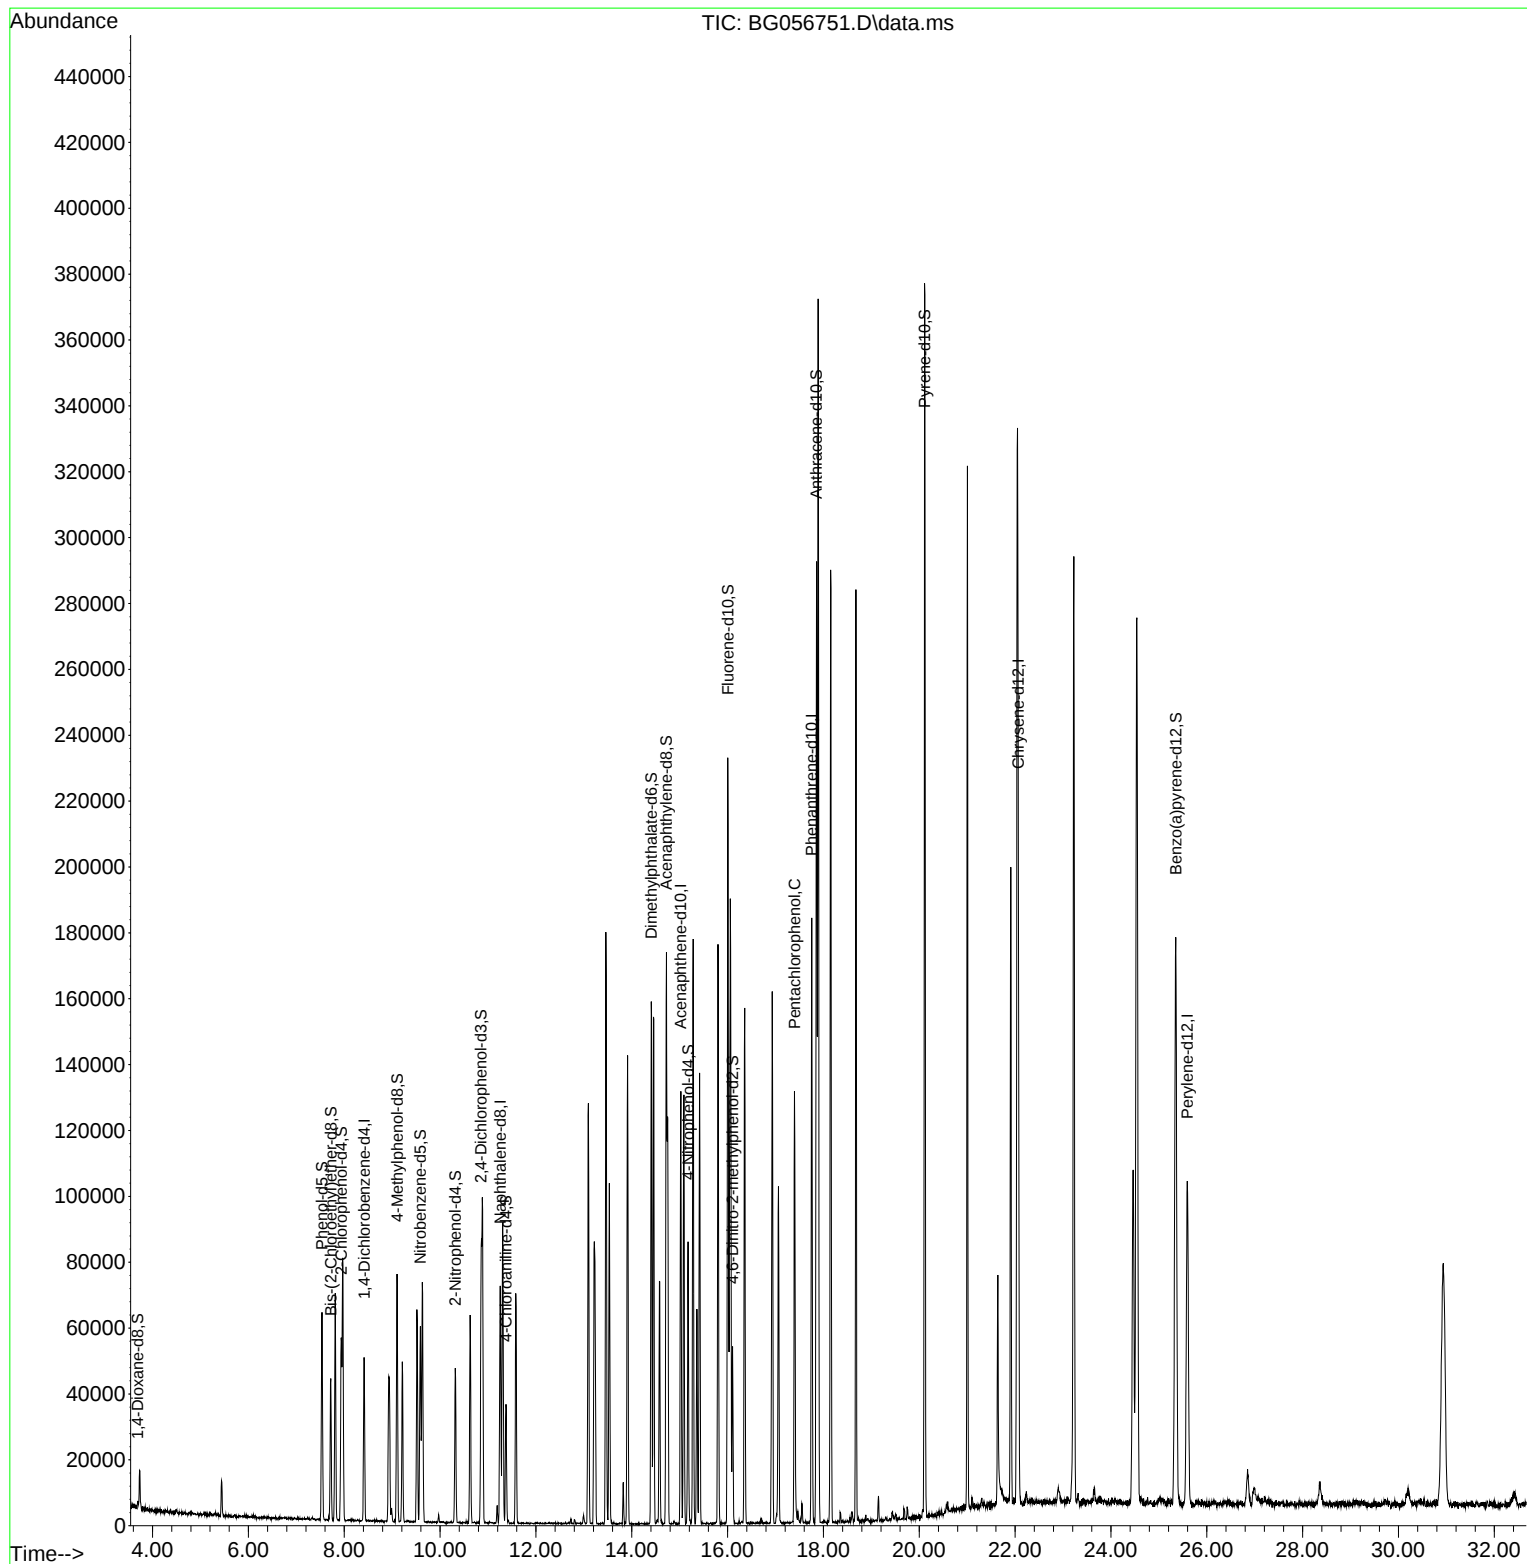

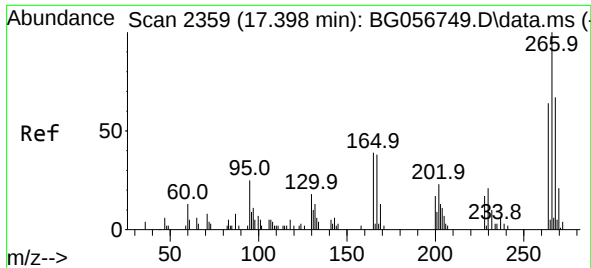

#71
 Pentachlorophenol
 Concen: 30.501 ng/ul
 RT: 17.397 min Scan# 21
 Delta R.T. -0.001 min
 Lab File: BG056751.D
 Acq: 28 Feb 2023 12:02

Instrument :
 BNA_G
 ClientSampleId :
 DBAF5

Tgt Ion:266 Resp: 27260
 Ion Ratio Lower Upper
 266 100
 264 60.2 49.9 74.9
 268 63.0 54.5 81.7

