

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
 Data File : BG056761.D
 Acq On : 28 Feb 2023 19:06
 Operator : CG/JU
 Sample : 01674-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.801	214	215	217	rBV2	1389	994	0.27%	0.059%
2	6.816	556	558	560	rVB3	921	663	0.18%	0.040%
3	6.840	560	562	563	rVB	783	518	0.14%	0.031%
4	6.857	563	565	568	rBV	696	681	0.18%	0.041%
5	6.945	578	580	581	rBV	705	475	0.13%	0.028%
6	7.092	604	605	608	rBV	884	629	0.17%	0.038%
7	7.204	622	624	628	rBV2	762	858	0.23%	0.051%
8	7.691	705	707	709	rBV2	560	518	0.14%	0.031%
9	7.750	715	717	721	rBV2	726	983	0.27%	0.059%
10	8.073	770	772	775	rBV2	620	796	0.22%	0.048%
11	8.297	809	810	812	rBV	984	507	0.14%	0.030%
12	8.367	818	822	823	rBV2	508	553	0.15%	0.033%
13	8.420	824	831	837	rVV	59963	100795	27.29%	6.031%
14	8.543	849	852	856	rBV2	853	1125	0.30%	0.067%
15	8.972	923	925	929	rBV2	427	497	0.13%	0.030%
16	9.912	1084	1085	1090	rVB	688	887	0.24%	0.053%
17	9.948	1090	1091	1094	rBV	400	479	0.13%	0.029%
18	9.989	1094	1098	1100	rVB2	513	606	0.16%	0.036%
19	10.200	1132	1134	1137	rBV	511	565	0.15%	0.034%
20	10.476	1178	1181	1183	rBV2	380	502	0.14%	0.030%
21	10.758	1227	1229	1231	rBV2	572	459	0.12%	0.027%
22	11.258	1306	1314	1322	rVB	89156	161460	43.71%	9.661%
23	12.075	1450	1453	1454	rBV2	562	573	0.16%	0.034%
24	12.598	1538	1542	1543	rBV2	375	557	0.15%	0.033%
25	12.950	1599	1602	1605	rVB2	452	563	0.15%	0.034%
26	13.749	1736	1738	1742	rVB	554	558	0.15%	0.033%
27	13.884	1759	1761	1768	rVB2	1419	1530	0.41%	0.092%
28	13.949	1768	1772	1773	rVB	442	548	0.15%	0.033%
29	14.008	1779	1782	1785	rVB	380	497	0.13%	0.030%
30	14.043	1785	1788	1791	rBV2	537	504	0.14%	0.030%
31	14.337	1836	1838	1841	rBV	380	447	0.12%	0.027%
32	14.542	1870	1873	1874	rBV	486	458	0.12%	0.027%
33	14.648	1887	1891	1893	rBV2	578	496	0.13%	0.030%
34	14.971	1942	1946	1948	rBV2	390	470	0.13%	0.028%
35	15.024	1948	1955	1961	rVB	175074	270322	73.19%	16.174%
36	15.353	2006	2011	2013	rBV	407	634	0.17%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
 Data File : BG056761.D
 Acq On : 28 Feb 2023 19:06
 Operator : CG/JU
 Sample : 01674-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

37	15.412	2017	2021	2023	rBV	567	553	0.15%	0.033%
38	15.447	2023	2027	2031	rVV	329	632	0.17%	0.038%
39	15.594	2049	2052	2055	rBV	381	470	0.13%	0.028%
40	15.964	2111	2115	2118	rBV	376	527	0.14%	0.032%
41	16.152	2143	2147	2150	rBV	457	498	0.13%	0.030%
42	16.851	2261	2266	2267	rBV	398	563	0.15%	0.034%
43	17.075	2302	2304	2307	rBV	428	543	0.15%	0.032%
44	17.216	2326	2328	2332	rBV	550	636	0.17%	0.038%
45	17.474	2366	2372	2374	rBV	429	519	0.14%	0.031%
46	17.498	2374	2376	2380	rVB	661	793	0.21%	0.047%
47	17.533	2380	2382	2384	rBV	661	781	0.21%	0.047%
48	17.756	2412	2420	2427	rBV	232593	345927	93.66%	20.698%
49	17.803	2427	2428	2431	rVB	634	572	0.15%	0.034%
50	17.833	2431	2433	2435	rBV	560	501	0.14%	0.030%
51	17.974	2456	2457	2461	rBV	681	647	0.18%	0.039%
52	18.026	2464	2466	2469	rVB	866	727	0.20%	0.043%
53	18.056	2469	2471	2473	rBV	649	690	0.19%	0.041%
54	18.191	2492	2494	2499	rVB	335	589	0.16%	0.035%
55	18.326	2516	2517	2521	rBV2	556	597	0.16%	0.036%
56	18.373	2523	2525	2528	rVB	738	831	0.22%	0.050%
57	18.496	2543	2546	2547	rBV2	521	486	0.13%	0.029%
58	18.661	2573	2574	2576	rBV	745	477	0.13%	0.029%
59	18.778	2592	2594	2597	rBV	614	528	0.14%	0.032%
60	18.908	2614	2616	2617	rVB	992	478	0.13%	0.029%
61	18.925	2617	2619	2621	rBV2	648	617	0.17%	0.037%
62	18.967	2621	2626	2628	rVB2	755	1202	0.33%	0.072%
63	19.113	2649	2651	2653	rBV	619	522	0.14%	0.031%
64	19.219	2667	2669	2671	rVB	621	477	0.13%	0.029%
65	19.325	2685	2687	2688	rBV	645	454	0.12%	0.027%
66	19.437	2703	2706	2710	rBV2	573	785	0.21%	0.047%
67	19.478	2710	2713	2717	rVV2	933	1048	0.28%	0.063%
68	19.601	2731	2734	2737	rBV3	409	542	0.15%	0.032%
69	19.636	2737	2740	2741	rBV	862	688	0.19%	0.041%
70	19.654	2741	2743	2744	rVB2	1594	849	0.23%	0.051%
71	19.666	2744	2745	2749	rBV3	1145	1266	0.34%	0.076%
72	19.707	2749	2752	2755	rBV2	1205	1950	0.53%	0.117%
73	19.766	2760	2762	2764	rBV2	1537	1794	0.49%	0.107%
74	19.883	2780	2782	2783	rBV	944	574	0.16%	0.034%
75	19.965	2794	2796	2797	rBV	1566	1300	0.35%	0.078%
76	20.194	2834	2835	2836	rBV	2145	822	0.22%	0.049%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
 Data File : BG056761.D
 Acq On : 28 Feb 2023 19:06
 Operator : CG/JU
 Sample : 01674-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

77	20.506	2886	2888	2890	rBV3	2149	1972	0.53%	0.118%
78	20.529	2890	2892	2893	rVV	2522	1216	0.33%	0.073%
79	20.547	2893	2895	2898	rVV4	2708	3130	0.85%	0.187%
80	22.063	3146	3153	3161	rBV2	203053	369348	100.00%	22.099%
81	23.402	3379	3381	3382	rBV2	3445	2660	0.72%	0.159%
82	25.230	3690	3692	3696	rVB4	2443	2502	0.68%	0.150%
83	25.582	3742	3752	3765	rVB2	114538	352126	95.34%	21.069%
84	27.621	4097	4099	4101	rBV3	2735	1663	0.45%	0.100%
85	27.838	4135	4136	4137	rBV	2420	1239	0.34%	0.074%
86	28.273	4208	4210	4213	rBV4	2611	1819	0.49%	0.109%
87	29.871	4480	4482	4485	rVB3	3212	2860	0.77%	0.171%
88	30.130	4525	4526	4527	rBV	2368	1250	0.34%	0.075%
89	32.433	4916	4918	4919	rVB2	3078	1365	0.37%	0.082%




Sum of corrected areas: 1671312

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
Data File : BG056761.D
Acq On : 28 Feb 2023 19:06
Operator : CG/JU
Sample : 01674-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

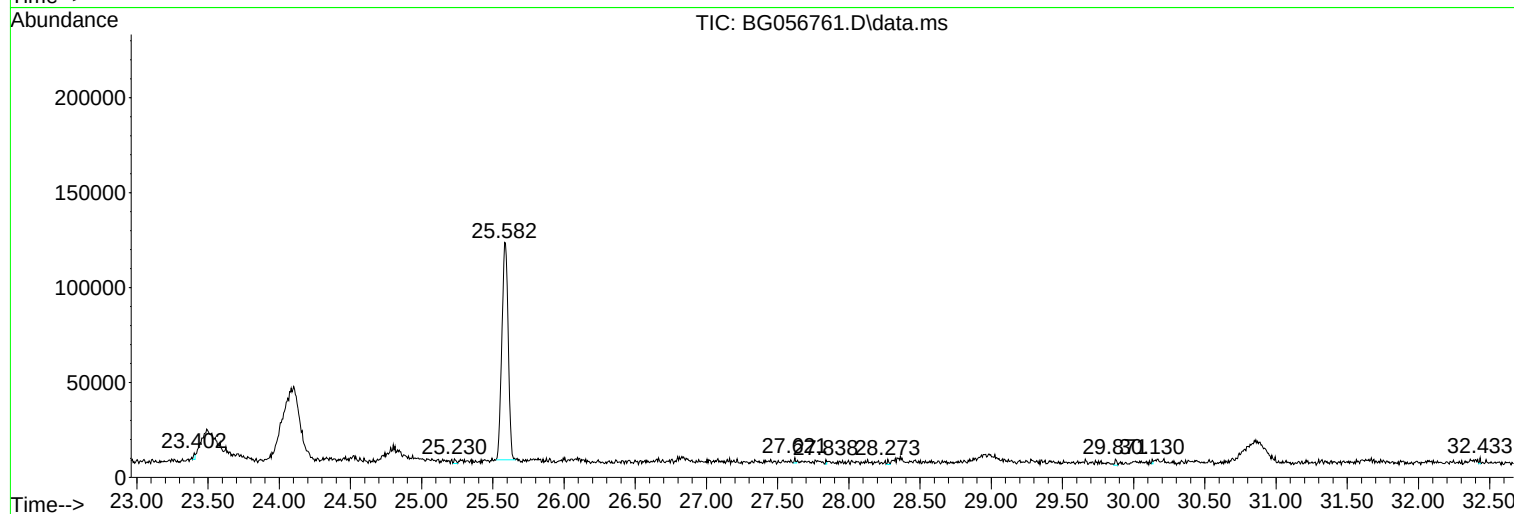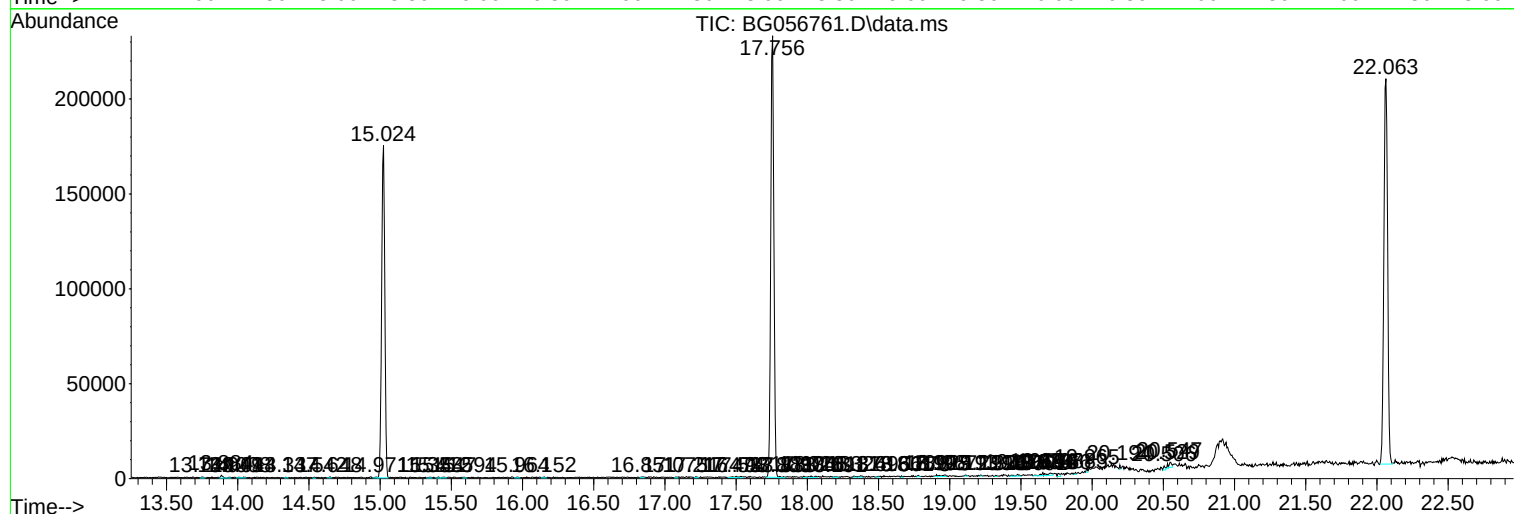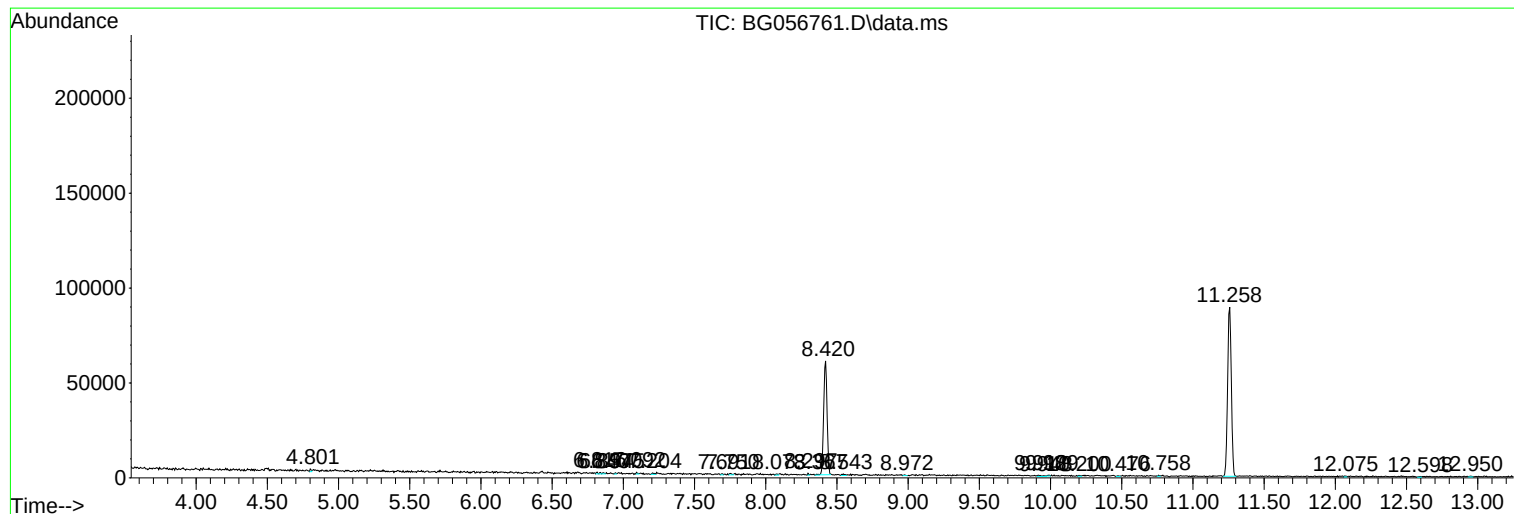

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
Data File : BG056761.D
Acq On : 28 Feb 2023 19:06
Operator : CG/JU
Sample : 01674-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
Data File : BG056761.D
Acq On : 28 Feb 2023 19:06
Operator : CG/JU
Sample : 01674-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc