


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022823\
Data File : BG056748.D
Acq On : 28 Feb 2023 8:38
Operator : CG/JU
Sample : DFTPP495
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP495

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Title : SVOA CALIBRATION
Last Update : Tue Feb 28 23:55:08 2023

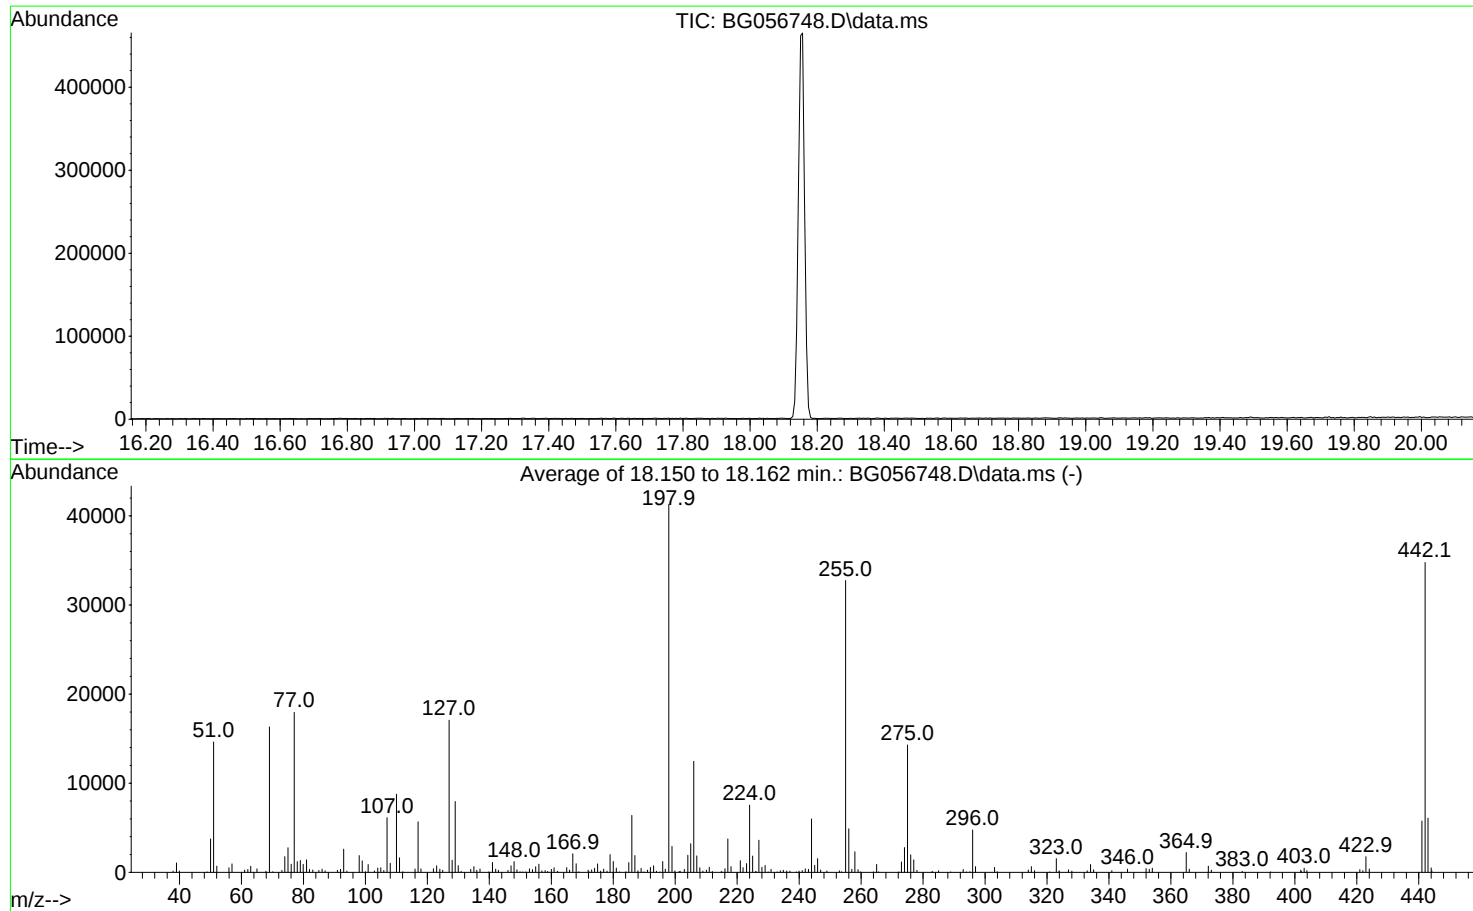

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	14628	PASS
68	69	0.00	2	0.8	130	PASS
69	198	0.00	100	39.5	16325	PASS
70	69	0.00	2	0.4	64	PASS
127	198	10	80	41.4	17074	PASS
197	198	0.00	2	0.9	352	PASS
198	198	100	100	100.0	41280	PASS
199	198	5	9	7.0	2904	PASS
275	198	10	60	34.6	14298	PASS
365	198	1	100	5.4	2222	PASS
441	198	0.01	100	14.0	5761	PASS
442	198	50	100	84.3	34789	PASS
443	442	15	24	17.5	6083	PASS

m/z	Abundance
44.00	859.0
206.90	155.0

Instrument :

BNA_G

ClientSampleId :

DFTPP495

m/z	Abundance
37.90	283.0
39.00	1583.0
40.00	209.0
43.90	825.0
50.00	5109.0
51.00	18968.0
52.10	904.0
56.00	767.0
57.00	1260.0
61.00	370.0
62.10	409.0
63.00	851.0
65.00	560.0
67.90	390.0
69.00	21976.0
70.10	192.0
73.10	197.0
74.00	2402.0
75.00	3395.0
76.10	1110.0
77.00	22288.0
78.00	1739.0
79.00	1889.0
79.90	1235.0
81.00	2001.0
81.90	406.0
83.00	441.0
85.00	221.0
86.00	385.0
87.00	279.0
91.00	347.0
92.00	428.0
93.00	3262.0
94.00	251.0
98.00	2226.0
99.00	1821.0
100.00	241.0
100.90	964.0
103.00	286.0
104.00	570.0
105.00	811.0
105.90	318.0
107.00	7581.0
108.00	1355.0
110.00	10860.0
111.00	2246.0
116.00	467.0
117.00	6766.0
117.90	545.0
122.00	426.0
123.00	991.0
124.00	478.0
125.00	176.0
127.00	20328.0
128.00	1696.0
129.00	9276.0
130.00	953.0
130.90	154.0
134.00	350.0
135.00	777.0
135.90	322.0
137.00	342.0
139.80	172.0
141.00	1445.0
142.00	355.0
142.90	156.0
146.00	322.0
147.00	991.0
148.00	1294.0
148.90	235.0
149.90	207.0
150.80	160.0
151.80	183.0
152.90	479.0
153.90	444.0
154.90	583.0
156.00	1048.0
156.90	269.0
158.10	203.0
158.90	162.0
160.00	340.0
160.90	645.0
162.00	192.0
164.90	814.0
165.90	313.0
166.90	2784.0
168.00	952.0
168.90	237.0
172.00	392.0
173.10	275.0
173.90	447.0
175.00	1114.0

Instrument :
BNA_G
ClientSampleId :
DFTPP495

175.90	249.0
176.90	303.0
178.10	246.0
179.00	2387.0
180.00	1295.0
181.00	522.0
182.00	151.0
184.10	241.0
185.00	1376.0
186.00	7136.0
187.00	2125.0
187.90	254.0
189.00	522.0
191.10	264.0
192.00	754.0
193.00	725.0
193.90	191.0
195.10	170.0
196.00	1336.0
196.90	523.0
198.00	47040.0
198.90	3311.0
199.90	198.0
201.60	216.0
202.90	396.0
204.00	2526.0
205.00	3946.0
206.00	14940.0
207.00	2355.0
208.00	629.0
208.90	249.0
210.10	352.0
211.00	734.0
211.90	167.0
214.80	183.0
216.00	492.0
217.00	4763.0
218.00	868.0
221.00	1659.0
221.90	588.0
223.00	1070.0
224.00	8411.0
225.00	2436.0
225.90	262.0
227.00	4224.0
228.00	658.0
229.00	883.0
231.00	386.0
232.90	154.0
233.90	406.0
234.90	421.0
236.10	270.0
237.00	205.0
240.00	201.0
241.00	260.0
242.00	377.0
243.00	318.0
244.00	6509.0
245.00	929.0
246.00	1884.0
247.00	415.0
249.00	278.0
253.00	155.0
255.00	36472.0
256.00	5160.0
257.00	485.0
258.00	2486.0
259.10	364.0
259.80	177.0
265.00	1070.0
273.00	1158.0
274.00	2843.0
275.00	16219.0
276.00	2133.0
277.00	1778.0
278.00	186.0
282.90	208.0
293.00	217.0
294.00	181.0
295.10	203.0
296.00	5405.0
296.90	677.0
303.10	518.0
314.00	201.0
314.90	647.0
316.00	227.0
320.90	159.0
323.00	1492.0
323.90	247.0
327.00	233.0
328.00	209.0
333.00	156.0
334.00	947.0
335.00	342.0
340.90	208.0
346.00	270.0

Instrument :
BNA_G
ClientSampleId :
DFTPP495

352.00	456.0
353.00	389.0
354.00	463.0
365.00	2197.0
365.90	429.0
372.00	605.0
373.10	271.0
392.20	180.0
401.90	383.0
403.10	350.0
403.90	166.0
421.00	199.0
422.00	320.0
422.90	1730.0
424.10	475.0
441.00	5577.0
442.10	33056.0
443.00	5915.0
444.00	699.0

Instrument :
BNA_G
ClientSampleId :
DFTPP495

m/z	Abundance
38.00	158.0
39.00	1092.0
39.90	279.0
44.00	793.0
48.90	174.0
50.00	3993.0
51.00	16384.0
52.00	866.0
55.90	642.0
56.90	1199.0
61.00	209.0
62.00	333.0
63.00	705.0
65.00	438.0
69.00	18016.0
73.00	233.0
74.00	2122.0
75.00	3314.0
76.00	1054.0
77.00	20760.0
78.00	1383.0
79.00	1358.0
79.90	965.0
81.00	1369.0
82.00	357.0
83.00	363.0
85.00	269.0
86.00	470.0
87.00	267.0
90.90	378.0
91.90	404.0
93.00	2925.0
94.00	191.0
98.00	2444.0
99.00	1376.0
100.90	1085.0
102.80	223.0
103.90	553.0
104.90	483.0
106.00	313.0
107.00	7025.0
108.00	1061.0
110.00	10354.0
111.00	1865.0
112.10	210.0
116.10	451.0
117.00	7004.0
118.00	406.0
121.90	473.0
123.00	885.0
124.00	382.0
124.90	272.0
127.00	20216.0
128.00	1693.0
129.00	9444.0
129.90	868.0
130.90	179.0
134.00	469.0
135.00	744.0
136.00	383.0
137.10	498.0
141.00	1294.0
142.10	475.0
142.90	305.0
146.00	384.0
147.00	739.0
148.00	1625.0
148.90	432.0
153.00	346.0
153.90	287.0
155.00	884.0
156.00	1100.0
157.00	214.0
158.10	167.0
158.80	172.0
160.00	400.0
160.90	551.0
162.10	200.0
165.00	542.0
165.90	439.0
167.00	2230.0
168.00	1219.0
171.90	211.0
172.20	213.0
172.90	284.0
174.00	592.0
174.90	1096.0
175.90	180.0
176.90	563.0
177.90	199.0
178.90	2298.0
180.00	1579.0

Instrument :
BNA_G
ClientSampleId :
DFTPP495

181.00	632.0
185.00	1248.0
186.00	7749.0
187.00	2292.0
188.00	291.0
189.00	536.0
189.90	175.0
191.00	361.0
192.00	491.0
193.00	953.0
194.00	195.0
195.90	1590.0
196.70	533.0
197.90	49112.0
199.00	3170.0
199.90	294.0
201.30	329.0
203.00	330.0
204.10	1881.0
205.00	3602.0
206.00	14923.0
207.00	2266.0
207.90	504.0
209.00	208.0
210.00	404.0
211.00	629.0
212.00	169.0
215.00	277.0
216.10	420.0
217.00	4245.0
218.00	762.0
221.00	1372.0
221.90	650.0
223.00	1117.0
224.00	8625.0
225.00	1964.0
226.10	218.0
227.00	4257.0
228.00	680.0
229.00	973.0
230.00	169.0
230.90	468.0
233.90	162.0
234.90	270.0
235.90	211.0
237.00	242.0
239.10	171.0
239.90	247.0
241.00	316.0
242.00	580.0
243.00	497.0
244.00	7258.0
245.00	971.0
245.90	1662.0
246.80	217.0
248.90	231.0
253.00	170.0
255.00	38504.0
256.00	5880.0
257.00	322.0
258.00	2756.0
258.90	366.0
264.00	166.0
265.00	1017.0
272.20	190.0
273.00	1562.0
274.00	3266.0
275.00	16302.0
276.00	2315.0
277.00	1552.0
278.10	203.0
283.10	209.0
285.00	314.0
288.90	156.0
293.00	493.0
296.00	5400.0
297.00	874.0
303.00	608.0
303.90	204.0
313.90	348.0
315.00	887.0
316.00	392.0
323.00	1765.0
323.90	284.0
327.00	374.0
328.00	215.0
332.90	184.0
334.10	1017.0
335.10	320.0
341.00	379.0
346.00	561.0
352.00	456.0
353.00	320.0
354.00	603.0
365.00	2756.0
366.00	300.0

Instrument :
BNA_G
ClientSampleId :
DFTPP495

372.10	951.0
373.00	292.0
383.00	358.0
401.90	364.0
403.00	525.0
404.00	258.0
420.90	458.0
423.00	1864.0
424.00	381.0
441.00	6826.0
442.00	40968.0
443.00	7215.0
444.00	798.0

Instrument :
BNA_G
ClientSampleId :
DFTPP495

m/z	Abundance
39.00	501.0
44.00	696.0
50.00	2158.0
51.00	8531.0
51.90	326.0
55.90	177.0
56.90	425.0
60.90	190.0
62.10	223.0
63.00	482.0
65.00	167.0
69.00	8982.0
73.00	237.0
74.00	736.0
74.90	1585.0
76.00	559.0
77.00	10844.0
78.00	494.0
78.90	733.0
79.90	517.0
80.90	843.0
82.00	186.0
84.90	160.0
86.00	208.0
92.00	207.0
93.00	1603.0
98.00	988.0
98.80	677.0
100.90	576.0
104.10	330.0
105.00	280.0
107.00	3796.0
108.00	650.0
110.00	5098.0
110.90	776.0
115.90	240.0
117.00	3272.0
117.90	216.0
122.00	360.0
122.90	312.0
123.90	210.0
125.00	267.0
127.00	10679.0
128.00	708.0
129.00	5120.0
130.00	438.0
134.00	199.0
134.90	392.0
136.90	309.0
141.00	607.0
142.00	239.0
142.90	240.0
147.10	482.0
147.90	677.0
148.90	211.0
152.90	347.0
154.00	200.0
155.00	413.0
156.00	582.0
157.90	226.0
160.00	273.0
161.00	371.0
165.00	265.0
167.00	1266.0
168.00	726.0
171.80	165.0
173.10	286.0
174.00	361.0
175.00	640.0
177.00	195.0
179.00	1317.0
180.00	797.0
181.00	328.0
185.00	679.0
186.00	4313.0
187.00	1268.0
189.00	303.0
191.00	153.0
192.00	448.0
193.00	534.0
196.00	757.0
198.00	27688.0
198.90	2230.0
201.60	155.0
203.00	318.0
204.00	1355.0
205.00	2077.0
206.00	7542.0
207.00	1408.0
207.90	411.0
211.10	342.0
216.00	312.0

Instrument :
BNA_G
ClientSampleId :
DFTPP495

217.00	2265.0
218.00	328.0
221.00	880.0
221.80	358.0
223.00	763.0
224.00	5602.0
225.00	1089.0
227.00	2360.0
228.00	371.0
228.90	442.0
231.00	192.0
242.10	226.0
243.00	218.0
244.00	4228.0
245.00	458.0
245.90	1073.0
247.00	162.0
253.00	213.0
253.70	211.0
255.00	23264.0
256.00	3623.0
257.00	195.0
257.90	1689.0
258.90	197.0
265.00	606.0
265.70	171.0
272.90	804.0
274.00	2258.0
275.00	10372.0
276.00	1495.0
276.90	883.0
278.00	294.0
285.00	225.0
292.90	255.0
296.00	3445.0
296.90	369.0
303.00	565.0
313.90	243.0
315.00	421.0
323.00	1357.0
324.10	211.0
326.80	273.0
333.00	190.0
334.00	692.0
335.00	209.0
346.10	238.0
352.00	402.0
353.00	337.0
354.00	314.0
364.90	1714.0
365.80	344.0
372.00	559.0
373.10	187.0
402.10	336.0
402.90	507.0
403.80	157.0
421.10	280.0
421.90	264.0
423.00	1679.0
424.00	302.0
441.00	4879.0
442.00	30344.0
443.00	5120.0
444.20	526.0

Instrument :
BNA_G
ClientSampleId :
DFTPP495