

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG030119\
 Data File : BG039718.D
 Acq On : 2 Mar 2019 11:22
 Operator : JU/SJ
 Sample : K1675-36
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 Z-3-13-B

Quant Time: Mar 04 00:06:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 01 06:15:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	53499	20.00	ng	0.00
21) Naphthalene-d8	10.98	136	234361	20.00	ng	0.00
39) Acenaphthene-d10	14.79	164	152769	20.00	ng	0.00
64) Phenanthrene-d10	17.53	188	344182	20.00	ng	0.00
76) Chrysene-d12	21.82	240	357285	20.00	ng	-0.01
87) Perylene-d12	25.20	264	331192	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.71	112	401410	128.42	ng	0.00
7) Phenol-d6	7.31	99	520358	113.09	ng	0.00
23) Nitrobenzene-d5	9.34	82	383121	102.13	ng	0.00
42) 2,4,6-Tribromophenol	16.28	330	189920	115.45	ng	0.00
45) 2-Fluorobiphenyl	13.41	172	910501	85.50	ng	0.00
79) Terphenyl-d14	20.12	244	1349253	79.93	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG030119\
Data File : BG039718.D
Acq On : 2 Mar 2019 11:22
Operator : JU/SJ
Sample : K1675-36
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
Z-3-13-B

Quant Time: Mar 04 00:06:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 06:15:02 2019
Response via : Initial Calibration

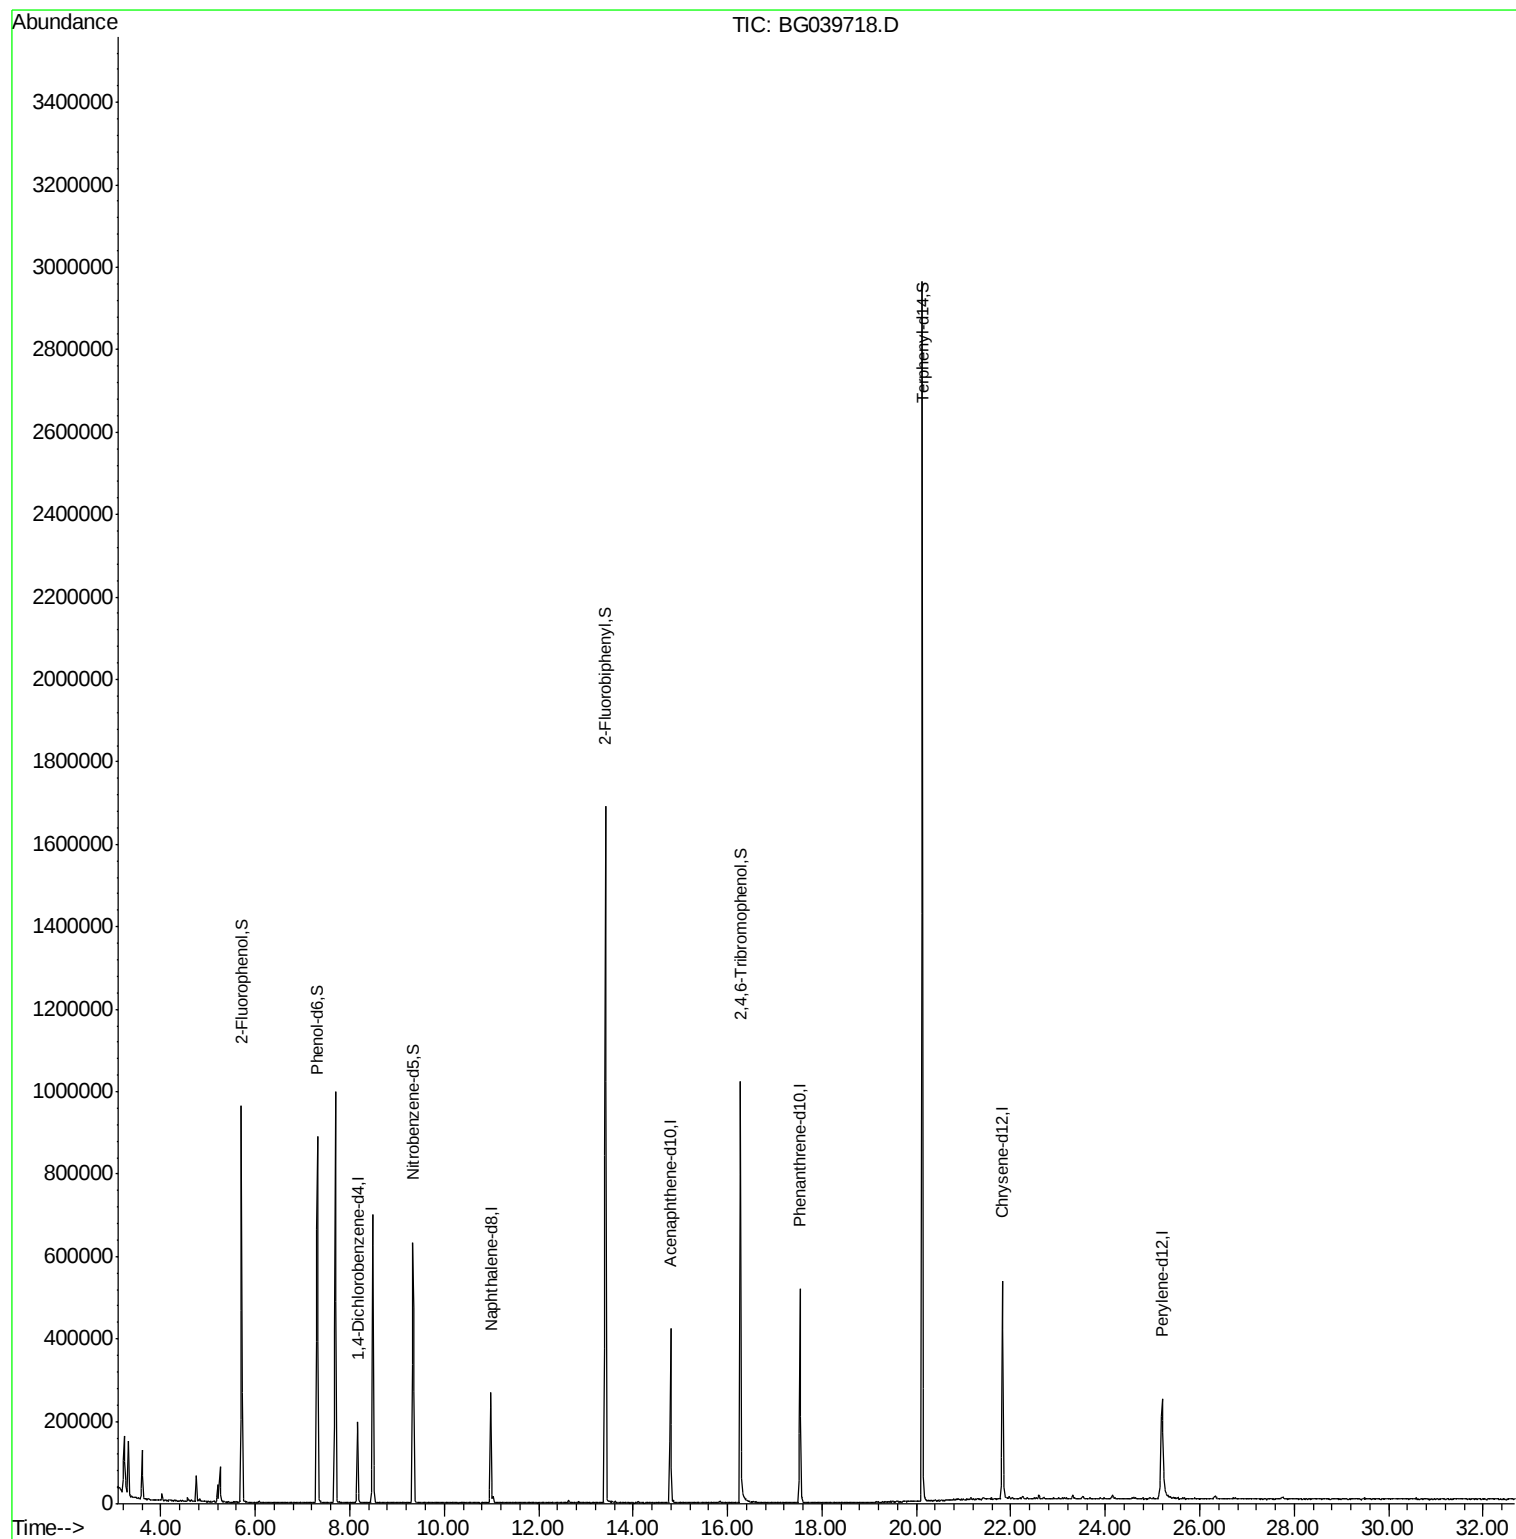

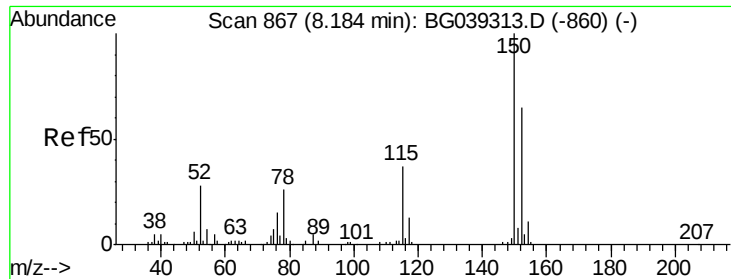


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.16 min Scan# 864
Delta R.T. -0.01 min
Lab File: BG039718.D
Acq: 2 Mar 2019 11:22

Instrument :
BNA_G
ClientSampleId :
Z-3-13-B

Tot Ion	Ratio	Lower	Upper
152	100		
150	161.9	123.7	185.5
115	65.6	45.9	68.9


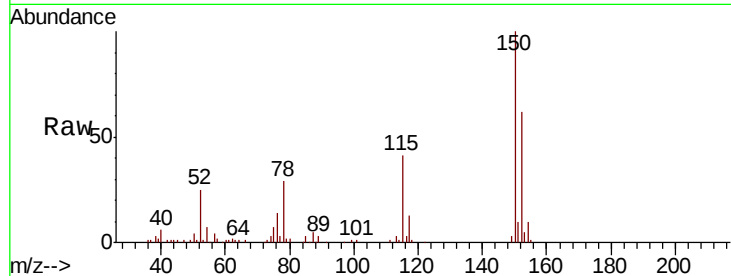


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

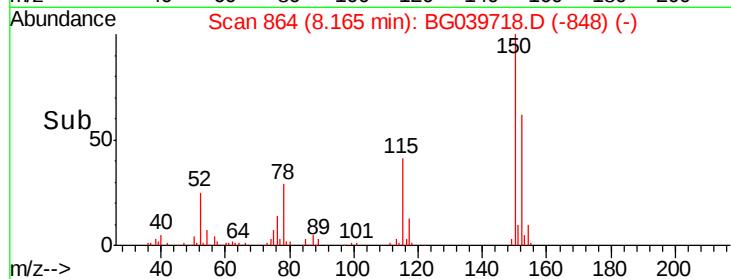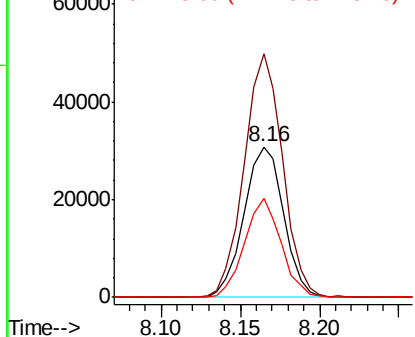

#5

2-Fluorophenol
Concen: 128.417 ng
RT: 5.71 min Scan# 446
Delta R.T. 0.00 min
Lab File: BG039718.D
Acq: 2 Mar 2019 11:22

Tgt Ion	Ratio	Lower	Upper
112	100		
64	69.9	57.8	86.8
63	37.6	29.8	44.6


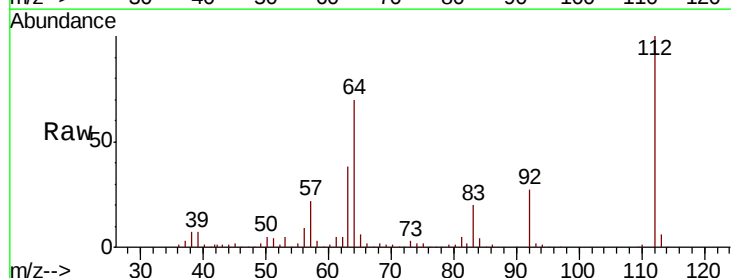


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

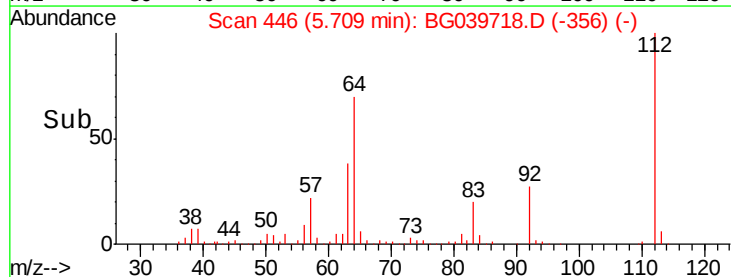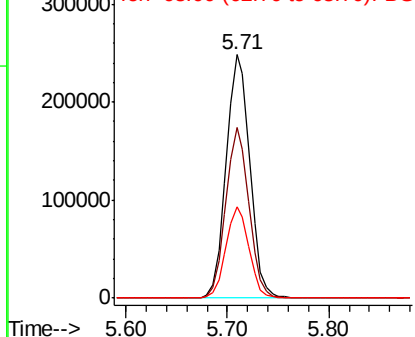



#7

Phenol-d6

Concen: 113.093 ng

RT: 7.31 min Scan# 719

Delta R.T. 0.00 min

Lab File: BG039718.D

Acq: 2 Mar 2019 11:22

Instrument :

BNA_G

ClientSampleId :

Z-3-13-B


Tot Ion: 99 Resp: 520358

Ion Ratio Lower Upper




99 100

42 20.4 18.2 27.2

71 35.9 28.0 42.0

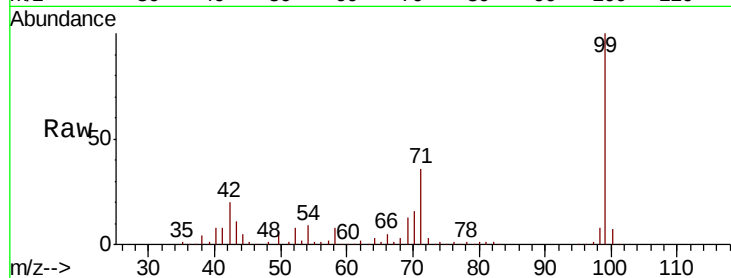

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

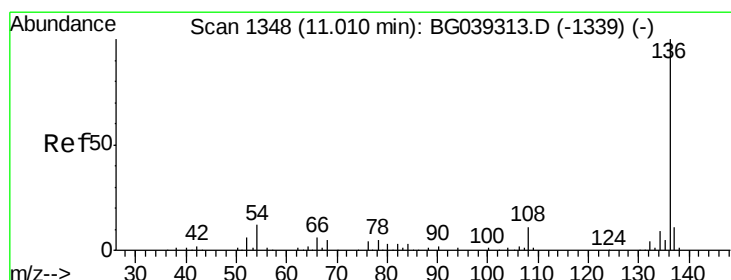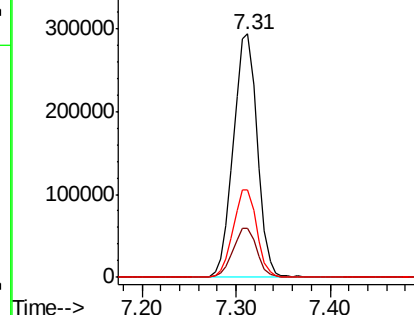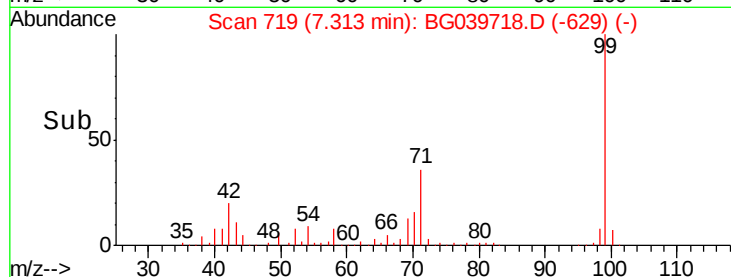

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.98 min Scan# 1344

Delta R.T. -0.01 min

Lab File: BG039718.D

Acq: 2 Mar 2019 11:22

Tgt Ion: 136 Resp: 234361


Ion Ratio Lower Upper

136 100



137 10.4 9.1 13.7

54 10.4 9.4 14.2

68 6.2 4.2 6.4

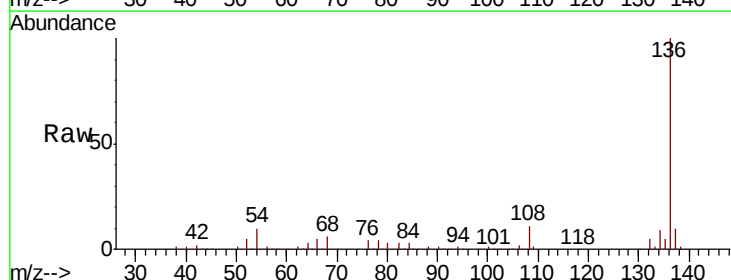

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

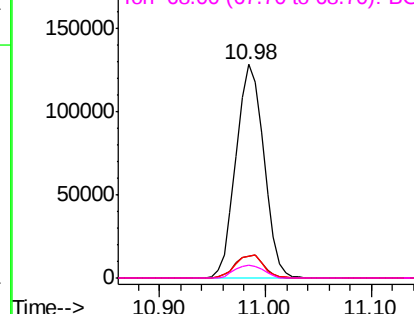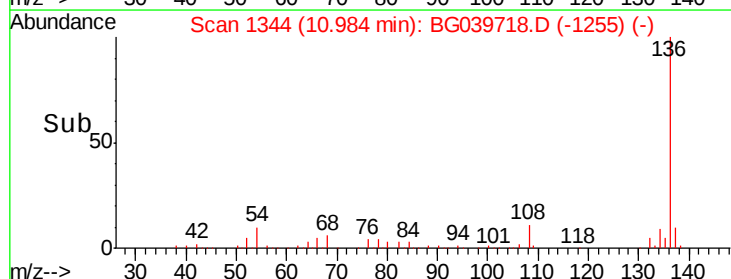



#23

Nitrobenzene-d5

Concen: 102.125 ng

RT: 9.34 min Scan# 1064

Delta R.T. -0.01 min

Lab File: BG039718.D

Acq: 2 Mar 2019 11:22

Instrument :

BNA_G

ClientSampled :

Z-3-13-B


Tot Ion: 82 Resp: 383121

Ion Ratio Lower Upper

82 100

128 41.4 31.3 46.9




54 60.2 50.9 76.3

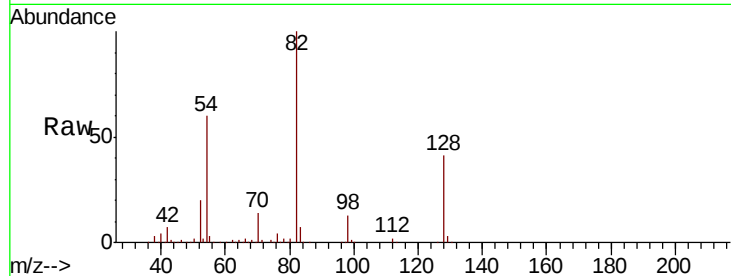

Abundance Ion 82.00 (81.70 to 82.70): BGC

Ion 128.00 (127.70 to 128.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

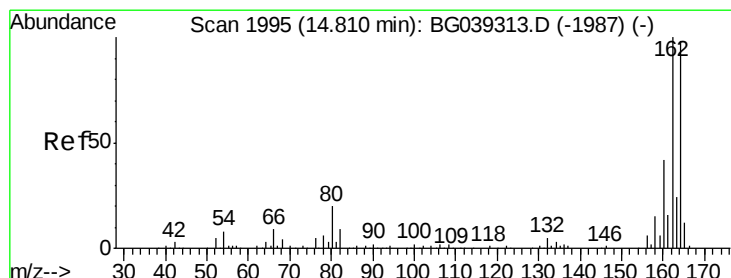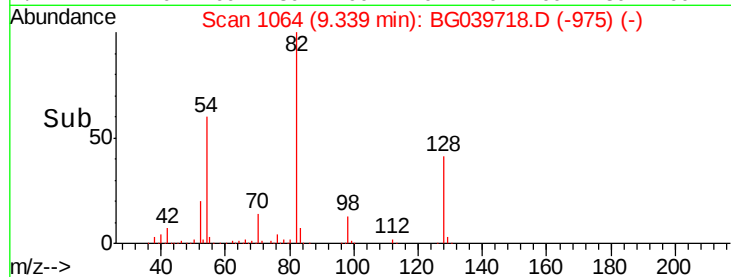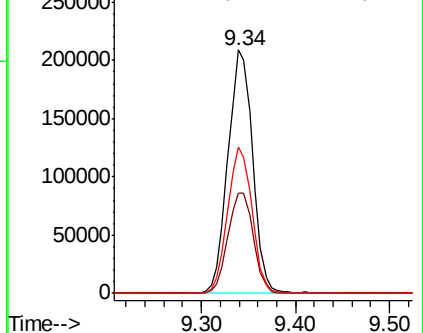

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.79 min Scan# 1992

Delta R.T. 0.00 min

Lab File: BG039718.D

Acq: 2 Mar 2019 11:22


Tgt Ion:164 Resp: 152769

Ion Ratio Lower Upper

164 100

162 103.4 81.6 122.4



160 44.2 34.2 51.2

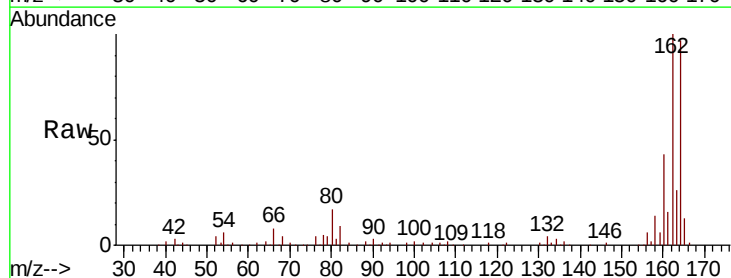


Abundance Ion 164.00 (163.70 to 164.70): BGC

Ion 162.00 (161.70 to 162.70): BGC

Ion 160.00 (159.70 to 160.70): BGC

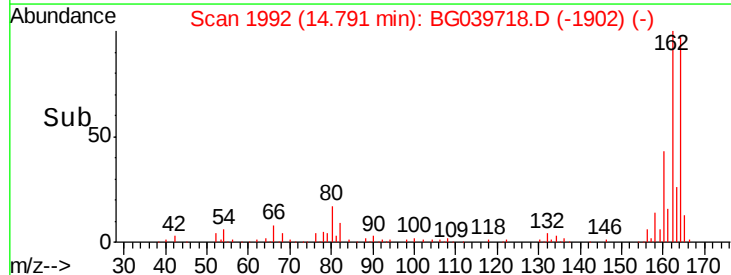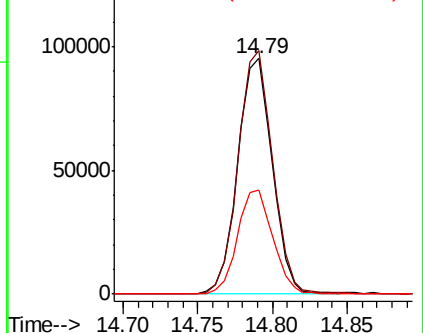


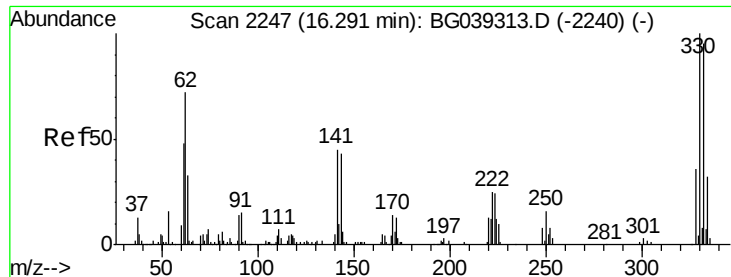




#42
 2,4,6-Tribromophenol
 Concen: 115.449 ng
 RT: 16.28 min Scan# 2245
 Delta R.T. 0.00 min
 Lab File: BG039718.D
 Acq: 2 Mar 2019 11:22

Instrument :
 BNA_G
 ClientSampleId :
 Z-3-13-B

Tot Ion:330 Resp: 189920
 Ion Ratio Lower Upper
 330 100
 332 95.1 75.7 113.5
 141 39.8 35.6 53.4

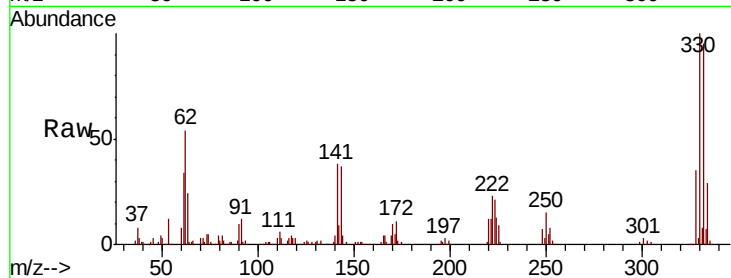


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

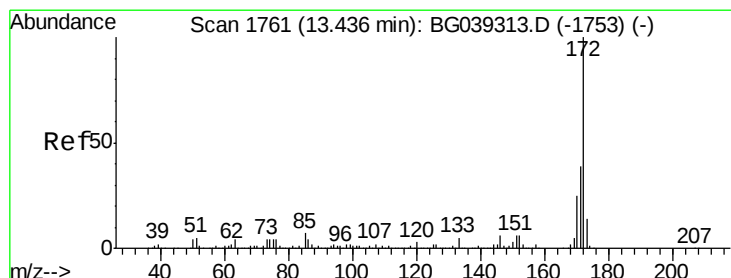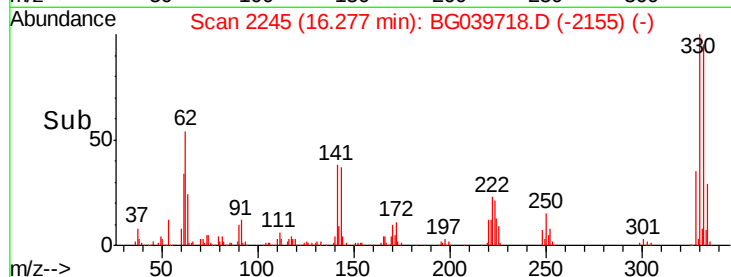
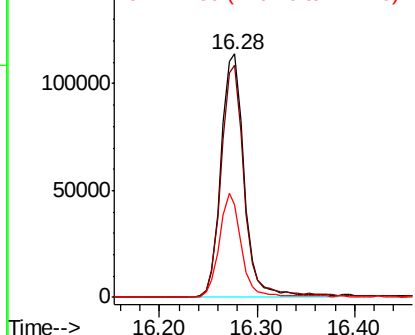


#45
 2-Fluorobiphenyl
 Concen: 85.499 ng
 RT: 13.41 min Scan# 1757
 Delta R.T. -0.01 min
 Lab File: BG039718.D
 Acq: 2 Mar 2019 11:22

Tgt Ion:172 Resp: 910501
 Ion Ratio Lower Upper
 172 100
 171 38.0 30.8 46.2
 170 24.4 20.2 30.4

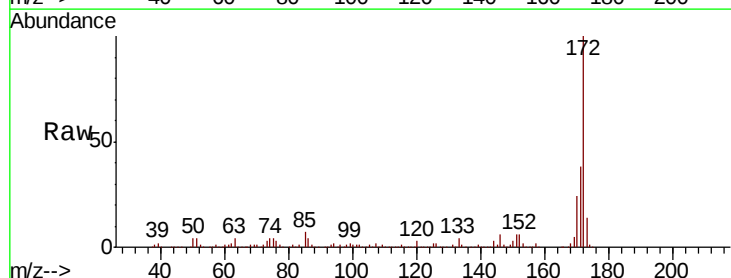

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

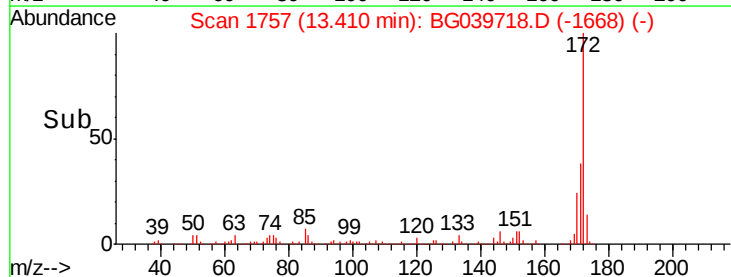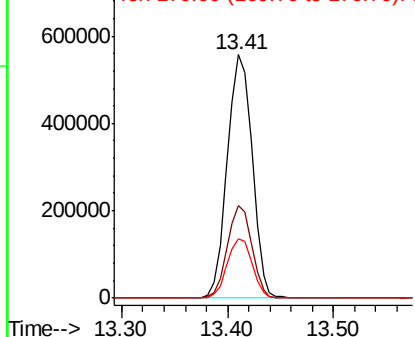



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.53 min Scan# 2458

Delta R.T. -0.01 min

Lab File: BG039718.D

Acq: 2 Mar 2019 11:22

Instrument :

BNA_G

ClientSampleId :

Z-3-13-B


Tot Ion:188 Resp: 344182

Ion Ratio Lower Upper

188 100

94 8.4 6.9 10.3



80 9.3 8.1 12.1

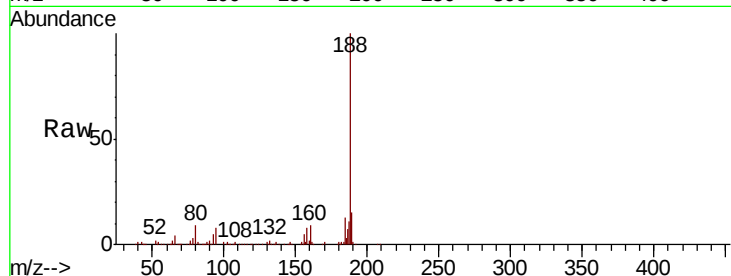

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

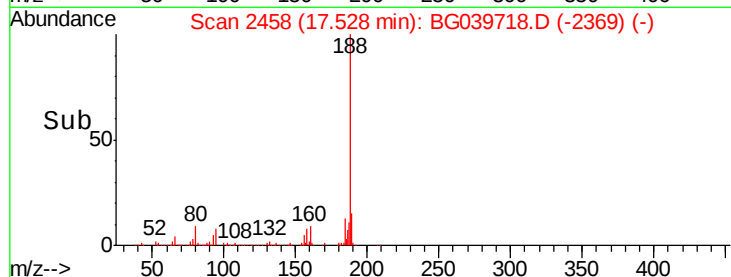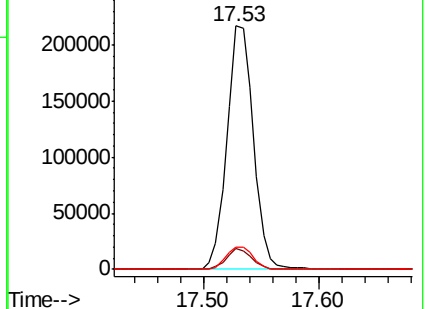

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.82 min Scan# 3188

Delta R.T. -0.01 min

Lab File: BG039718.D

Acq: 2 Mar 2019 11:22


Tgt Ion:240 Resp: 357285

Ion Ratio Lower Upper

240 100

120 8.6 7.0 10.6



236 25.2 21.0 31.4

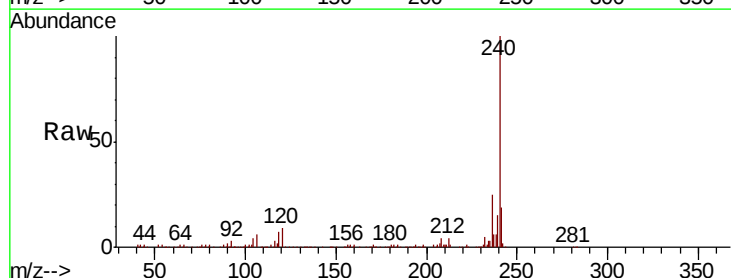


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



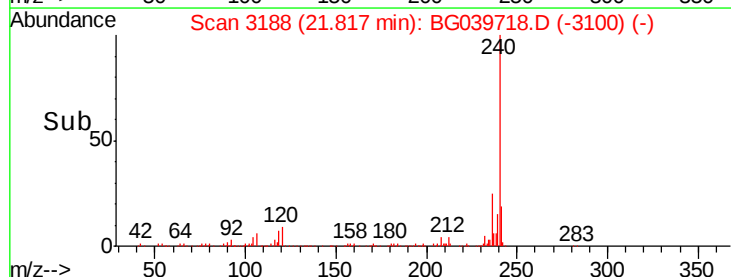
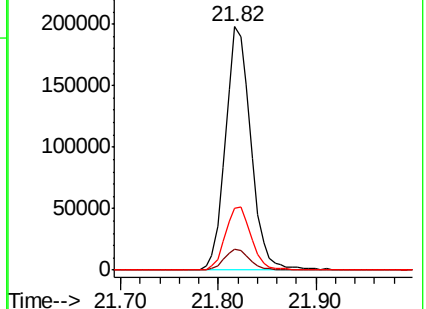


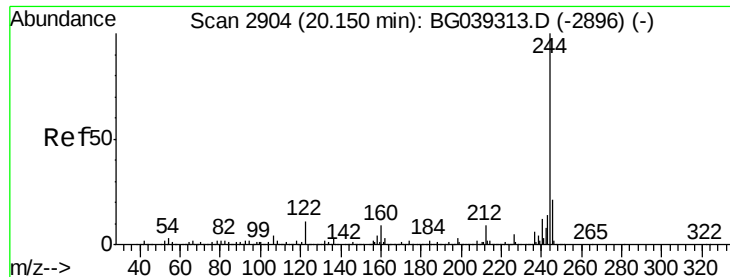

#79
 Terphenyl-d14
 Concen: 79.935 ng
 RT: 20.12 min Scan# 2900
 Delta R.T. 0.00 min
 Lab File: BG039718.D
 Acq: 2 Mar 2019 11:22

Instrument :
 BNA_G
 ClientSampleId :
 Z-3-13-B

Tot Ion:244 Resp: 1349253
 Ion Ratio Lower Upper
 244 100
 212 9.6 7.3 10.9
 122 10.0 8.4 12.6

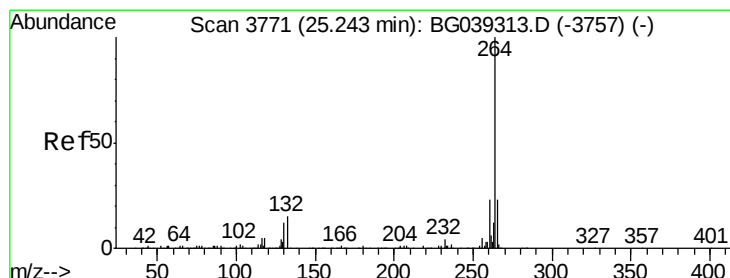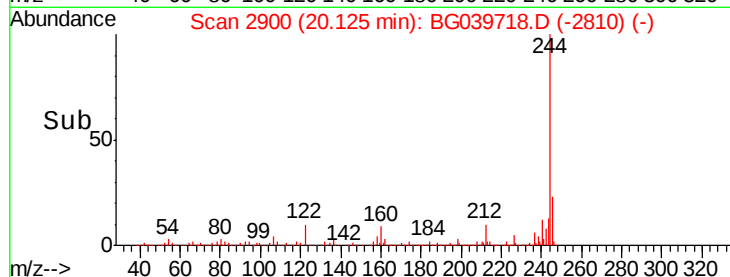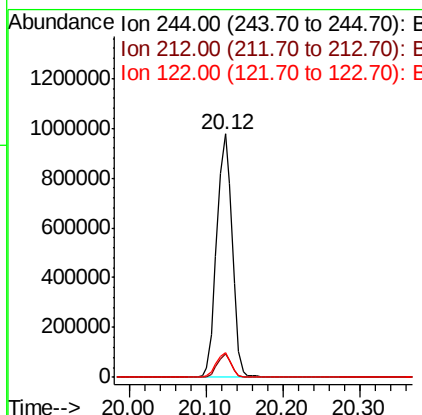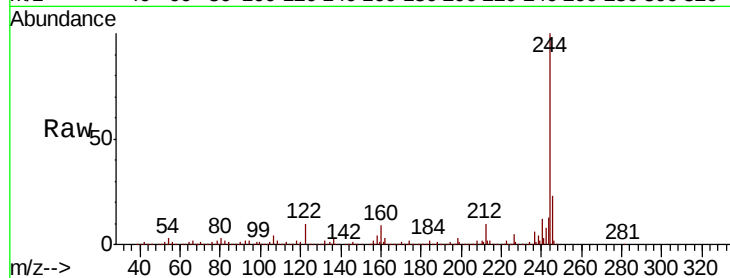

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.20 min Scan# 3764
 Delta R.T. 0.00 min
 Lab File: BG039718.D
 Acq: 2 Mar 2019 11:22

Tgt Ion:264 Resp: 331192
 Ion Ratio Lower Upper
 264 100
 260 22.2 18.2 27.4
 265 20.9 18.5 27.7

