


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG030119\
 Data File : BG039690.D
 Acq On : 1 Mar 2019 16:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 01 06:15:02 2019

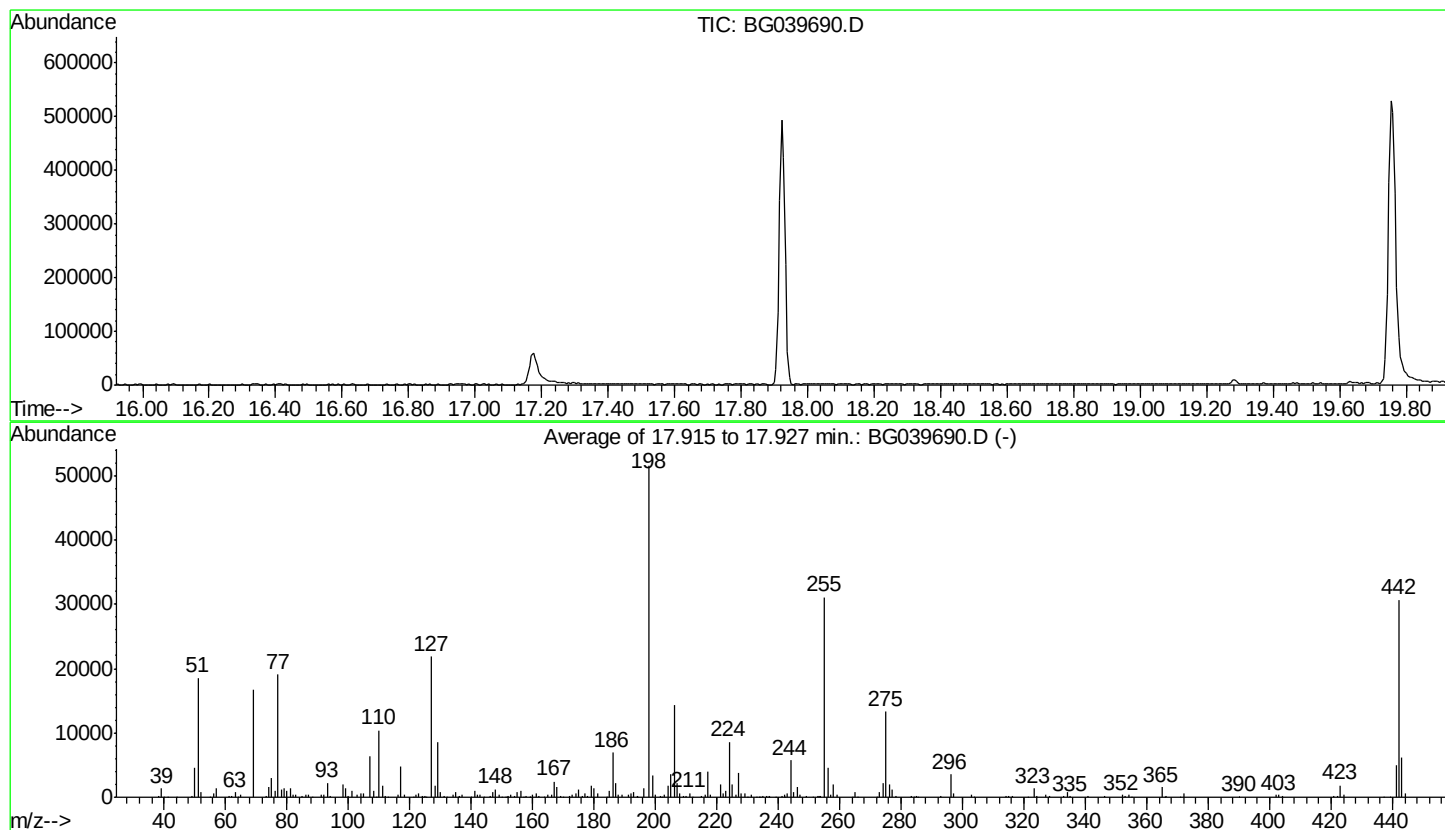

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	18580	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.6	16808	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.4	21864	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51560	PASS
199	198	5	9	6.7	3447	PASS
275	198	10	60	25.8	13278	PASS
365	198	1	100	3.0	1551	PASS
441	198	0.01	100	9.7	4978	PASS
442	198	50	100	59.5	30682	PASS
443	442	15	24	20.0	6144	PASS