


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030119\
 Data File : BG039707.D
 Acq On : 2 Mar 2019 4:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 01 06:15:02 2019

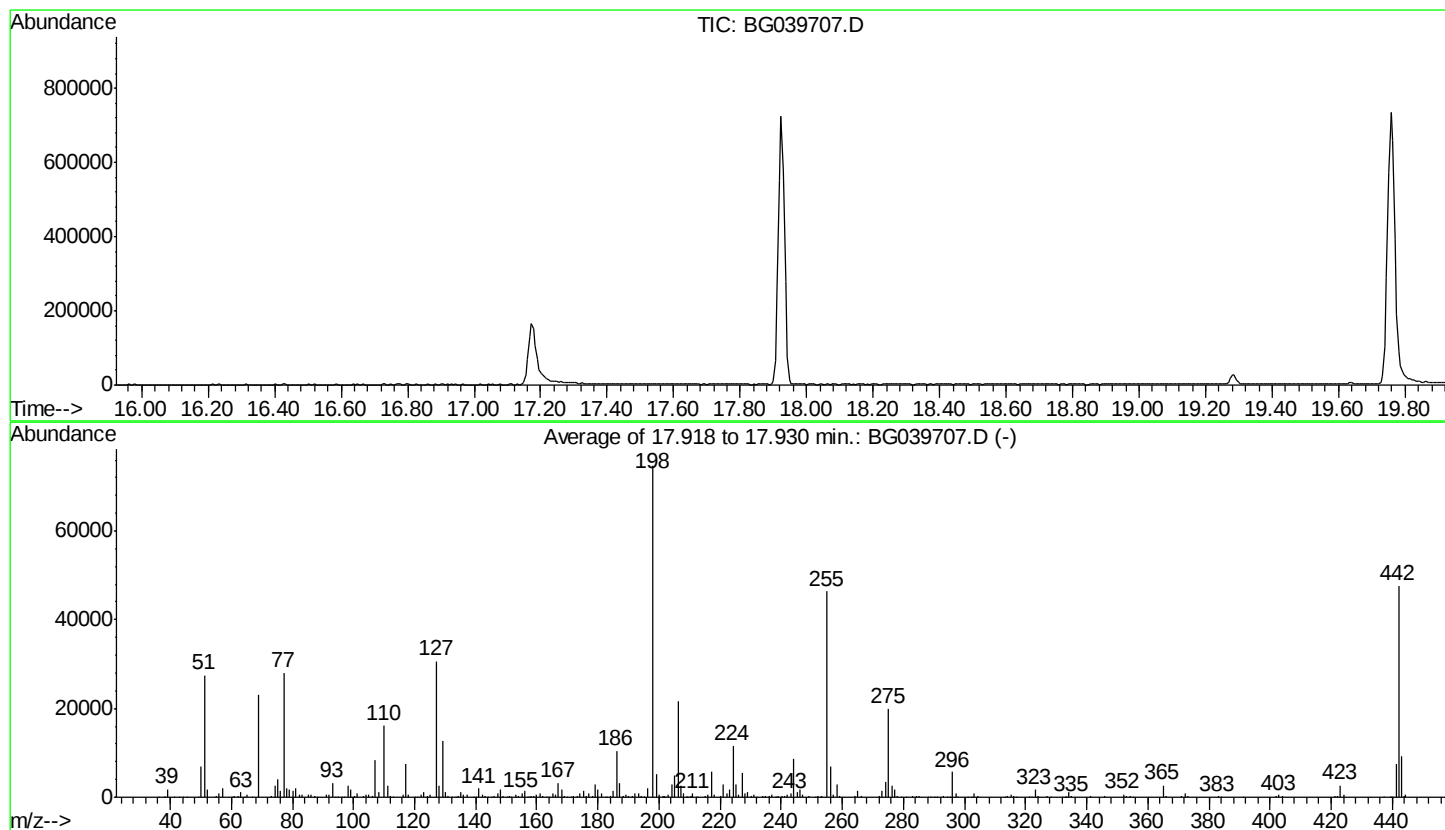

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	27506	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.1	23200	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.1	30672	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74709	PASS
199	198	5	9	7.1	5283	PASS
275	198	10	60	26.7	19970	PASS
365	198	1	100	3.6	2656	PASS
441	198	0.01	100	9.9	7431	PASS
442	198	50	100	63.8	47658	PASS
443	442	15	24	19.2	9135	PASS